




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010459.D
 Acq On : 21 May 2022 05:19
 Operator : CG/JU
 Sample : PB144974BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK974

Manual IntegrationsAPPROVED

Quant Time: May 21 06:05:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

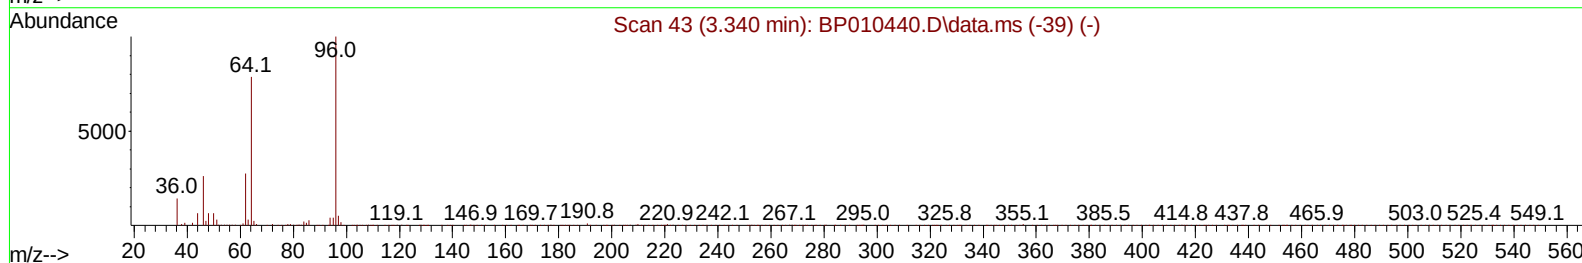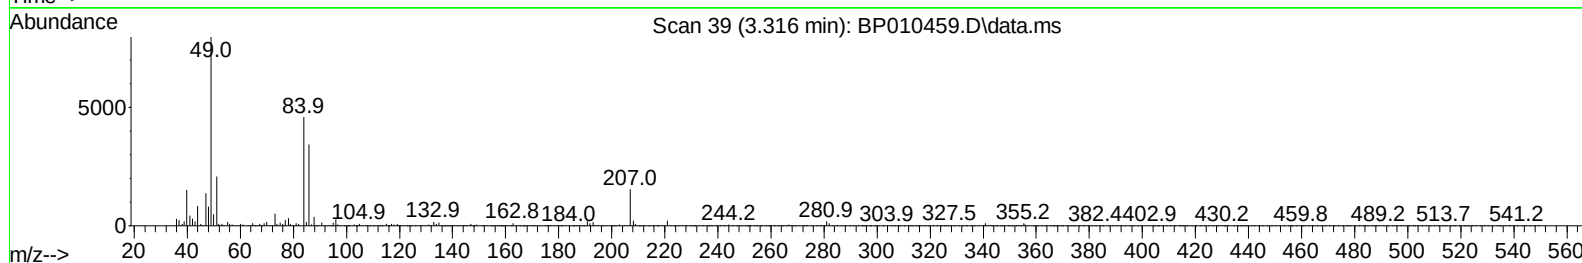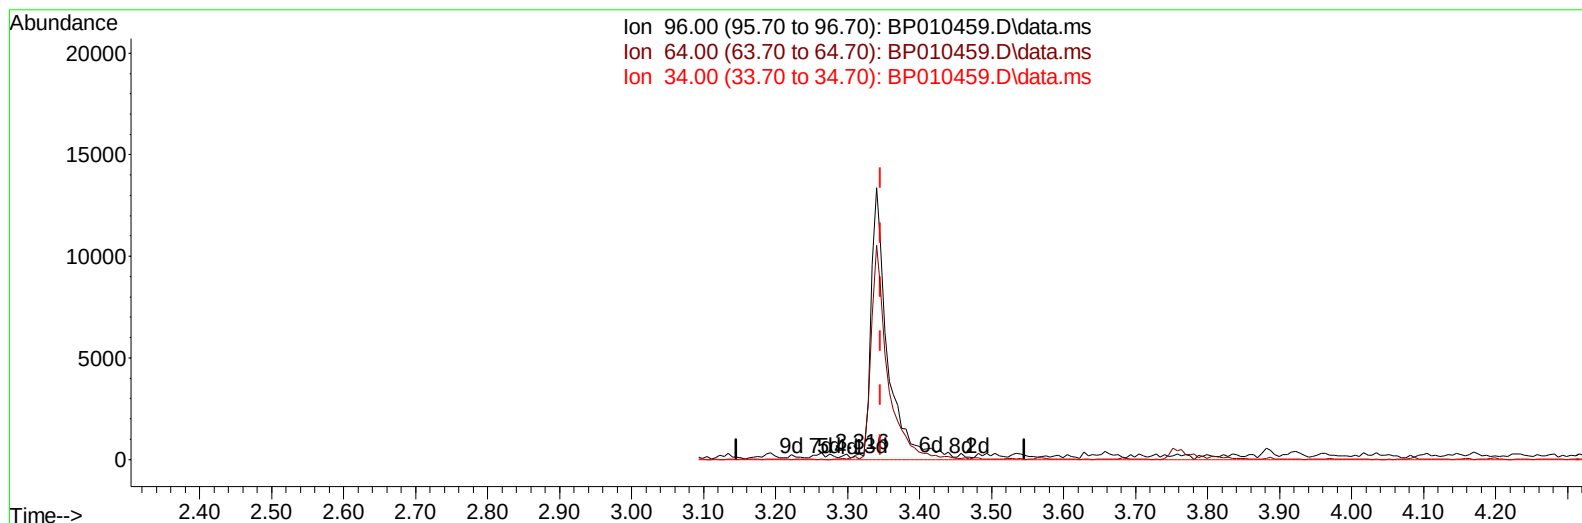

TIC: BP010459.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.316min (-0.030) 0.05 ng/uL

response 196

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	50.92
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010459.D
 Acq On : 21 May 2022 05:19
 Operator : CG/JU
 Sample : PB144974BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK974

Manual IntegrationsAPPROVED

Quant Time: May 21 06:05:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

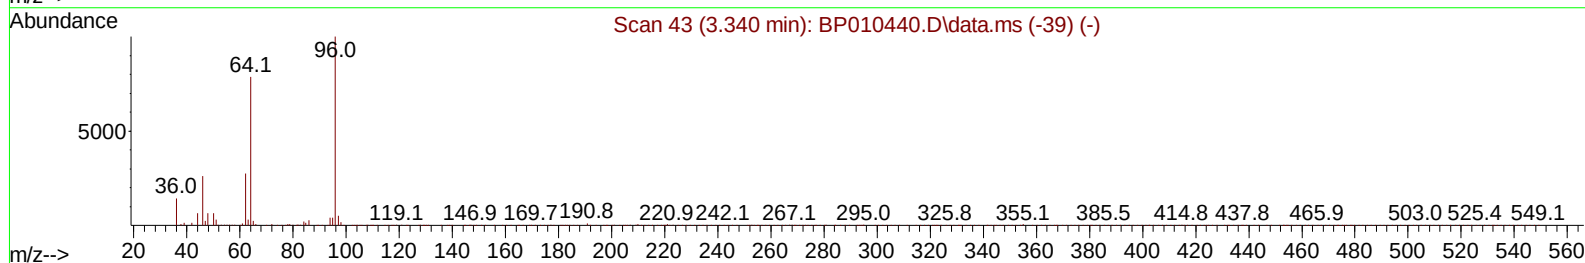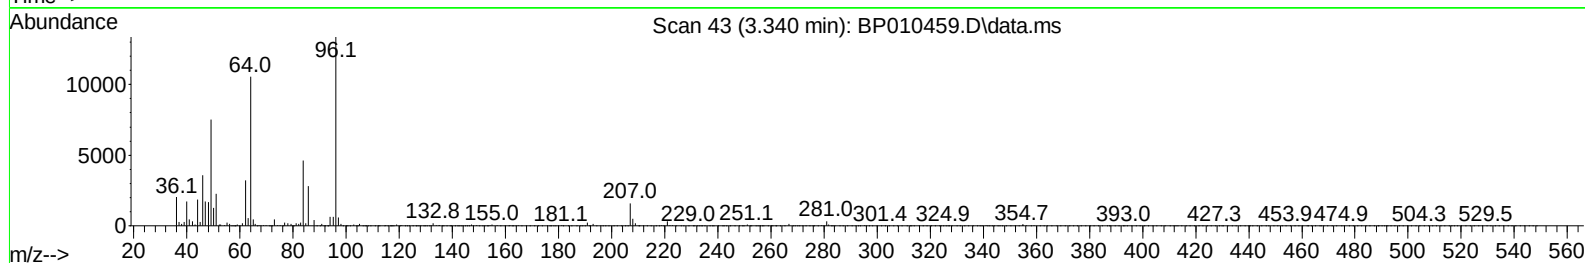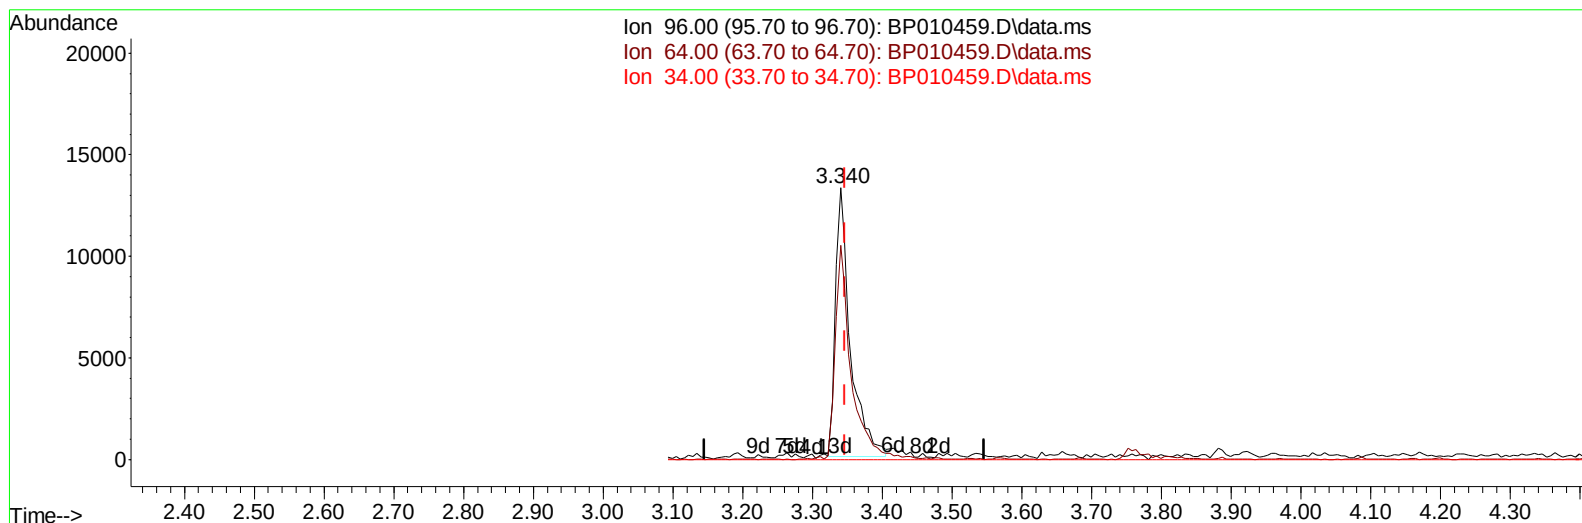

TIC: BP010459.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 5.04 ng/uL m

response 19704

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	78.95#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010459.D
 Acq On : 21 May 2022 05:19
 Operator : CG/JU
 Sample : PB144974BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK974

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 06:05:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	166696	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.687	136	749903	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.522	164	522183	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.275	188	1153538	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.357	240	1126251	20.000	ng/ul	# 0.00
88) Perylene-d12	23.780	264	995787	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	19704m	5.038	ng/uL	0.00
4) Pyridine-d5	3.758	84	305332	27.497	ng/ul	0.00
7) Phenol-d5	7.057	99	384825	27.505	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	267164	28.421	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.422	132	302067	28.215	ng/ul	-0.01
15) 4-Methylphenol-d8	8.599	113	332695	27.980	ng/ul	-0.01
21) Nitrobenzene-d5	9.046	128	166368	28.666	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.769	143	182424	29.660	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.310	165	311880	26.817	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.828	131	459485	26.572	ng/ul	-0.01
46) Dimethylphthalate-d6	13.934	166	1151293	29.925	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160	1273393	28.695	ng/ul	0.00
54) 4-Nitrophenol-d4	14.716	143	159639	23.312	ng/ul	-0.01
60) Fluorene-d10	15.516	176	977599	29.208	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	150208	22.265	ng/ul	0.00
73) Anthracene-d10	17.375	188	1602628	30.682	ng/ul	0.00
81) Pyrene-d10	19.604	212	1958341	32.742	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.621	264	1567811	31.355	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010459.D
Acq On : 21 May 2022 05:19
Operator : CG/JU
Sample : PB144974BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK974

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 21 06:05:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

