

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010445.D
 Acq On : 20 May 2022 20:51
 Operator : CG/JU
 Sample : N2843-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4H9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 20 23:04:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	136618	20.000	ng/u1	0.00
20) Naphthalene-d8	10.693	136	612292	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.522	164	426431	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.275	188	923549	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.357	240	879197	20.000	ng/u1	# 0.00
88) Perylene-d12	23.780	264	815919	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	18025m	5.624	ng/uL	0.00
4) Pyridine-d5	3.758	84	268438	29.497	ng/u1	0.00
7) Phenol-d5	7.058	99	361877	31.559	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	249132	32.338	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	288845	32.920	ng/u1	-0.01
15) 4-Methylphenol-d8	8.599	113	313894	32.211	ng/u1	-0.01
21) Nitrobenzene-d5	9.052	128	156194	32.961	ng/u1	0.00
24) 2-Nitrophenol-d4	9.775	143	170728	33.996	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	300671	31.664	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.828	131	435205m	30.824	ng/u1	-0.01
46) Dimethylphthalate-d6	13.934	166	1042654	33.186	ng/u1	0.00
49) Acenaphthylene-d8	14.216	160	1205521	33.265	ng/u1	0.00
54) 4-Nitrophenol-d4	14.722	143	137680	24.620	ng/u1	0.00
60) Fluorene-d10	15.516	176	903958	33.072	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	121421	22.480	ng/u1	-0.01
73) Anthracene-d10	17.375	188	1391053	33.263	ng/u1	0.00
81) Pyrene-d10	19.604	212	1689374	36.182	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.621	264	1408518	34.379	ng/u1	-0.01

Target Compounds					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.269	149	666883	20.071	ng/u1#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010445.D
Acq On : 20 May 2022 20:51
Operator : CG/JU
Sample : N2843-09
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
EW4H9

Quant Time: May 20 23:04:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 05/23/2022
Supervised By :mohammad ahmed 05/25/2022

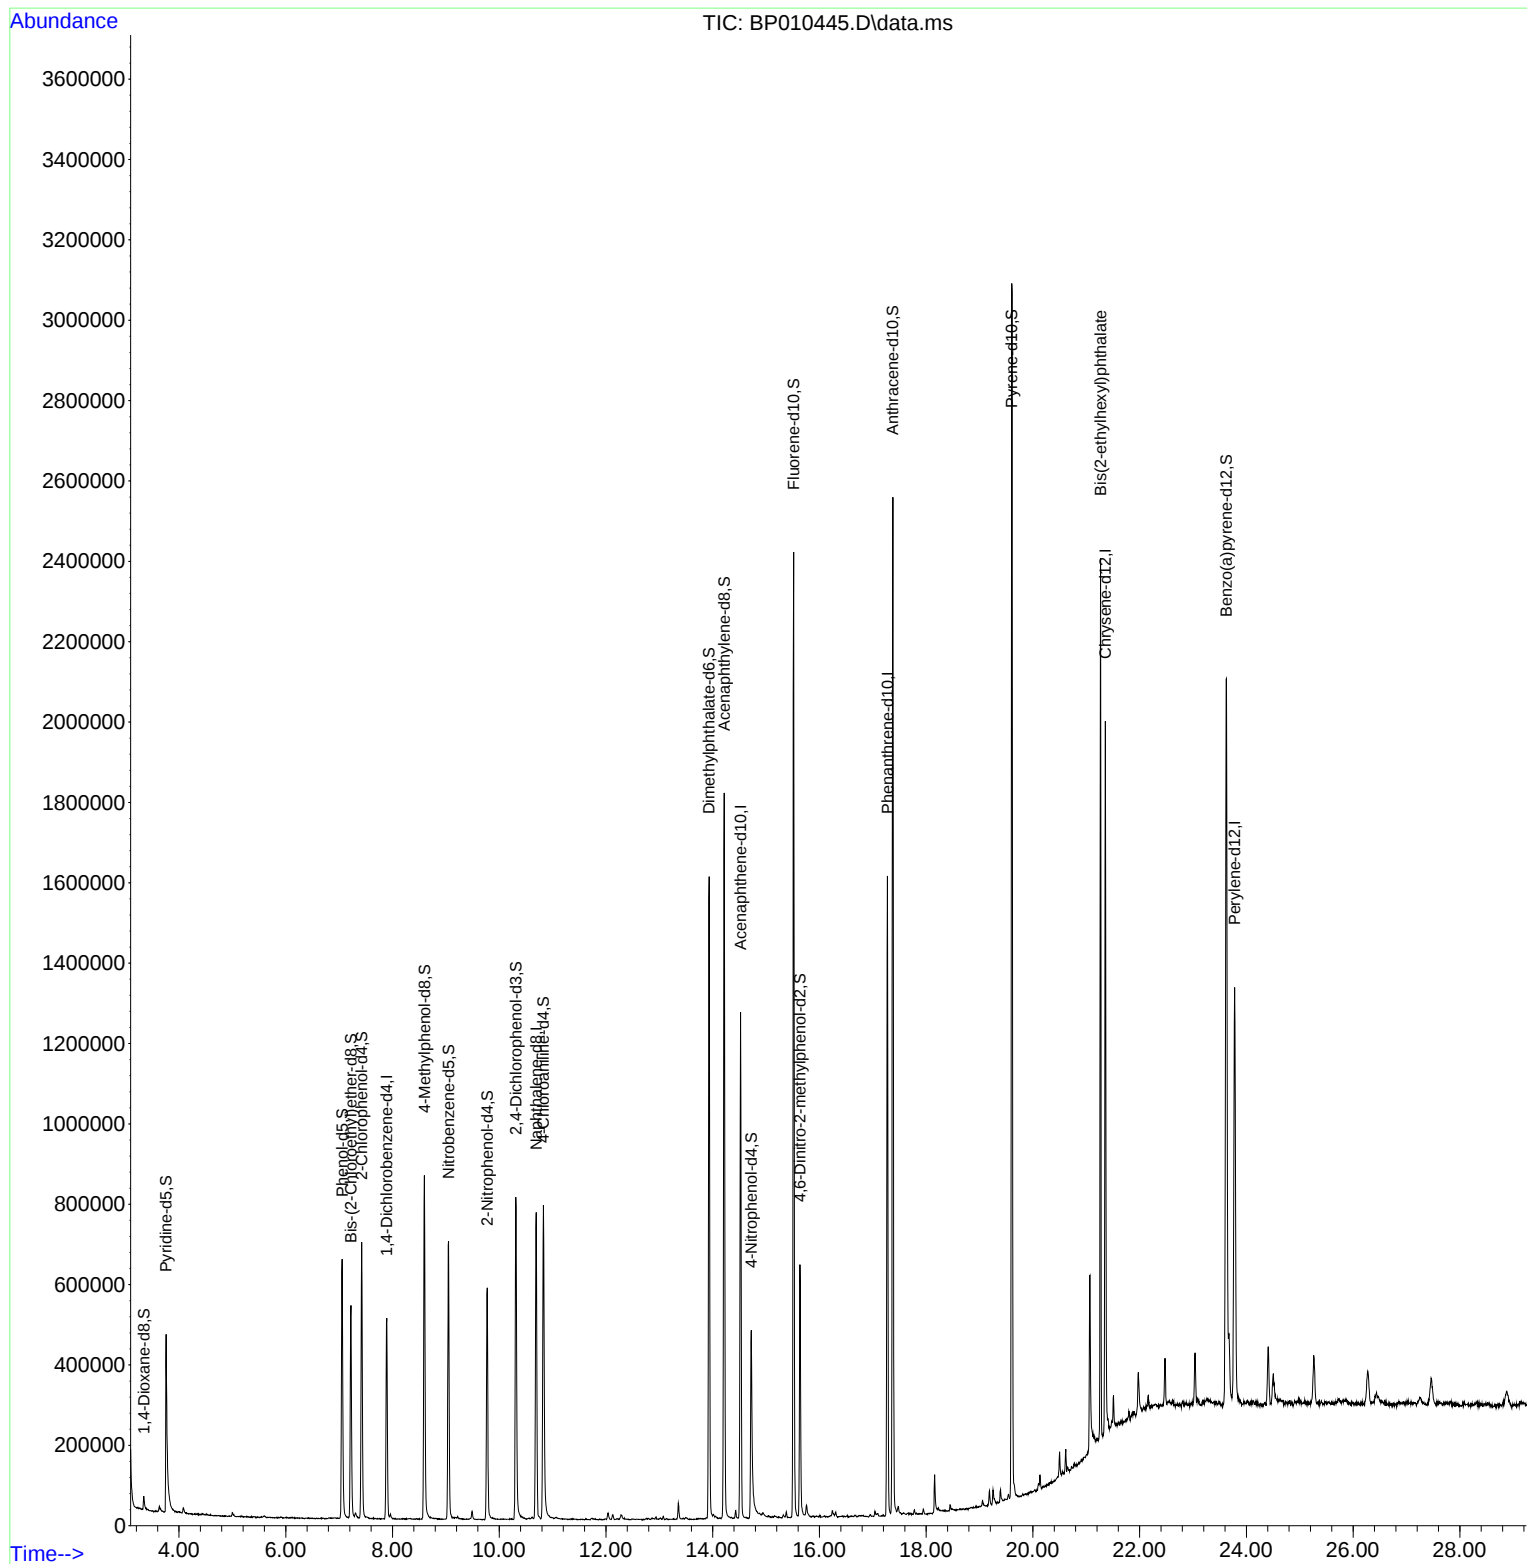

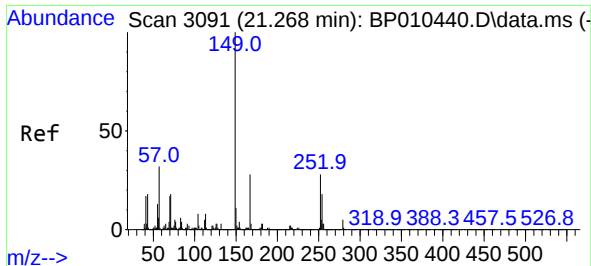

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 20.071 ng/ul
 RT: 21.269 min Scan# 3091
 Delta R.T. 0.000 min
 Lab File: BP010445.D
 Acq: 20 May 2022 20:51

Instrument :
 BNA_P
 ClientSampleId :
 EW4H9

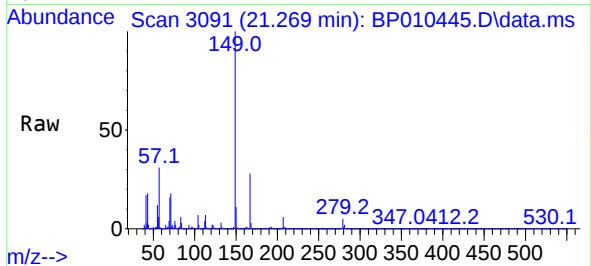

Tgt Ion:149 Resp: 666883
 Ion Ratio Lower Upper
 149 100
 167 28.1 32.8 49.2
 279 5.1 5.6 8.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/23/2022
 Supervised By :mohammad ahmed 05/25/2022

