

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010429.D
 Acq On : 20 May 2022 10:22
 Operator : CG/JU
 Sample : PB144950BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK950

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	19	rVB5	9058	11855	0.25%	0.026%
2	3.340	39	43	53	rBV	38140	59564	1.25%	0.131%
3	3.758	111	114	138	rBV	519654	1036982	21.84%	2.284%
4	4.087	164	170	178	rVB	28072	47949	1.01%	0.106%
5	7.058	666	675	691	rBV	700855	1201121	25.29%	2.645%
6	7.222	696	703	719	rVB	567817	942722	19.85%	2.076%
7	7.422	730	737	751	rBV	717040	1192507	25.11%	2.626%
8	7.893	809	817	827	rBV	473233	794554	16.73%	1.750%
9	8.599	929	937	955	rBV	915989	1533214	32.29%	3.376%
10	9.052	1004	1014	1031	rBV	759444	1318190	27.76%	2.903%
11	9.775	1129	1137	1155	rBV	633228	1087181	22.89%	2.394%
12	10.316	1220	1229	1247	rBV	826653	1541093	32.45%	3.394%
13	10.693	1284	1293	1307	rBV	693995	1194057	25.15%	2.630%
14	10.828	1307	1316	1339	rBV	838369	1638752	34.51%	3.609%
15	12.293	1559	1565	1575	rBV4	12450	29068	0.61%	0.064%
16	13.498	1767	1770	1775	rVB7	3514	5056	0.11%	0.011%
17	13.934	1837	1844	1857	rBV	1799198	2519368	53.05%	5.548%
18	14.034	1859	1861	1871	rVB10	4808	9986	0.21%	0.022%
19	14.216	1884	1892	1905	rBV	1881988	2805731	59.08%	6.179%
20	14.522	1937	1944	1956	rBV	1099087	1665145	35.07%	3.667%
21	14.722	1972	1978	1994	rBV	554310	1081882	22.78%	2.383%
22	15.198	2056	2059	2064	rVB7	3169	5212	0.11%	0.011%
23	15.516	2106	2113	2127	rBV	2444710	3588479	75.57%	7.903%
24	15.640	2127	2134	2150	rVV	772467	1147365	24.16%	2.527%
25	15.757	2150	2154	2162	rVB2	30053	50926	1.07%	0.112%
26	16.222	2226	2233	2236	rVB9	3336	6317	0.13%	0.014%
27	16.310	2243	2248	2253	rVB6	9931	18034	0.38%	0.040%
28	16.951	2352	2357	2364	rBV6	5407	10179	0.21%	0.022%
29	17.275	2405	2412	2421	rBV	1434990	2050847	43.19%	4.516%
30	17.375	2422	2429	2446	rVV2	2648023	3976628	83.74%	8.757%
31	17.945	2523	2526	2529	rBV4	4570	7010	0.15%	0.015%
32	19.186	2733	2737	2742	rBV2	35185	43688	0.92%	0.096%
33	19.257	2744	2749	2756	rBV2	30691	46496	0.98%	0.102%
34	19.610	2803	2809	2820	rBV	3424755	4748659	100.00%	10.458%
35	21.357	3101	3106	3123	rBV	1517524	2178774	45.88%	4.798%
36	23.627	3485	3492	3508	rVB2	1873841	3952497	83.23%	8.704%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010429.D
Acq On : 20 May 2022 10:22
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION

37 23.786 3512 3519 3531 rVB2 859021 1862034 39.21% 4.101%


Sum of corrected areas: 45409122

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010429.D
Acq On : 20 May 2022 10:22
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

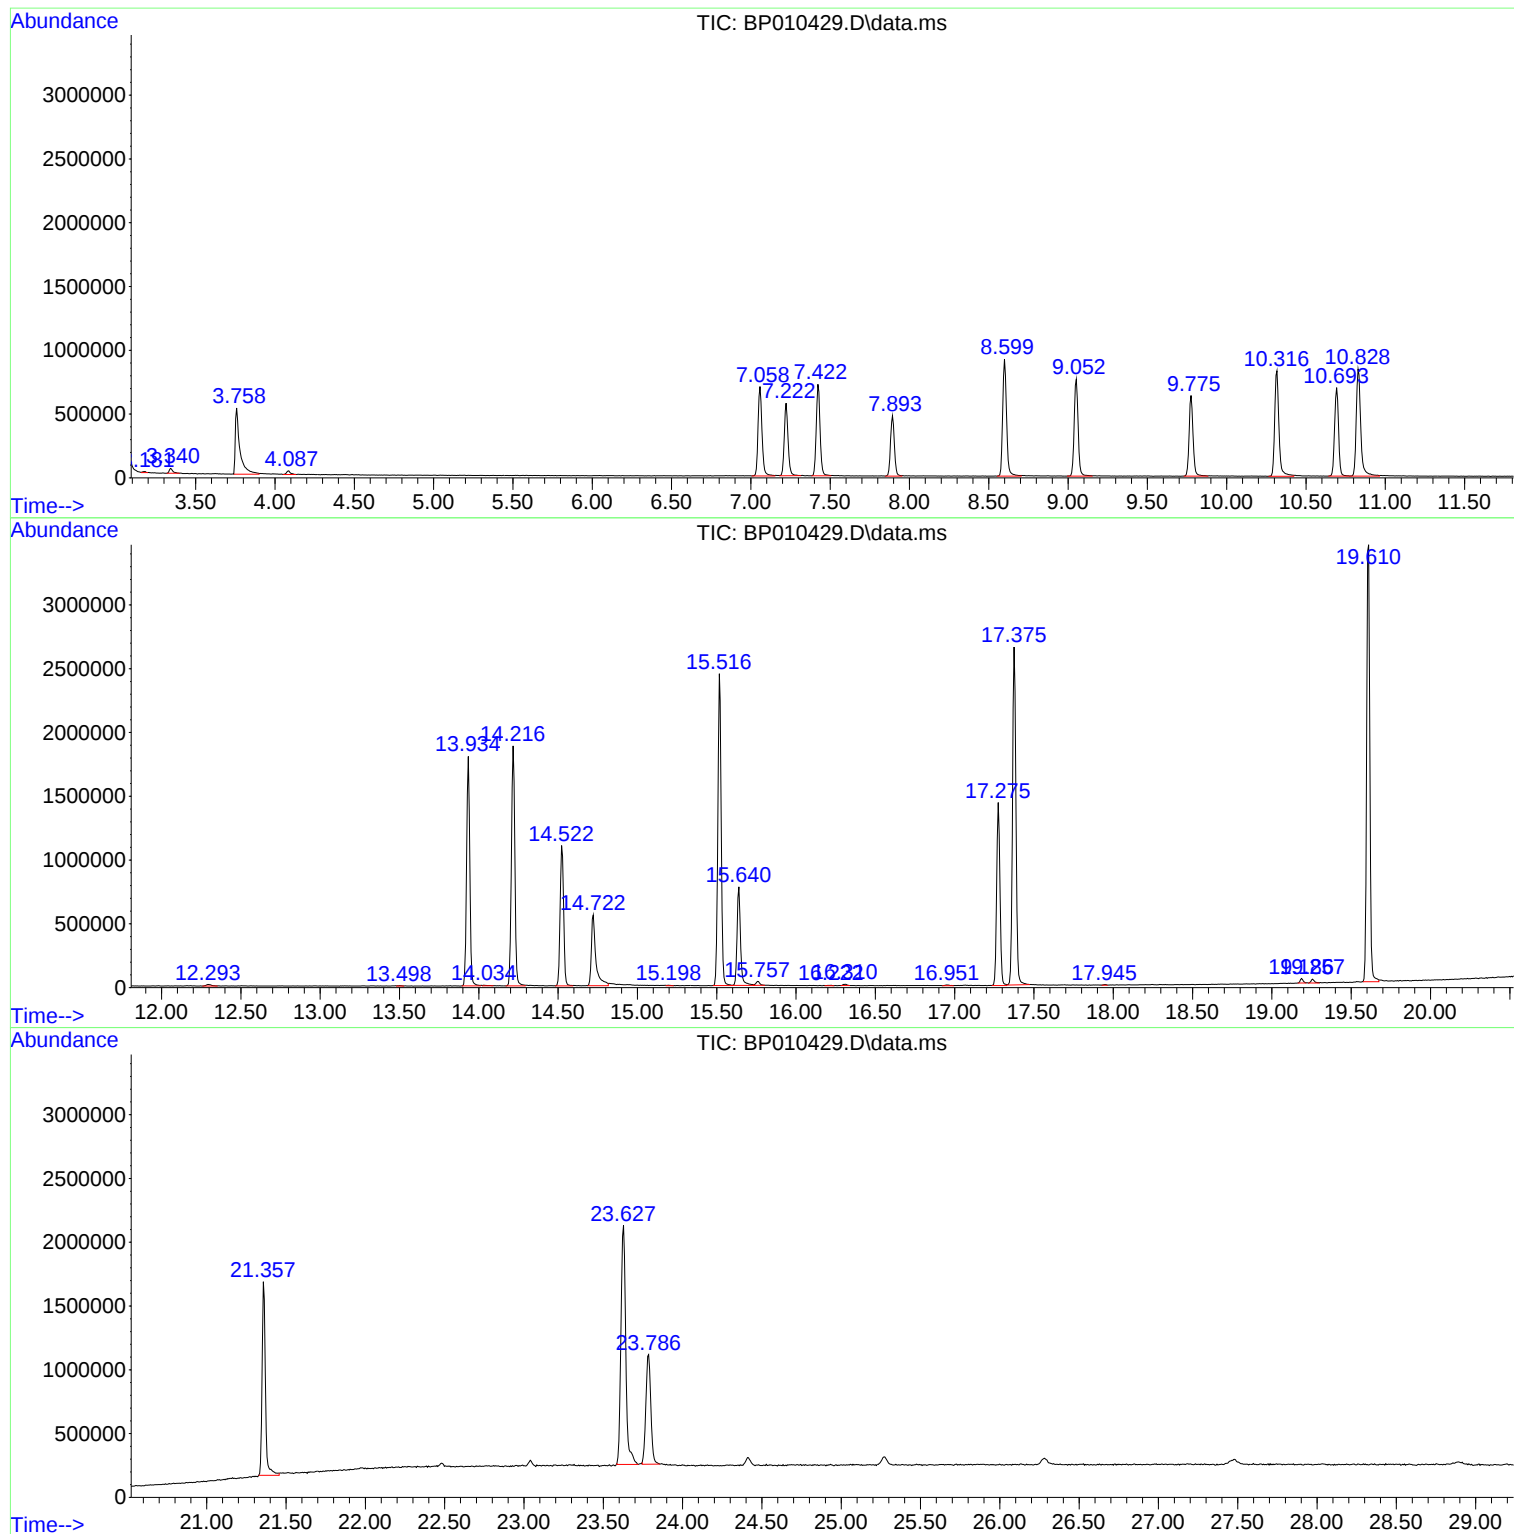

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010429.D
Acq On : 20 May 2022 10:22
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010429.D
Acq On : 20 May 2022 10:22
Operator : CG/JU
Sample : PB144950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------