

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010435.D
 Acq On : 20 May 2022 14:58
 Operator : CG/JU
 Sample : N2918-07DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.810	119	123	125	rBV3	7263	10940	0.25%	0.048%
2	4.081	163	169	174	rBV4	8187	15258	0.34%	0.067%
3	5.904	474	479	485	rBV4	11425	19102	0.43%	0.083%
4	7.063	672	676	684	rBV2	8524	16477	0.37%	0.072%
5	7.228	698	704	712	rBV	45794	81125	1.83%	0.355%
6	7.428	731	738	746	rBV	41079	77155	1.74%	0.337%
7	7.546	753	758	763	rVB7	4273	8311	0.19%	0.036%
8	7.616	763	770	776	rBV2	43872	76514	1.73%	0.334%
9	7.893	810	817	830	rBV	525686	879300	19.87%	3.842%
10	8.016	833	838	843	rVB7	5231	10021	0.23%	0.044%
11	8.434	903	909	916	rBV2	25336	48016	1.09%	0.210%
12	8.610	933	939	948	rVV4	29591	57318	1.30%	0.250%
13	8.740	955	961	969	rBV2	45857	83459	1.89%	0.365%
14	8.998	1001	1005	1008	rBV6	3406	5586	0.13%	0.024%
15	9.057	1008	1015	1027	rVB	56226	120053	2.71%	0.525%
16	9.251	1043	1048	1056	rVB5	10513	20440	0.46%	0.089%
17	9.322	1056	1060	1063	rBV6	5095	8977	0.20%	0.039%
18	9.375	1063	1069	1075	rVV3	28101	60988	1.38%	0.267%
19	9.440	1077	1080	1084	rVB5	6833	10415	0.24%	0.046%
20	9.587	1101	1105	1108	rVB6	3175	5070	0.11%	0.022%
21	9.781	1129	1138	1146	rBV3	40625	81108	1.83%	0.354%
22	9.910	1151	1160	1168	rBV8	9292	22032	0.50%	0.096%
23	10.104	1184	1193	1195	rBV7	7380	11296	0.26%	0.049%
24	10.328	1225	1231	1243	rBV2	54870	123842	2.80%	0.541%
25	10.692	1286	1293	1297	rVV	795179	1339017	30.26%	5.851%
26	10.745	1297	1302	1313	rVV	2621901	4424987	100.00%	19.337%
27	10.863	1313	1322	1331	rVB	209270	432891	9.78%	1.892%
28	10.992	1340	1344	1349	rVB8	2883	5128	0.12%	0.022%
29	11.075	1356	1358	1370	rVB8	5907	15215	0.34%	0.066%
30	11.728	1465	1469	1474	rBV5	7472	13311	0.30%	0.058%
31	11.786	1474	1479	1483	rVV5	8690	14744	0.33%	0.064%
32	12.063	1522	1526	1529	rBV6	3553	6611	0.15%	0.029%
33	12.251	1552	1558	1563	rBV2	12179	23224	0.52%	0.101%
34	12.298	1563	1566	1569	rBV5	3951	5226	0.12%	0.023%
35	12.357	1569	1576	1582	rBV	200581	336654	7.61%	1.471%
36	12.475	1591	1596	1602	rVB4	8184	16682	0.38%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010435.D
 Acq On : 20 May 2022 14:58
 Operator : CG/JU
 Sample : N2918-07DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	12.569	1602	1612	1620	rBV	143274	257880	5.83%	1.127%
38	12.686	1627	1632	1636	rBV4	8858	14178	0.32%	0.062%
39	12.739	1636	1641	1647	rVV9	6659	13207	0.30%	0.058%
40	12.945	1672	1676	1681	rBV8	5020	9265	0.21%	0.040%
41	13.004	1682	1686	1691	rVV7	8142	19700	0.45%	0.086%
42	13.057	1691	1695	1702	rVB8	12152	24502	0.55%	0.107%
43	13.251	1723	1728	1729	rBV5	6457	8060	0.18%	0.035%
44	13.363	1740	1747	1755	rVB	56748	93920	2.12%	0.410%
45	13.504	1766	1771	1776	rBV8	4844	9312	0.21%	0.041%
46	13.563	1776	1781	1789	rBV5	9765	21675	0.49%	0.095%
47	13.704	1793	1805	1813	rBV6	31611	74799	1.69%	0.327%
48	13.769	1813	1816	1824	rVB10	4290	8210	0.19%	0.036%
49	13.851	1824	1830	1834	rBV2	17308	32542	0.74%	0.142%
50	13.933	1834	1844	1855	rVB	174920	267624	6.05%	1.169%
51	14.022	1855	1859	1865	rVB7	6178	9437	0.21%	0.041%
52	14.086	1866	1870	1873	rBV5	6841	11579	0.26%	0.051%
53	14.216	1887	1892	1907	rVB2	159869	291938	6.60%	1.276%
54	14.527	1937	1945	1951	rBV	1205129	1897146	42.87%	8.290%
55	14.586	1951	1955	1961	rVV	216222	320545	7.24%	1.401%
56	14.657	1961	1967	1977	rVV	92373	153425	3.47%	0.670%
57	14.763	1981	1985	1987	rBV5	4205	5950	0.13%	0.026%
58	14.804	1987	1992	1999	rVV	30854	53053	1.20%	0.232%
59	14.875	2001	2004	2006	rVV4	4273	5829	0.13%	0.025%
60	14.922	2006	2012	2021	rVB	130625	209588	4.74%	0.916%
61	15.075	2033	2038	2045	rBV3	39751	68970	1.56%	0.301%
62	15.157	2048	2052	2060	rVB7	15897	26276	0.59%	0.115%
63	15.516	2103	2113	2119	rBV	238764	366804	8.29%	1.603%
64	15.574	2119	2123	2129	rVV	100171	158672	3.59%	0.693%
65	15.651	2130	2136	2142	rVV3	61605	140298	3.17%	0.613%
66	15.698	2142	2144	2148	rVV5	15345	21624	0.49%	0.094%
67	15.751	2151	2153	2158	rVV6	8554	17230	0.39%	0.075%
68	15.798	2158	2161	2166	rVV5	11366	21802	0.49%	0.095%
69	15.869	2170	2173	2179	rVB7	8367	15187	0.34%	0.066%
70	15.951	2184	2187	2192	rVB7	4076	4869	0.11%	0.021%
71	16.016	2192	2198	2200	rBV5	7964	12417	0.28%	0.054%
72	16.210	2227	2231	2232	rVV4	4536	5234	0.12%	0.023%
73	16.251	2232	2238	2246	rVV6	26534	55356	1.25%	0.242%
74	16.463	2267	2274	2281	rBV2	14191	28827	0.65%	0.126%
75	16.539	2281	2287	2299	rBV	57143	104487	2.36%	0.457%
76	16.786	2323	2329	2332	rBV8	8150	14953	0.34%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010435.D
 Acq On : 20 May 2022 14:58
 Operator : CG/JU
 Sample : N2918-07DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.880	2341	2345	2348	rBV6	4470	6710	0.15%	0.029%
78	16.933	2348	2354	2361	rVB2	68855	111079	2.51%	0.485%
79	17.098	2380	2382	2385	rVB3	7569	6461	0.15%	0.028%
80	17.274	2406	2412	2418	rBV	1620873	2347547	53.05%	10.258%
81	17.316	2418	2419	2425	rVV2	69836	92934	2.10%	0.406%
82	17.374	2425	2429	2442	rVB	274451	426043	9.63%	1.862%
83	17.527	2452	2455	2460	rVB7	5398	7219	0.16%	0.032%
84	17.680	2472	2481	2493	rBV	451344	690347	15.60%	3.017%
85	17.839	2504	2508	2514	rBV	42305	69377	1.57%	0.303%
86	17.980	2530	2532	2537	rVB5	6699	8498	0.19%	0.037%
87	18.027	2537	2540	2543	rBV5	3487	5276	0.12%	0.023%
88	18.110	2550	2554	2558	rBV5	8718	13500	0.31%	0.059%
89	18.163	2560	2563	2564	rBV3	7115	7104	0.16%	0.031%
90	18.192	2564	2568	2571	rVB2	10775	16313	0.37%	0.071%
91	18.263	2578	2580	2584	rVB3	8060	10400	0.24%	0.045%
92	18.321	2587	2590	2594	rBV6	5694	8449	0.19%	0.037%
93	18.416	2604	2606	2608	rBV3	6097	6909	0.16%	0.030%
94	18.568	2629	2632	2638	rVB8	8383	12787	0.29%	0.056%
95	19.115	2723	2725	2730	rVB6	7431	7702	0.17%	0.034%
96	19.392	2770	2772	2779	rVB7	8644	14185	0.32%	0.062%
97	19.610	2803	2809	2815	rBV	386251	522389	11.81%	2.283%
98	21.362	3101	3107	3119	rBV	1844832	2626181	59.35%	11.476%
99	23.627	3487	3492	3497	rBV2	158037	314929	7.12%	1.376%
100	23.786	3512	3519	3533	rVB2	1041492	2188830	49.47%	9.565%




Sum of corrected areas: 22884032

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010435.D
Acq On : 20 May 2022 14:58
Operator : CG/JU
Sample : N2918-07DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

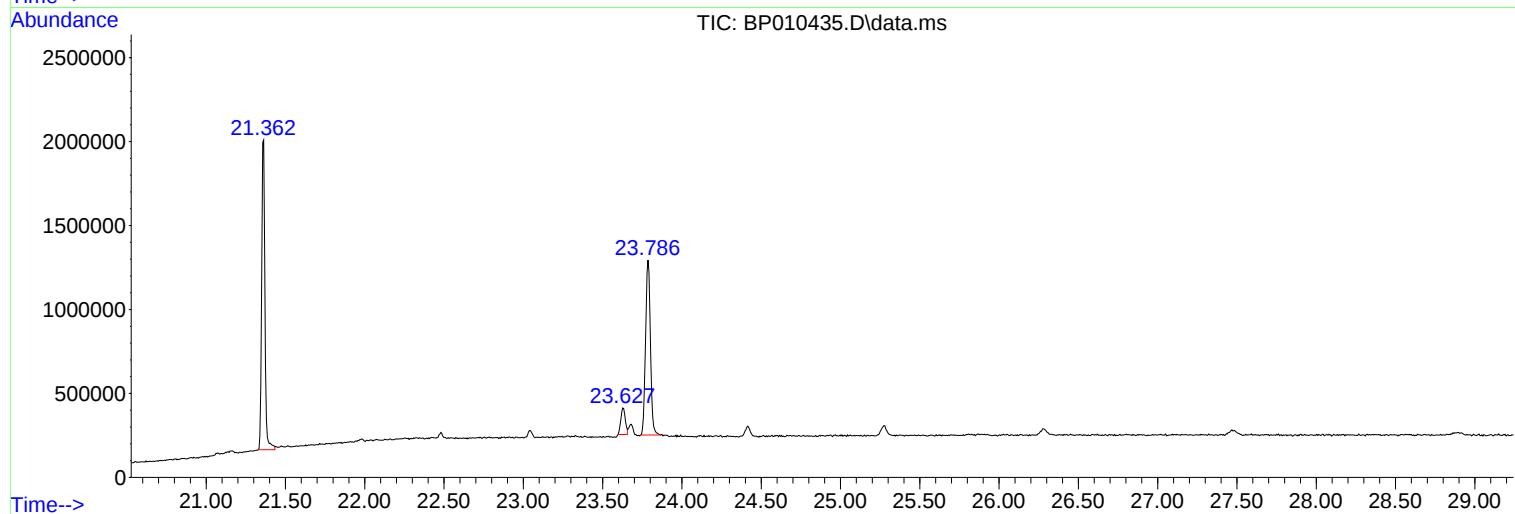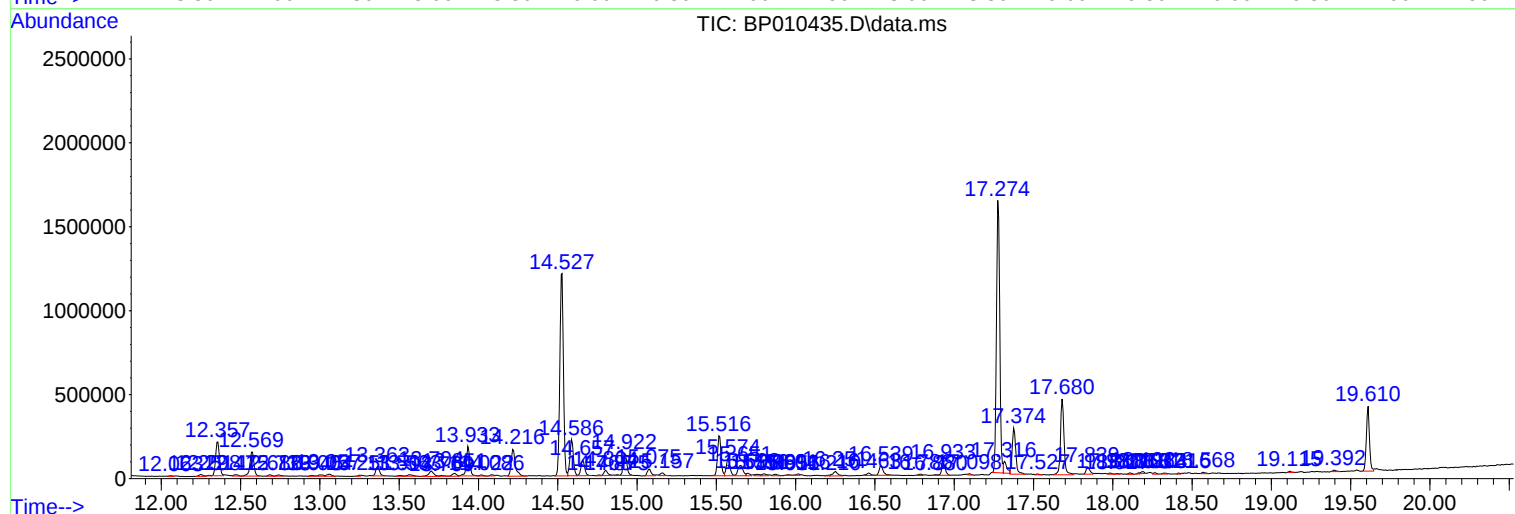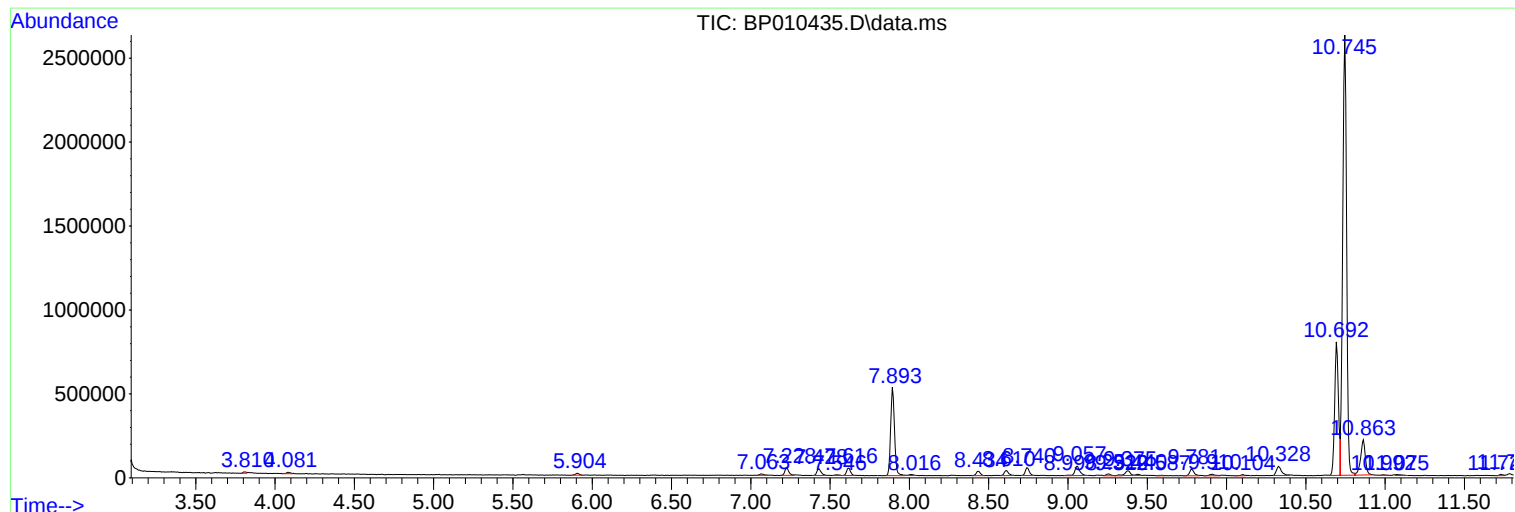

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010435.D
Acq On : 20 May 2022 14:58
Operator : CG/JU
Sample : N2918-07DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010435.D
Acq On : 20 May 2022 14:58
Operator : CG/JU
Sample : N2918-07DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------