

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010436.D
 Acq On : 20 May 2022 15:35
 Operator : CG/JU
 Sample : N2918-01DL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.805	118	122	125	rBV5	9155	15753	0.63%	0.088%
2	4.081	165	169	174	rVV6	7225	13879	0.56%	0.078%
3	4.123	174	176	177	rVB2	4256	2625	0.11%	0.015%
4	4.917	309	311	315	rVB4	2442	3240	0.13%	0.018%
5	5.146	348	350	355	rVB5	2054	2695	0.11%	0.015%
6	5.305	372	377	380	rBV6	2086	3047	0.12%	0.017%
7	5.905	475	479	484	rBV6	6764	11190	0.45%	0.063%
8	5.975	490	491	496	rVB6	2255	2680	0.11%	0.015%
9	7.064	672	676	686	rBV4	9767	20838	0.84%	0.116%
10	7.222	698	703	713	rBV	48207	89774	3.61%	0.502%
11	7.428	732	738	749	rVV	42347	85844	3.46%	0.480%
12	7.511	751	752	756	rVV4	2242	2683	0.11%	0.015%
13	7.617	764	770	777	rBV2	17466	31274	1.26%	0.175%
14	7.893	809	817	832	rBV	485794	831646	33.48%	4.646%
15	8.011	832	837	843	rVB9	3298	8163	0.33%	0.046%
16	8.258	877	879	886	rBV8	2538	5905	0.24%	0.033%
17	8.434	903	909	917	rBV3	10151	19607	0.79%	0.110%
18	8.611	934	939	947	rBV2	34000	64131	2.58%	0.358%
19	8.669	947	949	953	rVB5	2381	2869	0.12%	0.016%
20	8.746	955	962	970	rBV3	20710	36091	1.45%	0.202%
21	9.058	1008	1015	1024	rBV2	61139	121982	4.91%	0.681%
22	9.193	1032	1038	1042	rBV9	4576	8106	0.33%	0.045%
23	9.252	1045	1048	1056	rVV6	5720	10413	0.42%	0.058%
24	9.322	1056	1060	1064	rVV7	4093	7459	0.30%	0.042%
25	9.381	1064	1070	1077	rVV8	9564	23493	0.95%	0.131%
26	9.434	1077	1079	1086	rVB5	5240	8713	0.35%	0.049%
27	9.781	1130	1138	1145	rBV2	42477	84080	3.39%	0.470%
28	9.828	1145	1146	1154	rVB8	2469	3845	0.15%	0.021%
29	9.911	1156	1160	1164	rVV6	2834	4451	0.18%	0.025%
30	9.981	1169	1172	1176	rVB6	3058	4140	0.17%	0.023%
31	10.105	1190	1193	1197	rBV5	3428	5553	0.22%	0.031%
32	10.328	1221	1231	1245	rBV2	54046	128733	5.18%	0.719%
33	10.693	1282	1293	1297	rBV	721570	1243453	50.07%	6.946%
34	10.746	1297	1302	1313	rVV	1214110	2075305	83.56%	11.593%
35	10.863	1313	1322	1333	rVV2	127273	304662	12.27%	1.702%
36	10.940	1333	1335	1338	rVB4	1978	2514	0.10%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010436.D
 Acq On : 20 May 2022 15:35
 Operator : CG/JU
 Sample : N2918-01DL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	11.075	1352	1358	1360	rBV7	3299	3677	0.15%	0.021%
38	11.734	1467	1470	1475	rBV5	3529	5990	0.24%	0.033%
39	11.793	1475	1480	1481	rBV5	2519	3876	0.16%	0.022%
40	11.810	1481	1483	1488	rVB5	2395	2953	0.12%	0.016%
41	12.252	1553	1558	1562	rBV4	7558	13880	0.56%	0.078%
42	12.357	1570	1576	1585	rBV	95176	166077	6.69%	0.928%
43	12.481	1590	1597	1602	rVV9	4441	11460	0.46%	0.064%
44	12.575	1602	1613	1623	rVB	78388	141245	5.69%	0.789%
45	12.687	1629	1632	1637	rBV6	4420	6510	0.26%	0.036%
46	12.775	1645	1647	1653	rVB6	1972	3082	0.12%	0.017%
47	13.004	1682	1686	1687	rBV4	3013	3303	0.13%	0.018%
48	13.057	1691	1695	1703	rVB4	6619	12979	0.52%	0.073%
49	13.269	1726	1731	1737	rBV9	4117	10460	0.42%	0.058%
50	13.363	1737	1747	1758	rVV	38035	76078	3.06%	0.425%
51	13.563	1778	1781	1782	rBV3	3862	3209	0.13%	0.018%
52	13.581	1782	1784	1791	rVB7	4733	7956	0.32%	0.044%
53	13.704	1796	1805	1806	rBV8	6319	12548	0.51%	0.070%
54	13.851	1822	1830	1835	rVB6	10284	17162	0.69%	0.096%
55	13.940	1835	1845	1855	rBV	174775	281467	11.33%	1.572%
56	14.028	1855	1860	1865	rVB8	6070	9423	0.38%	0.053%
57	14.087	1867	1870	1874	rBV6	3554	5002	0.20%	0.028%
58	14.216	1886	1892	1906	rBV	172890	289833	11.67%	1.619%
59	14.528	1937	1945	1951	rBV	1161812	1800855	72.51%	10.060%
60	14.587	1951	1955	1963	rVV	120847	191069	7.69%	1.067%
61	14.663	1963	1968	1975	rVB	40565	65480	2.64%	0.366%
62	14.763	1982	1985	1987	rBV4	2811	3418	0.14%	0.019%
63	14.822	1991	1995	1996	rVV4	3860	5089	0.20%	0.028%
64	14.840	1996	1998	2003	rVV6	3402	4918	0.20%	0.027%
65	14.928	2007	2013	2023	rVV	88662	144456	5.82%	0.807%
66	14.998	2023	2025	2034	rVB10	2895	5191	0.21%	0.029%
67	15.081	2034	2039	2047	rBV6	20152	42086	1.69%	0.235%
68	15.163	2049	2053	2058	rVB7	8353	11858	0.48%	0.066%
69	15.522	2107	2114	2119	rBV	252128	381082	15.34%	2.129%
70	15.575	2119	2123	2130	rVB	33320	54787	2.21%	0.306%
71	15.646	2130	2135	2142	rBV4	41045	77040	3.10%	0.430%
72	15.757	2149	2154	2159	rBV9	5688	11548	0.46%	0.065%
73	15.804	2159	2162	2168	rVB8	4493	5998	0.24%	0.034%
74	15.875	2171	2174	2179	rVB7	4335	7526	0.30%	0.042%
75	15.957	2183	2188	2190	rBV6	3778	5366	0.22%	0.030%
76	16.010	2194	2197	2198	rBV3	3773	3100	0.12%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010436.D
 Acq On : 20 May 2022 15:35
 Operator : CG/JU
 Sample : N2918-01DL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.210	2226	2231	2232	rBV5	2568	3278	0.13%	0.018%
78	16.251	2232	2238	2244	rVV4	13187	25999	1.05%	0.145%
79	16.540	2282	2287	2292	rBV2	27642	49948	2.01%	0.279%
80	16.604	2296	2298	2303	rVV5	2853	4710	0.19%	0.026%
81	16.934	2349	2354	2364	rVB2	47127	77853	3.13%	0.435%
82	17.075	2374	2378	2379	rBV3	3048	3903	0.16%	0.022%
83	17.098	2379	2382	2387	rVB6	5950	7555	0.30%	0.042%
84	17.181	2392	2396	2397	rBV4	4011	4316	0.17%	0.024%
85	17.275	2403	2412	2419	rBV	1517695	2274752	91.59%	12.707%
86	17.375	2424	2429	2441	rVB2	270163	455260	18.33%	2.543%
87	17.681	2474	2481	2493	rVV	218887	346870	13.97%	1.938%
88	17.775	2495	2497	2502	rVB6	3163	3631	0.15%	0.020%
89	17.851	2505	2510	2516	rVV3	21262	37429	1.51%	0.209%
90	18.110	2551	2554	2559	rBV7	4713	7163	0.29%	0.040%
91	18.169	2559	2564	2565	rBV5	6111	8661	0.35%	0.048%
92	18.239	2573	2576	2579	rBV5	3738	6226	0.25%	0.035%
93	18.269	2579	2581	2586	rVB6	5939	7175	0.29%	0.040%
94	18.422	2603	2607	2609	rBV5	5313	7795	0.31%	0.044%
95	19.192	2736	2738	2741	rVB4	6167	5402	0.22%	0.030%
96	19.257	2747	2749	2751	rBV3	4458	3864	0.16%	0.022%
97	19.610	2803	2809	2816	rBV	399022	550813	22.18%	3.077%
98	21.363	3101	3107	3123	rBV	1723665	2483665	100.00%	13.874%
99	23.627	3487	3492	3497	rBV2	163714	313667	12.63%	1.752%
100	23.786	3512	3519	3533	rVB2	965087	2011183	80.98%	11.235%




Sum of corrected areas: 17900991

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010436.D
Acq On : 20 May 2022 15:35
Operator : CG/JU
Sample : N2918-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

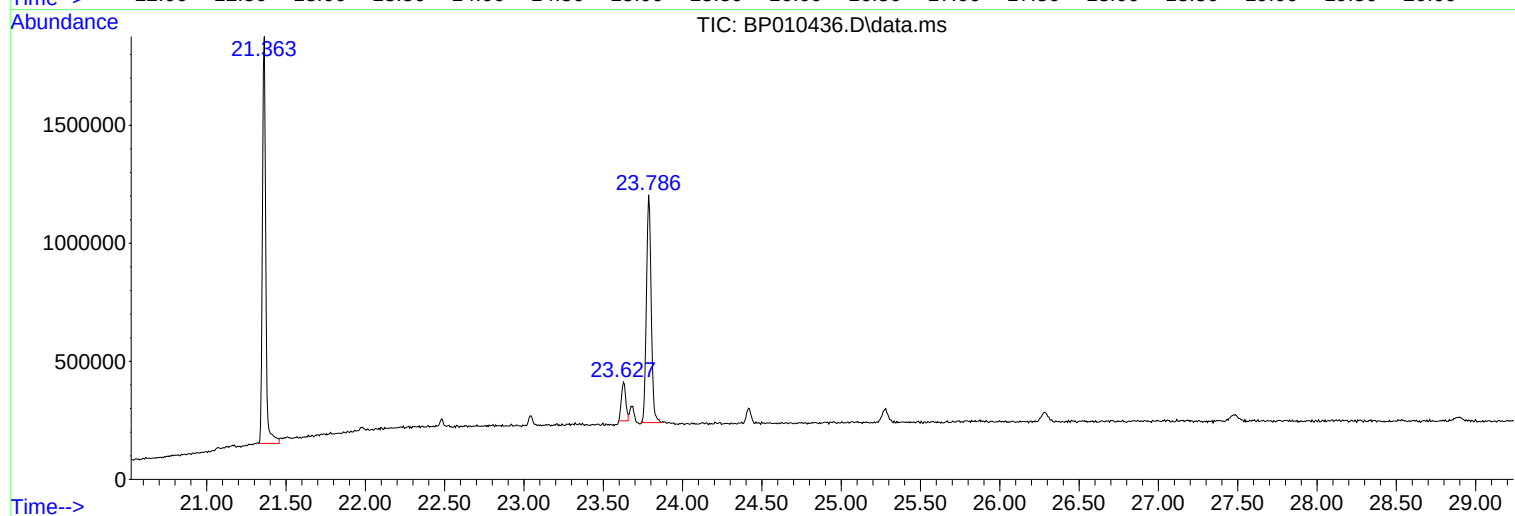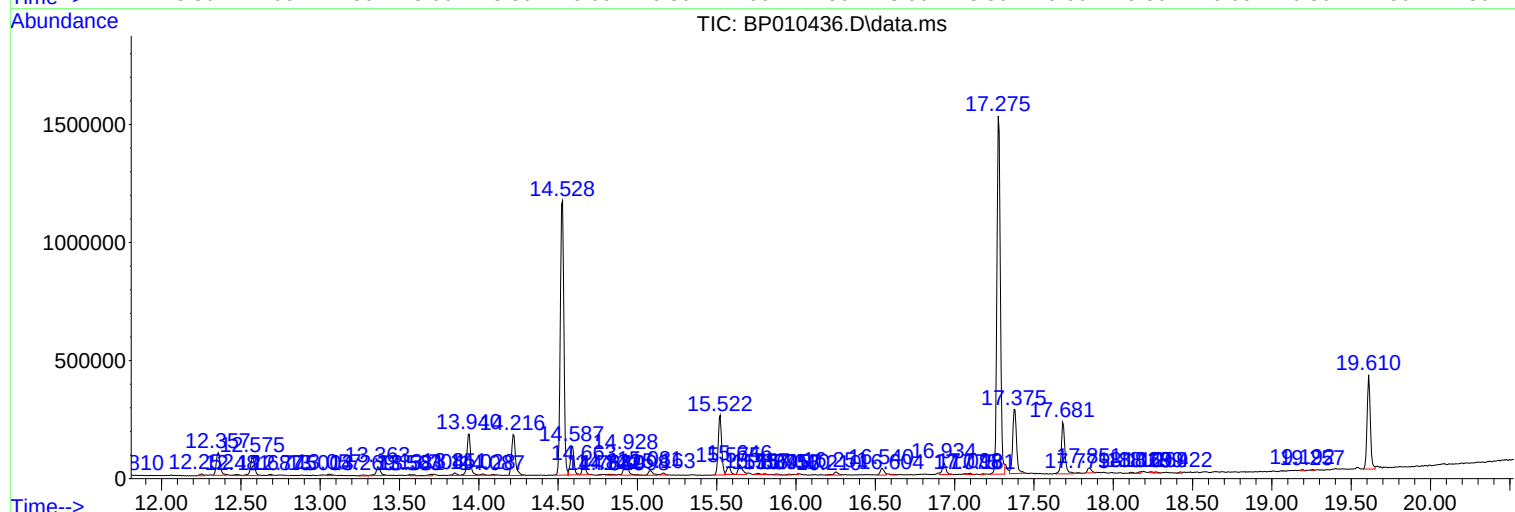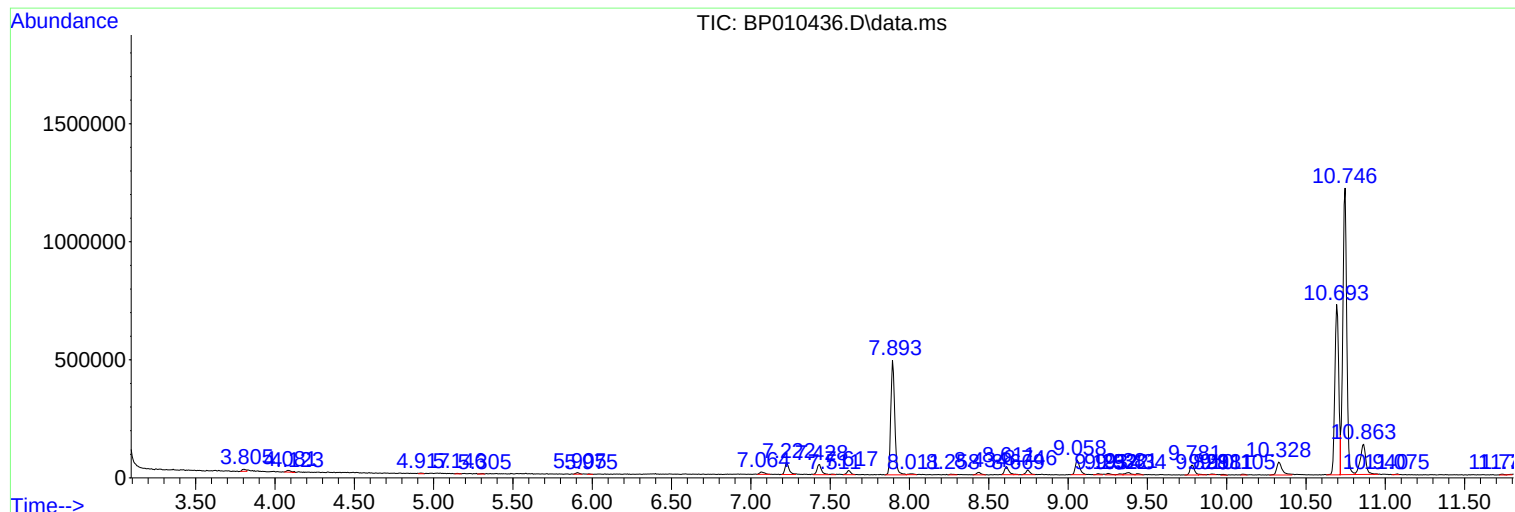

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010436.D
Acq On : 20 May 2022 15:35
Operator : CG/JU
Sample : N2918-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010436.D
Acq On : 20 May 2022 15:35
Operator : CG/JU
Sample : N2918-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------