

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010441.D
 Acq On : 20 May 2022 18:36
 Operator : CG/JU
 Sample : PB144914BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK914

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	54	rVB	38562	67565	1.40%	0.140%
2	3.758	111	114	134	rBV	539598	1031860	21.41%	2.131%
3	4.081	165	169	183	rVB	37484	61422	1.27%	0.127%
4	7.058	666	675	691	rBV	716250	1234730	25.62%	2.550%
5	7.222	696	703	715	rVV	585192	965994	20.04%	1.995%
6	7.422	728	737	748	rBV	746311	1238374	25.69%	2.558%
7	7.893	810	817	826	rBV	590807	999289	20.73%	2.064%
8	8.599	930	937	954	rBV	944064	1606768	33.34%	3.319%
9	9.052	1007	1014	1030	rBV	769576	1352927	28.07%	2.794%
10	9.775	1128	1137	1149	rBV	636263	1125187	23.35%	2.324%
11	10.310	1221	1228	1248	rBV	857519	1606455	33.33%	3.318%
12	10.693	1285	1293	1308	rBV	897528	1536405	31.88%	3.173%
13	10.828	1308	1316	1332	rBV	875260	1673893	34.73%	3.457%
14	12.293	1558	1565	1575	rBV4	13267	30910	0.64%	0.064%
15	13.487	1760	1768	1770	rBV9	3361	6274	0.13%	0.013%
16	13.934	1836	1844	1856	rBV	1827019	2620114	54.36%	5.412%
17	14.216	1881	1892	1906	rBV	1939011	2925896	60.71%	6.043%
18	14.522	1937	1944	1959	rBV	1435723	2153383	44.68%	4.448%
19	14.722	1970	1978	1998	rBV	548385	1137129	23.59%	2.349%
20	14.934	2012	2014	2020	rVB7	5197	7171	0.15%	0.015%
21	15.516	2106	2113	2127	rBV	2593832	3698137	76.73%	7.638%
22	15.640	2127	2134	2149	rVV	708828	1144555	23.75%	2.364%
23	15.757	2149	2154	2160	rVB	31698	51303	1.06%	0.106%
24	16.304	2241	2247	2255	rVB4	12109	23524	0.49%	0.049%
25	16.951	2353	2357	2362	rBV8	5909	10755	0.22%	0.022%
26	17.063	2369	2376	2381	rBV9	4706	9203	0.19%	0.019%
27	17.275	2405	2412	2422	rBV	1779175	2618554	54.33%	5.408%
28	17.375	2422	2429	2445	rVV2	2776489	4090625	84.87%	8.449%
29	18.233	2572	2575	2578	rBV5	3625	4991	0.10%	0.010%
30	19.186	2732	2737	2744	rBV2	35038	53668	1.11%	0.111%
31	19.257	2744	2749	2755	rBV	31107	52005	1.08%	0.107%
32	19.604	2802	2808	2824	rBV	3384832	4819611	100.00%	9.955%
33	21.357	3101	3106	3121	rBV	1903946	2680799	55.62%	5.537%
34	23.627	3484	3492	3499	rBV	1779144	3603354	74.76%	7.442%
35	23.780	3511	3518	3531	rVB	1028979	2173562	45.10%	4.489%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010441.D
Acq On : 20 May 2022 18:36
Operator : CG/JU
Sample : PB144914BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK914

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION


Sum of corrected areas: 48416392

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010441.D
Acq On : 20 May 2022 18:36
Operator : CG/JU
Sample : PB144914BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK914

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

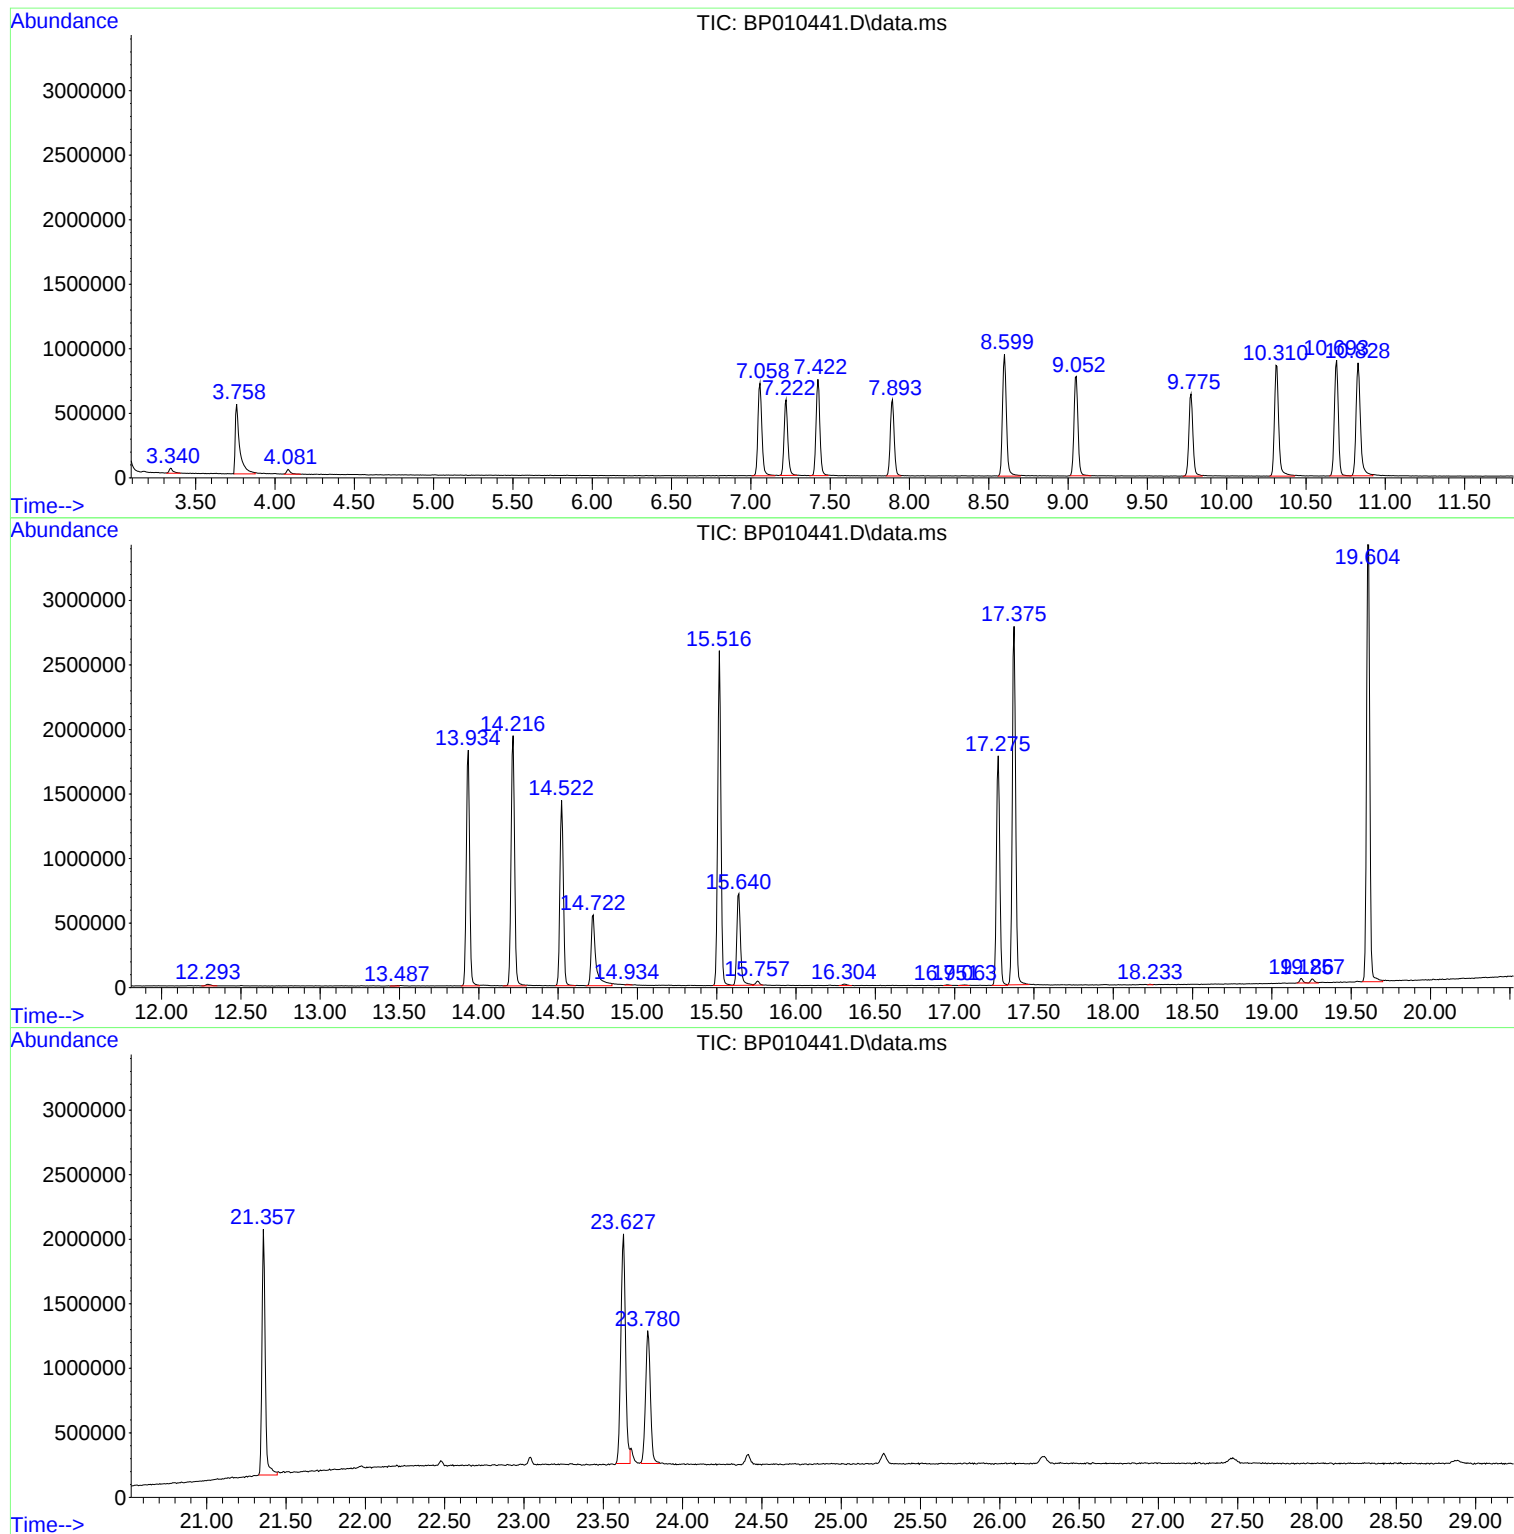

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010441.D
Acq On : 20 May 2022 18:36
Operator : CG/JU
Sample : PB144914BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK914

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010441.D
Acq On : 20 May 2022 18:36
Operator : CG/JU
Sample : PB144914BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK914

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------