

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010444.D
 Acq On : 20 May 2022 20:17
 Operator : CG/JU
 Sample : N2843-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	48	rBV2	14391	20987	0.82%	0.070%
2	3.793	117	120	128	rBV3	14821	33064	1.29%	0.110%
3	3.987	150	153	164	rVB6	11264	22847	0.89%	0.076%
4	4.081	166	169	173	rVV2	8594	10959	0.43%	0.036%
5	4.305	202	207	214	rBV	32220	49023	1.91%	0.163%
6	4.717	271	277	281	rBV2	17914	30549	1.19%	0.102%
7	5.005	320	326	336	rBV	452665	695678	27.06%	2.313%
8	5.252	365	368	370	rBV4	2575	3214	0.13%	0.011%
9	5.322	377	380	383	rBV5	2079	3474	0.14%	0.012%
10	5.405	391	394	396	rVB4	3211	3588	0.14%	0.012%
11	5.628	430	432	435	rVB4	3410	3800	0.15%	0.013%
12	5.669	435	439	440	rBV4	2688	3452	0.13%	0.011%
13	6.199	525	529	530	rBV4	2388	2882	0.11%	0.010%
14	6.275	541	542	546	rVB4	2245	2947	0.11%	0.010%
15	6.758	621	624	629	rBV7	3005	4205	0.16%	0.014%
16	7.058	668	675	691	rVV	319870	574931	22.36%	1.911%
17	7.222	696	703	714	rVV	257958	446630	17.37%	1.485%
18	7.311	714	718	725	rVB2	7791	16421	0.64%	0.055%
19	7.422	730	737	749	rVV	334213	561245	21.83%	1.866%
20	7.516	750	753	758	rVB4	5801	10042	0.39%	0.033%
21	7.893	810	817	826	rVV	520532	876394	34.09%	2.914%
22	7.963	826	829	835	rVB6	6133	11330	0.44%	0.038%
23	8.599	929	937	952	rBV	374123	668507	26.00%	2.222%
24	8.716	952	957	965	rVB	28810	50855	1.98%	0.169%
25	9.052	1007	1014	1024	rVV	332513	596851	23.22%	1.984%
26	9.122	1024	1026	1031	rVB6	6684	9359	0.36%	0.031%
27	9.222	1039	1043	1053	rVB6	5859	14093	0.55%	0.047%
28	9.493	1084	1089	1098	rVB3	12949	21698	0.84%	0.072%
29	9.775	1129	1137	1149	rBV	277173	487703	18.97%	1.621%
30	9.852	1149	1150	1153	rVB3	2886	2607	0.10%	0.009%
31	10.140	1192	1199	1203	rBV9	3400	7821	0.30%	0.026%
32	10.228	1209	1214	1218	rBV7	2043	2604	0.10%	0.009%
33	10.316	1222	1229	1250	rBV	377318	735866	28.62%	2.446%
34	10.693	1285	1293	1309	rBV	805351	1408858	54.80%	4.684%
35	10.828	1309	1316	1336	rBV	335698	714352	27.79%	2.375%
36	11.328	1397	1401	1404	rBV5	1388	2628	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010444.D
 Acq On : 20 May 2022 20:17
 Operator : CG/JU
 Sample : N2843-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	11.399	1411	1413	1417	rVB5	2469	2574	0.10%	0.009%
38	11.552	1438	1439	1443	rVB4	2763	2641	0.10%	0.009%
39	11.728	1464	1469	1474	rBV9	4207	8658	0.34%	0.029%
40	12.128	1532	1537	1545	rBV4	10255	18120	0.70%	0.060%
41	12.287	1559	1564	1567	rBV5	6902	12194	0.47%	0.041%
42	12.351	1571	1575	1577	rBV5	2363	2616	0.10%	0.009%
43	12.575	1611	1613	1618	rVB6	3945	4691	0.18%	0.016%
44	12.940	1670	1675	1678	rVB6	3312	5393	0.21%	0.018%
45	13.016	1682	1688	1692	rBV7	4298	6968	0.27%	0.023%
46	13.075	1695	1698	1703	rVV6	7976	10846	0.42%	0.036%
47	13.140	1705	1709	1715	rVB9	3234	6707	0.26%	0.022%
48	13.257	1727	1729	1734	rVB6	3155	5169	0.20%	0.017%
49	13.357	1740	1746	1754	rVB2	28837	45700	1.78%	0.152%
50	13.457	1759	1763	1766	rVB6	2565	3506	0.14%	0.012%
51	13.498	1766	1770	1772	rBV5	3517	4990	0.19%	0.017%
52	13.798	1818	1821	1824	rBV5	2125	4026	0.16%	0.013%
53	13.851	1828	1830	1833	rVV4	4692	4894	0.19%	0.016%
54	13.934	1836	1844	1854	rVV	809956	1198895	46.64%	3.986%
55	14.010	1855	1857	1861	rVB5	6087	8976	0.35%	0.030%
56	14.134	1876	1878	1882	rVB5	3066	3759	0.15%	0.012%
57	14.216	1882	1892	1904	rBV	888811	1390827	54.10%	4.624%
58	14.428	1924	1928	1932	rBV	16266	21552	0.84%	0.072%
59	14.522	1937	1944	1953	rBV	1389224	1974194	76.79%	6.563%
60	14.728	1970	1979	1993	rBV2	149027	375913	14.62%	1.250%
61	14.945	2010	2016	2020	rBV8	13441	22159	0.86%	0.074%
62	15.051	2031	2034	2040	rVB7	4801	7884	0.31%	0.026%
63	15.334	2077	2082	2085	rBV4	5510	10433	0.41%	0.035%
64	15.381	2086	2090	2094	rVB3	15591	20525	0.80%	0.068%
65	15.516	2106	2113	2121	rBV	1227424	1804008	70.17%	5.997%
66	15.640	2128	2134	2145	rBV	235454	390617	15.19%	1.299%
67	15.757	2150	2154	2157	rBV	13628	19096	0.74%	0.063%
68	15.934	2182	2184	2187	rBV4	3909	4410	0.17%	0.015%
69	16.004	2194	2196	2200	rVB5	3347	3667	0.14%	0.012%
70	16.204	2228	2230	2233	rBV4	2372	3002	0.12%	0.010%
71	16.245	2233	2237	2238	rBV2	13648	17469	0.68%	0.058%
72	16.304	2244	2247	2251	rVB5	6211	7573	0.29%	0.025%
73	16.581	2292	2294	2299	rBV6	3397	4691	0.18%	0.016%
74	16.822	2328	2335	2338	rBV8	12288	21395	0.83%	0.071%
75	16.851	2338	2340	2343	rVB4	3535	2789	0.11%	0.009%
76	17.039	2367	2372	2376	rBV4	18215	28530	1.11%	0.095%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010444.D
 Acq On : 20 May 2022 20:17
 Operator : CG/JU
 Sample : N2843-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	17.092	2378	2381	2386	rVB6	11727	17052	0.66%	0.057%
78	17.139	2386	2389	2393	rBV5	5522	7979	0.31%	0.027%
79	17.275	2405	2412	2417	rBV	1647620	2376383	92.44%	7.900%
80	17.375	2423	2429	2441	rVV	1249288	1860254	72.36%	6.184%
81	17.475	2443	2446	2451	rVB6	18018	24540	0.95%	0.082%
82	17.781	2494	2498	2501	rBV2	14006	16172	0.63%	0.054%
83	17.845	2507	2509	2511	rBV3	4119	3802	0.15%	0.013%
84	17.945	2522	2526	2531	rBB	29786	36600	1.42%	0.122%
85	18.010	2535	2537	2540	rBV4	4218	4679	0.18%	0.016%
86	18.104	2549	2553	2556	rBV5	11345	18276	0.71%	0.061%
87	18.157	2558	2562	2566	rBV3	58420	83501	3.25%	0.278%
88	18.334	2590	2592	2595	rVB3	13863	10583	0.41%	0.035%
89	18.445	2608	2611	2616	rBV3	16564	22693	0.88%	0.075%
90	19.181	2734	2736	2740	rVB4	23482	25698	1.00%	0.085%
91	19.251	2745	2748	2749	rBV2	20661	21427	0.83%	0.071%
92	19.281	2749	2753	2761	rVB	141036	200633	7.80%	0.667%
93	19.392	2769	2772	2777	rBV6	19915	29897	1.16%	0.099%
94	19.604	2803	2808	2820	rBV	1756712	2570758	100.00%	8.546%
95	20.498	2957	2960	2966	rVB	85359	94693	3.68%	0.315%
96	21.063	3053	3056	3066	rBV2	231882	405838	15.79%	1.349%
97	21.357	3101	3106	3111	rBV	1781310	2376094	92.43%	7.899%
98	23.039	3389	3392	3398	rVB2	138417	203982	7.93%	0.678%
99	23.621	3485	3491	3497	rBV2	895460	1793048	69.75%	5.961%
100	23.780	3511	3518	3536	rVB2	1029408	2271877	88.37%	7.553%




Sum of corrected areas: 30079980

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010444.D
Acq On : 20 May 2022 20:17
Operator : CG/JU
Sample : N2843-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

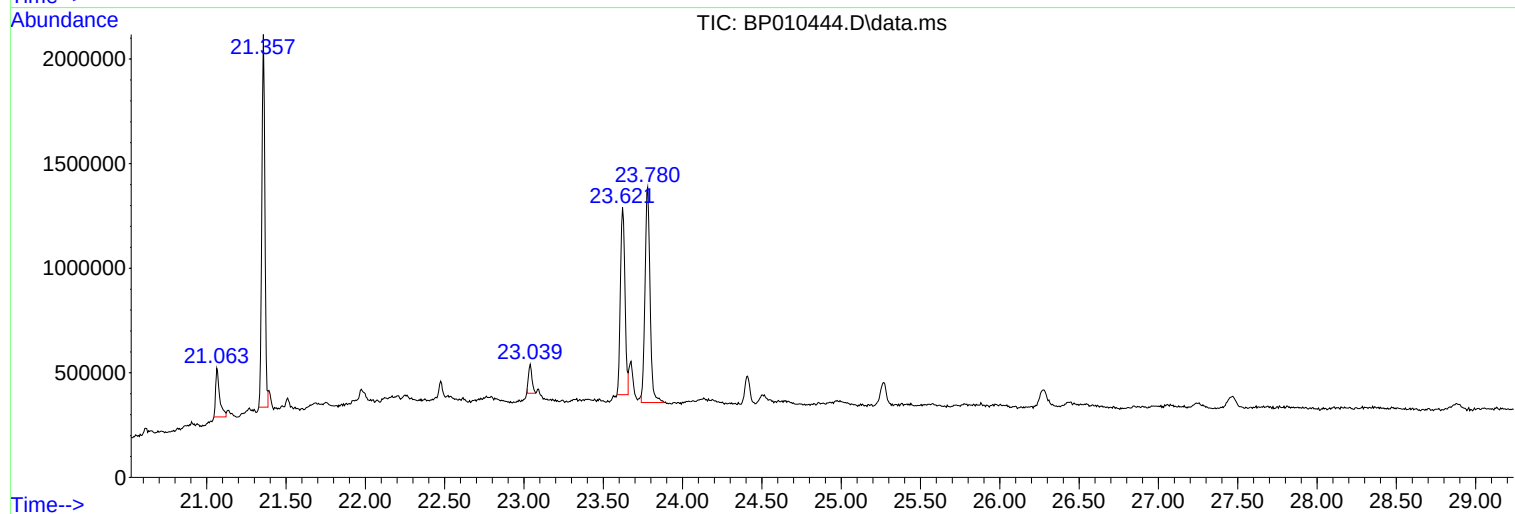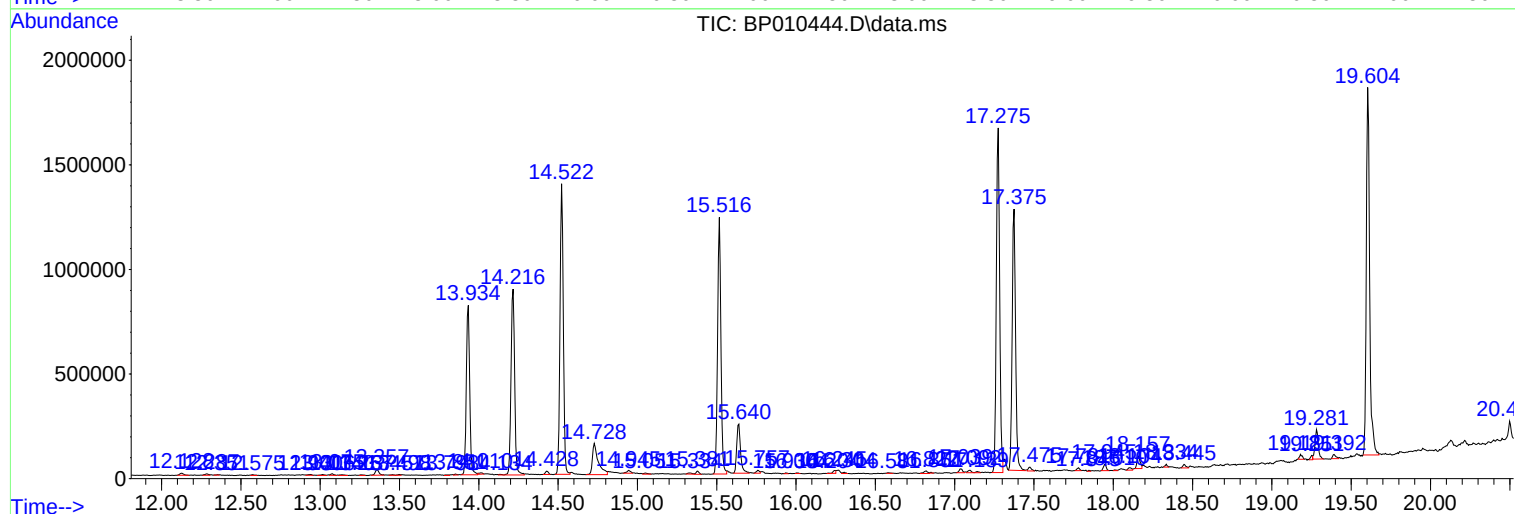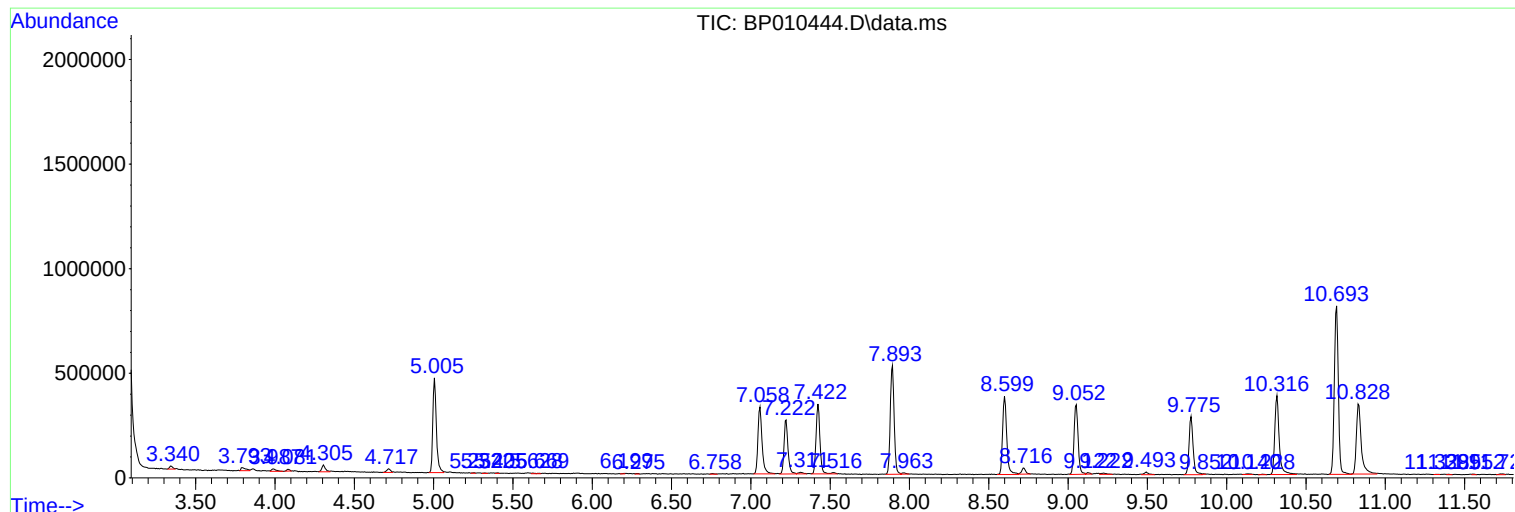

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010444.D
Acq On : 20 May 2022 20:17
Operator : CG/JU
Sample : N2843-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.005	15.88 ng/ul	695678	1,4-Dichlorobenzene-d4	7.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	46		
3	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42		
4	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	42		
5	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32		

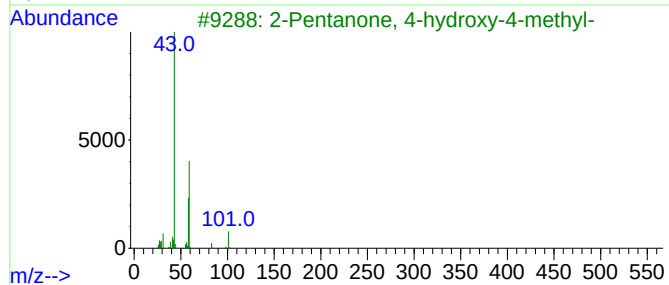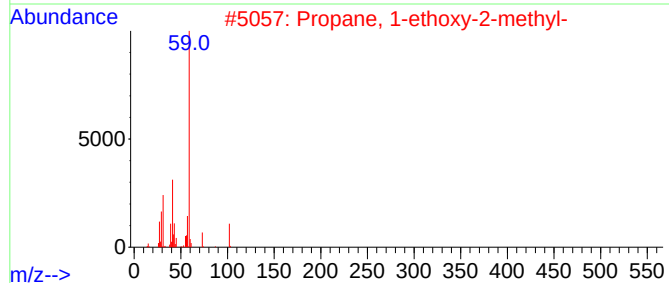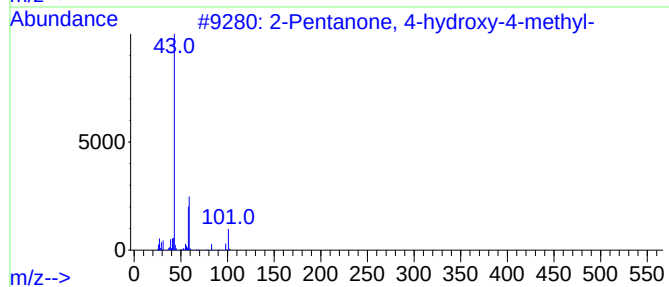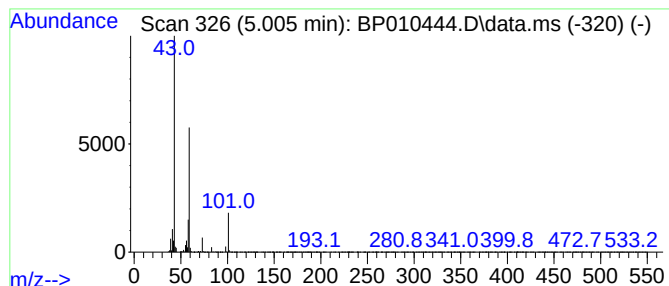

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010444.D
Acq On : 20 May 2022 20:17
Operator : CG/JU
Sample : N2843-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Octadecyl trifluoroacetate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.063	3.42 ng/ul	405838	Chrysene-d12	21.357

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Octadecyl trifluoroacetate	366	C20H37F3O2	079392-43-1	93
2			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	93
3			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	93
4			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	93
5			Pentacos-1-ene	350	C25H50	016980-85-1	93

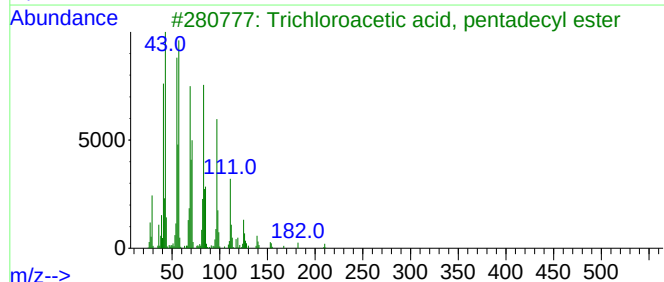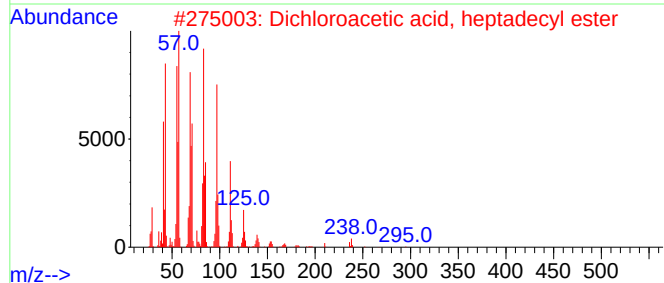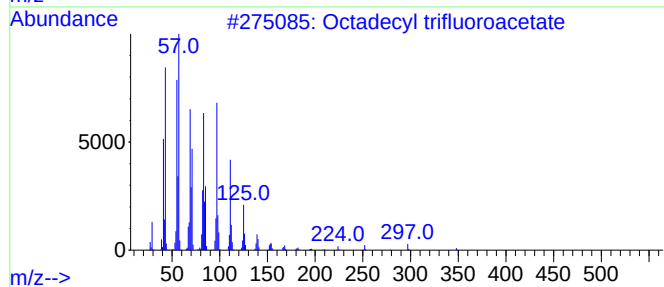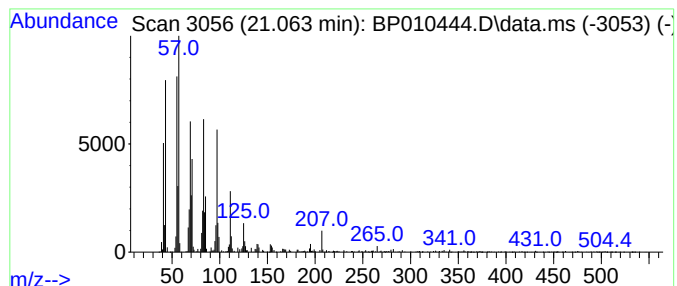

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010444.D
Acq On : 20 May 2022 20:17
Operator : CG/JU
Sample : N2843-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.005	15.9	ng/ul	695678	1	7.893	876394	20.0
Octadecyl trifl...	21.063	3.4	ng/ul	405838	5	21.357	2376090	20.0