

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010447.D
 Acq On : 20 May 2022 21:59
 Operator : CG/JU
 Sample : N2843-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	54	rVB	27022	47614	1.25%	0.114%
2	3.770	113	116	129	rBV	81621	173266	4.55%	0.414%
3	3.858	129	131	140	rVB2	15271	26801	0.70%	0.064%
4	3.987	151	153	159	rVB5	8470	11750	0.31%	0.028%
5	4.081	165	169	174	rBV4	12335	16547	0.43%	0.040%
6	4.305	203	207	220	rVB	37595	55814	1.47%	0.133%
7	4.717	273	277	281	rBV	17844	24721	0.65%	0.059%
8	4.999	320	325	332	rBV	29582	43538	1.14%	0.104%
9	5.105	341	343	351	rVB9	4333	7633	0.20%	0.018%
10	6.281	540	543	547	rVB6	3775	4427	0.12%	0.011%
11	7.058	667	675	691	rBV	468599	826857	21.73%	1.976%
12	7.222	696	703	715	rBV	369964	626885	16.48%	1.498%
13	7.317	715	719	722	rVB	5923	8405	0.22%	0.020%
14	7.422	729	737	748	rBV	480997	810043	21.29%	1.936%
15	7.522	751	754	760	rVB4	7977	12848	0.34%	0.031%
16	7.893	809	817	825	rBV	626324	1048634	27.56%	2.507%
17	7.964	825	829	834	rVB6	6697	13069	0.34%	0.031%
18	8.599	928	937	951	rBV	594403	1024149	26.92%	2.448%
19	8.716	953	957	963	rVB	27785	47064	1.24%	0.112%
20	9.052	1007	1014	1025	rBV	490975	866630	22.78%	2.072%
21	9.216	1039	1042	1047	rVB7	4437	6377	0.17%	0.015%
22	9.493	1083	1089	1094	rVB6	10467	17817	0.47%	0.043%
23	9.775	1128	1137	1146	rBV	403908	712908	18.74%	1.704%
24	9.987	1172	1173	1180	rVB7	3299	6146	0.16%	0.015%
25	10.046	1180	1183	1186	rBV5	2993	4135	0.11%	0.010%
26	10.316	1221	1229	1247	rBV	563827	1075490	28.27%	2.571%
27	10.693	1285	1293	1304	rBV	957663	1645543	43.25%	3.933%
28	10.828	1307	1316	1330	rBV	527475	1055810	27.75%	2.524%
29	11.740	1464	1471	1475	rBV10	5530	12815	0.34%	0.031%
30	12.122	1531	1536	1545	rBV	14252	25211	0.66%	0.060%
31	12.287	1558	1564	1573	rVB7	9674	18407	0.48%	0.044%
32	12.752	1639	1643	1647	rBV6	2412	4297	0.11%	0.010%
33	12.804	1647	1652	1655	rBV7	2178	4360	0.11%	0.010%
34	12.863	1657	1662	1665	rBV7	2537	4142	0.11%	0.010%
35	12.934	1669	1674	1678	rBV6	4928	5891	0.15%	0.014%
36	13.016	1684	1688	1693	rBV8	4468	4998	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010447.D
 Acq On : 20 May 2022 21:59
 Operator : CG/JU
 Sample : N2843-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.069	1693	1697	1702	rVV2	8205	11343	0.30%	0.027%
38	13.263	1725	1730	1735	rBV9	3122	7085	0.19%	0.017%
39	13.357	1739	1746	1753	rBV	33870	52930	1.39%	0.127%
40	13.493	1765	1769	1773	rBV7	2390	4000	0.11%	0.010%

41	13.857	1826	1831	1832	rBV5	4009	6071	0.16%	0.015%
42	13.928	1836	1843	1854	rVV	1205924	1794709	47.17%	4.290%
43	14.010	1855	1857	1861	rVV4	14015	21512	0.57%	0.051%
44	14.046	1861	1863	1871	rVB7	5487	12663	0.33%	0.030%
45	14.216	1882	1892	1904	rBV	1279508	2021446	53.13%	4.832%

46	14.428	1924	1928	1932	rBV	23147	32105	0.84%	0.077%
47	14.522	1937	1944	1961	rBV	1602244	2314246	60.83%	5.532%
48	14.722	1971	1978	1998	rBV	332378	753704	19.81%	1.802%
49	14.946	2011	2016	2021	rBV6	14742	26264	0.69%	0.063%
50	15.046	2032	2033	2039	rVB6	6451	7543	0.20%	0.018%

51	15.322	2076	2080	2082	rBV4	4863	6213	0.16%	0.015%
52	15.381	2086	2090	2094	rVB2	20112	25184	0.66%	0.060%
53	15.516	2106	2113	2125	rBV	1803247	2647057	69.58%	6.327%
54	15.634	2128	2133	2145	rVV	422400	667841	17.55%	1.596%
55	15.757	2150	2154	2157	rBV4	20624	31030	0.82%	0.074%

56	15.881	2171	2175	2179	rVB7	4452	7103	0.19%	0.017%
57	15.945	2182	2186	2189	rBV5	4063	5340	0.14%	0.013%
58	16.075	2206	2208	2211	rBV4	2970	4101	0.11%	0.010%
59	16.198	2226	2229	2230	rBV2	3585	4026	0.11%	0.010%
60	16.245	2232	2237	2238	rVV	27695	36019	0.95%	0.086%

61	16.269	2238	2241	2244	rVV2	26038	38321	1.01%	0.092%
62	16.304	2244	2247	2251	rVB6	9931	13553	0.36%	0.032%
63	16.651	2303	2306	2308	rBV4	4489	5281	0.14%	0.013%
64	16.822	2330	2335	2338	rBV6	7119	10542	0.28%	0.025%
65	16.940	2352	2355	2356	rBV3	3960	4175	0.11%	0.010%

66	16.951	2356	2357	2362	rVB5	5187	6332	0.17%	0.015%
67	17.040	2368	2372	2375	rBV	23430	28625	0.75%	0.068%
68	17.092	2377	2381	2387	rVB2	21056	30779	0.81%	0.074%
69	17.275	2405	2412	2422	rBV	1921160	2799492	73.58%	6.692%
70	17.375	2422	2429	2440	rVV	1877599	2816326	74.03%	6.732%

71	17.475	2442	2446	2451	rVB7	21470	36485	0.96%	0.087%
72	17.569	2459	2462	2463	rBV3	4443	5486	0.14%	0.013%
73	17.781	2493	2498	2503	rBV2	28023	39337	1.03%	0.094%
74	17.892	2514	2517	2520	rVB5	3971	4889	0.13%	0.012%
75	17.945	2523	2526	2531	rVB7	10519	15319	0.40%	0.037%

76	18.104	2549	2553	2556	rBV6	7836	10783	0.28%	0.026%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010447.D
 Acq On : 20 May 2022 21:59
 Operator : CG/JU
 Sample : N2843-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4J1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	18.157	2558	2562	2572	rBV	123330	205436	5.40%	0.491%
78	18.445	2608	2611	2615	rBV	26407	30872	0.81%	0.074%
79	19.057	2712	2715	2722	rVB	30868	39304	1.03%	0.094%
80	19.186	2733	2737	2743	rVB3	33750	51388	1.35%	0.123%
81	19.251	2745	2748	2751	rBV	29907	42892	1.13%	0.103%
82	19.392	2768	2772	2780	rBV6	36290	67411	1.77%	0.161%
83	19.604	2802	2808	2823	rBV	2691407	3804457	100.00%	9.094%
84	20.133	2895	2898	2902	rVB	53973	53918	1.42%	0.129%
85	20.616	2976	2980	2983	rBV	71455	87885	2.31%	0.210%
86	21.063	3052	3056	3066	rBV	664001	1062757	27.93%	2.540%
87	21.357	3101	3106	3117	rBV	2220996	2953911	77.64%	7.061%
88	21.504	3129	3131	3136	rVB2	91574	108155	2.84%	0.259%
89	21.975	3208	3211	3220	rVB3	96323	173327	4.56%	0.414%
90	22.475	3293	3296	3301	rVB2	108093	137500	3.61%	0.329%
91	23.033	3388	3391	3397	rVB	131331	197399	5.19%	0.472%
92	23.622	3484	3491	3498	rBV2	1535089	3191510	83.89%	7.629%
93	23.780	3511	3518	3529	rVB2	1330256	2706660	71.14%	6.470%
94	24.404	3621	3624	3634	rVB2	134032	254385	6.69%	0.608%




Sum of corrected areas: 41835469

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010447.D
Acq On : 20 May 2022 21:59
Operator : CG/JU
Sample : N2843-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

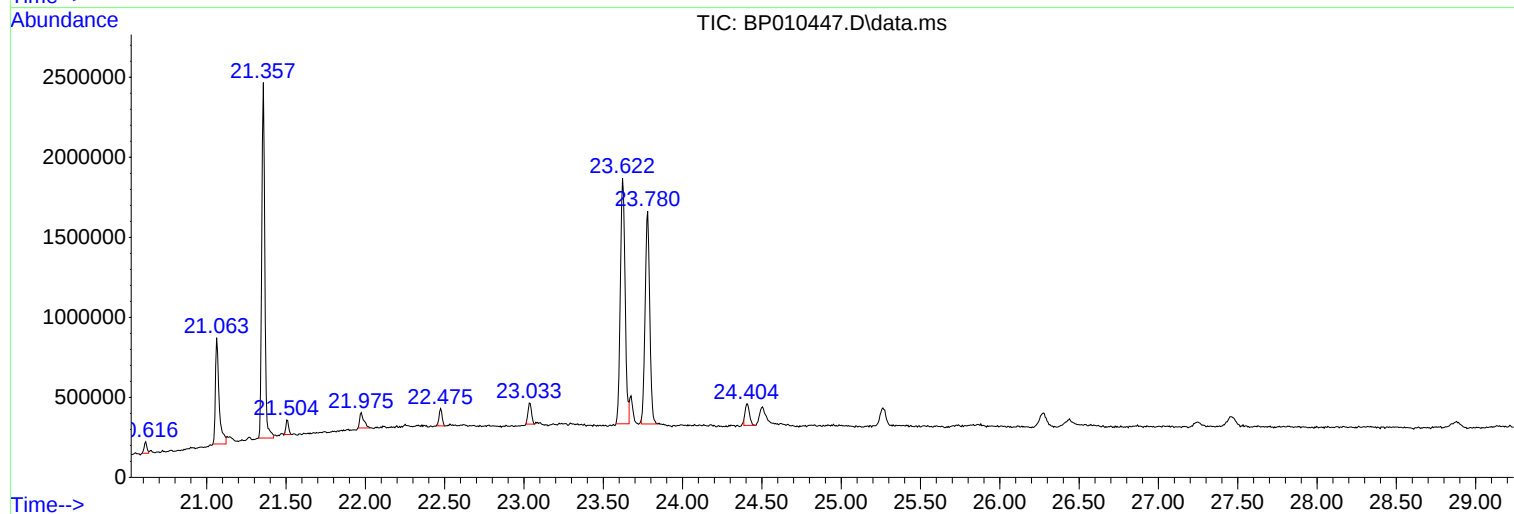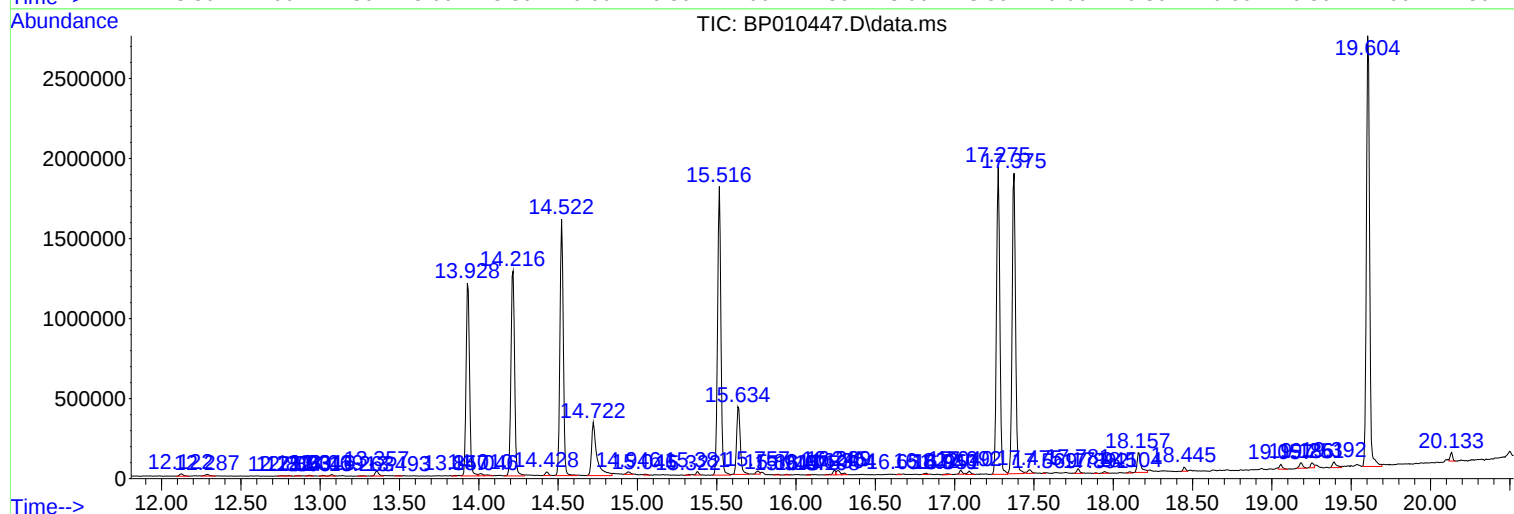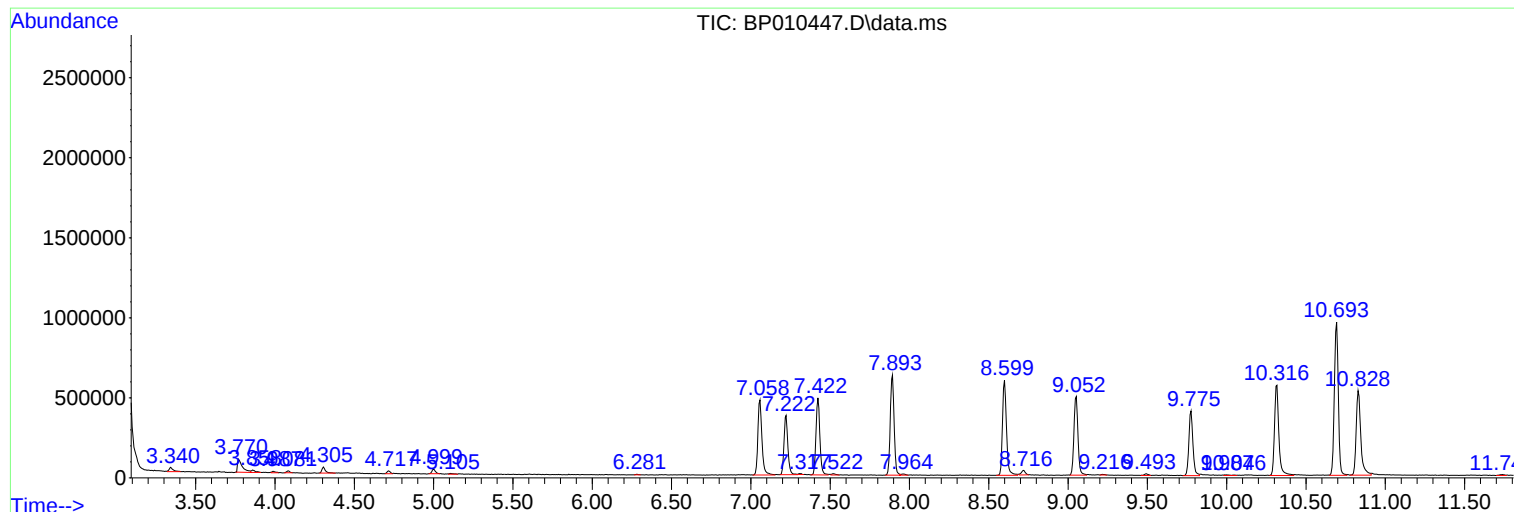

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010447.D
Acq On : 20 May 2022 21:59
Operator : CG/JU
Sample : N2843-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.063	7.20 ng/ul	1062760	Chrysene-d12	21.357

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1-Tetracosene	336	C24H48	010192-32-2	99
2		1-Tetracosene	336	C24H48	010192-32-2	99
3		Cyclotetracosane	336	C24H48	000297-03-0	95
4		Cyclotetracosane	336	C24H48	000297-03-0	94
5		Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94

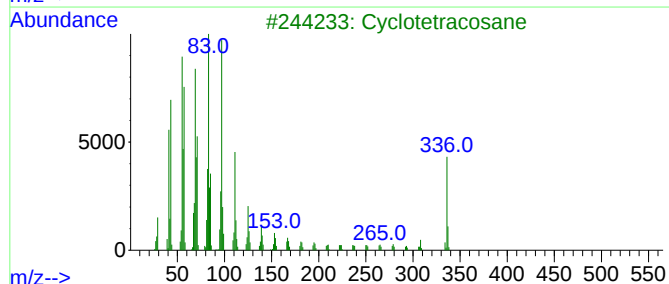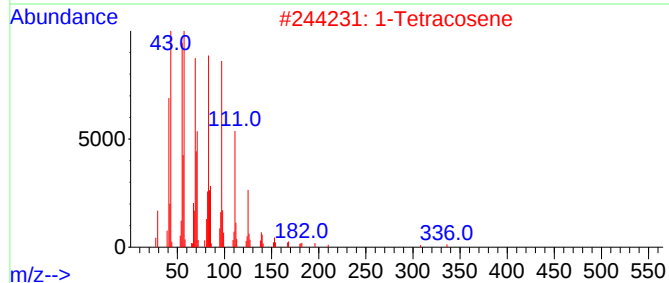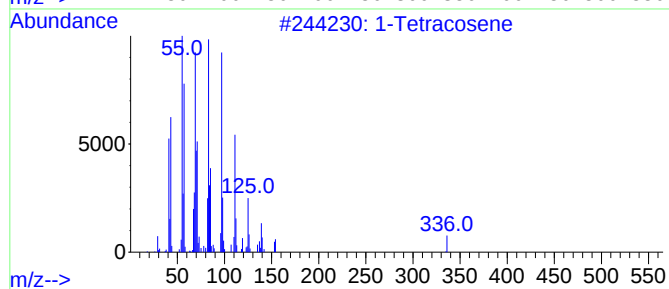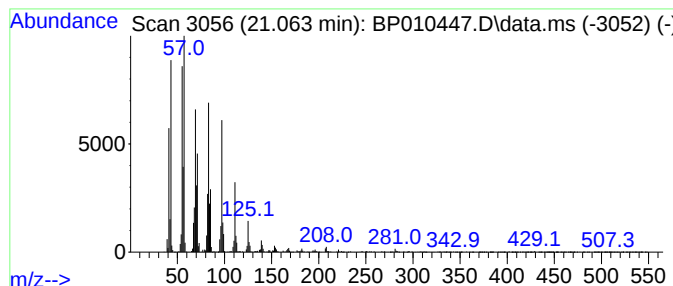

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010447.D
Acq On : 20 May 2022 21:59
Operator : CG/JU
Sample : N2843-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4J1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.063	7.2	ng/u1	1062760	5	21.357	2953910	20.0