

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010459.D
 Acq On : 21 May 2022 05:19
 Operator : CG/JU
 Sample : PB144974BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK974

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rBV	38115	52674	1.04%	0.104%
2	3.758	111	114	133	rBV	496149	1007491	19.86%	1.987%
3	4.081	165	169	173	rBV2	9007	12070	0.24%	0.024%
4	7.057	668	675	689	rBV	699810	1205509	23.76%	2.378%
5	7.216	696	702	715	rBV	543432	925748	18.25%	1.826%
6	7.422	729	737	752	rBV	726603	1216453	23.98%	2.399%
7	7.887	808	816	829	rBV	642820	1065573	21.00%	2.102%
8	8.599	930	937	950	rBV	910208	1559055	30.73%	3.075%
9	9.046	1005	1013	1028	rBV	785421	1348773	26.59%	2.660%
10	9.769	1128	1136	1149	rBV	639466	1122413	22.12%	2.214%
11	10.310	1221	1228	1243	rBV	868245	1563527	30.82%	3.084%
12	10.687	1283	1292	1306	rBV	959453	1657910	32.68%	3.270%
13	10.828	1308	1316	1331	rBV	857463	1661287	32.74%	3.277%
14	12.292	1558	1565	1573	rVB3	11646	25213	0.50%	0.050%
15	13.934	1836	1844	1853	rBV	1756564	2618574	51.61%	5.165%
16	14.216	1884	1892	1908	rBV	1866885	2880462	56.78%	5.682%
17	14.522	1936	1944	1953	rBV	1577258	2312040	45.57%	4.561%
18	14.716	1970	1977	1999	rBV	618699	1236261	24.37%	2.439%
19	15.516	2106	2113	2126	rBV	2535750	3697436	72.88%	7.293%
20	15.633	2127	2133	2147	rVV	779311	1175983	23.18%	2.320%
21	15.757	2149	2154	2163	rVB2	32848	54469	1.07%	0.107%
22	16.081	2203	2209	2212	rBV7	3578	6414	0.13%	0.013%
23	16.210	2228	2231	2236	rVB7	3195	5194	0.10%	0.010%
24	16.298	2242	2246	2251	rVB5	9147	15500	0.31%	0.031%
25	16.951	2353	2357	2364	rBV8	6157	10962	0.22%	0.022%
26	17.063	2370	2376	2383	rVB5	4322	8648	0.17%	0.017%
27	17.275	2405	2412	2422	rBV	2003993	2847184	56.12%	5.616%
28	17.375	2422	2429	2446	rVV	2793602	4220076	83.18%	8.324%
29	19.186	2732	2737	2741	rBV2	38070	54419	1.07%	0.107%
30	19.251	2744	2748	2753	rBV	31141	45746	0.90%	0.090%
31	19.539	2794	2797	2800	rBV4	6913	7299	0.14%	0.014%
32	19.604	2802	2808	2823	rBV	3814187	5073424	100.00%	10.007%
33	21.357	3100	3106	3118	rBV	2269955	3112948	61.36%	6.140%
34	23.621	3483	3491	3498	rBV2	2063012	4223582	83.25%	8.331%
35	23.780	3511	3518	3531	rVB2	1288578	2665998	52.55%	5.259%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010459.D
Acq On : 21 May 2022 05:19
Operator : CG/JU
Sample : PB144974BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK974

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 50696315

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010459.D
Acq On : 21 May 2022 05:19
Operator : CG/JU
Sample : PB144974BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK974

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

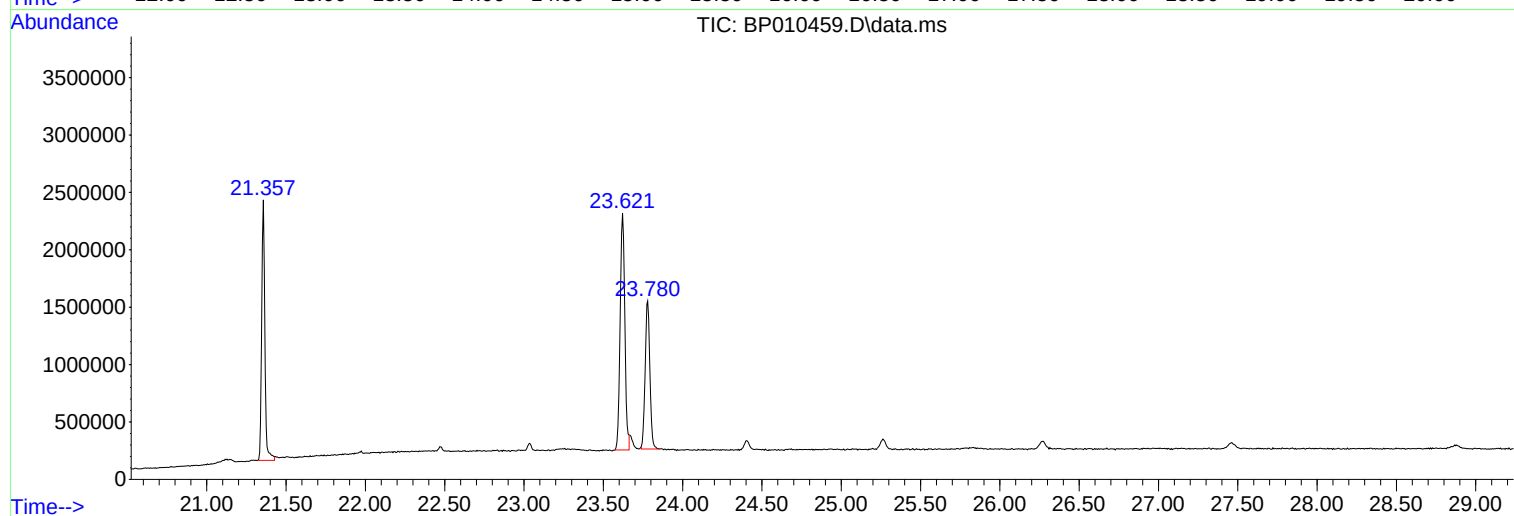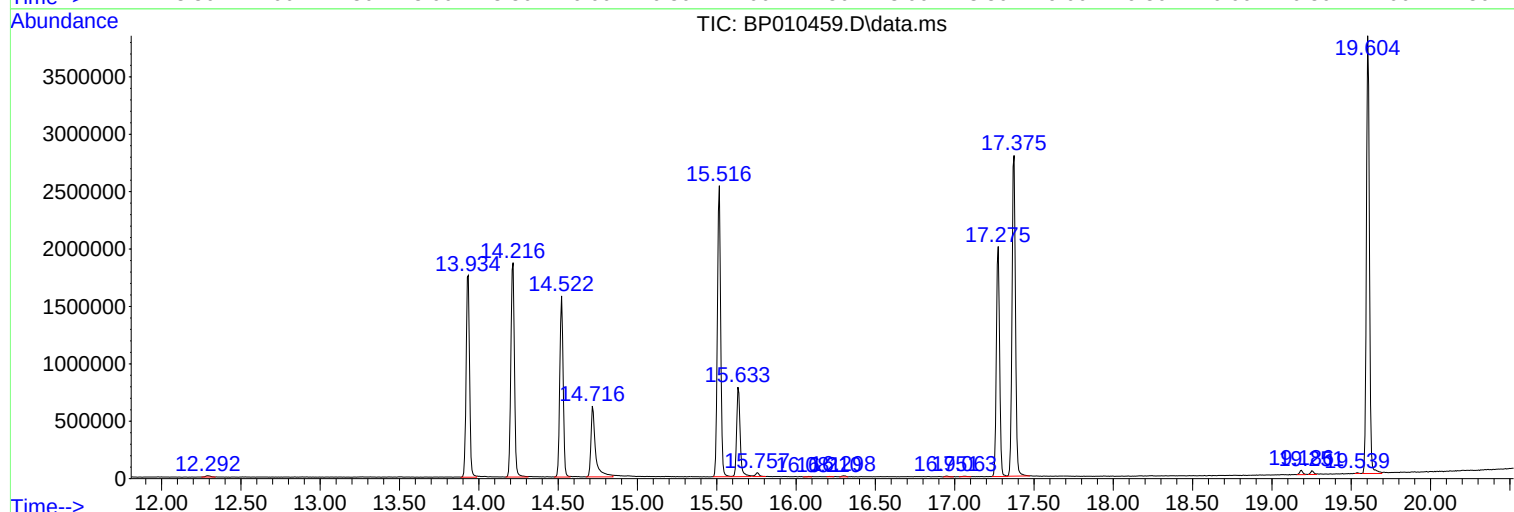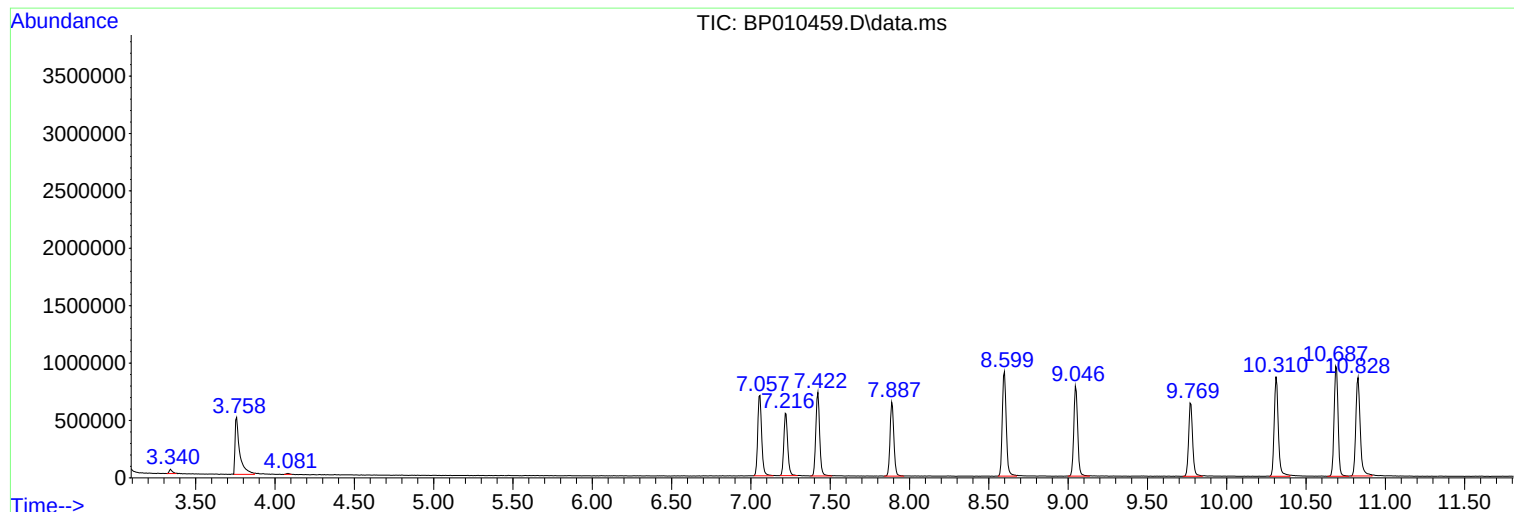

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010459.D
Acq On : 21 May 2022 05:19
Operator : CG/JU
Sample : PB144974BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK974

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010459.D
Acq On : 21 May 2022 05:19
Operator : CG/JU
Sample : PB144974BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK974

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------