

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010466.D
 Acq On : 21 May 2022 09:15
 Operator : CG/JU
 Sample : N2918-21
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	24	26	30	rVB5	10687	13052	0.17%	0.019%
2	3.340	40	43	54	rVB	45498	71159	0.94%	0.103%
3	3.764	112	115	143	rBV	200284	420835	5.56%	0.610%
4	3.993	148	154	160	rVB	30758	53090	0.70%	0.077%
5	4.081	166	169	176	rVB4	13253	20060	0.27%	0.029%
6	4.881	301	305	308	rBV6	5681	9096	0.12%	0.013%
7	5.011	319	327	338	rVB2	40637	77743	1.03%	0.113%
8	5.605	421	428	432	rBV3	8354	13765	0.18%	0.020%
9	7.058	668	675	687	rBV	252381	446442	5.90%	0.647%
10	7.222	695	703	717	rBV	984266	1606018	21.23%	2.327%
11	7.422	729	737	749	rBV	949784	1611434	21.30%	2.335%
12	7.522	749	754	762	rVB5	13859	29900	0.40%	0.043%
13	7.893	808	817	834	rBV	792764	1378031	18.21%	1.997%
14	8.246	870	877	882	rBV3	16080	30472	0.40%	0.044%
15	8.599	930	937	954	rBV	790978	1349664	17.84%	1.956%
16	8.740	957	961	968	rVB9	7583	15019	0.20%	0.022%
17	9.004	1000	1006	1007	rBV4	9063	15892	0.21%	0.023%
18	9.052	1007	1014	1028	rVB	1312394	2228245	29.45%	3.229%
19	9.775	1129	1137	1152	rBV	1066419	1804213	23.85%	2.615%
20	10.316	1221	1229	1248	rBV	1364932	2479902	32.78%	3.594%
21	10.469	1252	1255	1259	rVB5	5781	8974	0.12%	0.013%
22	10.557	1262	1270	1280	rVB3	50542	88404	1.17%	0.128%
23	10.693	1284	1293	1308	rBV	1151254	1984208	26.23%	2.875%
24	10.828	1308	1316	1333	rBV	989094	1851939	24.48%	2.684%
25	11.081	1354	1359	1365	rVB3	17056	31085	0.41%	0.045%
26	11.504	1425	1431	1440	rBV3	8281	22682	0.30%	0.033%
27	12.281	1556	1563	1571	rVV2	26848	52858	0.70%	0.077%
28	12.498	1593	1600	1604	rBV10	5141	9068	0.12%	0.013%
29	12.728	1631	1639	1650	rBV2	61969	122562	1.62%	0.178%
30	13.175	1710	1715	1720	rBV7	9539	15818	0.21%	0.023%
31	13.251	1720	1728	1734	rVV5	15924	35455	0.47%	0.051%
32	13.357	1734	1746	1753	rVV	178655	329128	4.35%	0.477%
33	13.428	1753	1758	1765	rVV3	29410	54423	0.72%	0.079%
34	13.492	1765	1769	1774	rVV8	6324	11482	0.15%	0.017%
35	13.557	1777	1780	1787	rVB9	5808	10257	0.14%	0.015%
36	13.934	1836	1844	1849	rBV	2987787	4099753	54.19%	5.941%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010466.D
 Acq On : 21 May 2022 09:15
 Operator : CG/JU
 Sample : N2918-21
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.981	1849	1852	1860	rVV	335841	453883	6.00%	0.658%
38	14.069	1863	1867	1872	rVB7	15631	25088	0.33%	0.036%
39	14.216	1881	1892	1908	rBV	3370097	4948530	65.41%	7.171%
40	14.428	1923	1928	1934	rVB9	4877	9114	0.12%	0.013%
41	14.522	1934	1944	1960	rBV	1767322	2742225	36.25%	3.974%
42	14.657	1961	1967	1974	rVB2	13243	24040	0.32%	0.035%
43	14.734	1974	1980	1990	rBV	150706	331898	4.39%	0.481%
44	14.851	1996	2000	2007	rVV2	44182	71312	0.94%	0.103%
45	14.922	2007	2012	2022	rVB	199530	300953	3.98%	0.436%
46	15.075	2033	2038	2042	rBV3	34936	57422	0.76%	0.083%
47	15.157	2048	2052	2056	rBV6	12307	19318	0.26%	0.028%
48	15.269	2065	2071	2075	rVB8	5554	12173	0.16%	0.018%
49	15.334	2077	2082	2087	rVV5	6192	12182	0.16%	0.018%
50	15.463	2097	2104	2106	rBV6	7285	14084	0.19%	0.020%
51	15.522	2107	2114	2119	rVV	4191498	6101757	80.65%	8.843%
52	15.569	2119	2122	2128	rVV	108269	173176	2.29%	0.251%
53	15.639	2128	2134	2147	rVV	825493	1235983	16.34%	1.791%
54	15.757	2148	2154	2163	rVB2	50847	90040	1.19%	0.130%
55	15.869	2168	2173	2179	rVB4	19470	36014	0.48%	0.052%
56	16.010	2192	2197	2202	rBV3	14627	23490	0.31%	0.034%
57	16.210	2226	2231	2232	rBV5	6107	8949	0.12%	0.013%
58	16.304	2243	2247	2255	rVB5	25147	44688	0.59%	0.065%
59	16.451	2269	2272	2277	rBV4	6188	10508	0.14%	0.015%
60	16.551	2286	2289	2293	rVB2	14395	15622	0.21%	0.023%
61	16.928	2349	2353	2363	rVB	89290	148801	1.97%	0.216%
62	17.039	2367	2372	2375	rBV3	14549	23796	0.31%	0.034%
63	17.092	2378	2381	2387	rVB2	27376	35244	0.47%	0.051%
64	17.275	2406	2412	2419	rBV	2197665	3159459	41.76%	4.579%
65	17.375	2422	2429	2442	rBV2	4791102	6823882	90.20%	9.889%
66	17.528	2448	2455	2464	rBV5	85215	201383	2.66%	0.292%
67	17.780	2495	2498	2506	rVB3	21616	28654	0.38%	0.042%
68	17.945	2522	2526	2530	rBV5	23359	34029	0.45%	0.049%
69	18.157	2559	2562	2569	rBV3	60443	92632	1.22%	0.134%
70	19.180	2733	2736	2742	rBV	66019	99576	1.32%	0.144%
71	19.257	2746	2749	2756	rVB	52640	82495	1.09%	0.120%
72	19.610	2803	2809	2817	rBV	5660951	7565638	100.00%	10.964%
73	21.063	3053	3056	3063	rBV	225087	329677	4.36%	0.478%
74	21.357	3101	3106	3122	rVB	2222654	3002394	39.68%	4.351%
75	23.633	3485	3493	3507	rVB2	2567282	5848069	77.30%	8.475%
76	23.786	3512	3519	3528	rVB2	1098239	2364493	31.25%	3.427%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010466.D
Acq On : 21 May 2022 09:15
Operator : CG/JU
Sample : N2918-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION


Sum of corrected areas: 69004799

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010466.D
Acq On : 21 May 2022 09:15
Operator : CG/JU
Sample : N2918-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

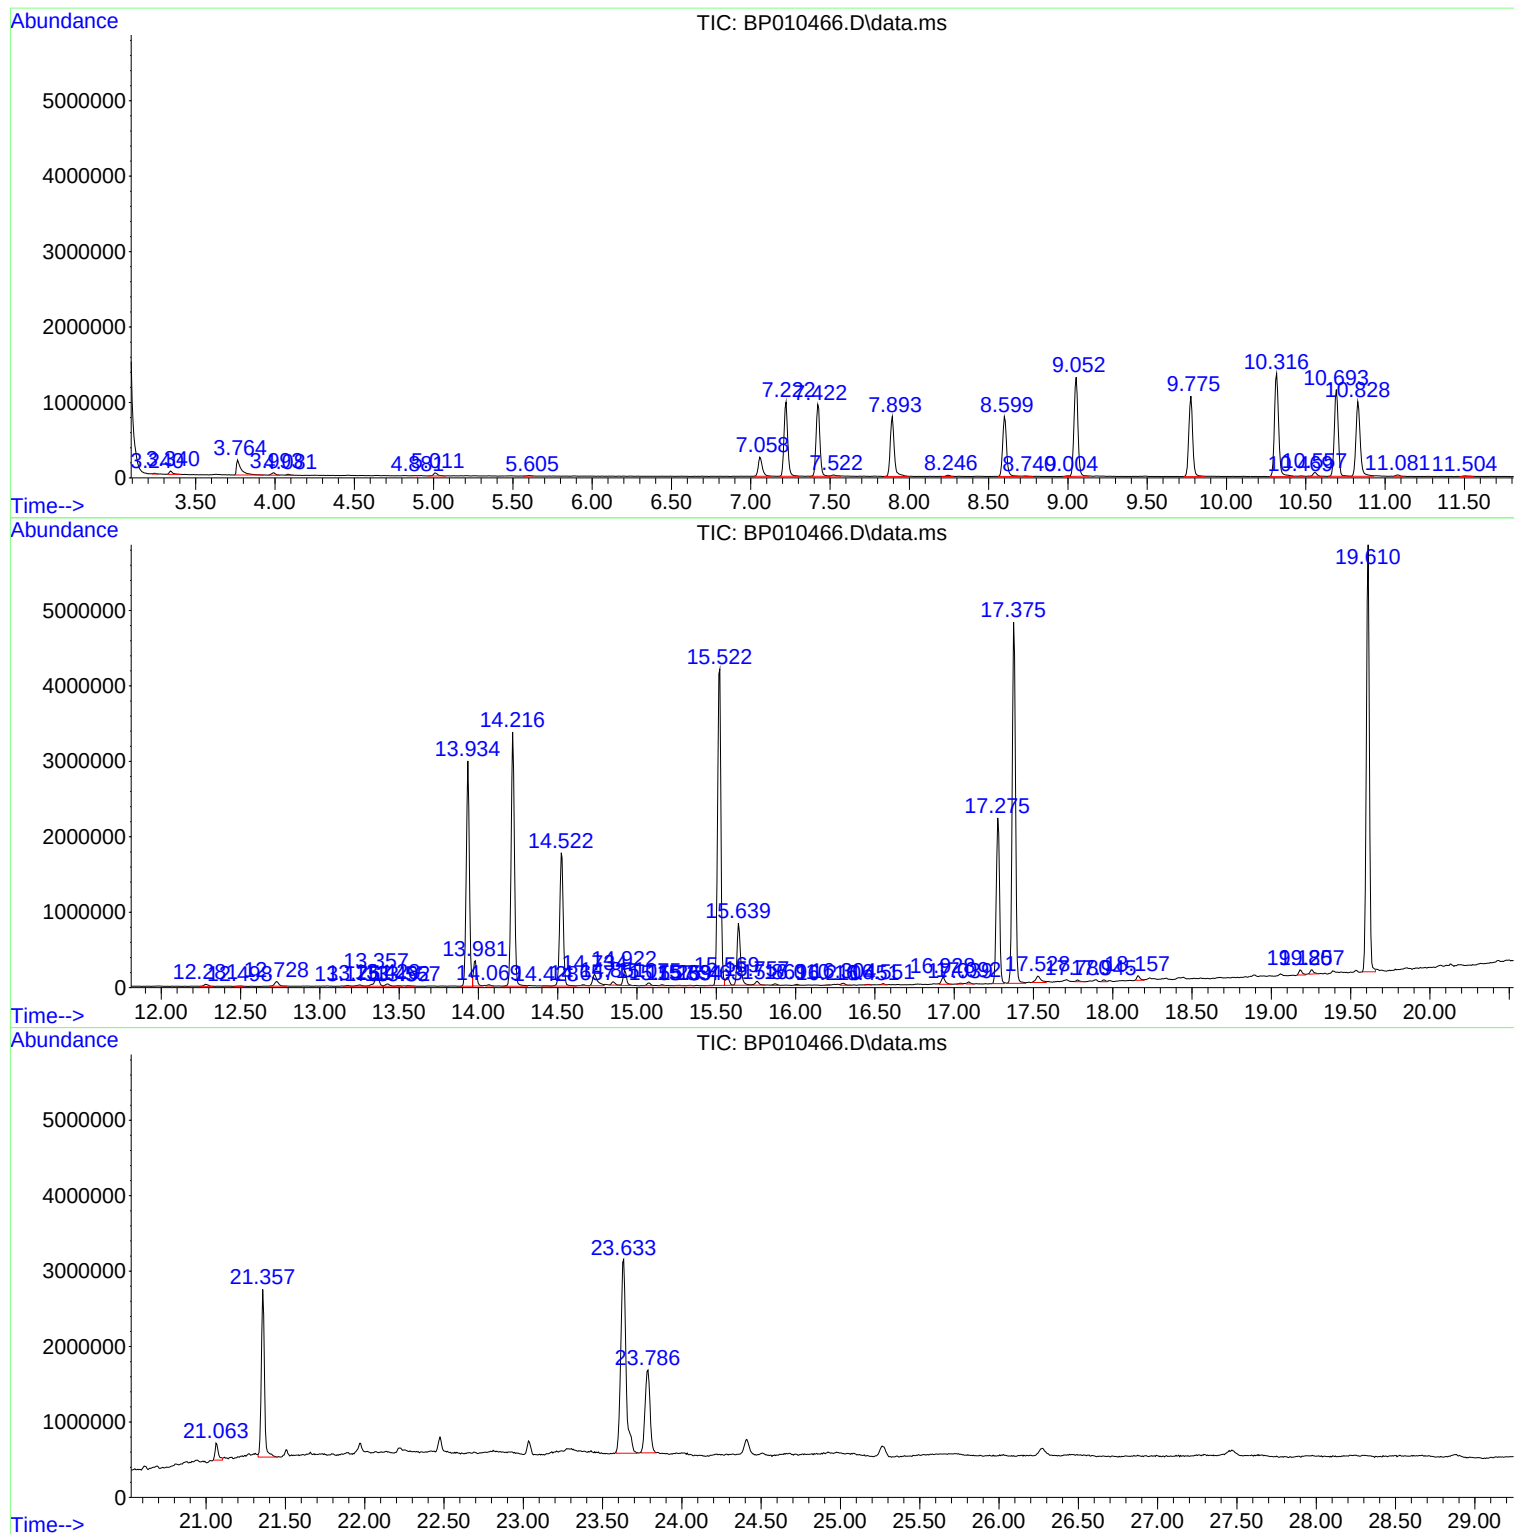

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010466.D
Acq On : 21 May 2022 09:15
Operator : CG/JU
Sample : N2918-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.063	2.20 ng/ul	329677	Chrysene-d12	21.357

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene		364	C26H52	018835-33-1	97
2	1-Tricosene		322	C23H46	018835-32-0	97
3	1-Hexacosene		364	C26H52	018835-33-1	95
4	9-Tricosene, (Z)-		322	C23H46	027519-02-4	93
5	1-Docosene		308	C22H44	001599-67-3	91

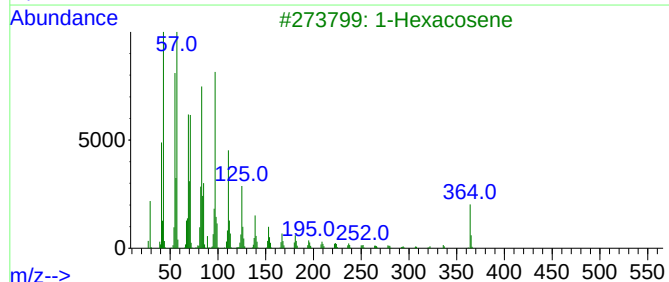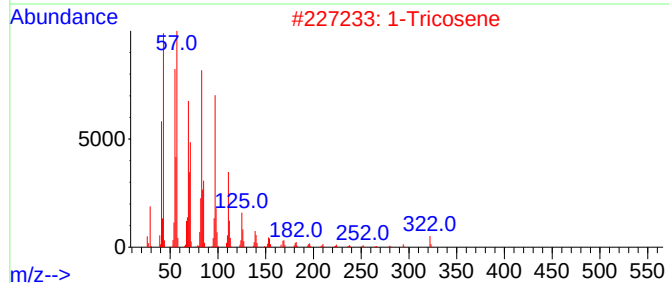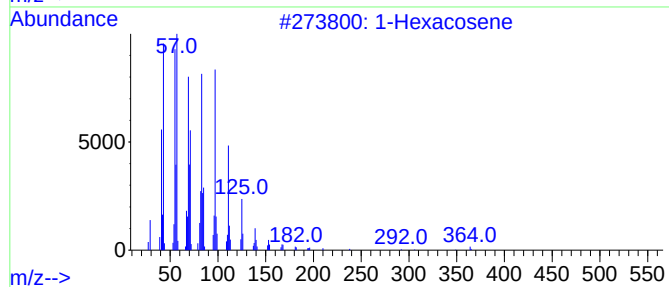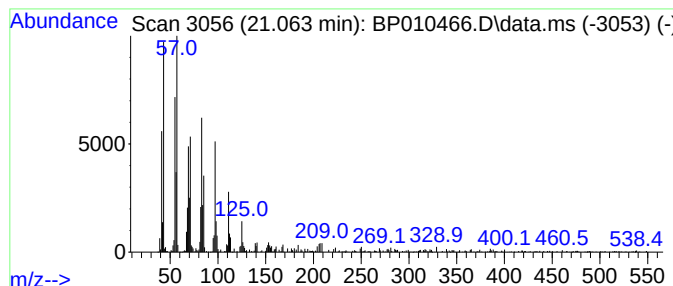

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010466.D
Acq On : 21 May 2022 09:15
Operator : CG/JU
Sample : N2918-21
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.063	2.2	ng/u1	329677	5	21.357	3002390	20.0