

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010467.D
 Acq On : 21 May 2022 09:49
 Operator : CG/JU
 Sample : N2918-22
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	53	rVB	34181	52677	0.80%	0.085%
2	3.764	112	115	131	rBV	162735	323513	4.89%	0.523%
3	3.987	149	153	160	rVB	22242	35721	0.54%	0.058%
4	4.452	229	232	238	rVB5	9587	16956	0.26%	0.027%
5	4.881	302	305	309	rBV6	4992	7267	0.11%	0.012%
6	5.005	322	326	340	rBV	157678	255955	3.87%	0.414%
7	5.211	355	361	366	rBV	22565	35316	0.53%	0.057%
8	5.605	424	428	433	rVB3	6786	11577	0.18%	0.019%
9	7.058	668	675	689	rVB	226087	405304	6.13%	0.656%
10	7.222	696	703	718	rBV	815362	1361296	20.58%	2.202%
11	7.422	726	737	750	rBV	841600	1407270	21.28%	2.276%
12	7.522	750	754	762	rVV8	12102	30705	0.46%	0.050%
13	7.616	766	770	774	rVB6	7231	13861	0.21%	0.022%
14	7.893	809	817	833	rBV	649077	1114834	16.85%	1.803%
15	8.246	870	877	885	rBV	110119	201329	3.04%	0.326%
16	8.434	904	909	916	rVB2	11477	20491	0.31%	0.033%
17	8.599	930	937	955	rBV	705689	1200844	18.16%	1.942%
18	8.740	955	961	971	rVV	49025	85682	1.30%	0.139%
19	9.052	1006	1014	1032	rVV	1102484	1906830	28.83%	3.084%
20	9.181	1032	1036	1040	rVB7	3957	6719	0.10%	0.011%
21	9.481	1086	1087	1094	rVB6	4966	7898	0.12%	0.013%
22	9.693	1116	1123	1128	rVB10	2826	6754	0.10%	0.011%
23	9.775	1128	1137	1151	rBV	900442	1550841	23.45%	2.508%
24	10.093	1186	1191	1196	rVB9	7312	14440	0.22%	0.023%
25	10.316	1218	1229	1247	rBV	1192683	2168249	32.78%	3.507%
26	10.469	1252	1255	1261	rVB8	7268	11455	0.17%	0.019%
27	10.557	1265	1270	1275	rBV5	10592	17108	0.26%	0.028%
28	10.693	1285	1293	1297	rBV	954824	1640427	24.80%	2.653%
29	10.740	1297	1301	1308	rVV	445165	769720	11.64%	1.245%
30	10.828	1308	1316	1334	rVV2	1022846	2017313	30.50%	3.263%
31	11.081	1355	1359	1370	rVB10	13391	29469	0.45%	0.048%
32	11.522	1426	1434	1437	rBV10	8450	18690	0.28%	0.030%
33	11.804	1476	1482	1488	rBV	37875	65512	0.99%	0.106%
34	11.987	1508	1513	1521	rBV	4012	7253	0.11%	0.012%
35	12.251	1552	1558	1559	rBV4	9540	16539	0.25%	0.027%
36	12.281	1559	1563	1570	rVV	24779	44092	0.67%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010467.D
 Acq On : 21 May 2022 09:49
 Operator : CG/JU
 Sample : N2918-22
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	12.351	1570	1575	1584	rVB2	30511	53670	0.81%	0.087%
38	12.569	1607	1612	1621	rVB2	30858	53424	0.81%	0.086%
39	12.681	1624	1631	1633	rVV8	5158	9842	0.15%	0.016%
40	12.728	1635	1639	1647	rVB9	16204	31228	0.47%	0.051%

41	13.010	1681	1687	1691	rBV9	4557	10599	0.16%	0.017%
42	13.040	1691	1692	1700	rVB8	6910	10076	0.15%	0.016%
43	13.251	1722	1728	1731	rBV8	6463	10606	0.16%	0.017%
44	13.357	1739	1746	1755	rBV	96873	158667	2.40%	0.257%
45	13.428	1755	1758	1764	rVB7	7761	11863	0.18%	0.019%

46	13.498	1764	1770	1774	rBV9	5207	9560	0.14%	0.015%
47	13.557	1774	1780	1788	rBV9	5825	14818	0.22%	0.024%
48	13.698	1797	1804	1812	rVB9	8475	21463	0.32%	0.035%
49	13.851	1824	1830	1834	rVB8	5781	11795	0.18%	0.019%
50	13.934	1836	1844	1849	rBV	2539137	3514546	53.14%	5.684%

51	13.981	1849	1852	1860	rVB	240536	319519	4.83%	0.517%
52	14.216	1879	1892	1906	rBV	2827297	4277416	64.67%	6.918%
53	14.522	1937	1944	1951	rBV	1482017	2239622	33.86%	3.622%
54	14.587	1951	1955	1961	rVB	43443	73349	1.11%	0.119%
55	14.657	1961	1967	1974	rVB	68514	104275	1.58%	0.169%

56	14.734	1974	1980	1988	rBV	142621	301436	4.56%	0.488%
57	14.798	1988	1991	1996	rVB3	26735	40491	0.61%	0.065%
58	14.922	2007	2012	2024	rVB	143999	249662	3.77%	0.404%
59	15.075	2031	2038	2043	rBV	100174	159547	2.41%	0.258%
60	15.157	2047	2052	2057	rVB3	28959	46804	0.71%	0.076%

61	15.245	2063	2067	2074	rVB7	7913	15448	0.23%	0.025%
62	15.328	2077	2081	2088	rVV8	6934	11918	0.18%	0.019%
63	15.516	2107	2113	2119	rBV	3521968	5210440	78.78%	8.427%
64	15.569	2119	2122	2128	rVV3	97350	163172	2.47%	0.264%
65	15.639	2128	2134	2145	rVV	691474	1061291	16.05%	1.716%

66	15.728	2145	2149	2151	rVV3	33640	57526	0.87%	0.093%
67	15.757	2151	2154	2159	rVB2	46034	67456	1.02%	0.109%
68	15.863	2169	2172	2180	rVB5	15614	27420	0.41%	0.044%
69	16.010	2193	2197	2207	rVB3	16177	33408	0.51%	0.054%
70	16.128	2213	2217	2224	rVB9	14692	23481	0.36%	0.038%

71	16.204	2226	2230	2232	rVV5	8694	11868	0.18%	0.019%
72	16.245	2233	2237	2240	rVV4	20469	37075	0.56%	0.060%
73	16.298	2243	2246	2253	rVB6	20065	34473	0.52%	0.056%
74	16.434	2267	2269	2271	rBV3	5954	6841	0.10%	0.011%
75	16.539	2281	2287	2295	rBV2	33418	77251	1.17%	0.125%

76	16.775	2320	2327	2333	rBV10	14546	38357	0.58%	0.062%
----	--------	------	------	------	-------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010467.D
 Acq On : 21 May 2022 09:49
 Operator : CG/JU
 Sample : N2918-22
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.875	2340	2344	2345	rBV4	22422	25925	0.39%	0.042%
78	16.928	2349	2353	2361	rVB2	125885	208219	3.15%	0.337%
79	17.034	2369	2371	2374	rBV4	7692	10671	0.16%	0.017%
80	17.092	2377	2381	2387	rVB	37388	58783	0.89%	0.095%
81	17.275	2406	2412	2417	rBV	1805385	2619994	39.61%	4.237%
82	17.316	2417	2419	2423	rVV	155967	195673	2.96%	0.316%
83	17.375	2423	2429	2439	rVB2	3900792	5656709	85.52%	9.149%
84	17.533	2449	2456	2465	rBV5	47362	110637	1.67%	0.179%
85	17.681	2472	2481	2488	rBV	140714	229331	3.47%	0.371%
86	17.839	2505	2508	2512	rBV4	17586	25740	0.39%	0.042%
87	17.892	2513	2517	2522	rVB8	20148	29372	0.44%	0.048%
88	17.975	2529	2531	2536	rVB5	11410	15784	0.24%	0.026%
89	18.163	2558	2563	2570	rBV	89747	151836	2.30%	0.246%
90	18.416	2603	2606	2609	rBV4	13444	17484	0.26%	0.028%
91	19.186	2733	2737	2743	rVB2	53995	73484	1.11%	0.119%
92	19.251	2745	2748	2751	rBV	51243	65927	1.00%	0.107%
93	19.392	2769	2772	2780	rBV8	36474	56601	0.86%	0.092%
94	19.610	2803	2809	2822	rBV	4992408	6614293	100.00%	10.697%
95	21.069	3053	3057	3062	rBV	237973	357654	5.41%	0.578%
96	21.357	3101	3106	3119	rVB	1926305	2603631	39.36%	4.211%
97	23.039	3389	3392	3396	rVB	138442	189468	2.86%	0.306%
98	23.627	3485	3492	3499	rBV2	2370718	4954912	74.91%	8.014%
99	23.786	3513	3519	3527	rVB2	1041846	2067202	31.25%	3.343%




Sum of corrected areas: 61830940

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010467.D
Acq On : 21 May 2022 09:49
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

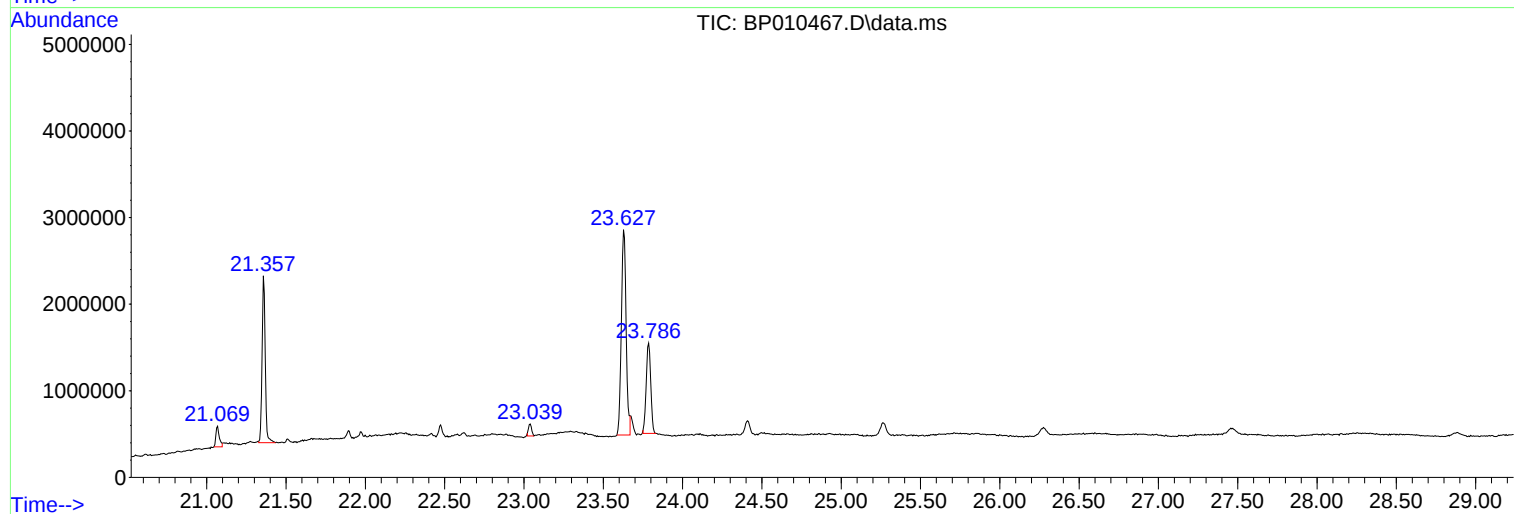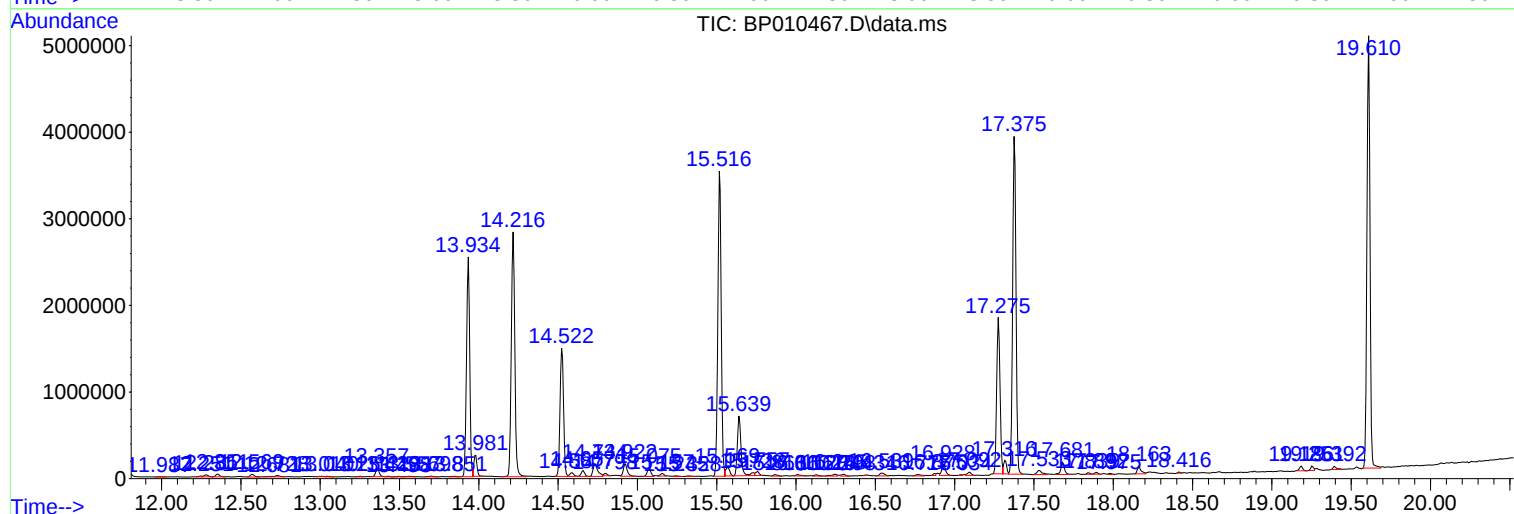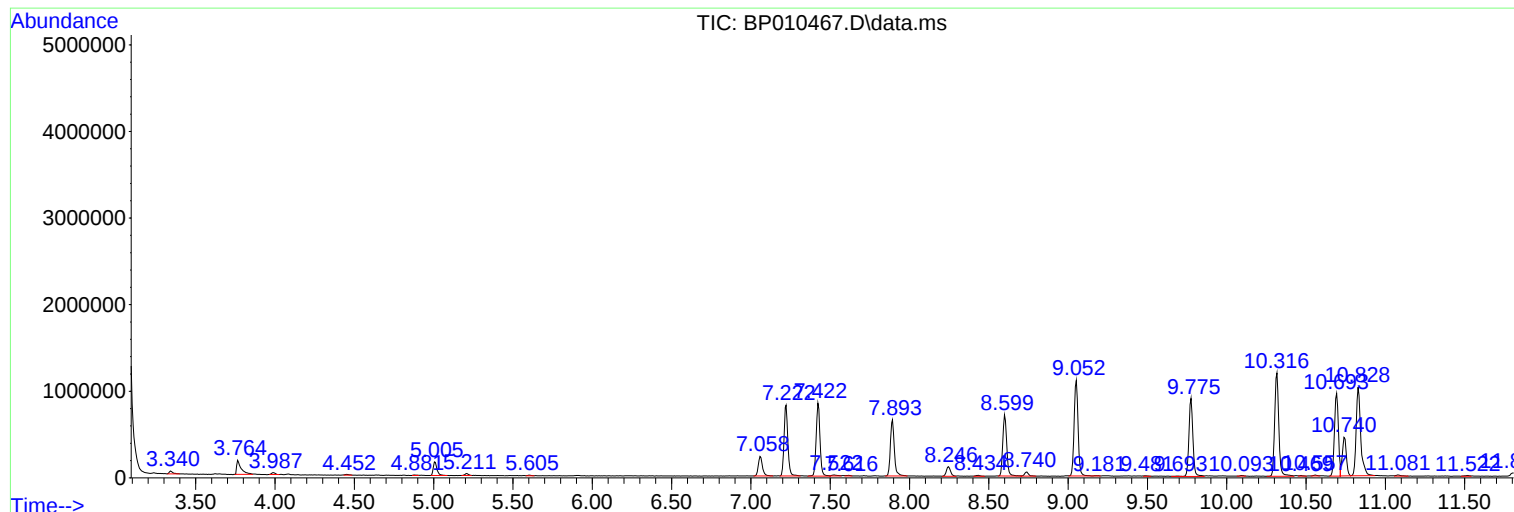

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010467.D
Acq On : 21 May 2022 09:49
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.005	4.59 ng/ul	255955	1,4-Dichlorobenzene-d4	7.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	38		
2	Hydrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	38		
3	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38		
4	Methyl 2,5,8,11-tetraoxatridecan...	236	C10H20O6	1000366-78-2	38		
5	Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	37		

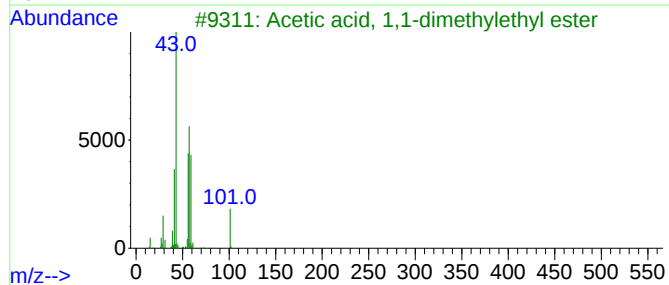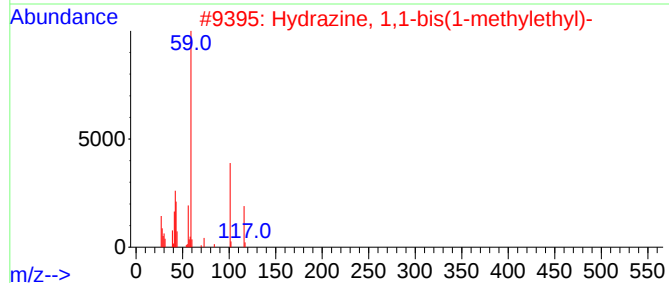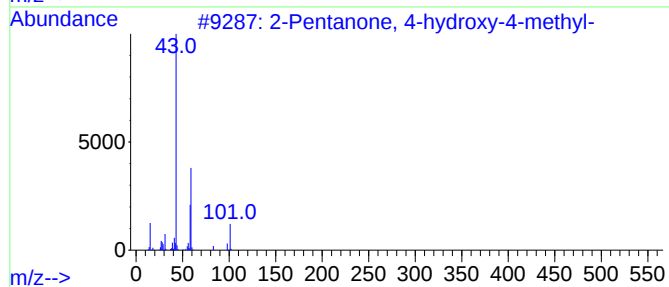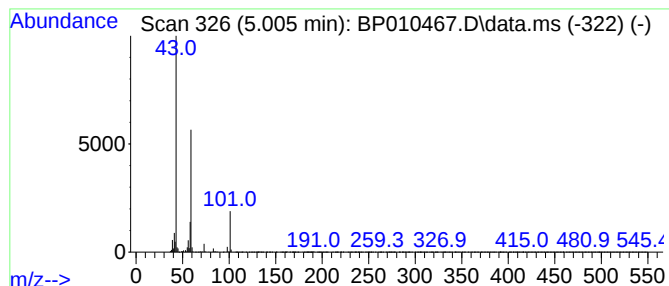

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010467.D
Acq On : 21 May 2022 09:49
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1,4-dichloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.246	3.61 ng/ul	201329	1,4-Dichlorobenzene-d4	7.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,4-dichloro-	146	C6H4Cl2	000106-46-7	97
2			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	97
3			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	97
4			Benzene, 1,3-dichloro-	146	C6H4Cl2	000541-73-1	96
5			Benzene, 1,2-dichloro-	146	C6H4Cl2	000095-50-1	96

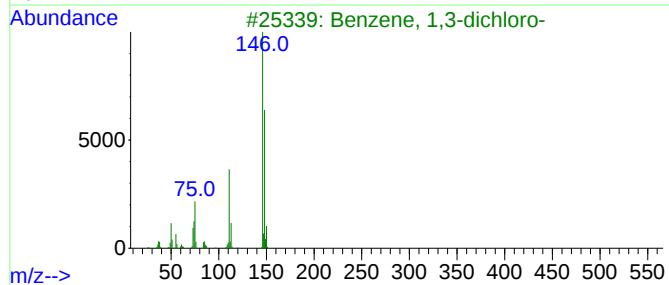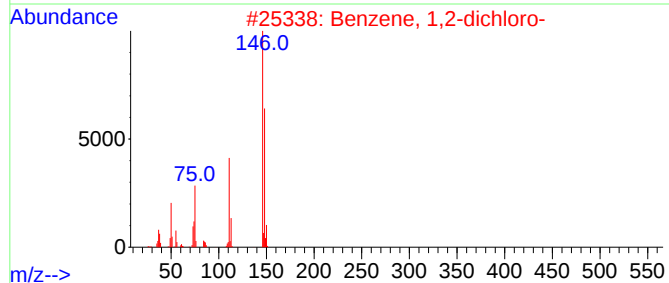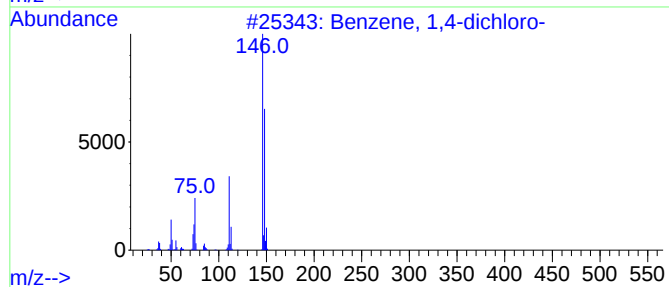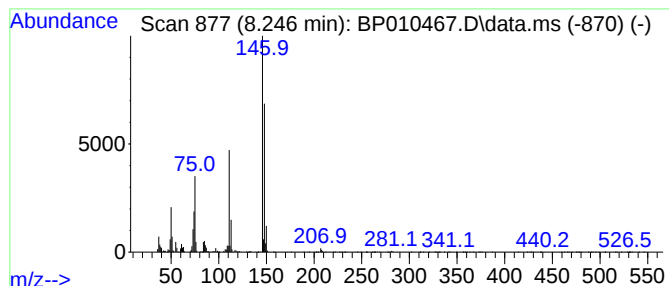

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010467.D
Acq On : 21 May 2022 09:49
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 (DEL) Alkane: Straight-Chai... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.069	2.75 ng/ul	357654	Chrysene-d12	21.357

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Nonadecene			266	C19H38	018435-45-5	94
2	Heptadecyl heptafluorobutyrate			452	C21H35F7O2	959085-66-6	94
3	Pentadecafluorooctanoic acid, oc...			666	C26H37F15O2	1000406-04-8	94
4	n-Nonadecanol-1			284	C19H40O	001454-84-8	93
5	1-Hexacosene			364	C26H52	018835-33-1	93

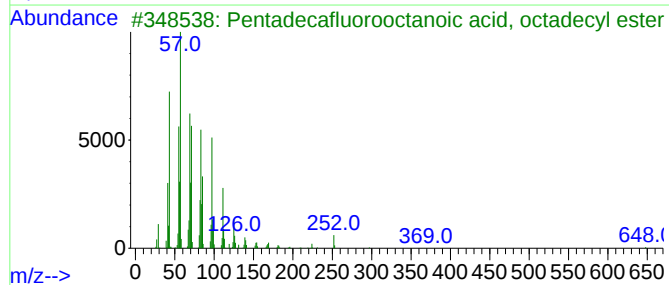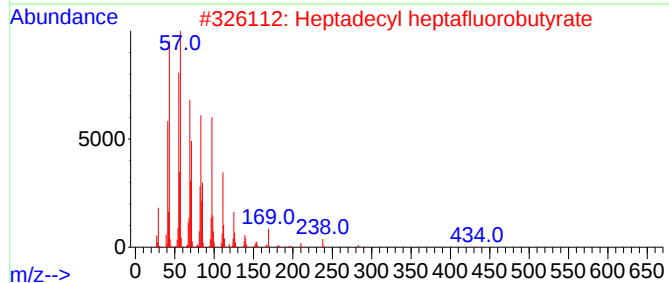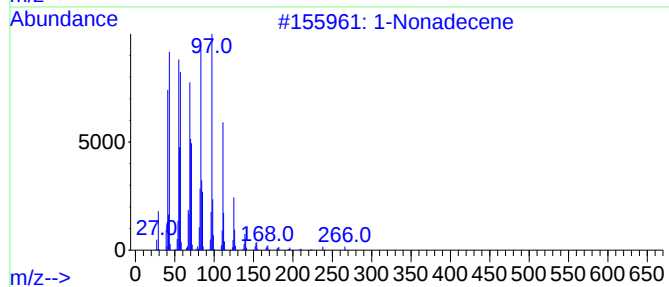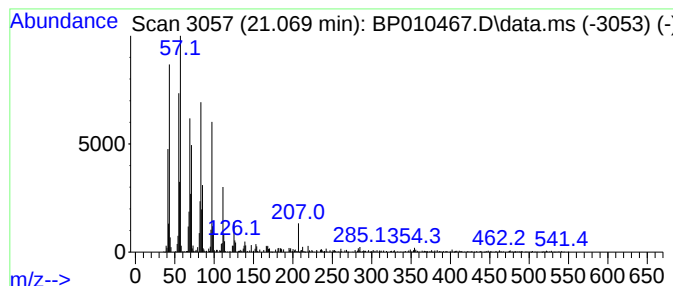

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010467.D
Acq On : 21 May 2022 09:49
Operator : CG/JU
Sample : N2918-22
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.005	4.6	ng/ul	255955	1	7.893	1114830	20.0
Benzene, 1,4-di...	8.246	3.6	ng/ul	201329	1	7.893	1114830	20.0
(DEL) Alkane: S...	21.069	2.8	ng/ul	357654	5	21.357	2603630	20.0