

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010468.D
 Acq On : 21 May 2022 10:23
 Operator : CG/JU
 Sample : N2918-23
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	56	rVB	40873	69016	0.92%	0.105%
2	3.640	87	94	97	rBV7	9524	22977	0.31%	0.035%
3	3.764	112	115	132	rBV	169620	333263	4.43%	0.508%
4	3.993	149	154	160	rVB	26041	42168	0.56%	0.064%
5	4.081	166	169	176	rVB3	13374	22029	0.29%	0.034%
6	4.881	300	305	308	rBV7	4752	7928	0.11%	0.012%
7	5.011	321	327	340	rVB	90869	154197	2.05%	0.235%
8	5.199	358	359	366	rVB7	6640	9892	0.13%	0.015%
9	5.611	424	429	433	rVB5	6333	11238	0.15%	0.017%
10	7.058	669	675	687	rBV	232858	411560	5.48%	0.628%
11	7.222	696	703	717	rBV	873796	1478527	19.67%	2.255%
12	7.422	728	737	749	rBV	885080	1478557	19.67%	2.255%
13	7.522	749	754	762	rVB2	16962	33890	0.45%	0.052%
14	7.893	806	817	826	rBV	784741	1320502	17.57%	2.014%
15	7.958	826	828	833	rVB3	9806	14061	0.19%	0.021%
16	8.246	870	877	885	rVB2	30206	54663	0.73%	0.083%
17	8.599	926	937	955	rBV	733266	1248673	16.61%	1.904%
18	9.052	1006	1014	1028	rBV	1207401	2053455	27.32%	3.132%
19	9.181	1033	1036	1040	rVV6	6101	11283	0.15%	0.017%
20	9.487	1082	1088	1097	rBV	28508	47405	0.63%	0.072%
21	9.775	1129	1137	1151	rBV	968855	1666819	22.18%	2.542%
22	10.316	1221	1229	1246	rBV	1258871	2265780	30.15%	3.456%
23	10.693	1284	1293	1308	rBV	1148619	2013965	26.80%	3.072%
24	10.828	1308	1316	1333	rBV	958700	1798867	23.94%	2.744%
25	11.075	1354	1358	1367	rVB	8837	17058	0.23%	0.026%
26	11.516	1426	1433	1440	rBV9	14226	36070	0.48%	0.055%
27	11.987	1506	1513	1519	rVB2	33938	57235	0.76%	0.087%
28	12.281	1556	1563	1572	rBV2	24279	46652	0.62%	0.071%
29	12.893	1662	1667	1669	rBV6	5869	8560	0.11%	0.013%
30	13.369	1744	1748	1752	rVV4	7300	11720	0.16%	0.018%
31	13.428	1752	1758	1765	rVB	71810	115328	1.53%	0.176%
32	13.934	1836	1844	1849	rBV	2903334	3909053	52.01%	5.962%
33	13.981	1849	1852	1861	rVV	316643	439928	5.85%	0.671%
34	14.040	1861	1862	1870	rVB8	8220	13686	0.18%	0.021%
35	14.216	1882	1892	1907	rBV	3006416	4548509	60.52%	6.937%
36	14.522	1937	1944	1953	rBV	1807409	2683608	35.71%	4.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
 Data File : BP010468.D
 Acq On : 21 May 2022 10:23
 Operator : CG/JU
 Sample : N2918-23
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	14.657	1962	1967	1971	rVB6	6822	10006	0.13%	0.015%
38	14.734	1973	1980	1997	rBV	144836	366303	4.87%	0.559%
39	14.851	1997	2000	2004	rVV5	10770	21388	0.28%	0.033%
40	14.887	2004	2006	2009	rVV4	7795	9571	0.13%	0.015%
41	14.945	2011	2016	2026	rVB4	14401	35999	0.48%	0.055%
42	15.075	2033	2038	2044	rVB10	7412	14883	0.20%	0.023%
43	15.269	2067	2071	2077	rVB2	16824	24680	0.33%	0.038%
44	15.328	2077	2081	2086	rBV3	12254	22183	0.30%	0.034%
45	15.516	2106	2113	2127	rBV	3984644	5898271	78.48%	8.996%
46	15.640	2127	2134	2148	rVV	910584	1370382	18.23%	2.090%
47	15.757	2148	2154	2160	rVB2	46181	78016	1.04%	0.119%
48	15.887	2169	2176	2178	rVB8	5390	11550	0.15%	0.018%
49	16.304	2242	2247	2251	rVB4	19642	28874	0.38%	0.044%
50	16.775	2322	2327	2331	rBV5	7496	11640	0.15%	0.018%
51	16.875	2340	2344	2349	rVV8	8558	10991	0.15%	0.017%
52	16.934	2349	2354	2361	rVB7	25343	51218	0.68%	0.078%
53	17.204	2396	2400	2404	rVB5	14054	15821	0.21%	0.024%
54	17.275	2405	2412	2422	rBV	2224944	3163405	42.09%	4.825%
55	17.375	2422	2429	2446	rVV2	4554046	6674991	88.82%	10.181%
56	17.534	2450	2456	2468	rVV4	43111	114404	1.52%	0.174%
57	17.892	2512	2517	2522	rBV3	60590	78014	1.04%	0.119%
58	17.939	2522	2525	2530	rVV6	15837	17840	0.24%	0.027%
59	18.157	2558	2562	2569	rBV	106219	165334	2.20%	0.252%
60	18.886	2683	2686	2693	rVB3	24510	34984	0.47%	0.053%
61	19.057	2712	2715	2723	rBV10	10229	18083	0.24%	0.028%
62	19.186	2733	2737	2743	rVB	61020	84876	1.13%	0.129%
63	19.251	2744	2748	2753	rBV	59950	88551	1.18%	0.135%
64	19.392	2768	2772	2775	rBV5	37914	54572	0.73%	0.083%
65	19.533	2793	2796	2799	rVB5	23177	28276	0.38%	0.043%
66	19.610	2803	2809	2824	rVV	5646477	7515442	100.00%	11.462%
67	21.063	3052	3056	3063	rBV	344916	552382	7.35%	0.842%
68	21.357	3101	3106	3119	rVB	2199955	2761135	36.74%	4.211%
69	23.033	3388	3391	3396	rVB	155114	214007	2.85%	0.326%
70	23.627	3484	3492	3506	rVB2	2472119	5323999	70.84%	8.120%
71	23.780	3512	3518	3532	rVB2	1064074	2235657	29.75%	3.410%




Sum of corrected areas: 65565850

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010468.D
Acq On : 21 May 2022 10:23
Operator : CG/JU
Sample : N2918-23
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

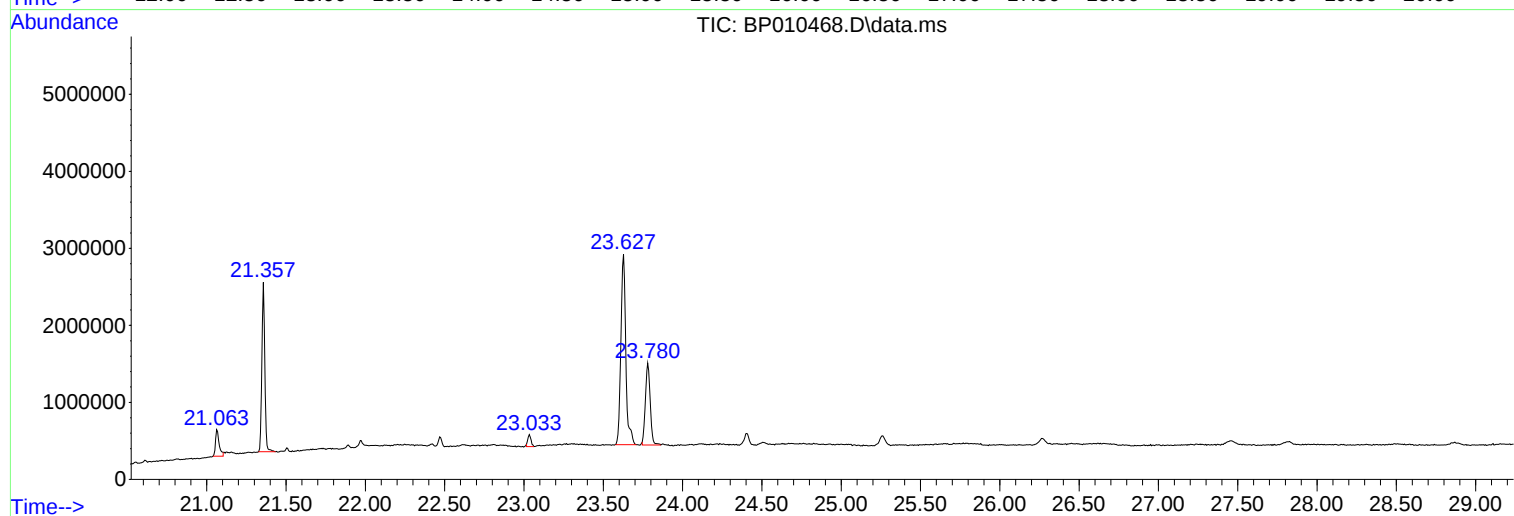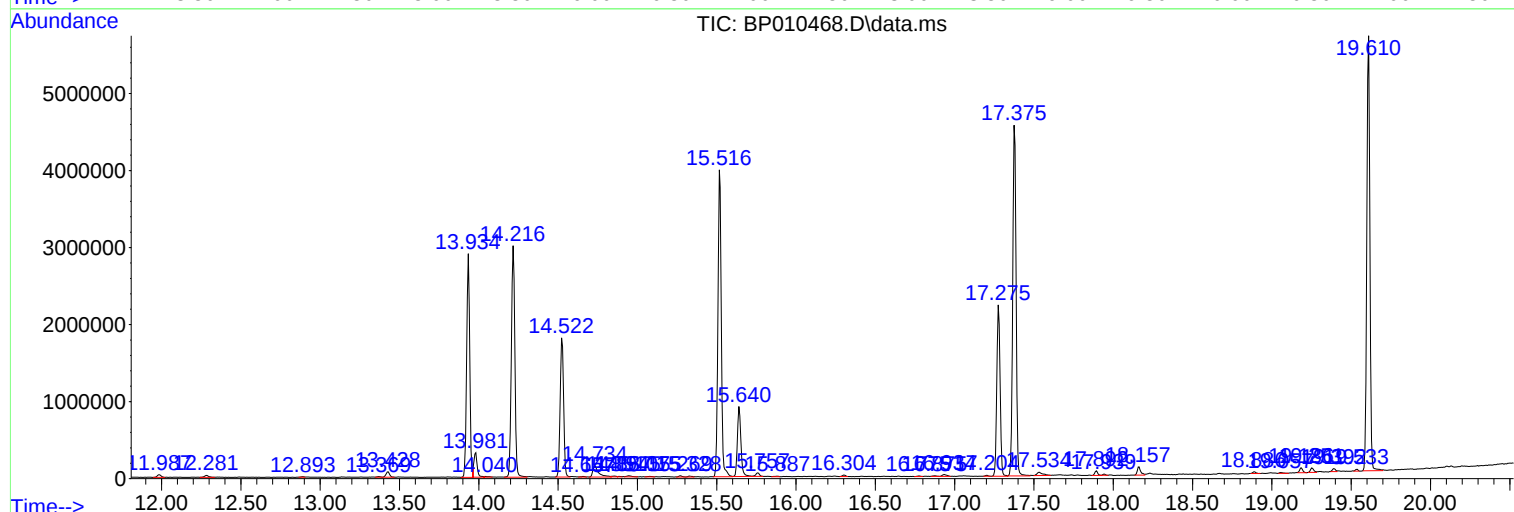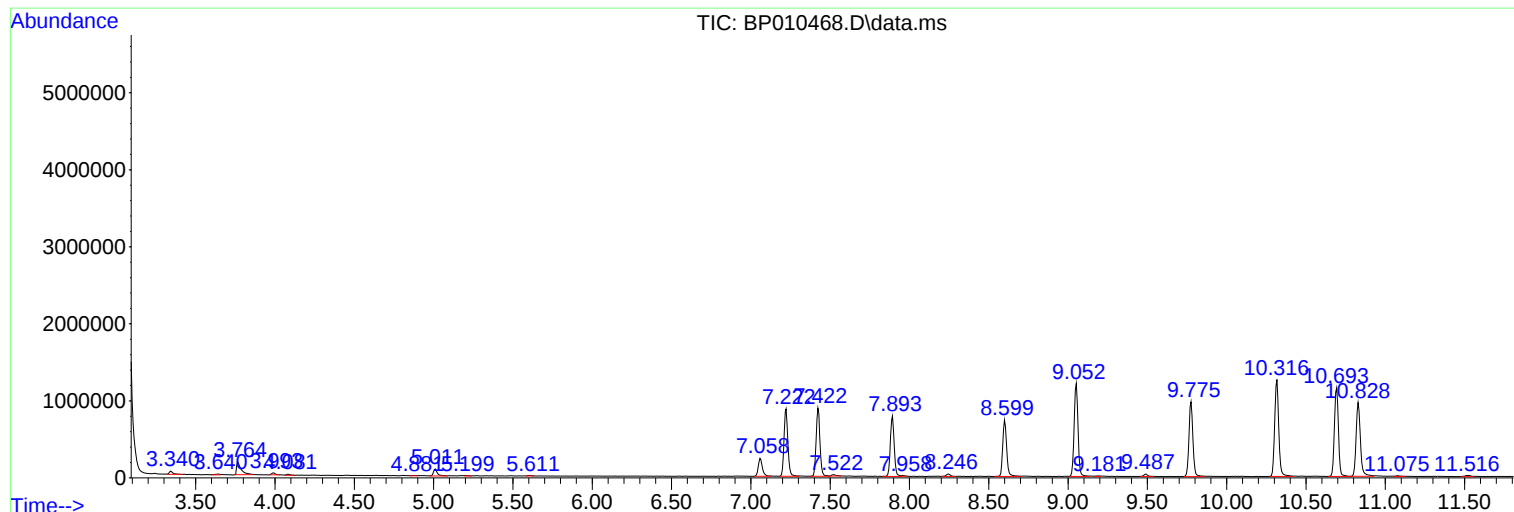

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010468.D
Acq On : 21 May 2022 10:23
Operator : CG/JU
Sample : N2918-23
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.011	2.34 ng/ul	154197	1,4-Dichlorobenzene-d4	7.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
3	Propane, 1,1-dipropoxy-	160	C9H20O2	004744-11-0	38		
4	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	28		
5	3-Octanol	130	C8H18O	000589-98-0	28		

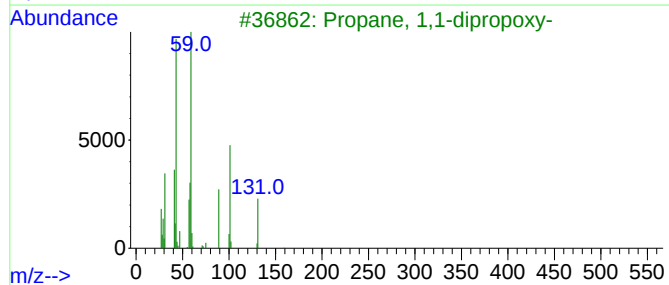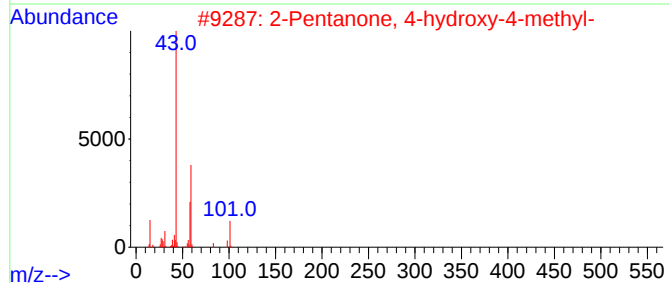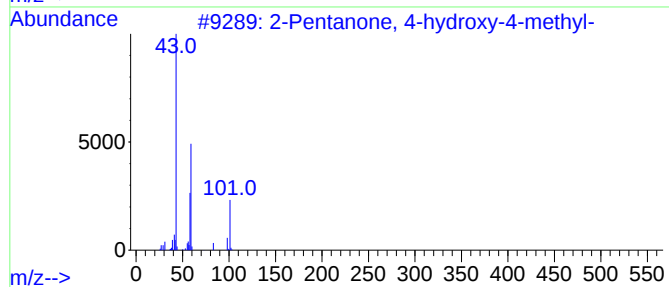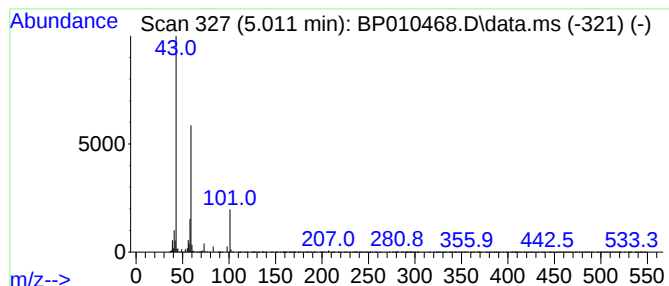

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010468.D
Acq On : 21 May 2022 10:23
Operator : CG/JU
Sample : N2918-23
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic21.063 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.063	4.00 ng/ul	552382	Chrysene-d12	21.357

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	99
2			Pentafluoropropionic acid, hepta...	402	C20H35F5O2	959218-78-1	94
3			Heptadecyl trifluoroacetate	352	C19H35F3O2	1010351-87-0	94
4			Heptafluorobutyric acid, hexadec...	438	C20H33F7O2	006385-15-5	94
5			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94

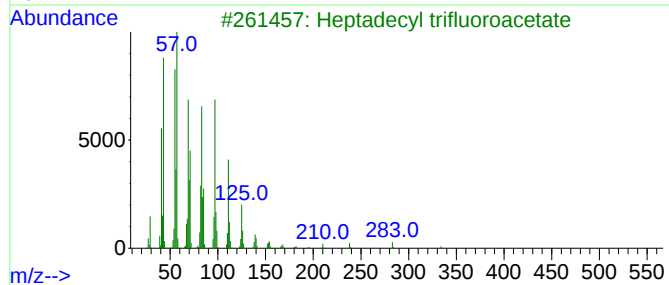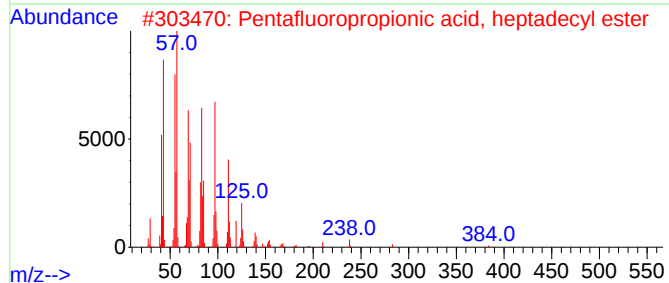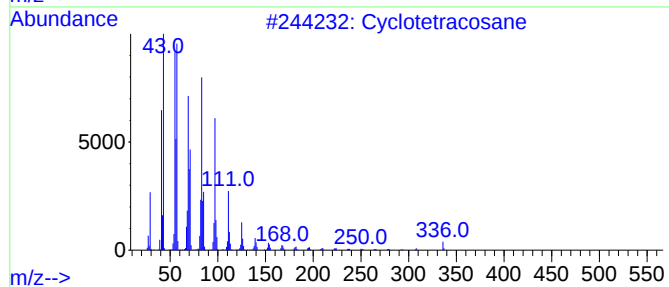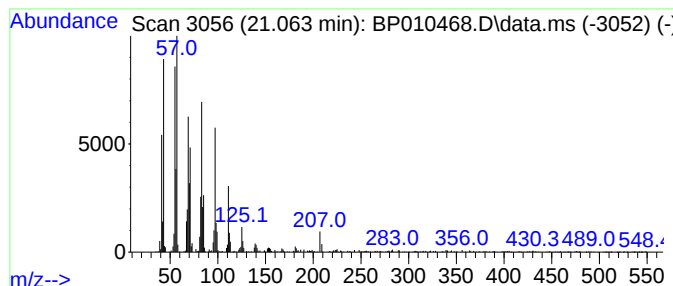

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052022\
Data File : BP010468.D
Acq On : 21 May 2022 10:23
Operator : CG/JU
Sample : N2918-23
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.011	2.3	ng/u1	154197	1	7.893	1320500	20.0
(DEL) Alkane: C...	21.063	4.0	ng/u1	552382	5	21.357	2761140	20.0