
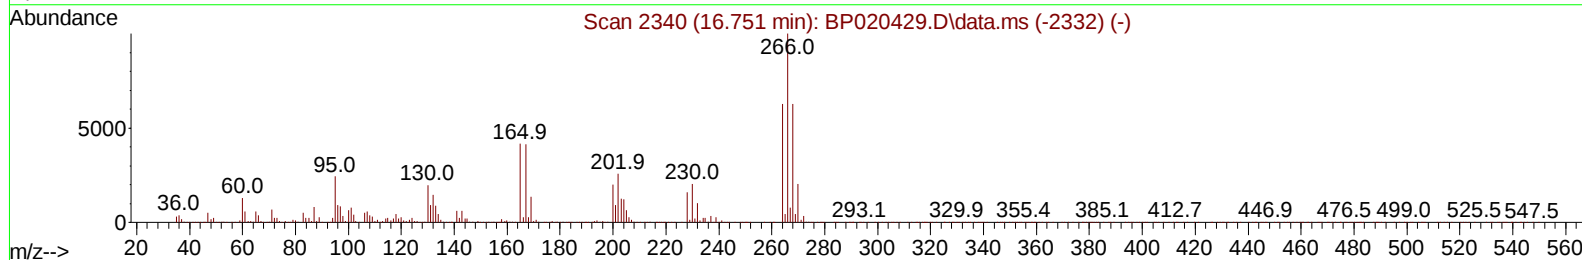
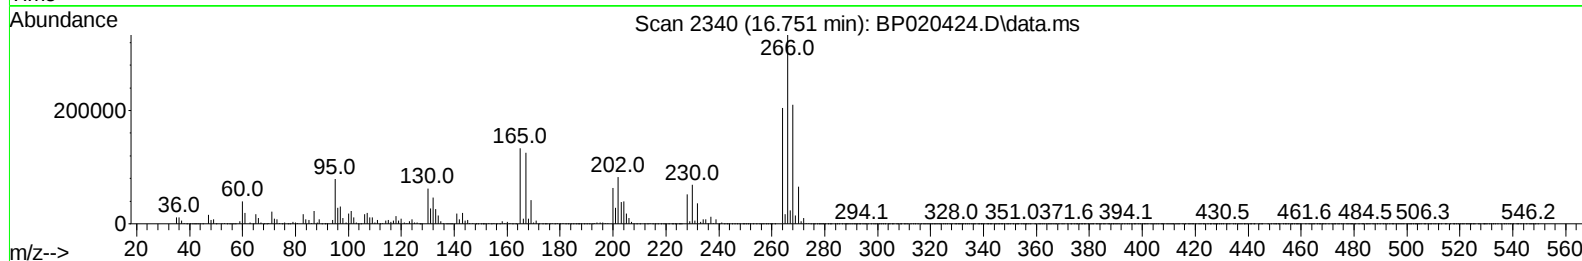


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052024\
Data File : BP020424.D
Acq On : 20 May 2024 12:26
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 01:58:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 21 01:48:44 2024
Response via : Initial Calibration

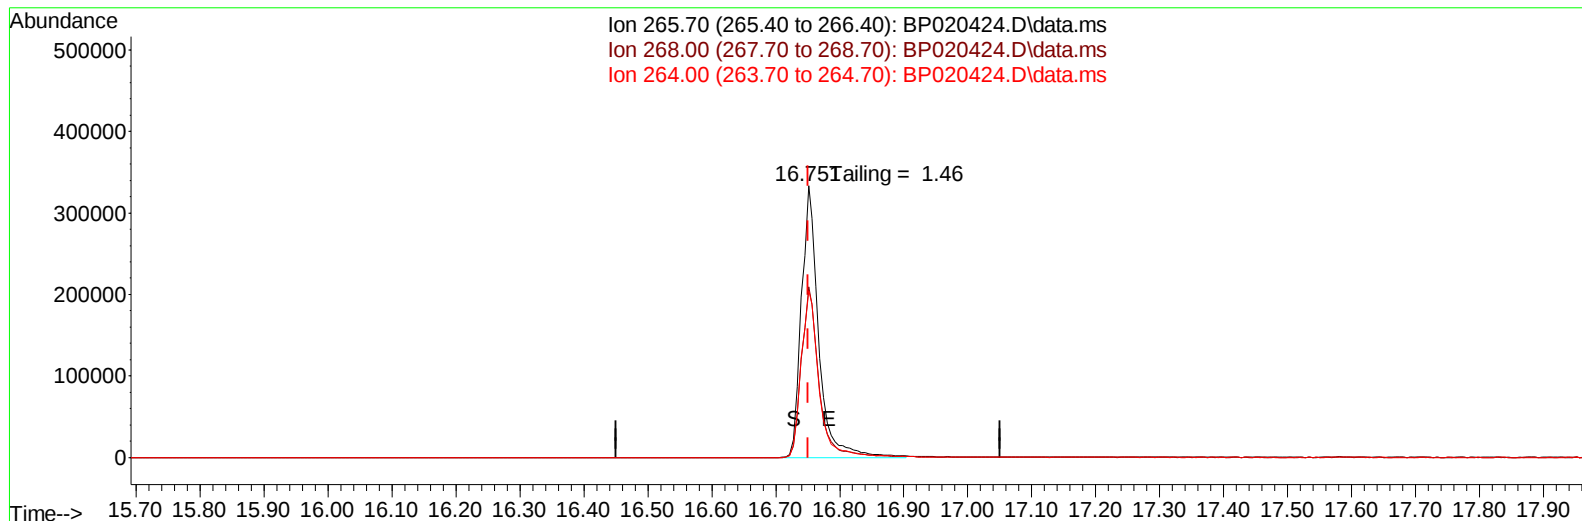

TIC: BP020424.D\data.ms

(70) Pentachlorophenol (C)




16.751min (+ 0.000) 7611111.94 ng

response 636368

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.93
264.00	62.80	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052024\
Data File : BP020424.D
Acq On : 20 May 2024 12:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 01:58:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 21 01:48:44 2024
Response via : Initial Calibration

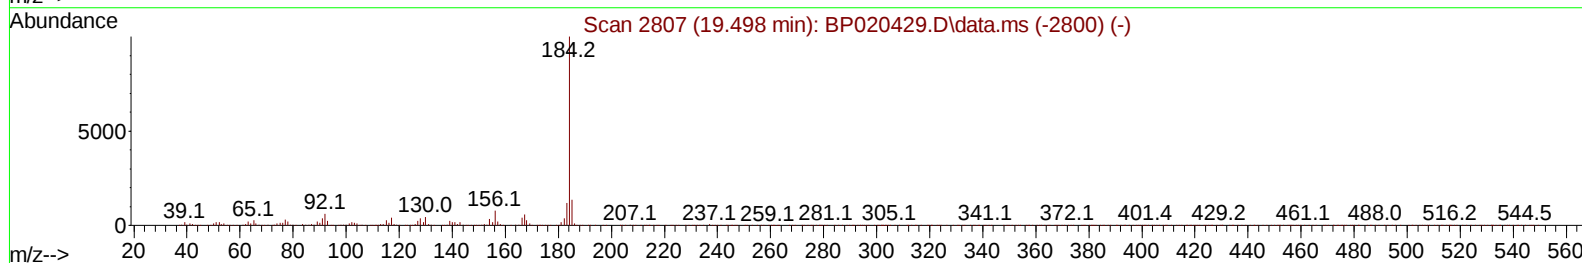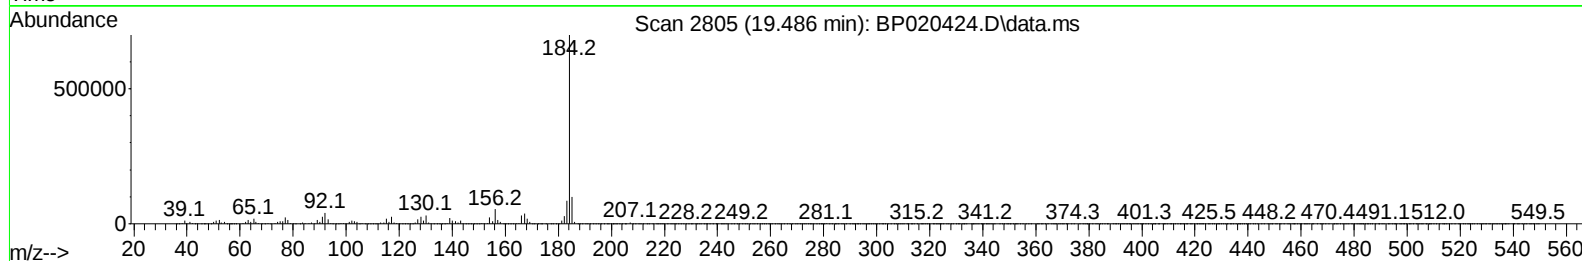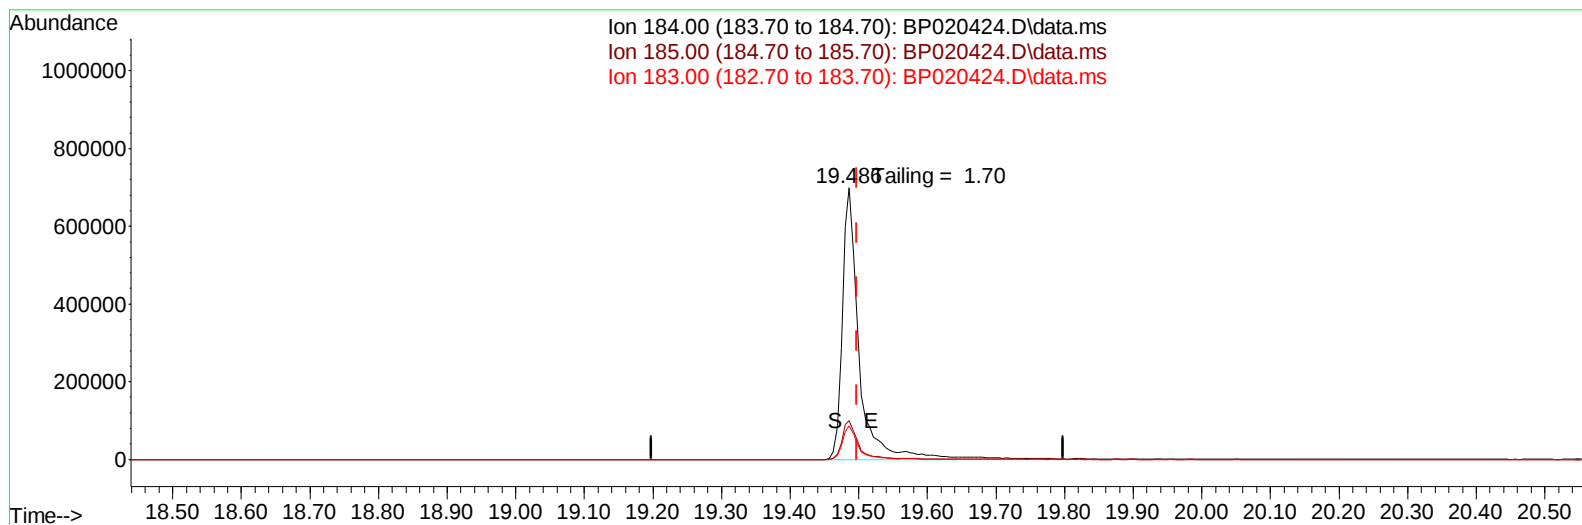

TIC: BP020424.D\data.ms

(77) Benzidine**19.486min (-0.012) 4109206.68 ng****response 1115093**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.30
183.00	11.90	12.37
0.00	0.00	0.00