


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052024\
Data File : BP020424.D
Acq On : 20 May 2024 12:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 21 01:48:44 2024

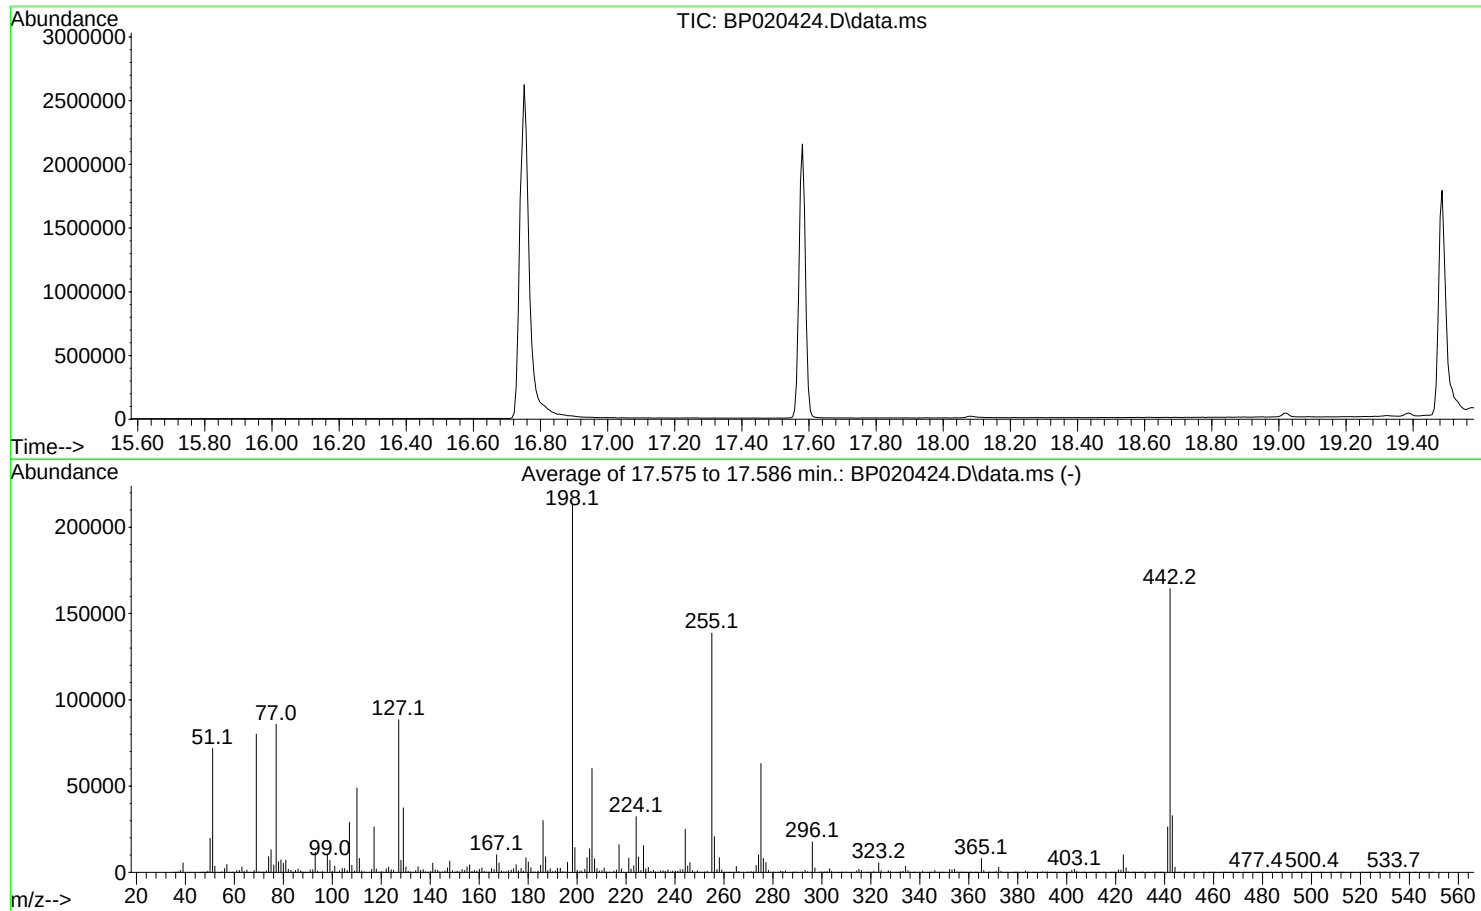




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	71778	PASS
68	69	0.00	2	1.4	1155	PASS
69	198	0.00	100	37.6	80127	PASS
70	69	0.00	2	0.6	472	PASS
127	198	10	80	41.5	88440	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	213203	PASS
199	198	5	9	6.8	14398	PASS
275	198	10	60	29.6	63076	PASS
365	198	1	100	3.8	8014	PASS
441	198	0.01	100	12.4	26354	PASS
442	442	100	100	100.0	164387	PASS
443	442	15	24	19.9	32795	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052024\
Data File : BP020424.D
Acq On : 20 May 2024 12:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 21 01:58:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 21 01:48:44 2024
Response via : Initial Calibration

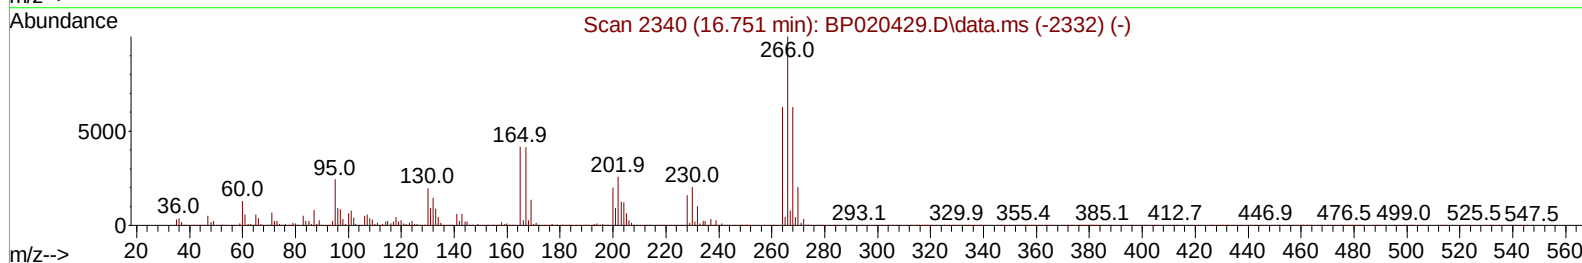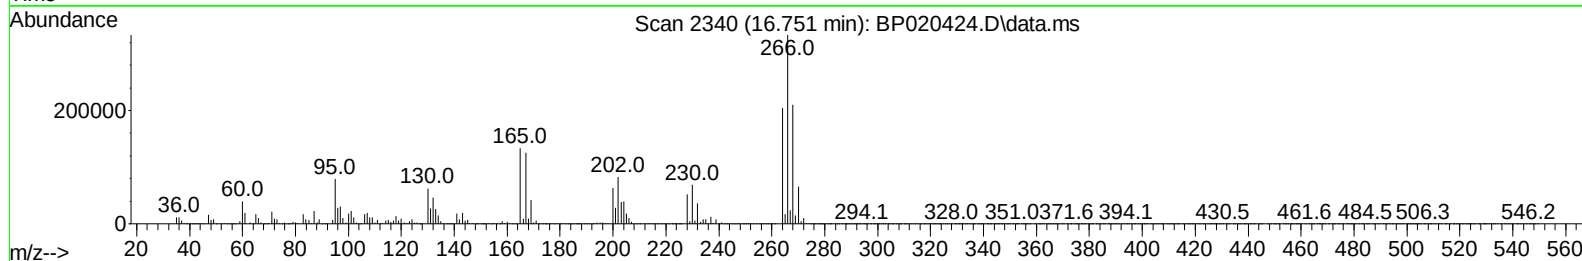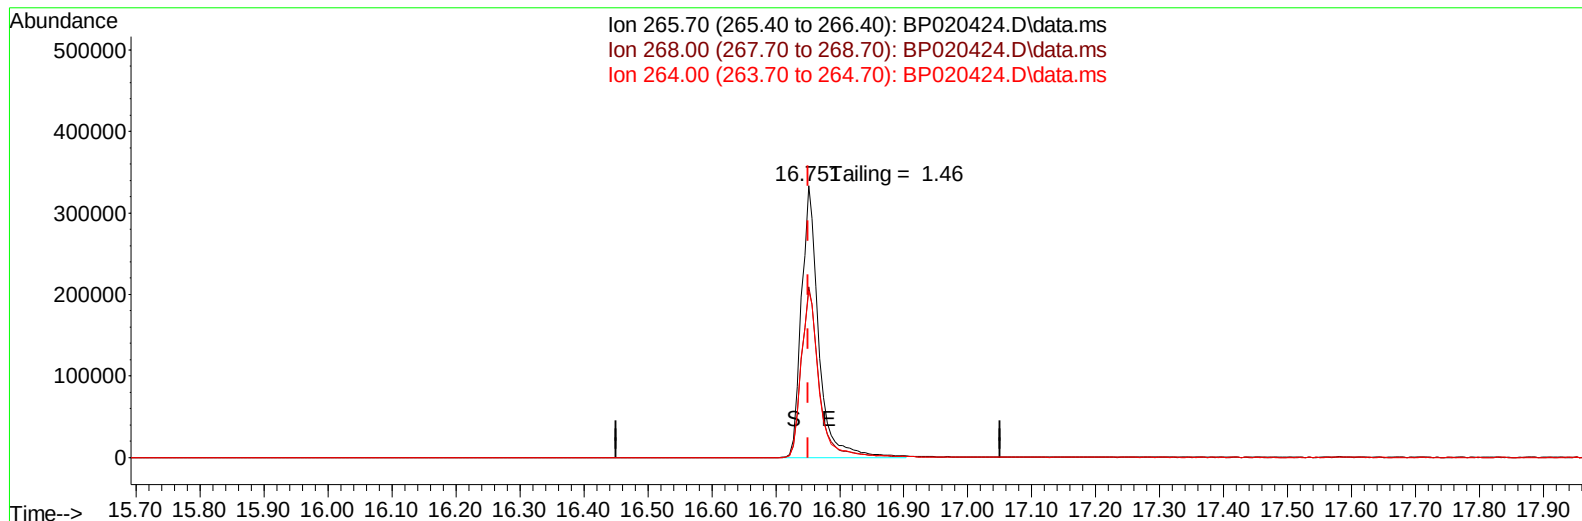

TIC: BP020424.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.000) 7611111.94 ng




response 636368

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.93
264.00	62.80	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052024\
Data File : BP020424.D
Acq On : 20 May 2024 12:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 21 01:58:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 21 01:48:44 2024
Response via : Initial Calibration

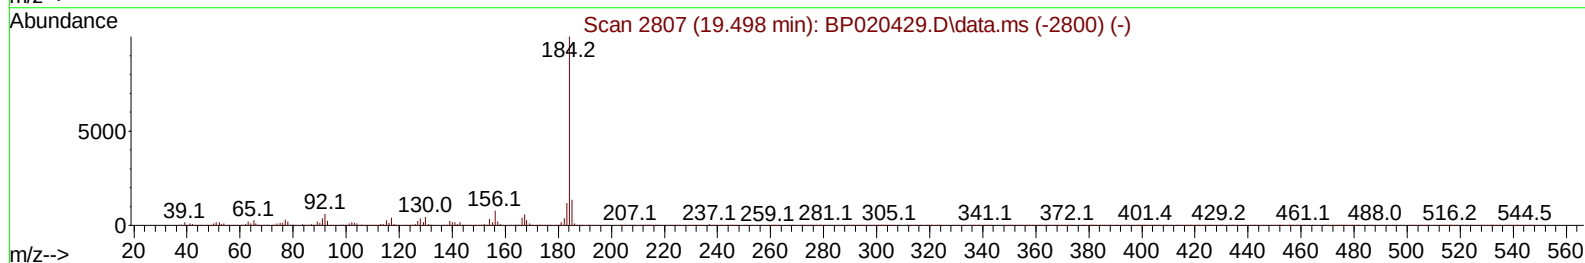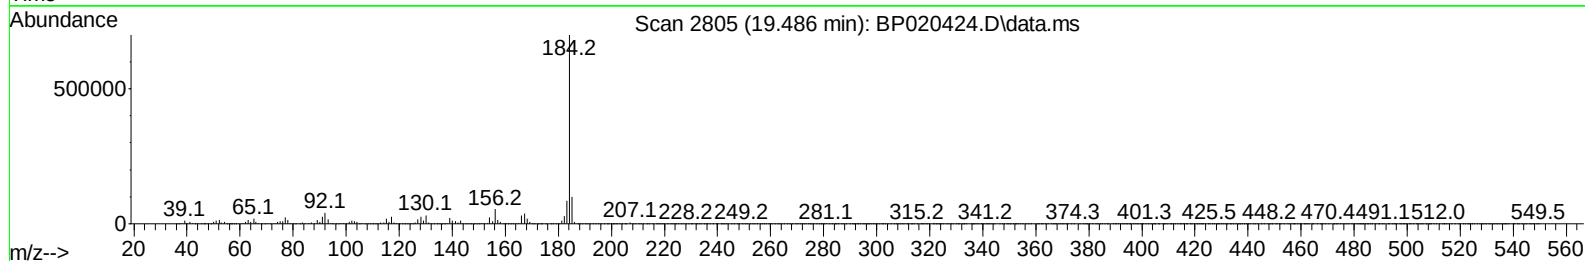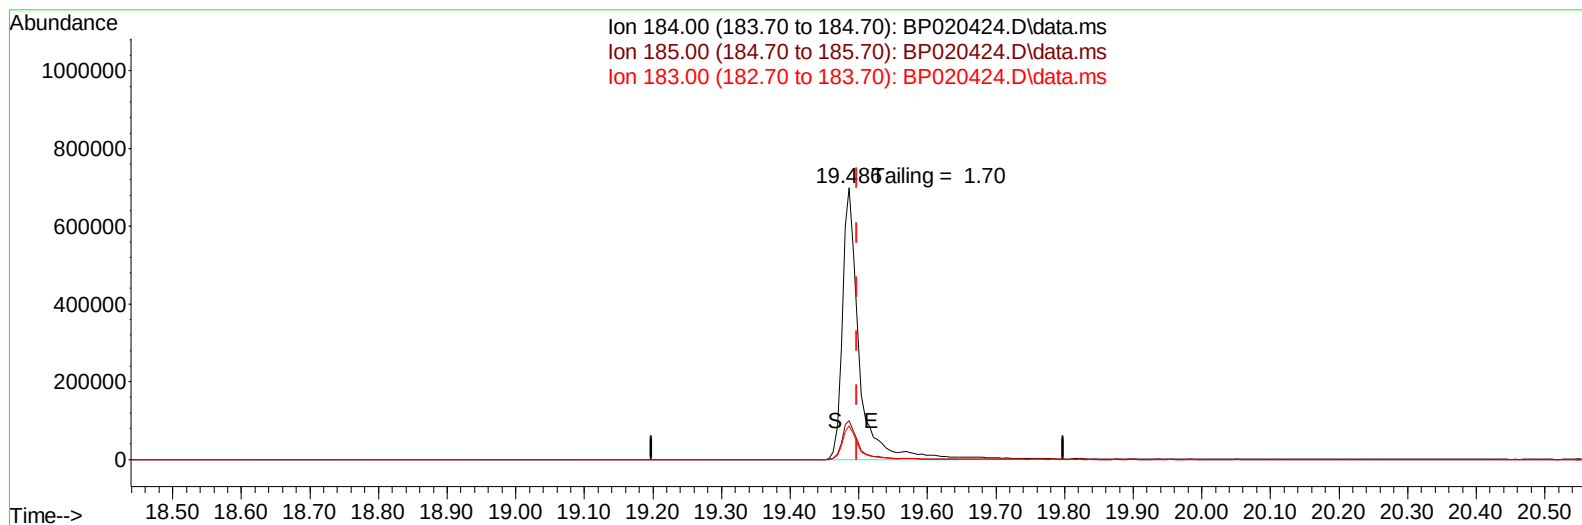

TIC: BP020424.D\data.ms

(77) Benzidine

19.486min (-0.012) 4109206.68 ng

response 1115093

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.30
183.00	11.90	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2024	BNA_P	<u>BP020424.D</u>
Compound Name	Response	Retention Time
DDT	758336	20.774
DDD	7182	20.351
DDE	1010	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8192	766528	1.07

Instrument :
BNA_P
ClientSampleId :
DFTPP