
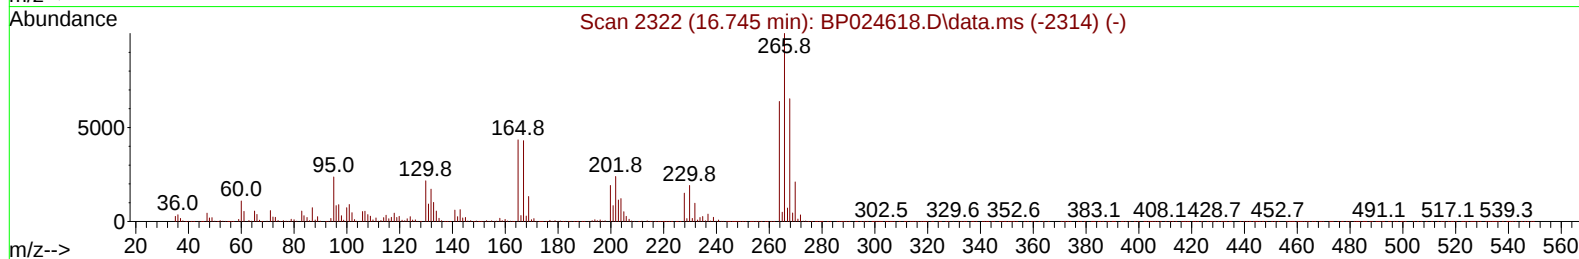
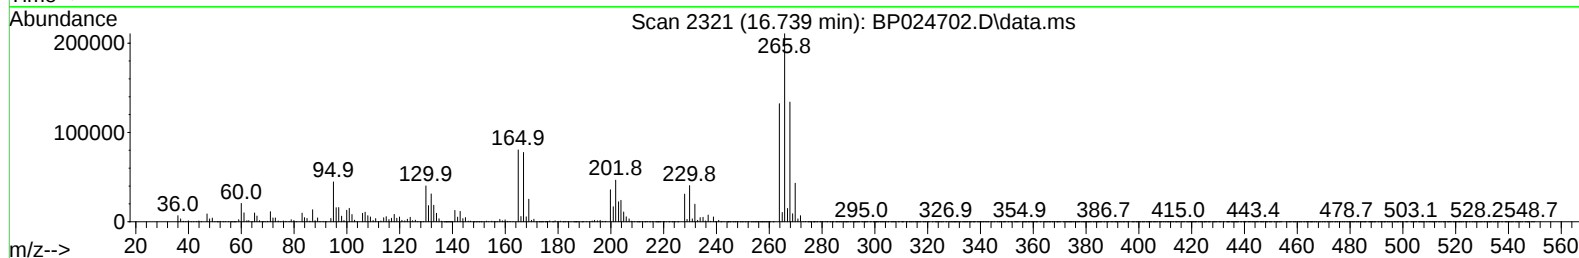


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052025\  
Data File : BP024702.D  
Acq On : 20 May 2025 10:31  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 12:58:55 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 13 16:21:39 2025  
Response via : Initial Calibration

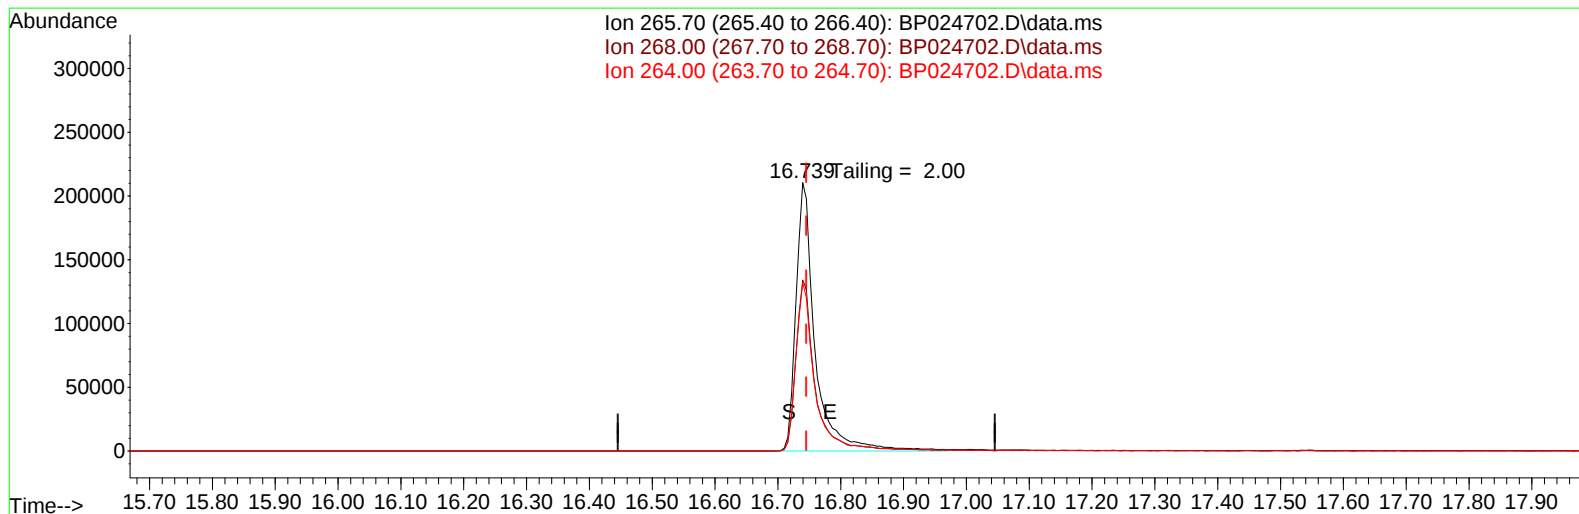

TIC: BP024702.D\data.ms

**(70) Pentachlorophenol (C)**




**16.739min (-0.006) 1977139.32 ng**

**response 448686**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.30  | 63.67  |
| 264.00 | 63.90  | 62.85  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052025\  
Data File : BP024702.D  
Acq On : 20 May 2025 10:31  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 12:58:55 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 13 16:21:39 2025  
Response via : Initial Calibration

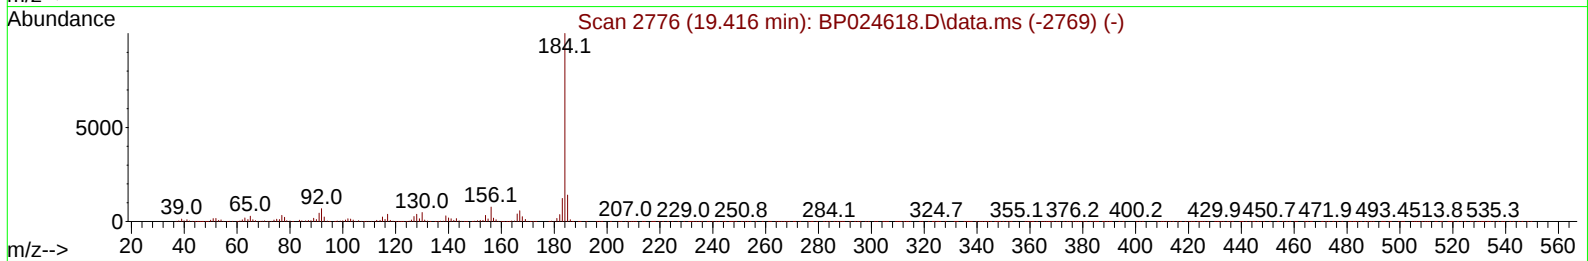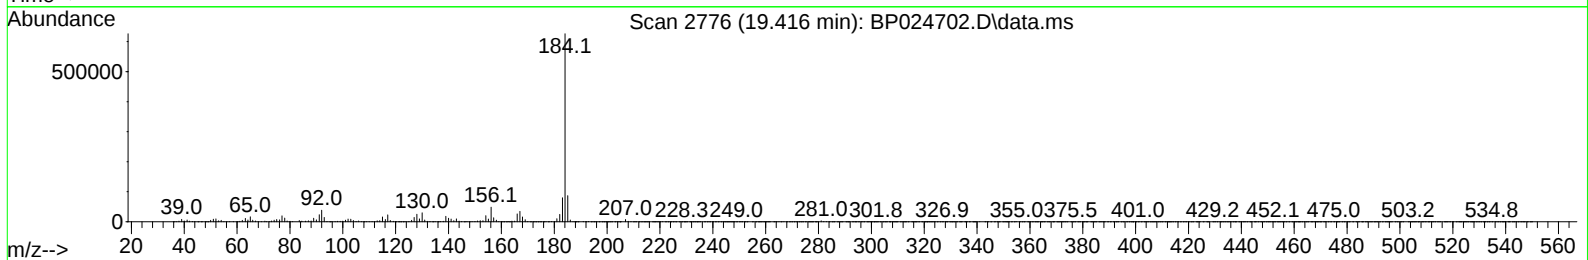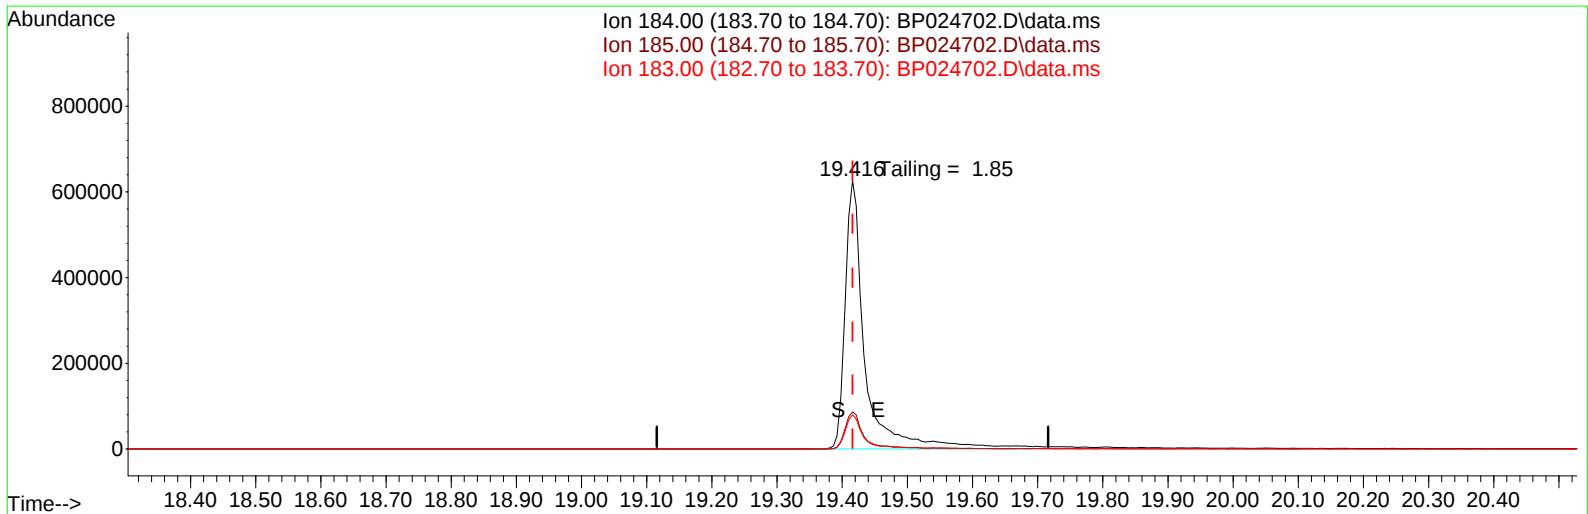

TIC: BP024702.D\data.ms

**(77) Benzidine****19.416min (-0.000) 89911.52 ng****response 1248901**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 13.86  |
| 183.00 | 12.30  | 12.78  |
| 0.00   | 0.00   | 0.00   |