
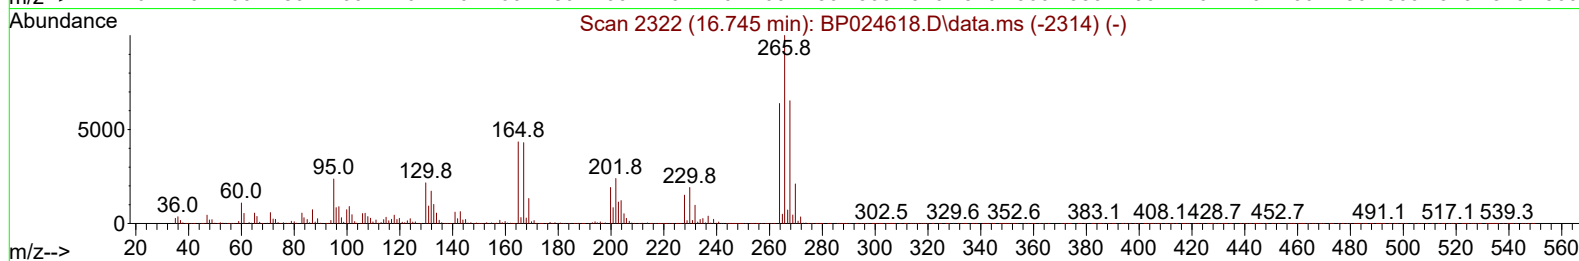
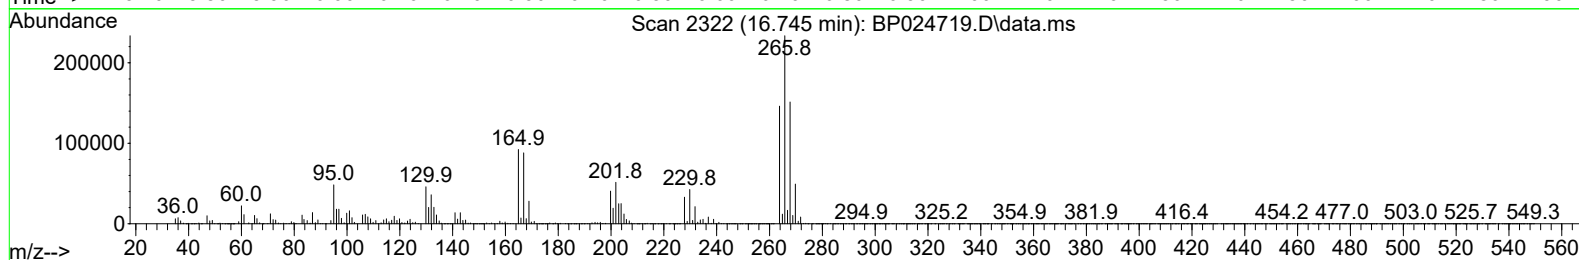


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024719.D
Acq On : 21 May 2025 00:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 02:08:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

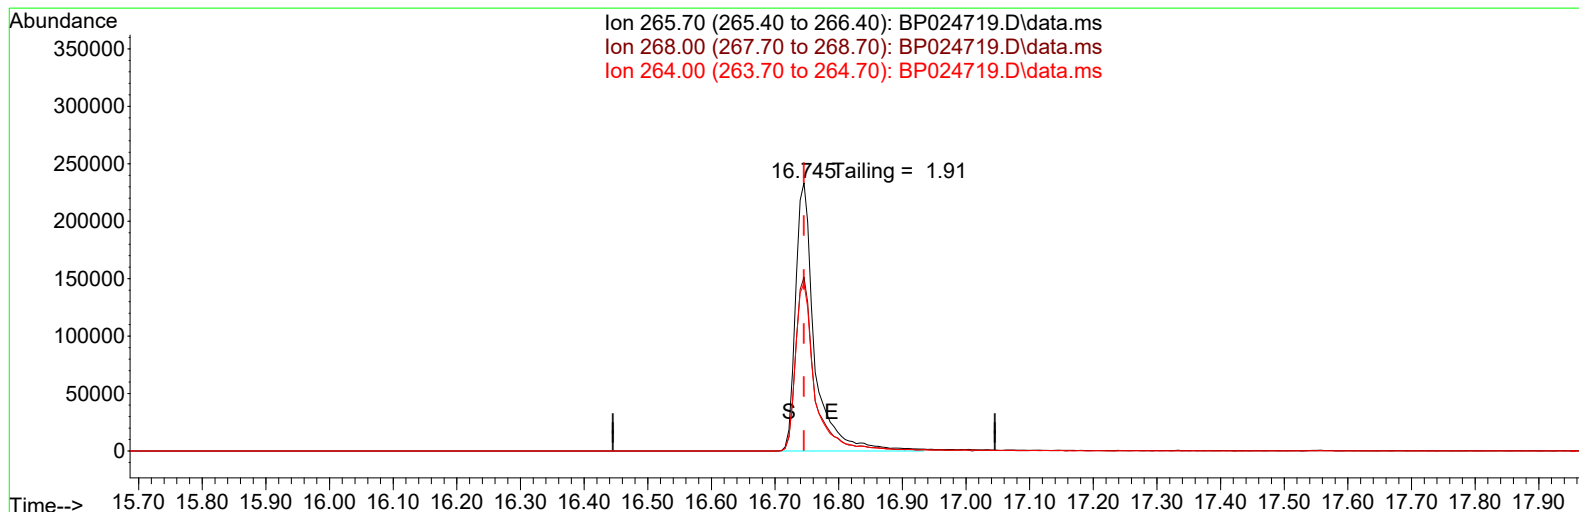

TIC: BP024719.D\data.ms

(70) Pentachlorophenol (C)




16.745min (+ 0.000) 574282.04 ng

response 492342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.77
264.00	63.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024719.D
Acq On : 21 May 2025 00:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 02:08:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

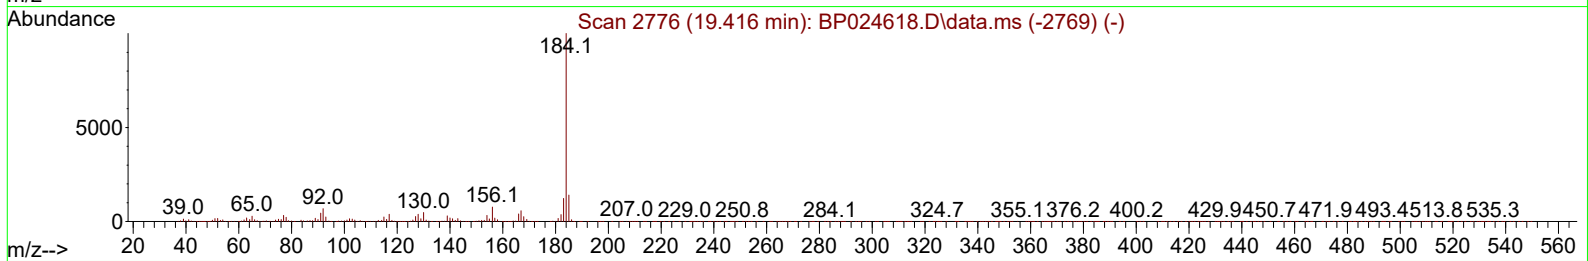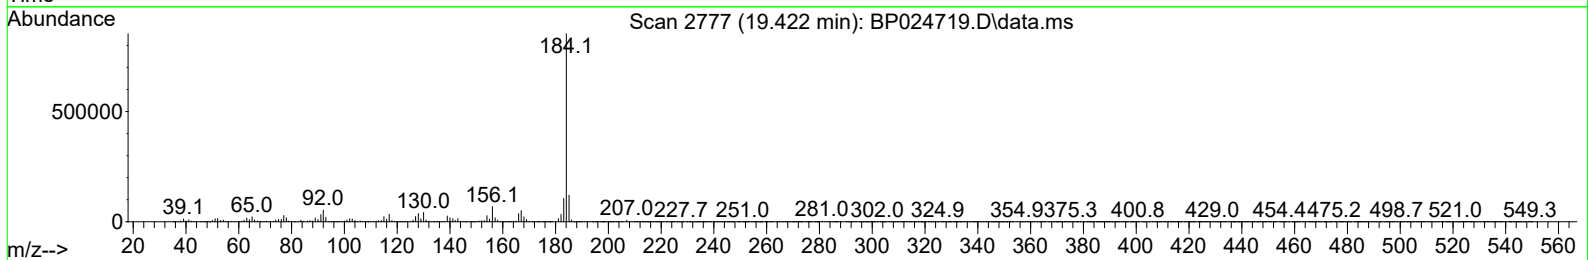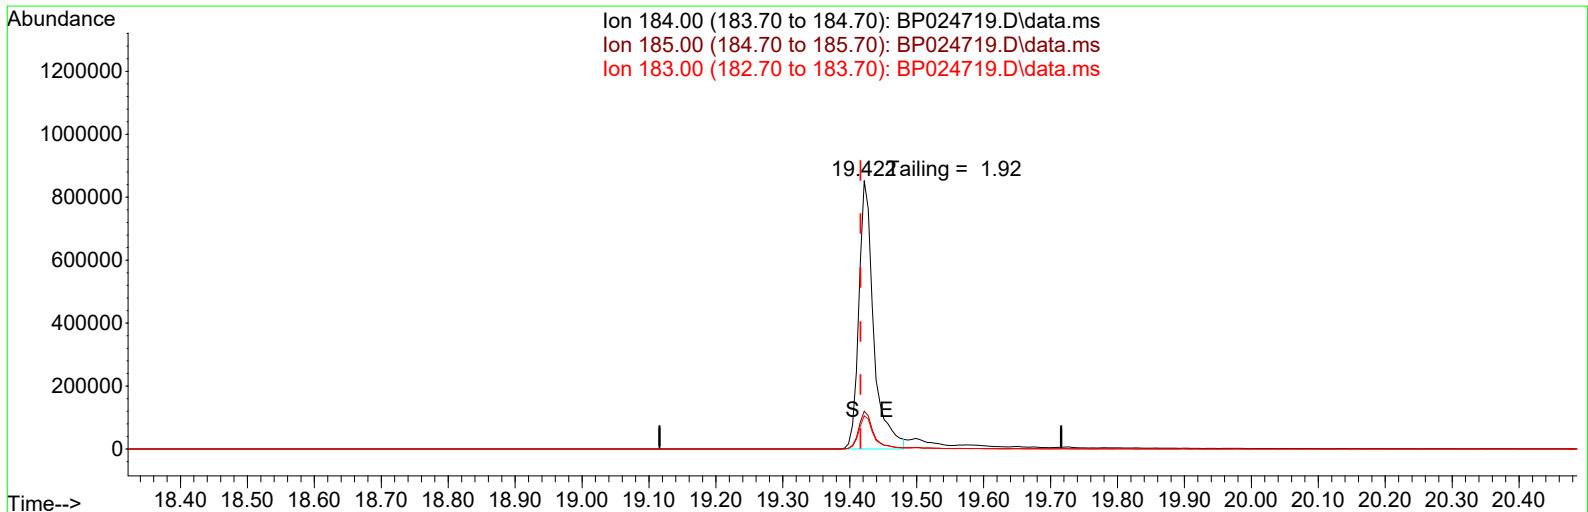

TIC: BP024719.D\data.ms

(77) Benzidine

19.422min (+ 0.006) 97951.15 ng

response 1323225

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.13
183.00	12.30	12.40
0.00	0.00	0.00