

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052025\  
 Data File : BP024724.D  
 Acq On : 21 May 2025 03:30  
 Operator : RC/JU  
 Sample : Q1984-09  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 OU4-TS-25-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024724.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.470       | 61            | 65          | 80           | rBV      | 47786          | 81560         | 1.67%           | 0.253%        |
| 2         | 4.823       | 289           | 295         | 307          | rBV      | 121770         | 177465        | 3.64%           | 0.550%        |
| 3         | 5.287       | 368           | 374         | 390          | rBV      | 1297142        | 2030213       | 41.64%          | 6.289%        |
| 4         | 6.858       | 634           | 641         | 668          | rBV      | 1181383        | 2139338       | 43.87%          | 6.627%        |
| 5         | 7.652       | 768           | 776         | 786          | rBV      | 483084         | 744535        | 15.27%          | 2.306%        |
| 6         | 8.805       | 965           | 972         | 988          | rBV      | 859837         | 1446296       | 29.66%          | 4.480%        |
| 7         | 10.428      | 1237          | 1248        | 1263         | rBV      | 632728         | 1089032       | 22.33%          | 3.374%        |
| 8         | 11.187      | 1370          | 1377        | 1391         | rBV      | 35838          | 103743        | 2.13%           | 0.321%        |
| 9         | 12.899      | 1660          | 1668        | 1683         | rBV      | 2229182        | 3473964       | 71.24%          | 10.762%       |
| 10        | 13.469      | 1759          | 1765        | 1769         | rBV3     | 42519          | 63998         | 1.31%           | 0.198%        |
| 11        | 14.287      | 1896          | 1904        | 1912         | rBV      | 905674         | 1466166       | 30.07%          | 4.542%        |
| 12        | 14.516      | 1935          | 1943        | 1956         | rBV      | 358459         | 806455        | 16.54%          | 2.498%        |
| 13        | 15.804      | 2156          | 2162        | 2183         | rBV      | 2177385        | 3409284       | 69.92%          | 10.561%       |
| 14        | 17.075      | 2372          | 2378        | 2391         | rBV      | 1175176        | 1756541       | 36.02%          | 5.441%        |
| 15        | 17.945      | 2522          | 2526        | 2531         | rVB      | 42744          | 57205         | 1.17%           | 0.177%        |
| 16        | 18.016      | 2532          | 2538        | 2552         | rBV2     | 284599         | 498788        | 10.23%          | 1.545%        |
| 17        | 18.322      | 2585          | 2590        | 2593         | rBV2     | 123289         | 174952        | 3.59%           | 0.542%        |
| 18        | 18.457      | 2610          | 2613        | 2620         | rBV6     | 32400          | 51222         | 1.05%           | 0.159%        |
| 19        | 19.210      | 2734          | 2741        | 2745         | rBV      | 105869         | 217733        | 4.47%           | 0.674%        |
| 20        | 19.345      | 2760          | 2764        | 2773         | rBV3     | 80936          | 129915        | 2.66%           | 0.402%        |
| 21        | 19.581      | 2801          | 2804        | 2808         | rBV      | 76923          | 96125         | 1.97%           | 0.298%        |
| 22        | 19.798      | 2836          | 2841        | 2852         | rBV      | 3734278        | 4876211       | 100.00%         | 15.106%       |
| 23        | 20.139      | 2896          | 2899        | 2903         | rVB      | 49337          | 56582         | 1.16%           | 0.175%        |
| 24        | 20.475      | 2952          | 2956        | 2960         | rBV2     | 236661         | 277404        | 5.69%           | 0.859%        |
| 25        | 20.651      | 2982          | 2986        | 2991         | rBV2     | 118412         | 174247        | 3.57%           | 0.540%        |
| 26        | 21.175      | 3071          | 3075        | 3083         | rVB      | 250350         | 369141        | 7.57%           | 1.144%        |
| 27        | 21.504      | 3125          | 3131        | 3138         | rBV      | 1264109        | 2080676       | 42.67%          | 6.446%        |
| 28        | 22.369      | 3274          | 3278        | 3283         | rBV      | 164262         | 296043        | 6.07%           | 0.917%        |
| 29        | 23.910      | 3534          | 3540        | 3548         | rVB      | 498433         | 1070594       | 21.96%          | 3.316%        |
| 30        | 24.780      | 3680          | 3688        | 3698         | rBV      | 777752         | 2060067       | 42.25%          | 6.382%        |
| 31        | 26.057      | 3896          | 3905        | 3912         | rBV3     | 337240         | 1005492       | 20.62%          | 3.115%        |




Sum of corrected areas: 32280987

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052025\  
Data File : BP024724.D  
Acq On : 21 May 2025 03:30  
Operator : RC/JU  
Sample : Q1984-09  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

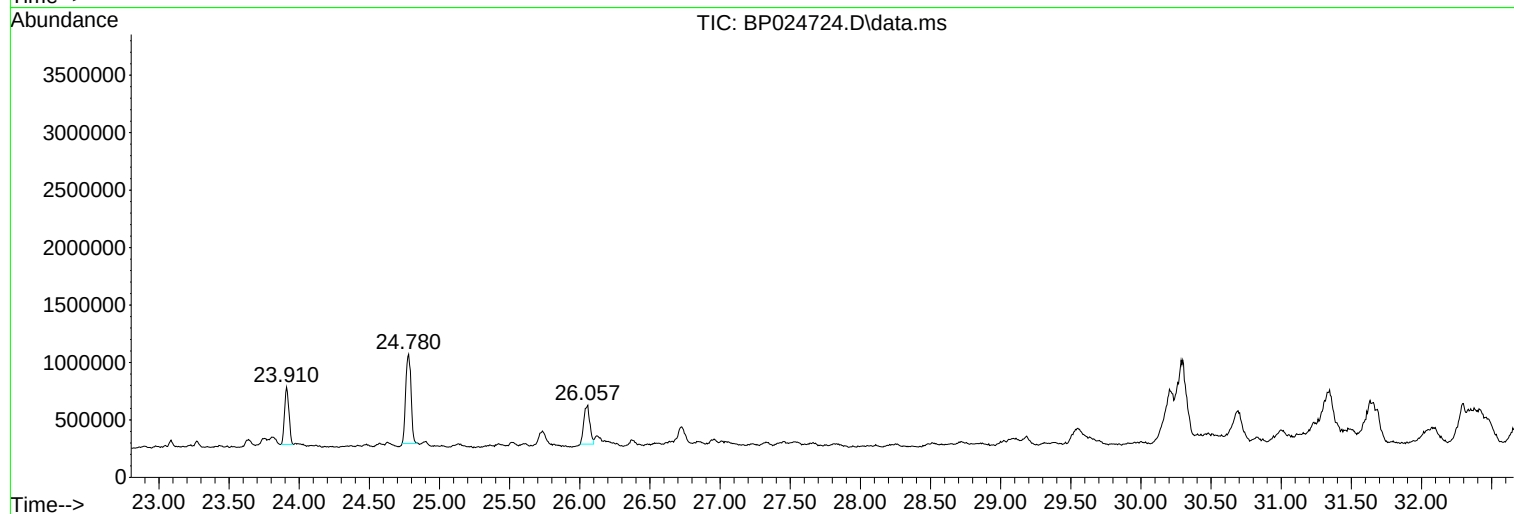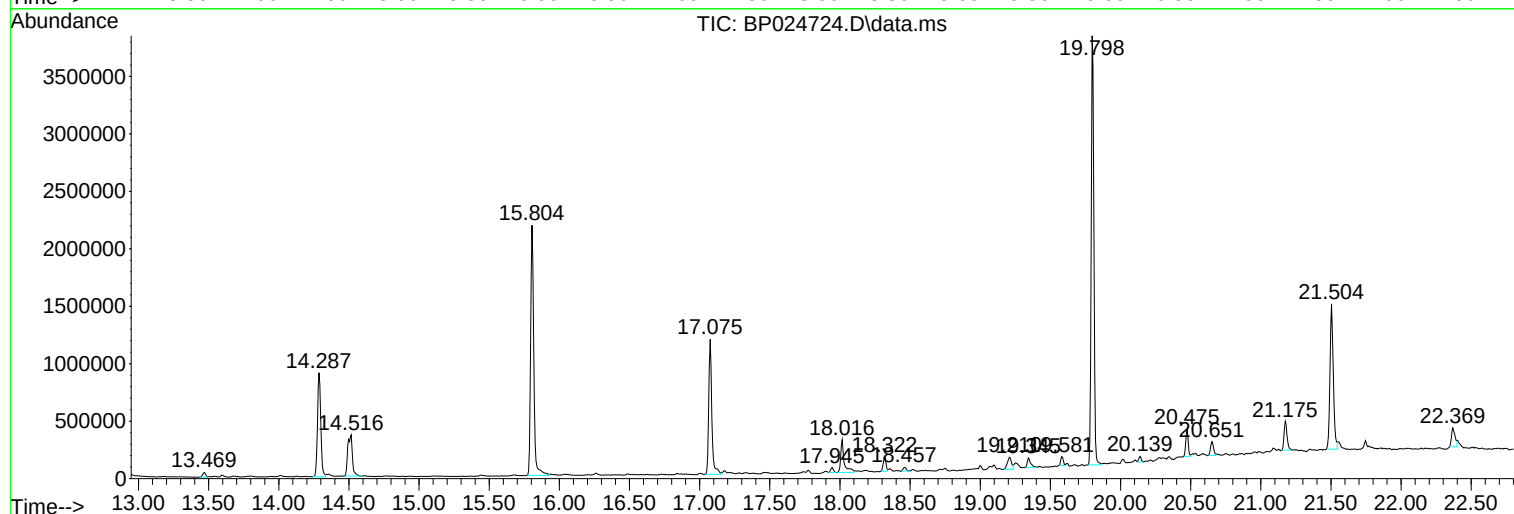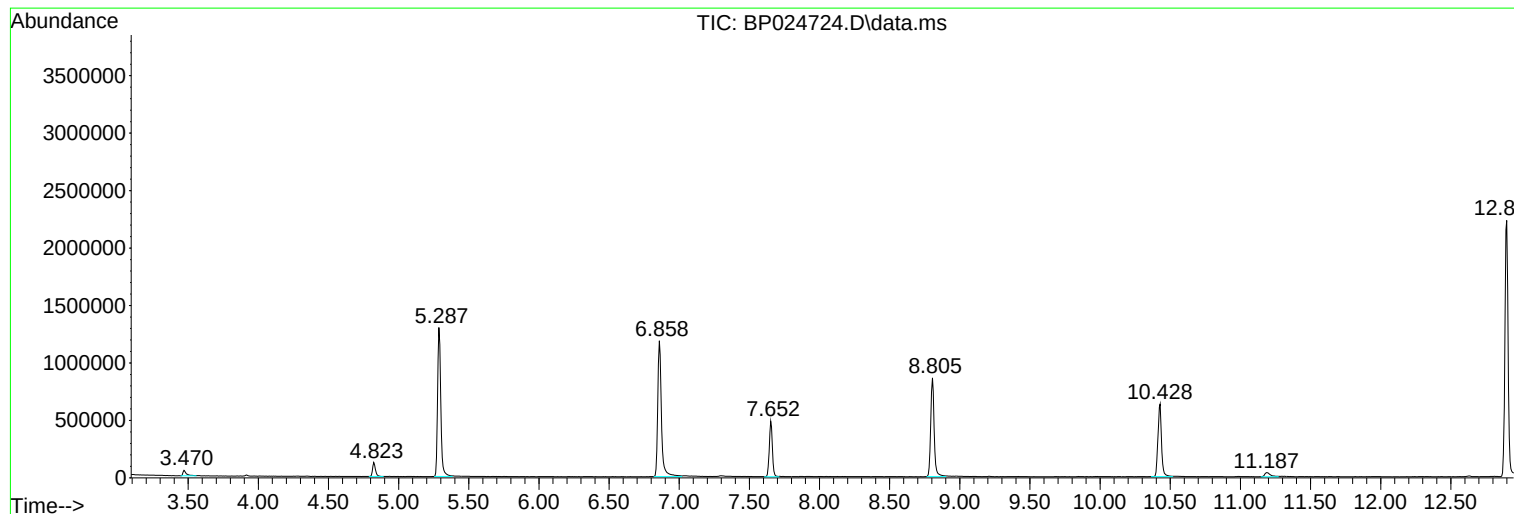

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052025\  
Data File : BP024724.D  
Acq On : 21 May 2025 03:30  
Operator : RC/JU  
Sample : Q1984-09  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052025\  
Data File : BP024724.D  
Acq On : 21 May 2025 03:30  
Operator : RC/JU  
Sample : Q1984-09  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|