

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
 Data File : BP024725.D
 Acq On : 21 May 2025 04:10
 Operator : RC/JU
 Sample : Q1984-13RX
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-27-050725RX

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.475	62	66	79	rBV	51797	90447	1.85%	0.238%
2	4.822	288	295	304	rBV	130761	196764	4.03%	0.519%
3	5.293	368	375	397	rBV	1409814	2204588	45.20%	5.810%
4	6.863	635	642	659	rBV	1345195	2377485	48.75%	6.265%
5	7.657	769	777	794	rBV	536327	895350	18.36%	2.359%
6	8.804	964	972	993	rBV	952169	1629181	33.41%	4.293%
7	10.428	1239	1248	1262	rBV	704379	1271257	26.07%	3.350%
8	11.181	1367	1376	1387	rBV	53931	133521	2.74%	0.352%
9	12.898	1660	1668	1681	rBV	2478707	3685351	75.57%	9.712%
10	13.463	1756	1764	1769	rBV2	45731	71320	1.46%	0.188%
11	14.286	1896	1904	1913	rBV	1023575	1671038	34.26%	4.403%
12	14.510	1934	1942	1955	rBV	1243834	2572530	52.75%	6.779%
13	15.669	2134	2139	2150	rBV	31796	62436	1.28%	0.165%
14	15.804	2155	2162	2178	rBV	2068580	3449381	70.73%	9.090%
15	17.080	2372	2379	2385	rBV	1191947	1808849	37.09%	4.767%
16	17.945	2523	2526	2530	rVB	49742	60216	1.23%	0.159%
17	18.016	2533	2538	2547	rBV	342046	536828	11.01%	1.415%
18	18.322	2585	2590	2594	rBV	128218	184915	3.79%	0.487%
19	18.457	2610	2613	2619	rBV6	34464	56001	1.15%	0.148%
20	19.204	2735	2740	2745	rBV	135611	283234	5.81%	0.746%
21	19.345	2760	2764	2773	rBV2	105768	184546	3.78%	0.486%
22	19.586	2801	2805	2808	rBV	113231	144381	2.96%	0.380%
23	19.663	2816	2818	2826	rVB6	72532	120229	2.47%	0.317%
24	19.804	2836	2842	2851	rBV	4057779	4876883	100.00%	12.852%
25	20.474	2952	2956	2960	rBV2	252732	310275	6.36%	0.818%
26	20.651	2983	2986	2991	rVB3	89808	120877	2.48%	0.319%
27	21.174	3071	3075	3083	rVB2	224448	375971	7.71%	0.991%
28	21.510	3125	3132	3137	rBV	1383878	2320038	47.57%	6.114%
29	21.633	3151	3153	3163	rVB5	167314	380808	7.81%	1.004%
30	22.045	3216	3223	3231	rBV3	387396	1203158	24.67%	3.171%
31	22.374	3275	3279	3291	rVB3	155194	413780	8.48%	1.090%
32	23.927	3538	3543	3544	rBV	332936	447012	9.17%	1.178%
33	24.786	3681	3689	3700	rBV	798525	2250608	46.15%	5.931%
34	26.062	3901	3906	3916	rVB	257816	663944	13.61%	1.750%
35	30.221	4604	4613	4618	rBV8	244254	894754	18.35%	2.358%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024725.D
Acq On : 21 May 2025 04:10
Operator : RC/JU
Sample : Q1984-13RX
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-27-050725RX

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 37947956

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024725.D
Acq On : 21 May 2025 04:10
Operator : RC/JU
Sample : Q1984-13RX
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-27-050725RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

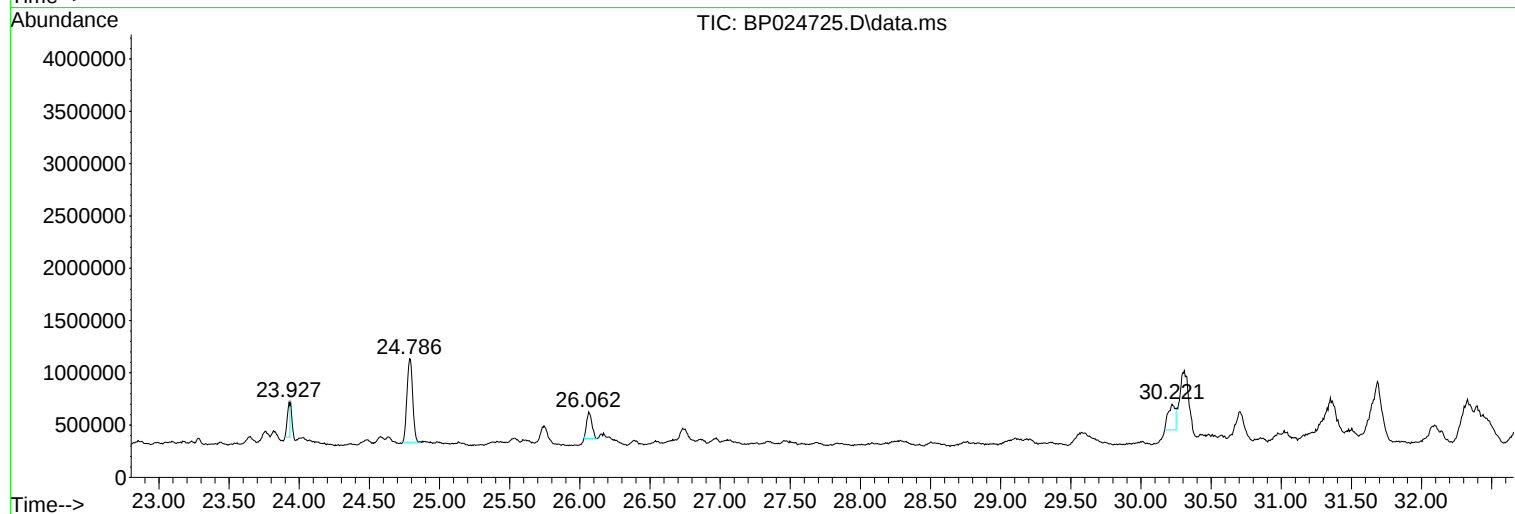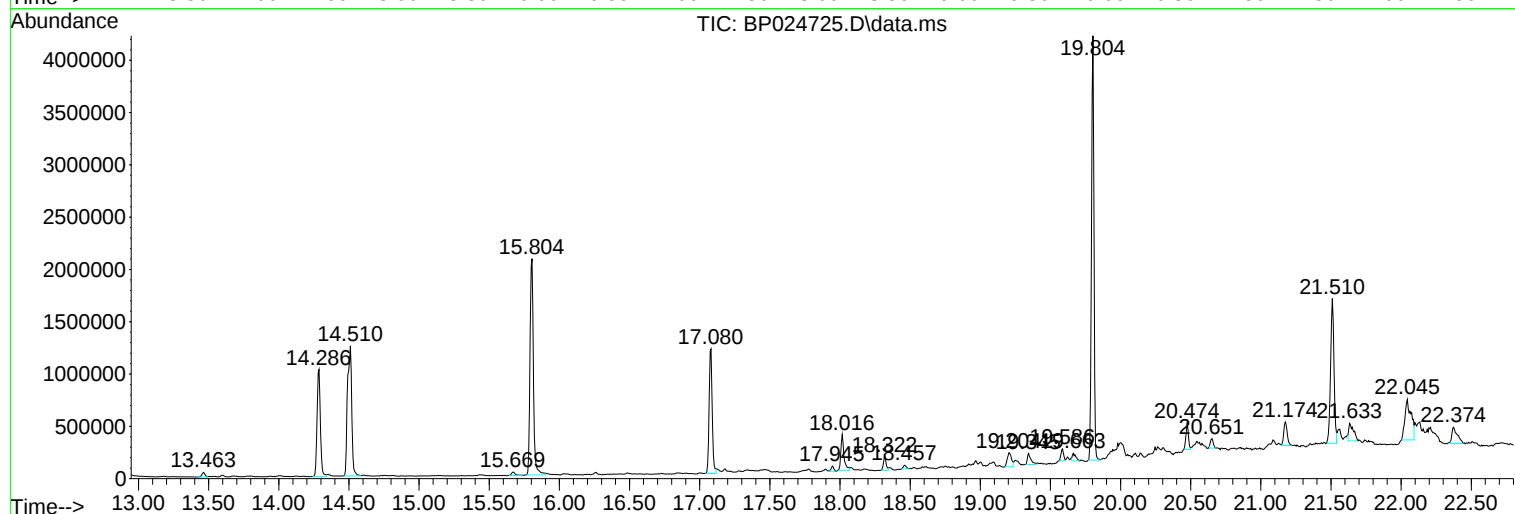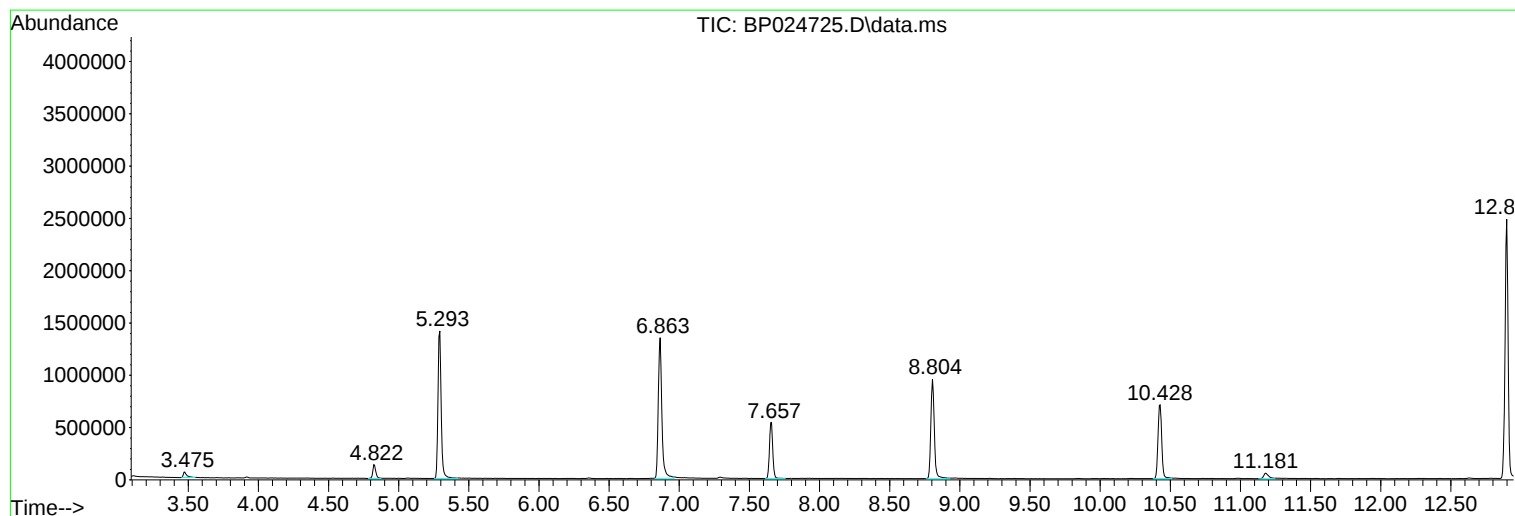

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024725.D
Acq On : 21 May 2025 04:10
Operator : RC/JU
Sample : Q1984-13RX
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-27-050725RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024725.D
Acq On : 21 May 2025 04:10
Operator : RC/JU
Sample : Q1984-13RX
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-27-050725RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------