

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
 Data File : BP015207.D
 Acq On : 22 May 2023 10:29
 Operator : CG/JU
 Sample : PB152888BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK888

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	37	41	48	rVB	66154	88276	1.68%	0.143%
2	3.869	113	116	138	rBV	801807	1267712	24.07%	2.052%
3	4.211	171	174	181	rVB	12638	20193	0.38%	0.033%
4	7.269	687	694	711	rBV	995126	1642376	31.19%	2.658%
5	7.440	717	723	736	rVB	836319	1337186	25.39%	2.164%
6	7.646	751	758	769	rBV	1063355	1706840	32.41%	2.762%
7	8.122	831	839	849	rBV	903768	1433259	27.21%	2.319%
8	8.834	951	960	974	rBV	1293096	2183846	41.47%	3.534%
9	9.299	1031	1039	1047	rBV	1057689	1716960	32.60%	2.779%
10	9.693	1102	1106	1109	rBV6	3078	5433	0.10%	0.009%
11	10.028	1155	1163	1175	rBV	868248	1489040	28.27%	2.410%
12	10.563	1247	1254	1276	rBV	1302590	2285910	43.40%	3.699%
13	10.951	1312	1320	1331	rVB	1309680	2190031	41.58%	3.544%
14	11.087	1335	1343	1361	rBV	1307389	2305651	43.78%	3.731%
15	12.534	1583	1589	1599	rBV2	17341	38216	0.73%	0.062%
16	13.645	1771	1778	1784	rBV2	23556	40603	0.77%	0.066%
17	13.740	1789	1794	1800	rVB9	3909	8862	0.17%	0.014%
18	14.163	1859	1866	1877	rBV	2408167	3445460	65.42%	5.576%
19	14.275	1883	1885	1892	rVB8	3645	7008	0.13%	0.011%
20	14.457	1909	1916	1928	rBV	2798636	4121905	78.27%	6.670%
21	14.681	1950	1954	1958	rVB7	2979	5620	0.11%	0.009%
22	14.763	1958	1968	1982	rBV	1992889	3016134	57.27%	4.881%
23	14.951	1992	2000	2019	rBV	787625	1390036	26.39%	2.249%
24	15.169	2034	2037	2044	rVB9	7422	12165	0.23%	0.020%
25	15.422	2076	2080	2085	rVB8	3039	6020	0.11%	0.010%
26	15.751	2126	2136	2149	rBV	3376080	4931391	93.64%	7.980%
27	15.869	2150	2156	2171	rVV	803929	1128893	21.44%	1.827%
28	15.992	2173	2177	2183	rVB3	18149	31102	0.59%	0.050%
29	16.539	2266	2270	2275	rVB8	4855	9028	0.17%	0.015%
30	17.298	2397	2399	2404	rVB5	5634	8897	0.17%	0.014%
31	17.516	2429	2436	2444	rBV	2432665	3450152	65.51%	5.583%
32	17.616	2446	2453	2466	rVV	3530068	5106303	96.96%	8.264%
33	19.410	2754	2758	2764	rBV2	43807	62534	1.19%	0.101%
34	19.480	2766	2770	2777	rVB	40310	55445	1.05%	0.090%
35	19.833	2824	2830	2843	rBV	3925152	5266532	100.00%	8.523%
36	21.586	3123	3128	3137	rBV	1871026	2720051	51.65%	4.402%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015207.D
Acq On : 22 May 2023 10:29
Operator : CG/JU
Sample : PB152888BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK888

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	23.980	3528	3535	3549	rVB	2209371	4596650	87.28%	7.439%
38	24.145	3557	3563	3577	rVB	1243560	2661703	50.54%	4.307%




Sum of corrected areas: 61793423

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015207.D
Acq On : 22 May 2023 10:29
Operator : CG/JU
Sample : PB152888BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK888

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

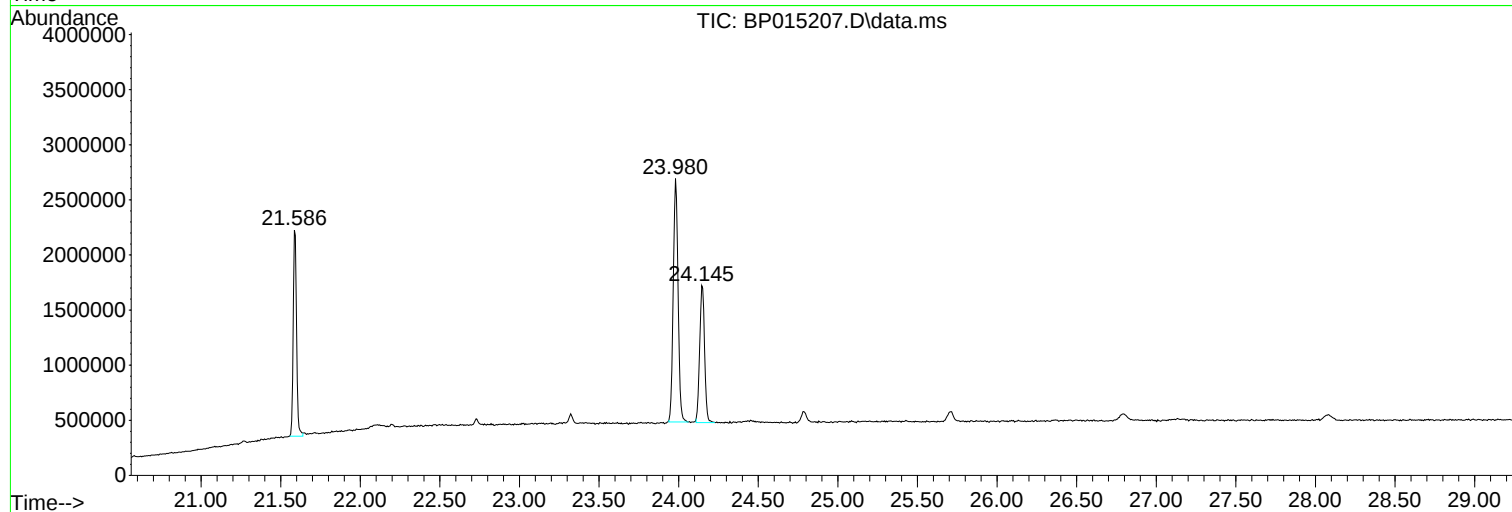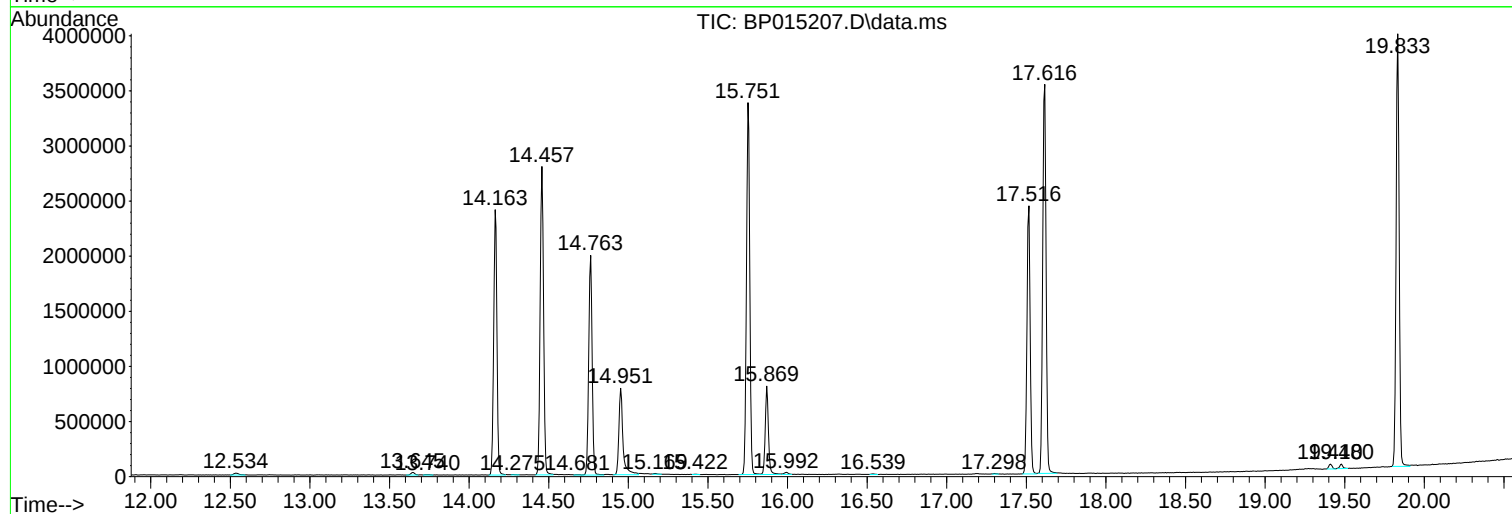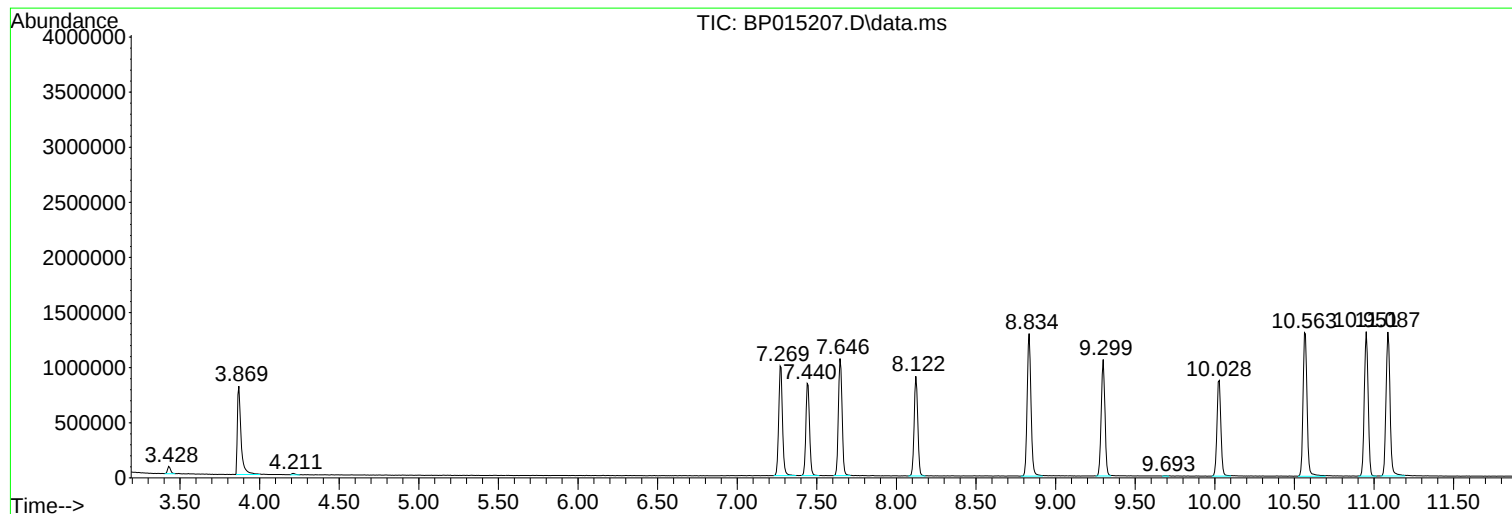

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015207.D
Acq On : 22 May 2023 10:29
Operator : CG/JU
Sample : PB152888BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK888

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015207.D
Acq On : 22 May 2023 10:29
Operator : CG/JU
Sample : PB152888BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK888

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------