

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
 Data File : BP015211.D
 Acq On : 22 May 2023 12:47
 Operator : CG/JU
 Sample : 02822-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	38	42	47	rVB	40247	54623	1.99%	0.187%
2	3.876	115	117	131	rBV	210964	340481	12.41%	1.164%
3	4.105	154	156	162	rVB5	4977	9049	0.33%	0.031%
4	4.211	170	174	180	rVB	14163	21356	0.78%	0.073%
5	4.670	249	252	257	rBV	5032	7935	0.29%	0.027%
6	5.093	323	324	331	rVB6	2158	3454	0.13%	0.012%
7	5.658	416	420	421	rBV4	3318	3412	0.12%	0.012%
8	5.775	438	440	447	rVB6	4185	7520	0.27%	0.026%
9	7.222	683	686	689	rBV4	4713	6107	0.22%	0.021%
10	7.275	689	695	707	rVB	207747	357762	13.04%	1.223%
11	7.440	715	723	733	rBV	295729	475928	17.34%	1.627%
12	7.646	751	758	771	rBV	308388	516505	18.82%	1.765%
13	8.122	831	839	850	rBV	745317	1190482	43.38%	4.069%
14	8.834	951	960	972	rBV	336471	586190	21.36%	2.003%
15	9.122	1005	1009	1012	rBV5	2239	2924	0.11%	0.010%
16	9.299	1032	1039	1055	rBV	353252	598629	21.82%	2.046%
17	9.693	1101	1106	1113	rVB	15323	25228	0.92%	0.086%
18	10.028	1156	1163	1173	rBV	242412	418396	15.25%	1.430%
19	10.569	1246	1255	1275	rBV	385459	708104	25.80%	2.420%
20	10.952	1312	1320	1330	rBV	1075672	1811451	66.01%	6.191%
21	11.087	1335	1343	1358	rBV	367176	731082	26.64%	2.499%
22	11.381	1391	1393	1398	rVB7	2700	2997	0.11%	0.010%
23	11.552	1417	1422	1424	rVB6	1990	2769	0.10%	0.009%
24	12.187	1525	1530	1535	rVB	11154	17085	0.62%	0.058%
25	12.369	1558	1561	1565	rVB6	2053	2808	0.10%	0.010%
26	12.534	1584	1589	1600	rBV7	6544	14627	0.53%	0.050%
27	12.763	1626	1628	1632	rVB5	2608	3258	0.12%	0.011%
28	13.381	1728	1733	1739	rVB10	1999	4641	0.17%	0.016%
29	13.575	1760	1766	1770	rBV9	4268	6649	0.24%	0.023%
30	13.646	1772	1778	1786	rVV2	23147	38777	1.41%	0.133%
31	13.740	1789	1794	1797	rVB7	2852	4130	0.15%	0.014%
32	14.163	1857	1866	1880	rBV	961274	1330344	48.48%	4.547%
33	14.275	1883	1885	1889	rVB4	2313	3024	0.11%	0.010%
34	14.457	1909	1916	1933	rBV	987322	1500824	54.69%	5.129%
35	14.757	1961	1967	1978	rBV	1668558	2500009	91.11%	8.544%
36	14.957	1995	2001	2016	rBV2	60634	170177	6.20%	0.582%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
 Data File : BP015211.D
 Acq On : 22 May 2023 12:47
 Operator : CG/JU
 Sample : 02822-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	15.198	2040	2042	2045	rVB4	2471	2820	0.10%	0.010%
38	15.498	2091	2093	2097	rBV5	1823	2889	0.11%	0.010%
39	15.710	2122	2129	2130	rBV3	10746	15244	0.56%	0.052%
40	15.751	2130	2136	2148	rVV	1324367	1907660	69.52%	6.520%
41	15.869	2151	2156	2168	rVB2	96921	156520	5.70%	0.535%
42	15.993	2173	2177	2180	rVB6	4345	7503	0.27%	0.026%
43	16.116	2192	2198	2205	rBV	136696	204231	7.44%	0.698%
44	16.681	2287	2294	2301	rBV5	13657	24247	0.88%	0.083%
45	16.957	2337	2341	2346	rBV2	7389	10778	0.39%	0.037%
46	17.187	2378	2380	2386	rVB7	3674	4274	0.16%	0.015%
47	17.298	2396	2399	2407	rVB6	3957	7625	0.28%	0.026%
48	17.510	2429	2435	2446	rBV	1930049	2744093	100.00%	9.378%
49	17.610	2446	2452	2464	rVV2	1404483	2074179	75.59%	7.089%
50	18.022	2519	2522	2528	rVB5	8043	11258	0.41%	0.038%
51	18.375	2577	2582	2586	rBV6	12921	21368	0.78%	0.073%
52	18.928	2673	2676	2679	rBV3	8666	9857	0.36%	0.034%
53	19.410	2755	2758	2763	rVB5	17508	22340	0.81%	0.076%
54	19.828	2824	2829	2841	rBV	1546497	2103977	76.67%	7.191%
55	21.586	3123	3128	3136	rBV	1567193	2189315	79.78%	7.482%
56	23.974	3528	3534	3545	rVB	907313	2005932	73.10%	6.856%
57	24.145	3556	3563	3574	rVB	1041613	2255331	82.19%	7.708%




Sum of corrected areas: 29260178

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015211.D
Acq On : 22 May 2023 12:47
Operator : CG/JU
Sample : 02822-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONM2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

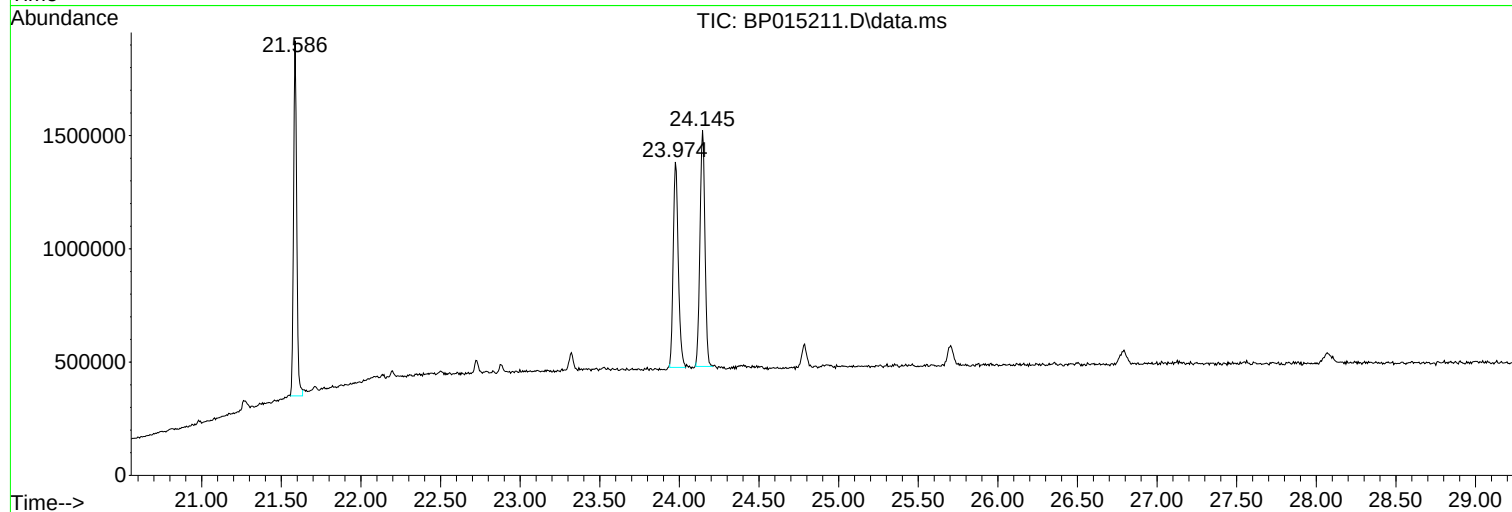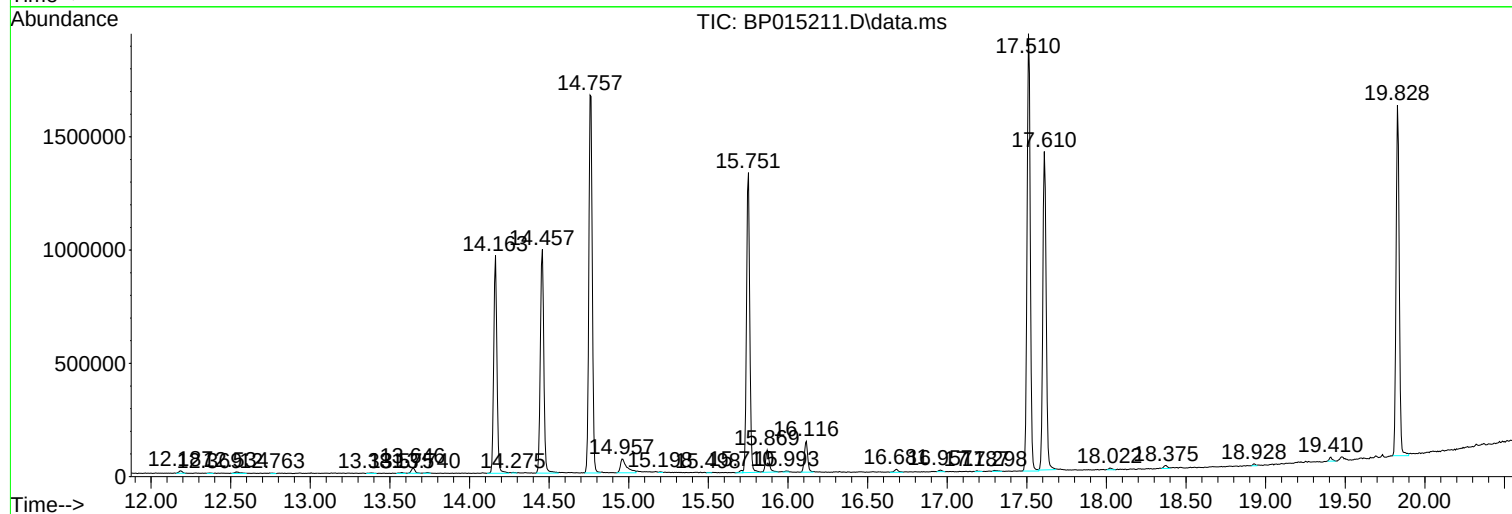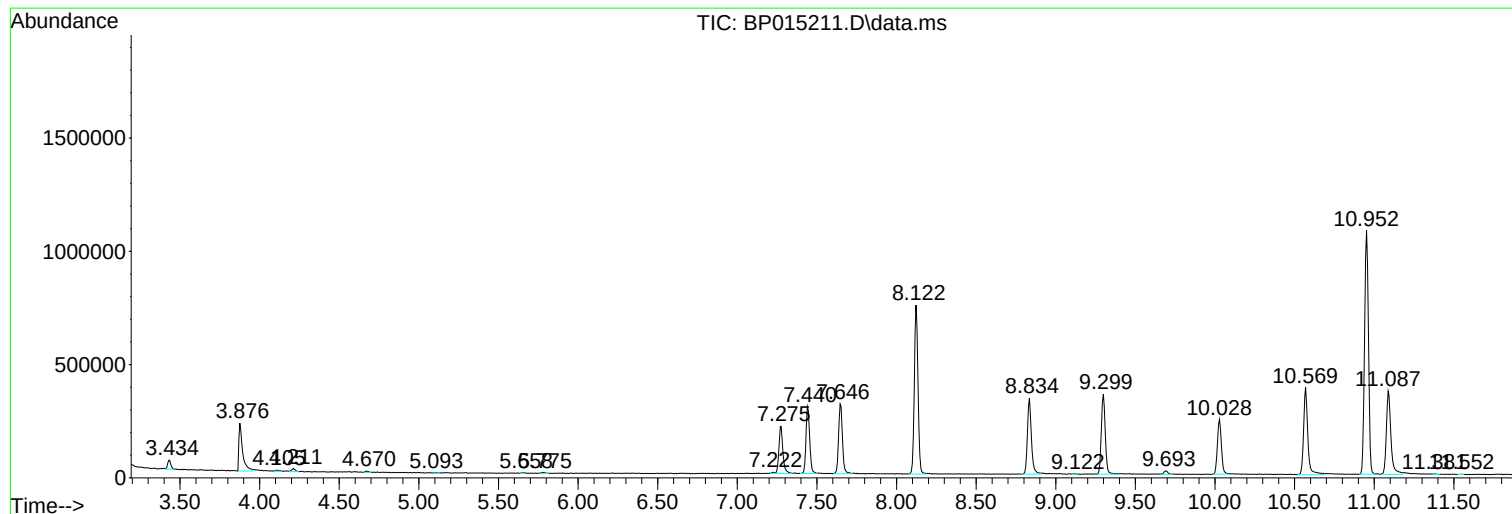

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015211.D
Acq On : 22 May 2023 12:47
Operator : CG/JU
Sample : 02822-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONM2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015211.D
Acq On : 22 May 2023 12:47
Operator : CG/JU
Sample : 02822-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONM2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------