

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
 Data File : BP015227.D
 Acq On : 22 May 2023 22:19
 Operator : CG/JU
 Sample : 02664-09DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREA4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.916	123	124	131	rBV5	7149	9412	0.15%	0.031%
2	3.981	132	135	140	rVB2	20190	27020	0.43%	0.089%
3	4.110	154	157	162	rVB4	9595	15345	0.24%	0.051%
4	4.210	170	174	180	rVB	16792	27355	0.43%	0.090%
5	4.669	248	252	256	rVB	14235	20230	0.32%	0.067%
6	5.163	332	336	342	rVB4	6968	11292	0.18%	0.037%
7	5.775	436	440	448	rVB4	8521	16398	0.26%	0.054%
8	6.622	579	584	589	rBV9	3959	7168	0.11%	0.024%
9	7.222	680	686	689	rBV4	9375	16545	0.26%	0.055%
10	7.269	689	694	704	rVB	73798	137268	2.17%	0.454%
11	7.440	716	723	731	rBV	75826	126499	2.00%	0.418%
12	7.646	752	758	768	rVB	94096	153379	2.42%	0.507%
13	8.122	831	839	853	rBV	1120035	1788587	28.23%	5.912%
14	8.834	953	960	970	rBV	75091	150829	2.38%	0.499%
15	8.957	975	981	989	rBV	43753	79910	1.26%	0.264%
16	9.298	1032	1039	1047	rBV	80905	145356	2.29%	0.480%
17	9.410	1051	1058	1063	rVB	3076	7310	0.12%	0.024%
18	9.687	1100	1105	1111	rVB	31101	47169	0.74%	0.156%
19	10.028	1155	1163	1173	rBV2	58266	114090	1.80%	0.377%
20	10.387	1214	1224	1229	rBV2	4471	10779	0.17%	0.036%
21	10.569	1247	1255	1266	rBV	81294	177569	2.80%	0.587%
22	10.951	1311	1320	1331	rBV	1545985	2642684	41.71%	8.735%
23	11.098	1339	1345	1359	rBV2	32037	77861	1.23%	0.257%
24	11.734	1447	1453	1455	rBV7	5028	8865	0.14%	0.029%
25	11.957	1484	1491	1495	rBV10	3455	7472	0.12%	0.025%
26	12.181	1524	1529	1534	rBV	20897	31173	0.49%	0.103%
27	13.286	1711	1717	1724	rBV9	6191	12031	0.19%	0.040%
28	13.569	1761	1765	1772	rVB6	8890	14716	0.23%	0.049%
29	13.645	1772	1778	1784	rBV2	18237	32801	0.52%	0.108%
30	14.163	1859	1866	1872	rBV	219764	344639	5.44%	1.139%
31	14.222	1873	1876	1881	rVB6	14170	19034	0.30%	0.063%
32	14.451	1909	1915	1926	rBV	246517	400535	6.32%	1.324%
33	14.633	1943	1946	1951	rBV2	17691	24115	0.38%	0.080%
34	14.710	1955	1959	1960	rBV4	4710	6470	0.10%	0.021%
35	14.757	1960	1967	1976	rBV	2348360	3452388	54.50%	11.411%
36	14.963	1998	2002	2014	rBV7	20965	55318	0.87%	0.183%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
 Data File : BP015227.D
 Acq On : 22 May 2023 22:19
 Operator : CG/JU
 Sample : 02664-09DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREA4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	15.304	2057	2060	2066	rVB7	12720	16546	0.26%	0.055%
38	15.539	2095	2100	2102	rBV6	10057	17125	0.27%	0.057%
39	15.580	2104	2107	2111	rVB	30346	39359	0.62%	0.130%
40	15.704	2122	2128	2131	rBV4	20831	33563	0.53%	0.111%
41	15.751	2131	2136	2141	rVV	350089	499296	7.88%	1.650%
42	15.869	2152	2156	2165	rVB2	39066	64934	1.02%	0.215%
43	15.992	2173	2177	2182	rVB	31406	47252	0.75%	0.156%
44	16.110	2194	2197	2202	rVB	35599	40339	0.64%	0.133%
45	16.451	2251	2255	2256	rBV2	55738	70516	1.11%	0.233%
46	16.469	2256	2258	2264	rVB2	77503	102077	1.61%	0.337%
47	16.869	2323	2326	2330	rVB3	38986	46143	0.73%	0.153%
48	17.157	2371	2375	2381	rBV	178614	251399	3.97%	0.831%
49	17.245	2386	2390	2394	rBV	69883	86234	1.36%	0.285%
50	17.298	2395	2399	2403	rVV	79347	115385	1.82%	0.381%
51	17.510	2429	2435	2441	rBV	2770202	3912208	61.75%	12.931%
52	17.610	2447	2452	2456	rBV	366960	514515	8.12%	1.701%
53	17.910	2499	2503	2506	rBV4	48715	79335	1.25%	0.262%
54	17.980	2512	2515	2520	rVB2	92674	103967	1.64%	0.344%
55	18.104	2533	2536	2541	rVB4	75075	107154	1.69%	0.354%
56	18.363	2577	2580	2583	rBV3	88469	113512	1.79%	0.375%
57	18.645	2625	2628	2634	rBV	91054	105915	1.67%	0.350%
58	19.251	2728	2731	2734	rBV	105064	133702	2.11%	0.442%
59	19.504	2770	2774	2779	rBV	241580	299252	4.72%	0.989%
60	19.827	2825	2829	2832	rBV	401152	519708	8.20%	1.718%
61	21.468	3103	3108	3114	rBV	5353539	6335108	100.00%	20.939%
62	21.586	3123	3128	3133	rBV	2308810	3174435	50.11%	10.492%
63	24.145	3556	3563	3570	rVB	1513655	3206557	50.62%	10.598%




Sum of corrected areas: 30255148

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP052227.D
Acq On : 22 May 2023 22:19
Operator : CG/JU
Sample : 02664-09DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREA4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

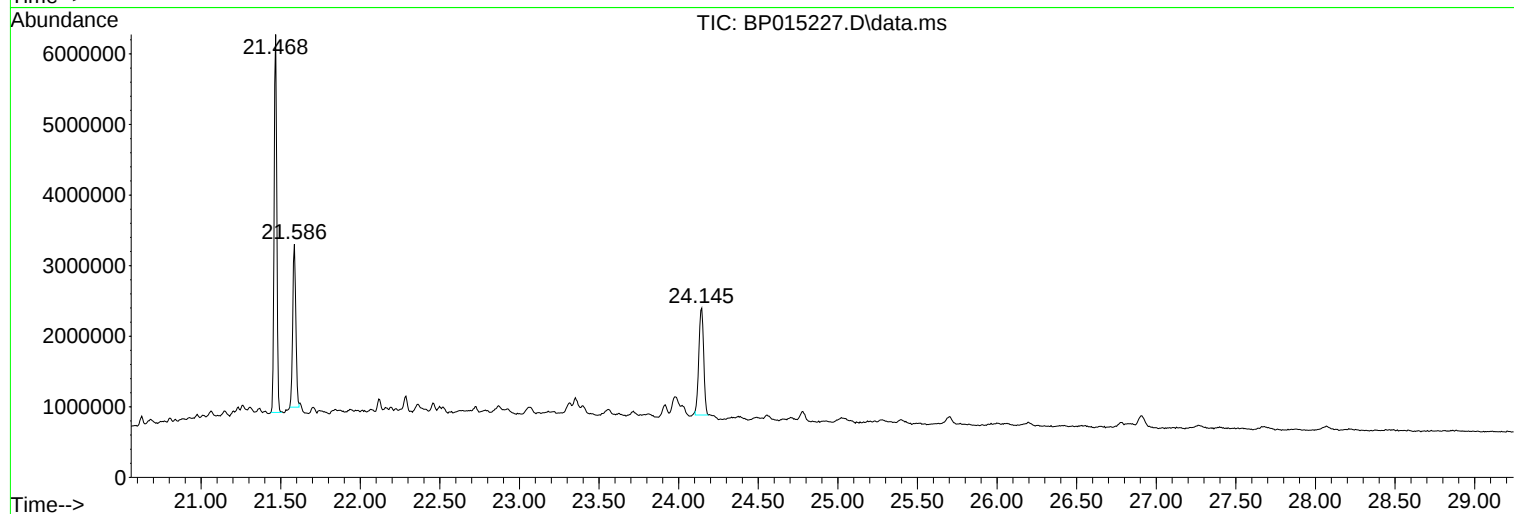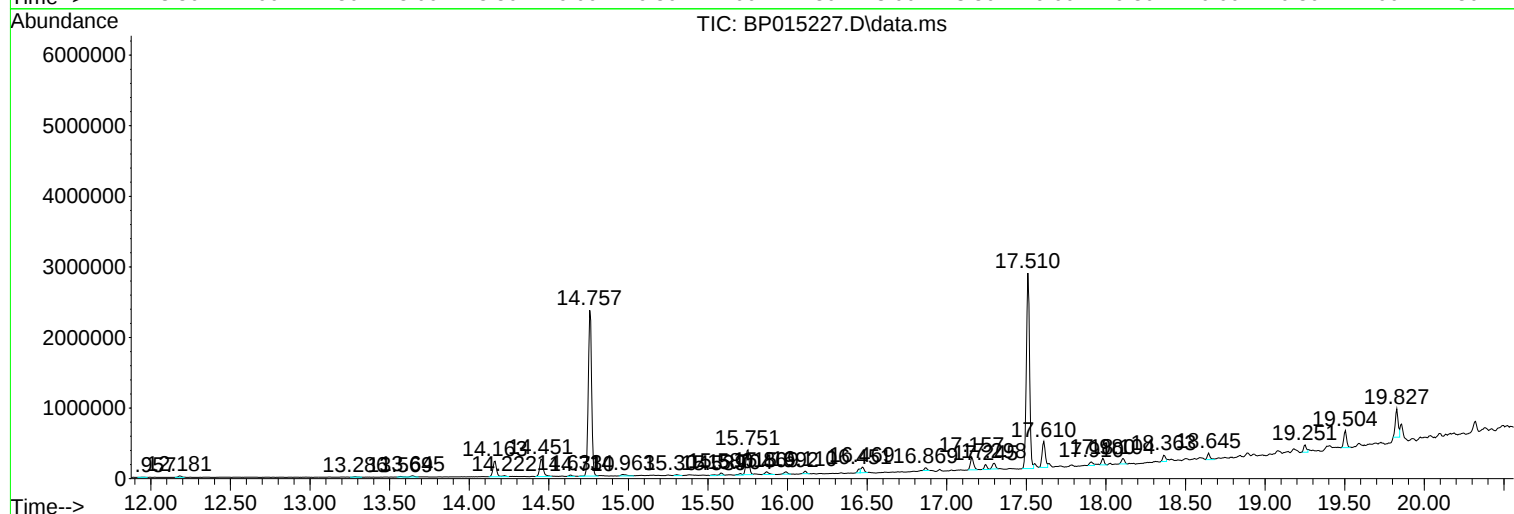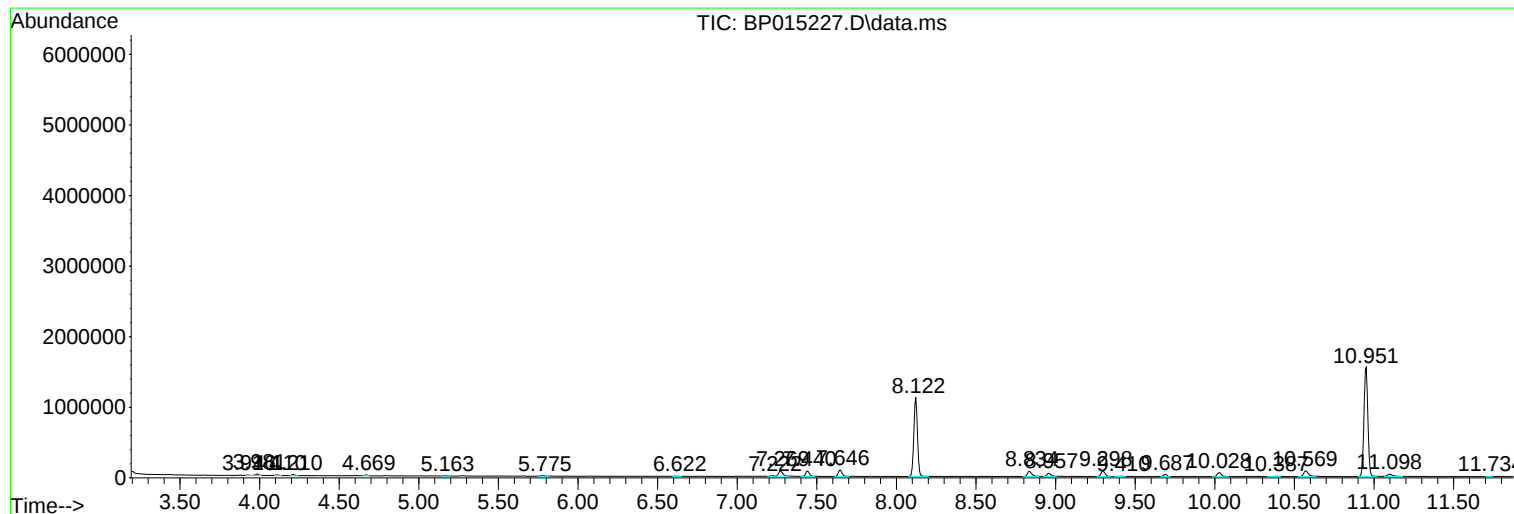

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015227.D
Acq On : 22 May 2023 22:19
Operator : CG/JU
Sample : 02664-09DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREA4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052223\
Data File : BP015227.D
Acq On : 22 May 2023 22:19
Operator : CG/JU
Sample : 02664-09DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREA4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc