
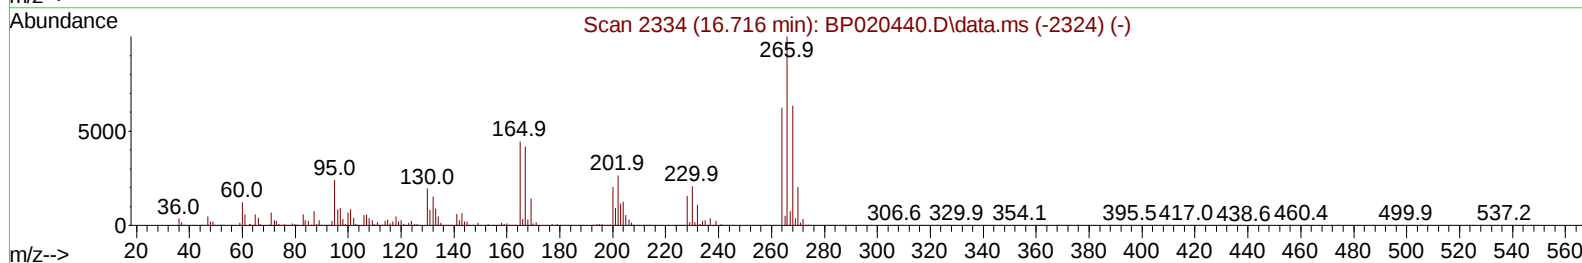
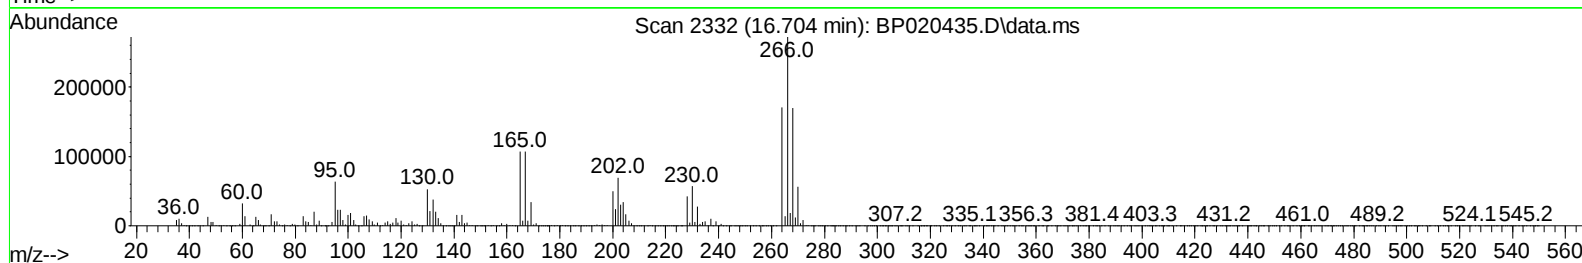


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052224\
Data File : BP020435.D
Acq On : 22 May 2024 13:15
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 02:23:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

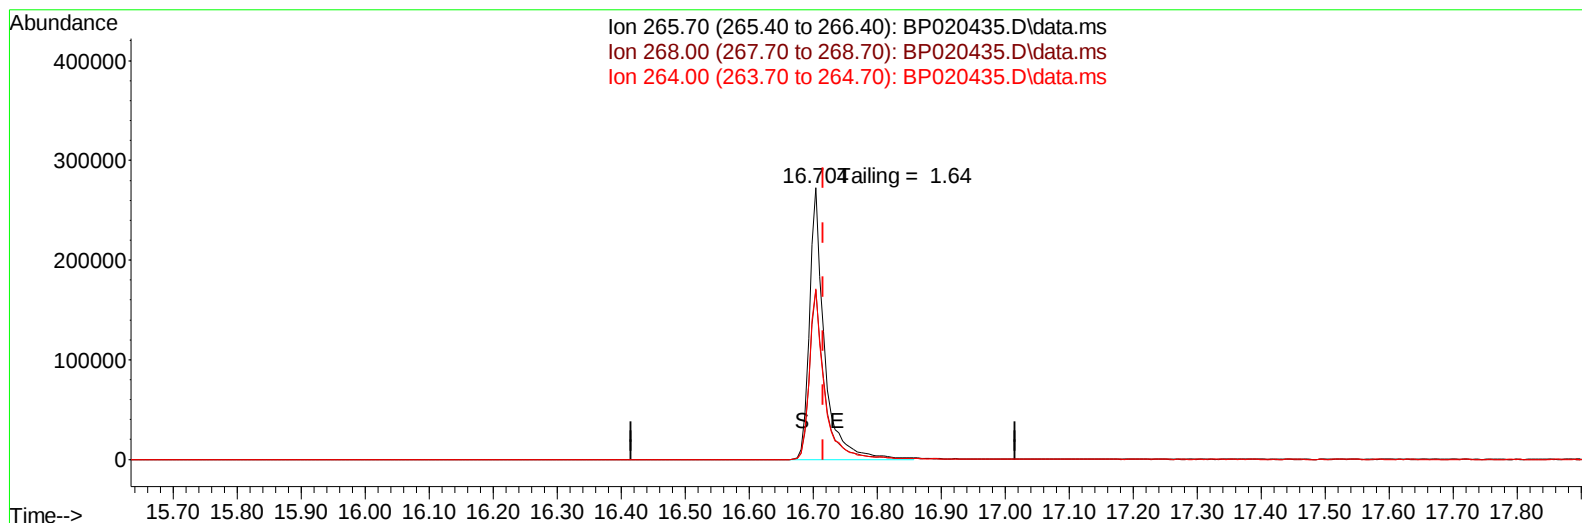

TIC: BP020435.D\data.ms

(70) Pentachlorophenol (C)




16.704min (-0.012) 2966197.22 ng

response 448378

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.36
264.00	62.40	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052224\
Data File : BP020435.D
Acq On : 22 May 2024 13:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 02:23:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

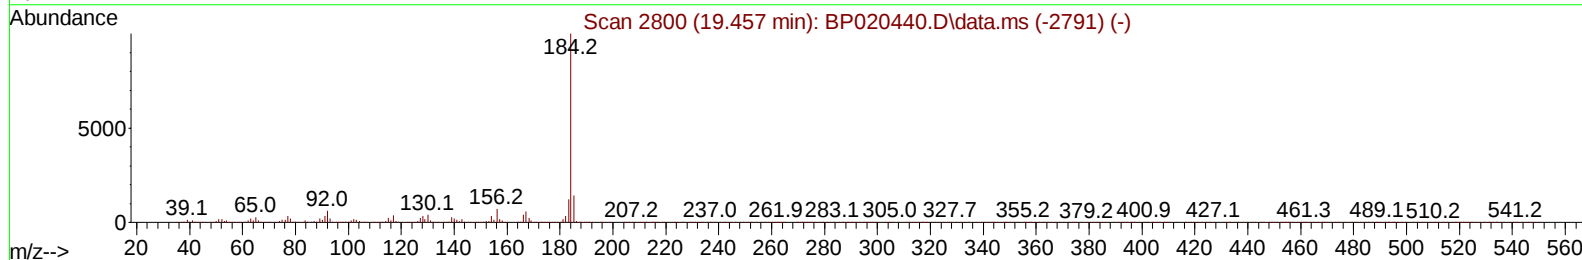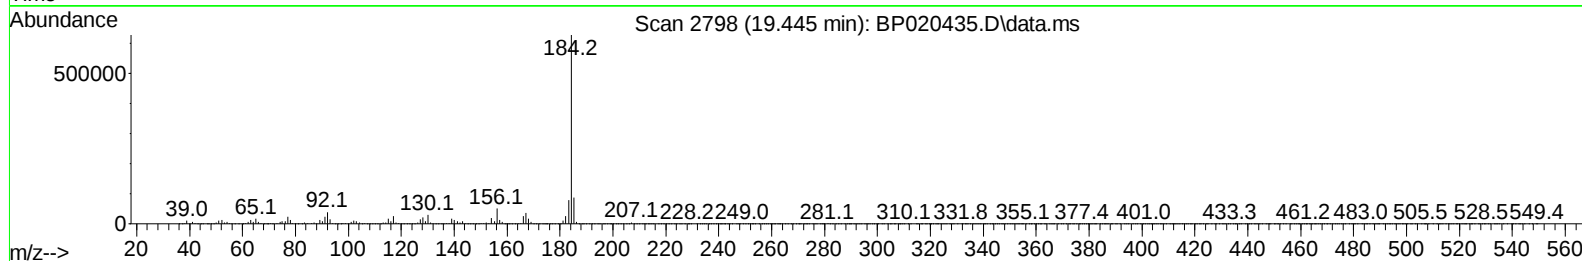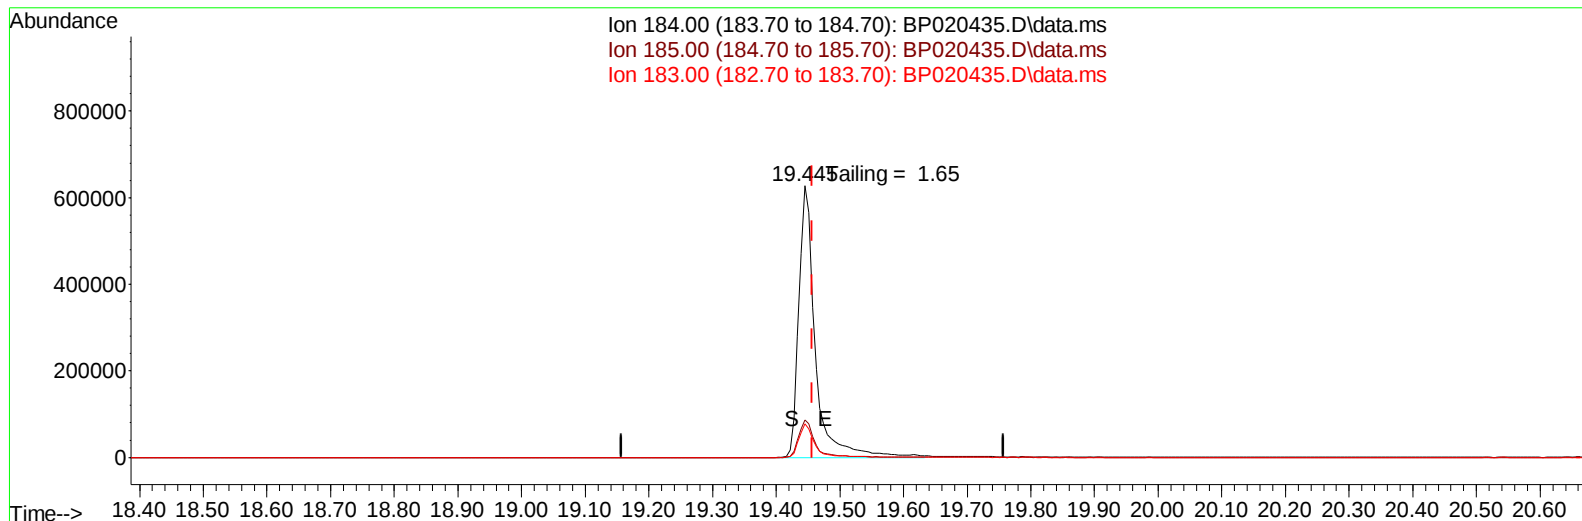

TIC: BP020435.D\data.ms

(77) Benzidine**19.445min (-0.012) 3139472.16 ng****response 1142027**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.89
183.00	12.20	12.46
0.00	0.00	0.00