

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052224\  
Data File : BP020445.D  
Acq On : 22 May 2024 22:24  
Operator : MA/JU  
Sample : PB160983BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB160983BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052224.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP020445.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.181       | 367           | 373         | 402          | rBV      | 2325385        | 3753076       | 50.28%          | 10.639%       |
| 2         | 6.746       | 632           | 639         | 659          | rBV      | 2175777        | 3859011       | 51.70%          | 10.940%       |
| 3         | 7.552       | 769           | 776         | 793          | rBV      | 437326         | 792246        | 10.61%          | 2.246%        |
| 4         | 8.716       | 965           | 974         | 1002         | rBV      | 1178568        | 2448851       | 32.81%          | 6.942%        |
| 5         | 10.322      | 1239          | 1247        | 1271         | rBV      | 424280         | 1071085       | 14.35%          | 3.036%        |
| 6         | 12.816      | 1664          | 1671        | 1696         | rBV      | 3173853        | 5590571       | 74.90%          | 15.848%       |
| 7         | 14.228      | 1903          | 1911        | 1928         | rBV      | 752050         | 1424367       | 19.08%          | 4.038%        |
| 8         | 15.769      | 2166          | 2173        | 2197         | rBV      | 2558584        | 4423054       | 59.26%          | 12.539%       |
| 9         | 17.069      | 2388          | 2394        | 2422         | rBV      | 860950         | 1698115       | 22.75%          | 4.814%        |
| 10        | 19.833      | 2858          | 2864        | 2877         | rBV      | 4931490        | 7464399       | 100.00%         | 21.160%       |
| 11        | 21.563      | 3151          | 3158        | 3172         | rBV      | 782727         | 1481093       | 19.84%          | 4.199%        |
| 12        | 24.857      | 3711          | 3718        | 3741         | rVB      | 468831         | 1269553       | 17.01%          | 3.599%        |




Sum of corrected areas: 35275421

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052224\  
Data File : BP020445.D  
Acq On : 22 May 2024 22:24  
Operator : MA/JU  
Sample : PB160983BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB160983BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

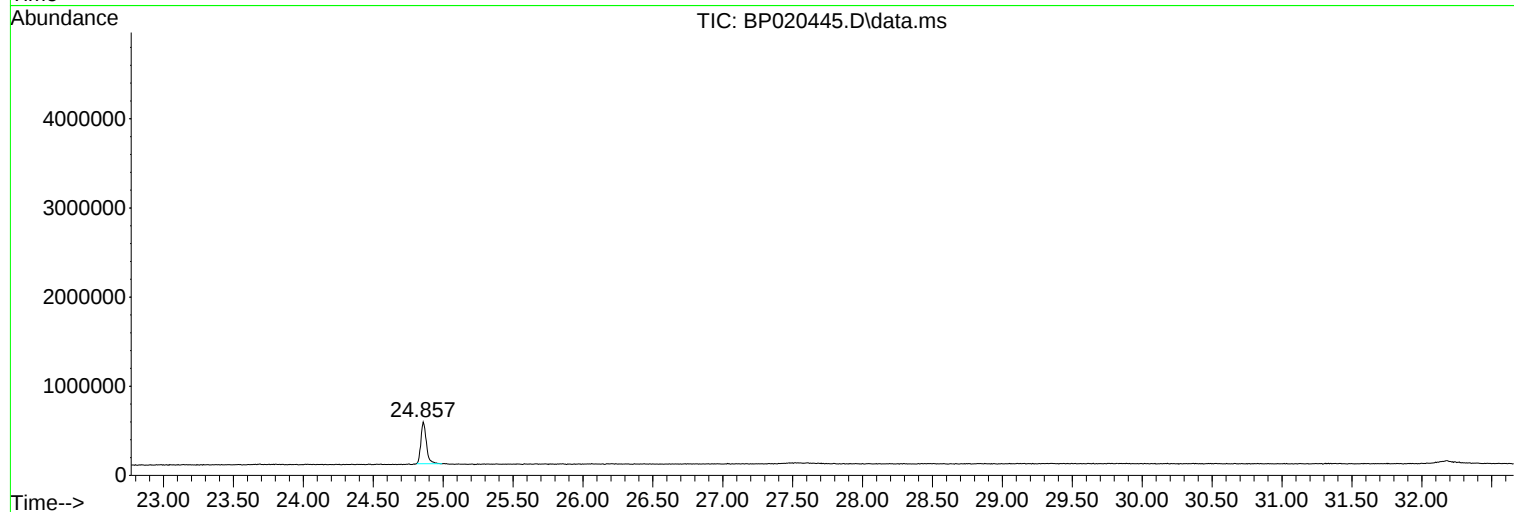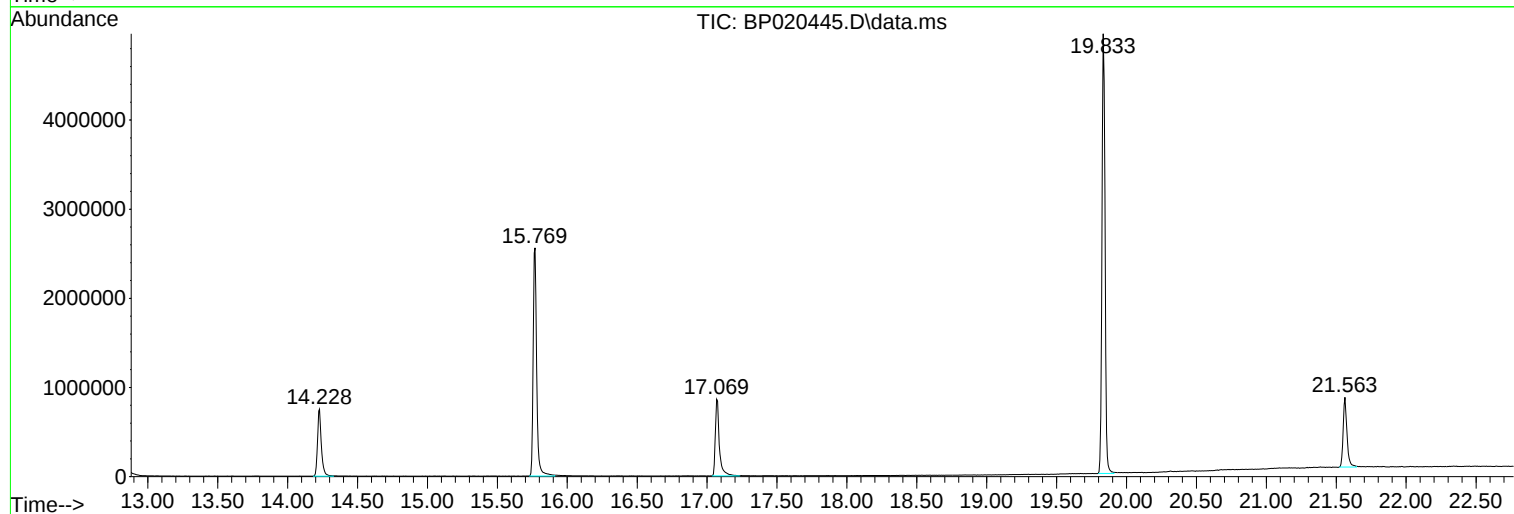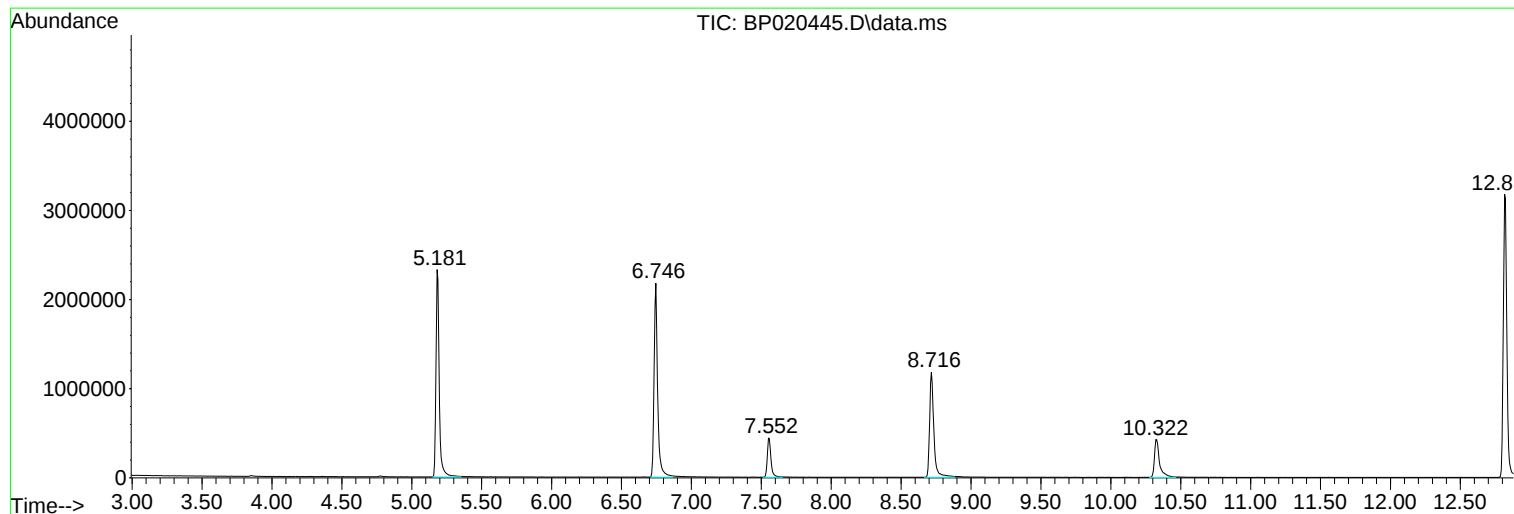

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052224\  
Data File : BP020445.D  
Acq On : 22 May 2024 22:24  
Operator : MA/JU  
Sample : PB160983BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB160983BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052224\  
Data File : BP020445.D  
Acq On : 22 May 2024 22:24  
Operator : MA/JU  
Sample : PB160983BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB160983BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|