
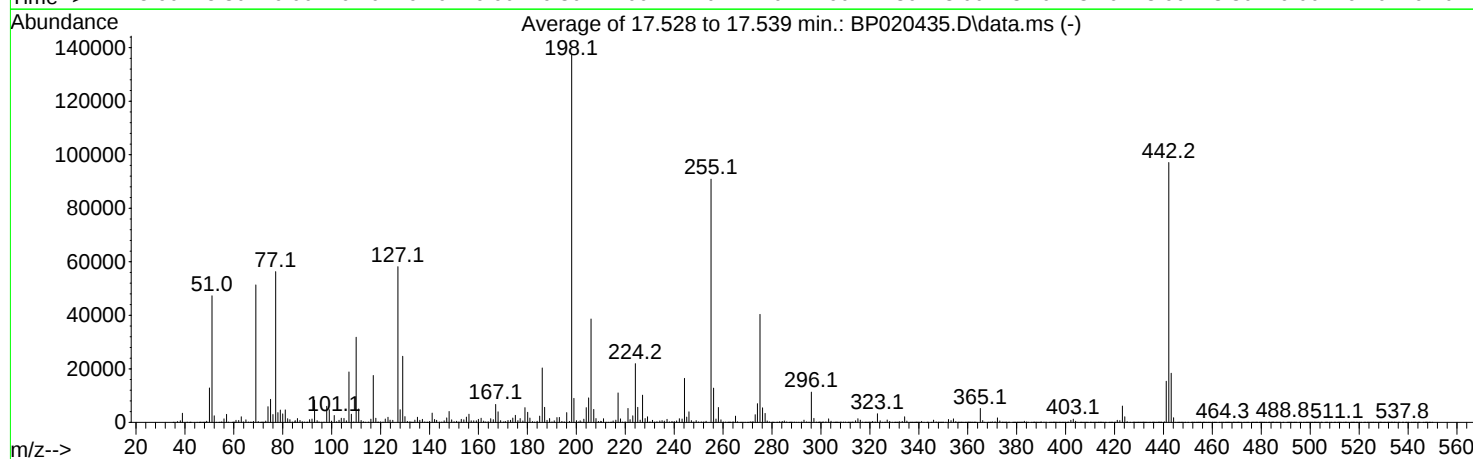


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052224\
Data File : BP020435.D
Acq On : 22 May 2024 13:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 23 02:14:59 2024

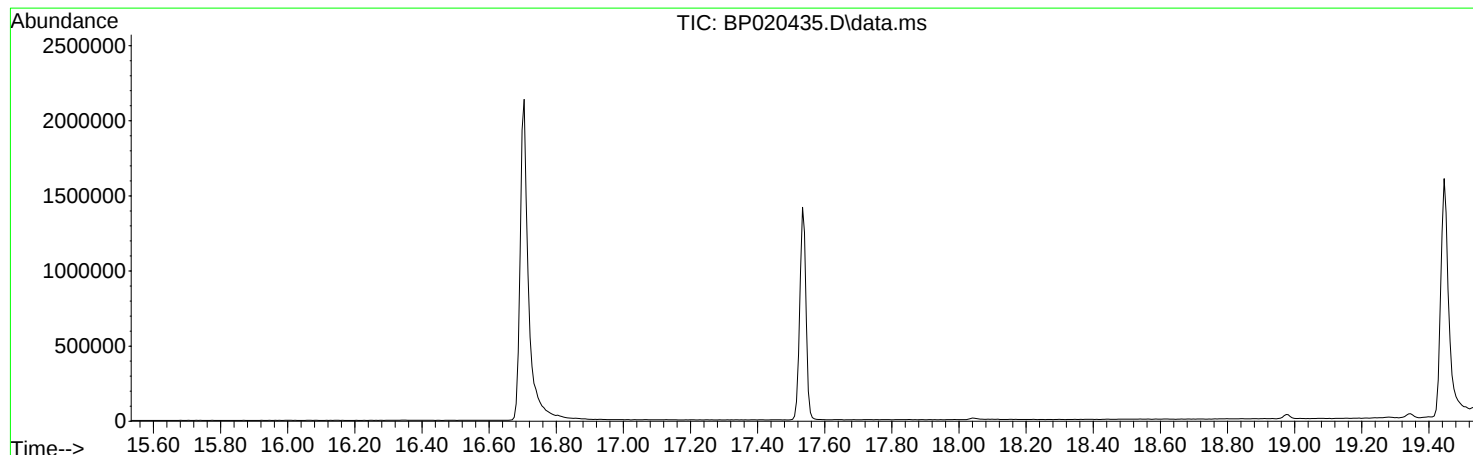




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	47304	PASS
68	69	0.00	2	0.7	373	PASS
69	198	0.00	100	37.4	51343	PASS
70	69	0.00	2	0.6	285	PASS
127	198	10	80	42.3	58156	PASS
197	198	0.00	2	0.3	358	PASS
198	198	100	100	100.0	137461	PASS
199	198	5	9	6.5	8985	PASS
275	198	10	60	29.4	40355	PASS
365	198	1	100	3.8	5178	PASS
441	198	0.01	100	11.2	15380	PASS
442	442	100	100	100.0	97120	PASS
443	442	15	24	18.9	18338	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052224\
Data File : BP020435.D
Acq On : 22 May 2024 13:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 23 02:23:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

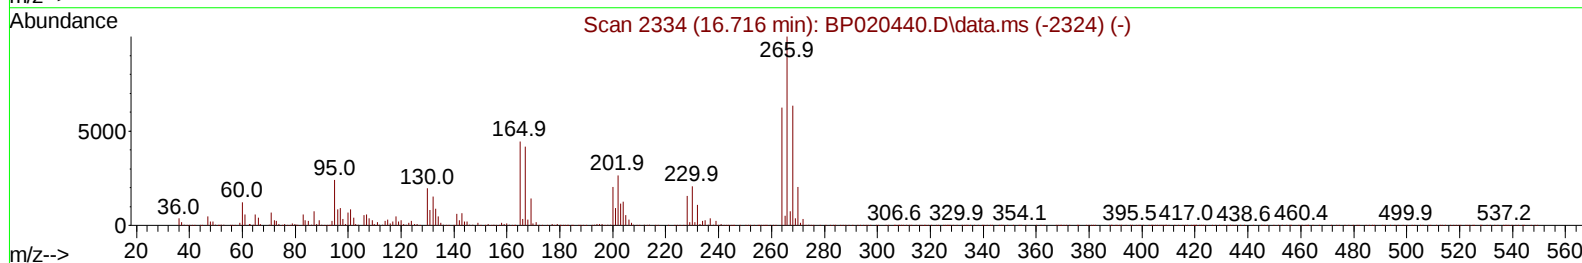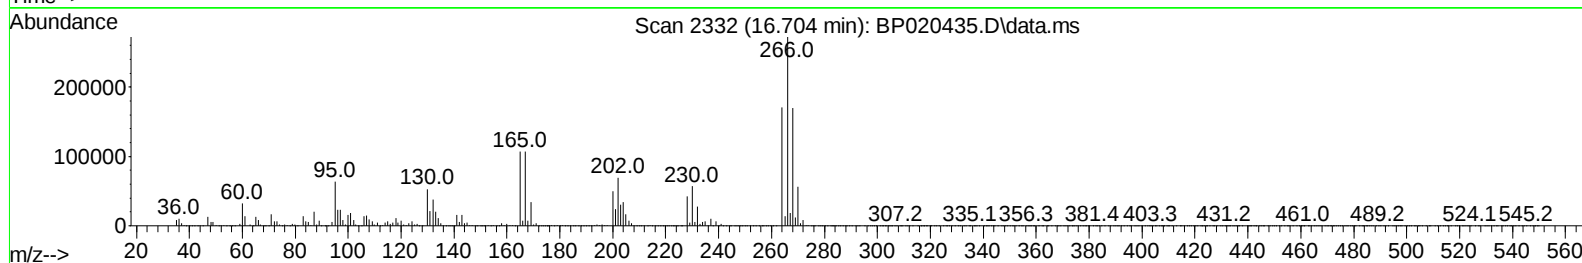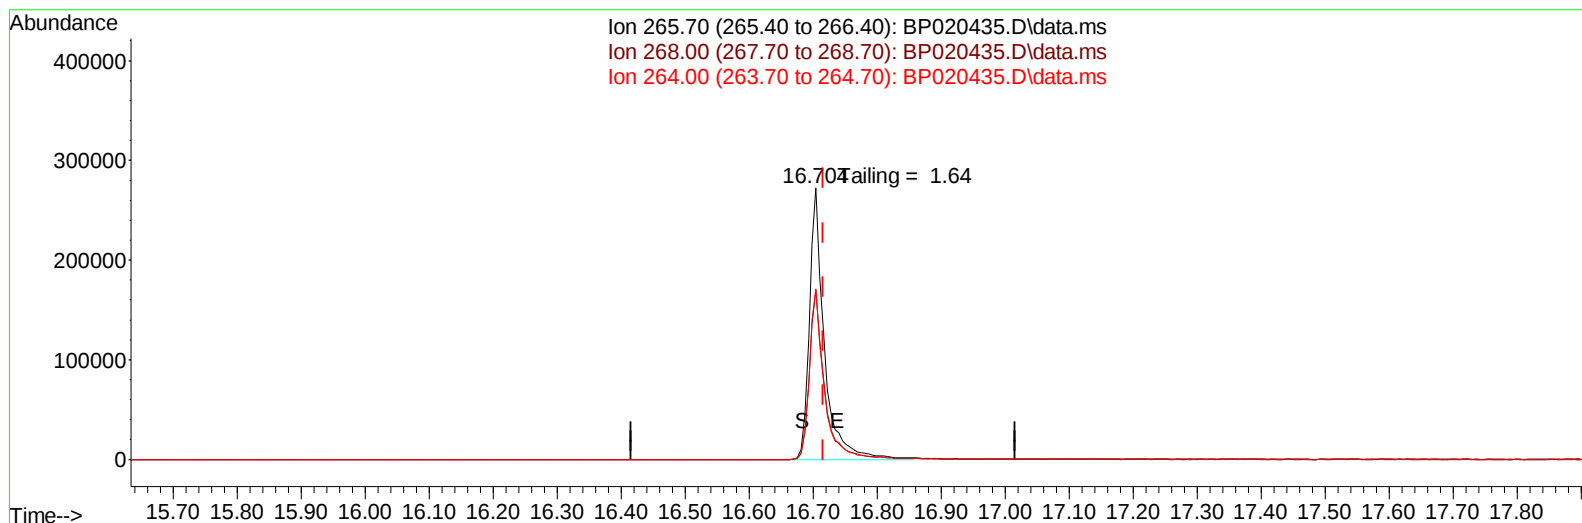

TIC: BP020435.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.012) 2966197.22 ng




response 448378

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	62.36
264.00	62.40	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052224\
Data File : BP020435.D
Acq On : 22 May 2024 13:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 23 02:23:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 02:14:59 2024
Response via : Initial Calibration

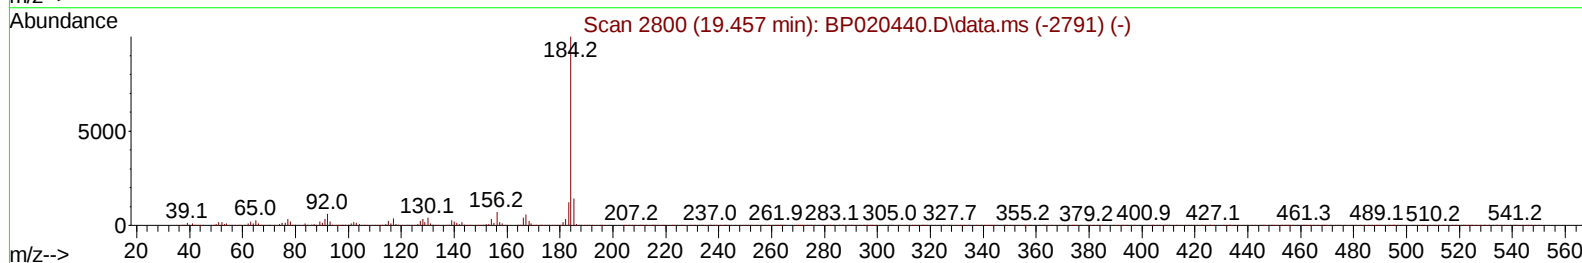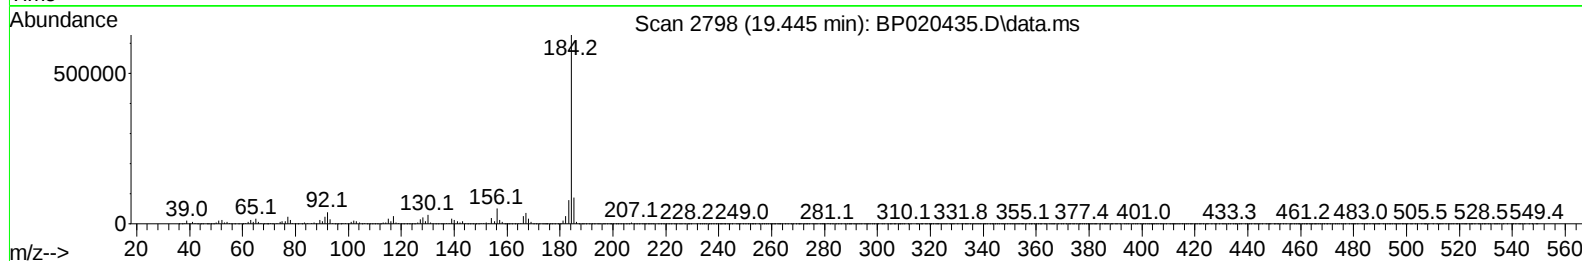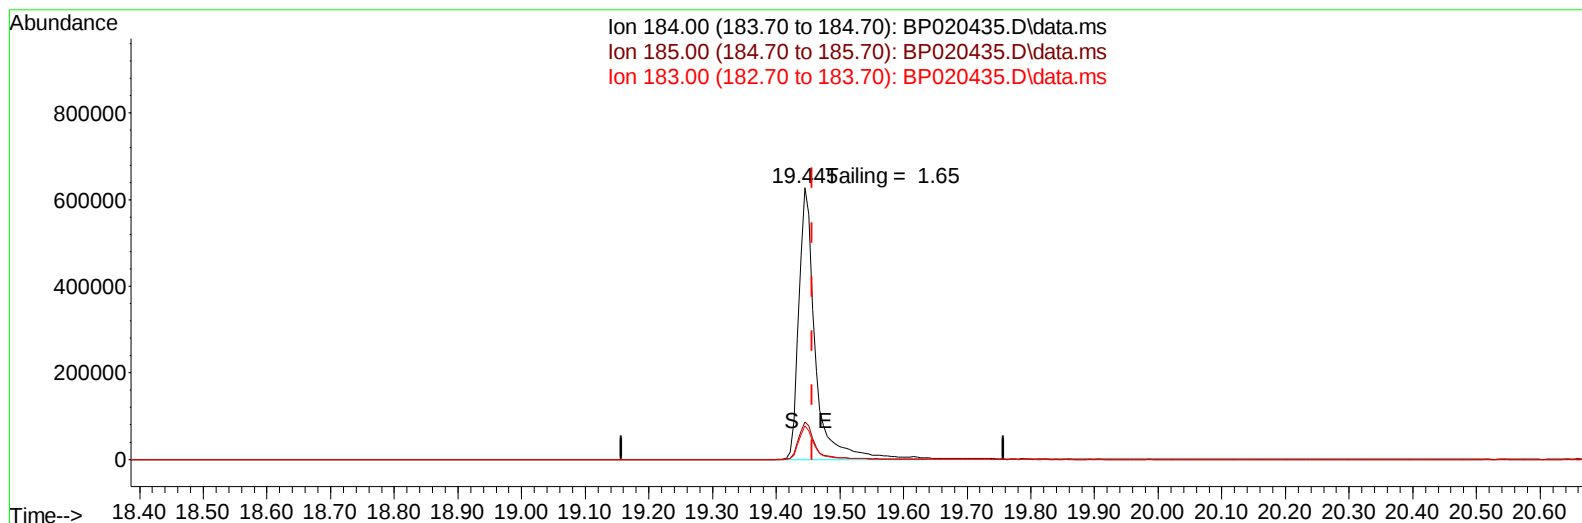

TIC: BP020435.D\data.ms

(77) Benzidine

19.445min (-0.012) 3139472.16 ng

response 1142027

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.89
183.00	12.20	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/22/2024	BNA_P	<u>BP020435.D</u>
Compound Name	Response	Retention Time
DDT	570084	20.727
DDD	6697	20.316
DDE	862	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7559	577643	1.31

Instrument :
BNA_P
ClientSampleId :
DFTPP