

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024764.D
 Acq On : 22 May 2025 18:24
 Operator : RC/JU
 Sample : Q2097-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:57:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.440	152	28	40.000	ng	0.18
2) Naphthalene-d8	11.910	136	52	40.000	ng	# 0.19
3) Acenaphthene-d10	15.175	164	246	40.000	ng	# 0.27
4) Phenanthrene-d10	15.339	188	48	40.000	ng	# 0.25
8) Chrysene-d12	31.450	240	60	40.000	ng	# 0.52
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.604	246	16	N.D.		
6) DDD	11.022	235	57	N.D.		
7) DDT	11.369	235	38	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024764.D
Acq On : 22 May 2025 18:24
Operator : RC/JU
Sample : Q2097-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: May 23 02:57:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

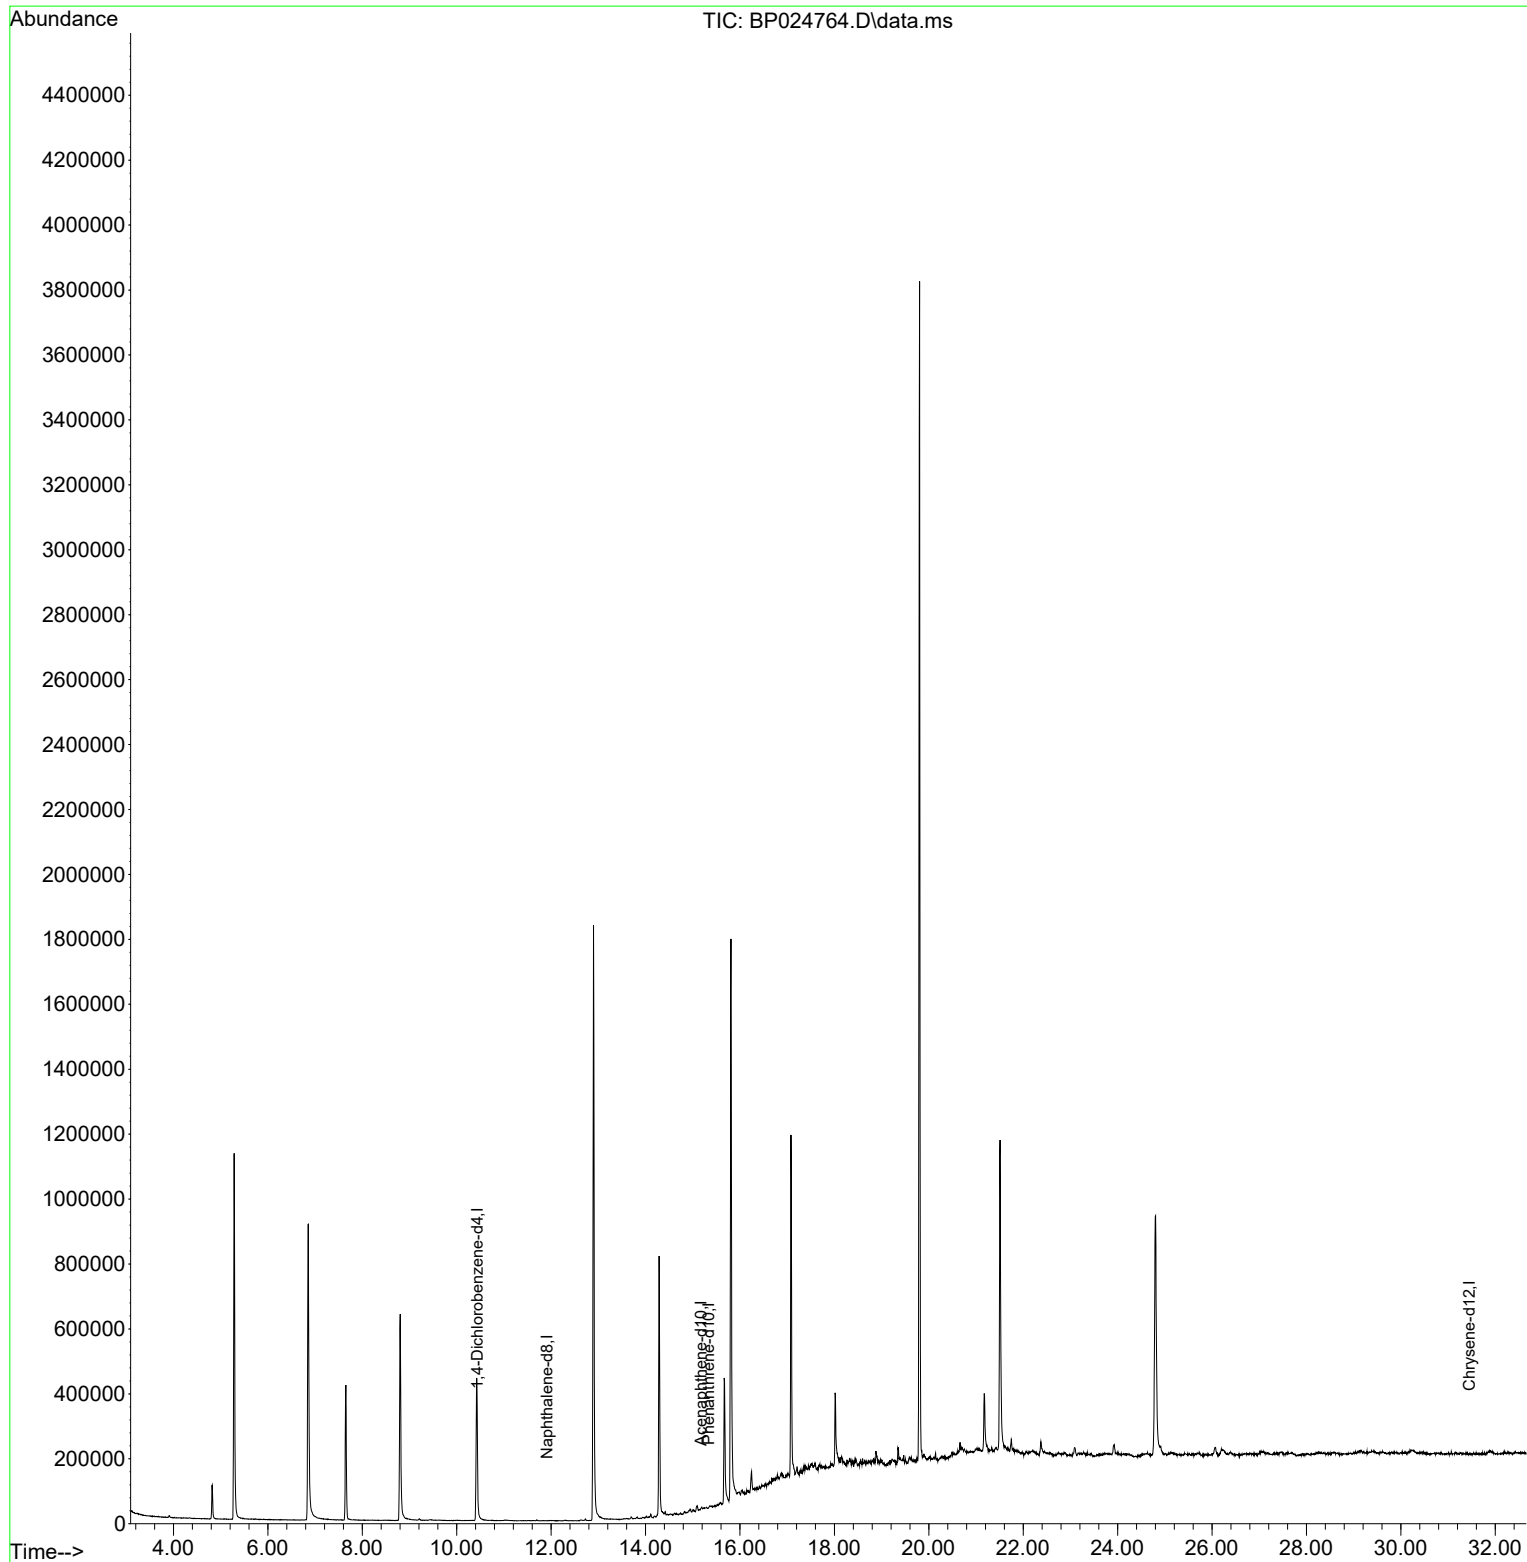



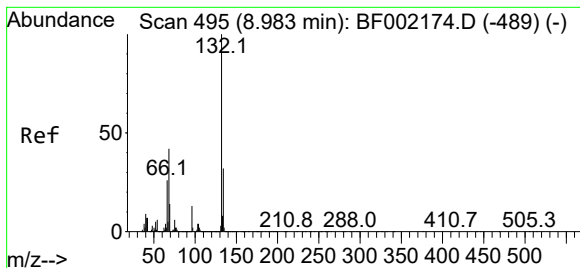


#5
DDE
Concen: Below Cal
RT: 10.604 min Scan# 11
Delta R.T. 0.165 min
Lab File: BP024764.D
Acq: 22 May 2025 18:24

Instrument :
BNA_P
ClientSampleId :



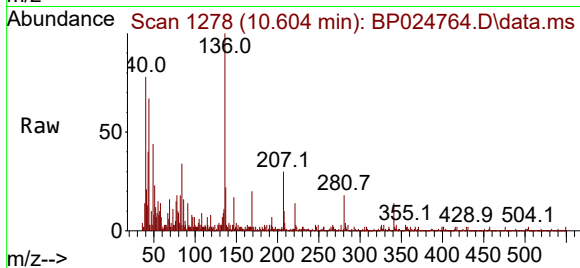



Tgt Ion:246 Resp: 16
Ion Ratio Lower Upper
246 100
248 25.0 1434.9 2152.3#
318 0.0 161.5 242.3#
176 156.3 3844.2 5766.4#

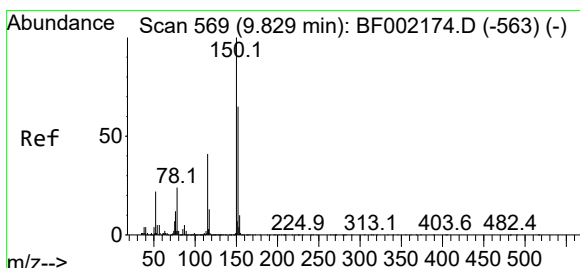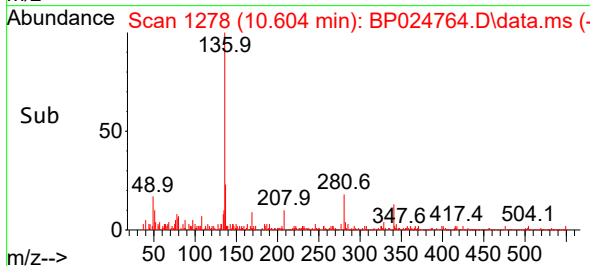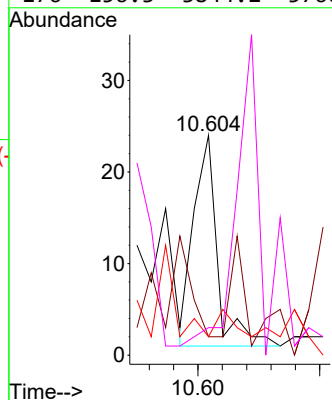

#6
DDD
Concen: Below Cal
RT: 11.022 min Scan# 1349
Delta R.T. 0.189 min
Lab File: BP024764.D
Acq: 22 May 2025 18:24


Tgt Ion:235 Resp: 57
Ion Ratio Lower Upper
235 100
237 12.3 4800.0 7200.0#
165 73.7 4800.0 7200.0#

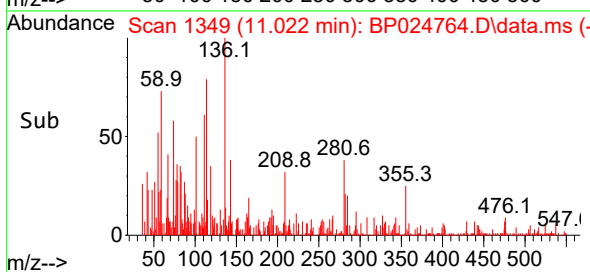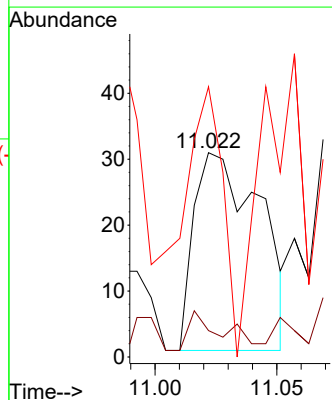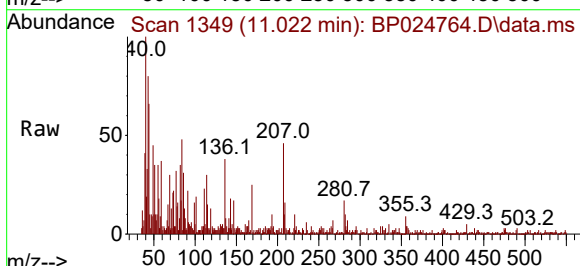

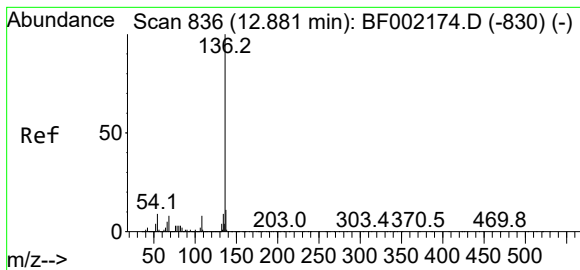

#7
DDT
Concen: Below Cal
RT: 11.369 min Scan# 14
Delta R.T. 0.177 min
Lab File: BP024764.D
Acq: 22 May 2025 18:24

Instrument :
BNA_P
ClientSampleId :

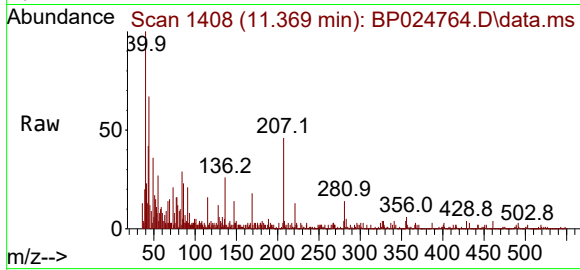

Tgt Ion: 235 Resp: 38
Ion Ratio Lower Upper
235 100
237 0.0 0.0 0.0
165 36.8 0.2 0.2#

