

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024765.D
 Acq On : 22 May 2025 19:04
 Operator : RC/JU
 Sample : Q2097-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:57:52 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	9.852	152	11	40.000	ng	-0.41
2) Naphthalene-d8	11.252	136	109	40.000	ng	#-0.47
3) Acenaphthene-d10	14.287	164	228808	40.000	ng	#-0.62
4) Phenanthrene-d10	14.445	188	14	40.000	ng	#-0.65
8) Chrysene-d12	29.574	240	97	40.000	ng	#-1.35
9) Perylene-d12	32.621	264	80	40.000	ng	#-1.93
Target Compounds						Qvalue
5) DDE	9.999	246	5	N.D.		
6) DDD	10.375	235	16	N.D.		
7) DDT	10.728	235	26	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024765.D
Acq On : 22 May 2025 19:04
Operator : RC/JU
Sample : Q2097-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: May 23 02:57:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

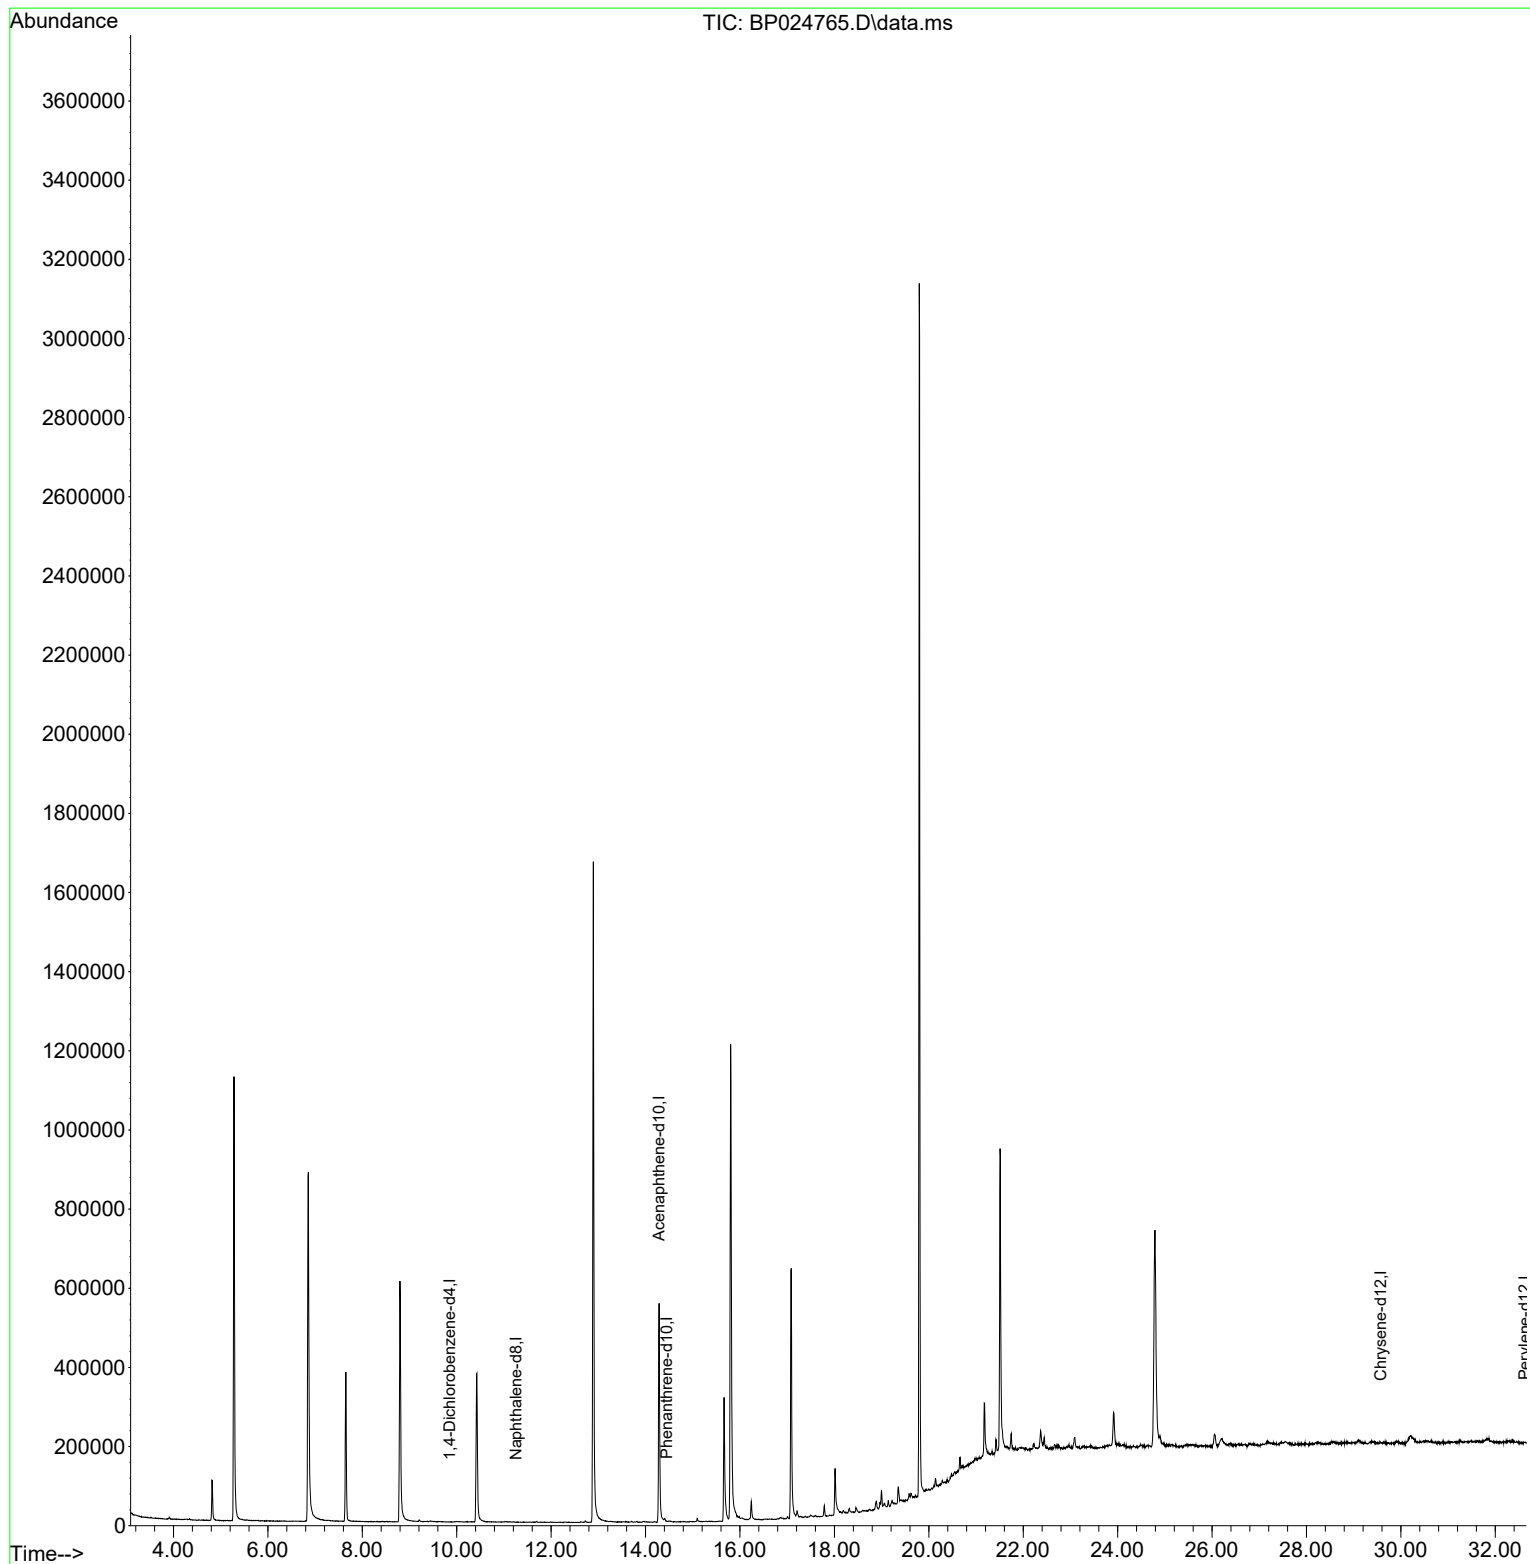



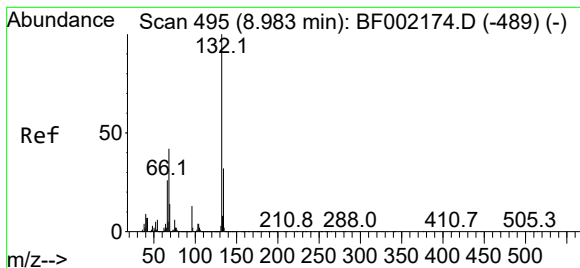


#5
DDE
Concen: Below Cal
RT: 9.999 min Scan# 1175
Delta R.T. -0.440 min
Lab File: BP024765.D
Acq: 22 May 2025 19:04

Instrument :
BNA_P
ClientSampleId :



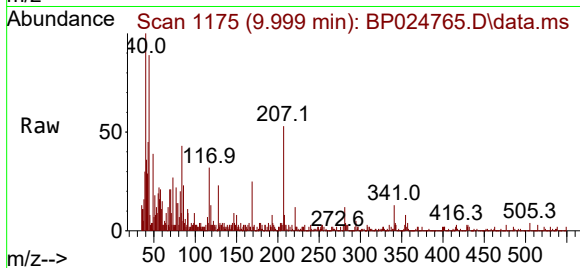



Tgt Ion:246 Resp: 5
Ion Ratio Lower Upper
246 100
248 260.0 1434.9 2152.3#
318 80.0 161.5 242.3#
176 0.0 3844.2 5766.4#

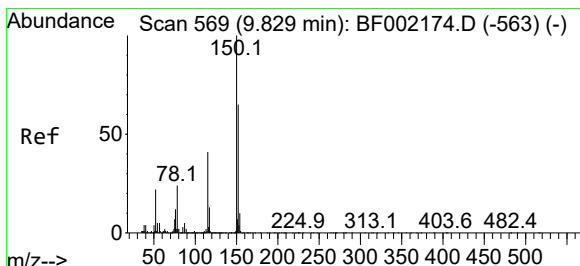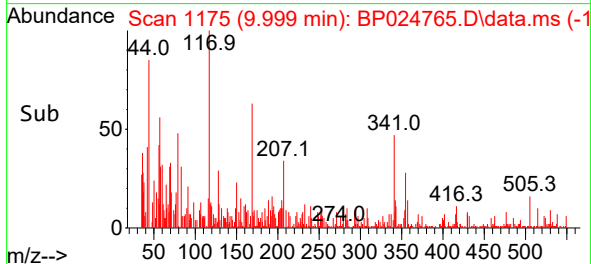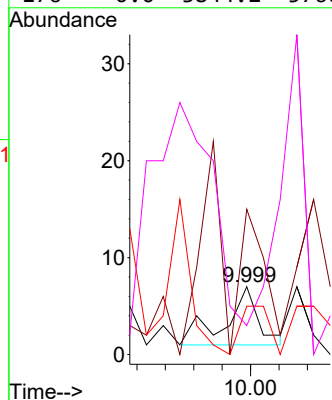

#6
DDD
Concen: Below Cal
RT: 10.375 min Scan# 1239
Delta R.T. -0.458 min
Lab File: BP024765.D
Acq: 22 May 2025 19:04


Tgt Ion:235 Resp: 16
Ion Ratio Lower Upper
235 100
237 0.0 4800.0 7200.0#
165 0.0 4800.0 7200.0#

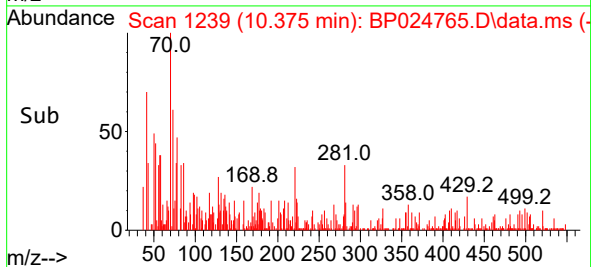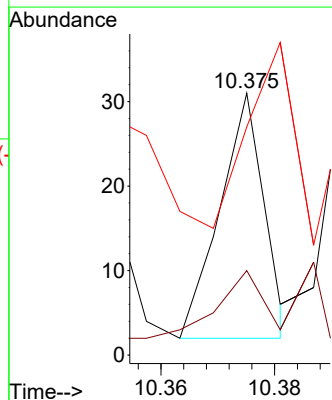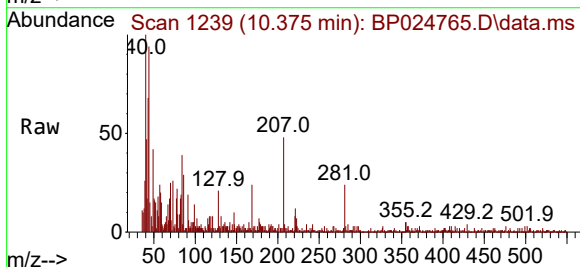

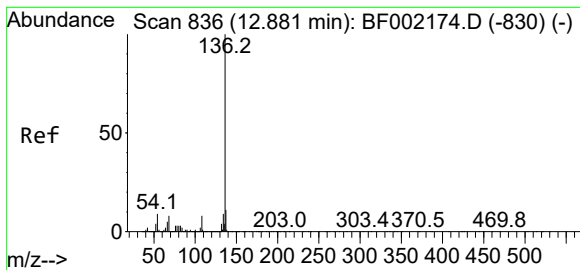

#7
DDT
Concen: Below Cal
RT: 10.728 min Scan# 11
Delta R.T. -0.464 min
Lab File: BP024765.D
Acq: 22 May 2025 19:04

Instrument :
BNA_P
ClientSampleId :

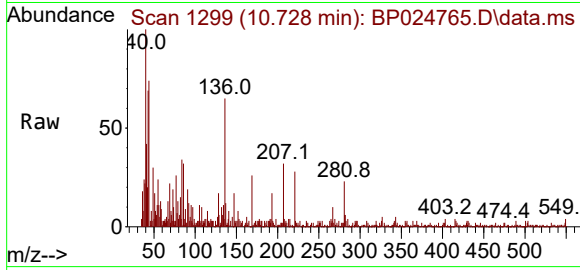

Tgt Ion: 235 Resp: 26
Ion Ratio Lower Upper
235 100
237 57.7 0.0 0.0#
165 30.8 0.2 0.2#

