

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024766.D
 Acq On : 22 May 2025 19:45
 Operator : RC/JU
 Sample : Q2097-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:57:58 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.263	152	12	40.000	ng	# 0.00
2) Naphthalene-d8	11.722	136	75	40.000	ng	# 0.00
3) Acenaphthene-d10	14.916	164	58	40.000	ng	# 0.00
4) Phenanthrene-d10	15.098	188	52	40.000	ng	# 0.00
8) Chrysene-d12	30.950	240	87	40.000	ng	# 0.02
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.452	246	3	N.D.		
6) DDD	10.828	235	34	N.D.		
7) DDT	11.204	235	6	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024766.D
Acq On : 22 May 2025 19:45
Operator : RC/JU
Sample : Q2097-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:57:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




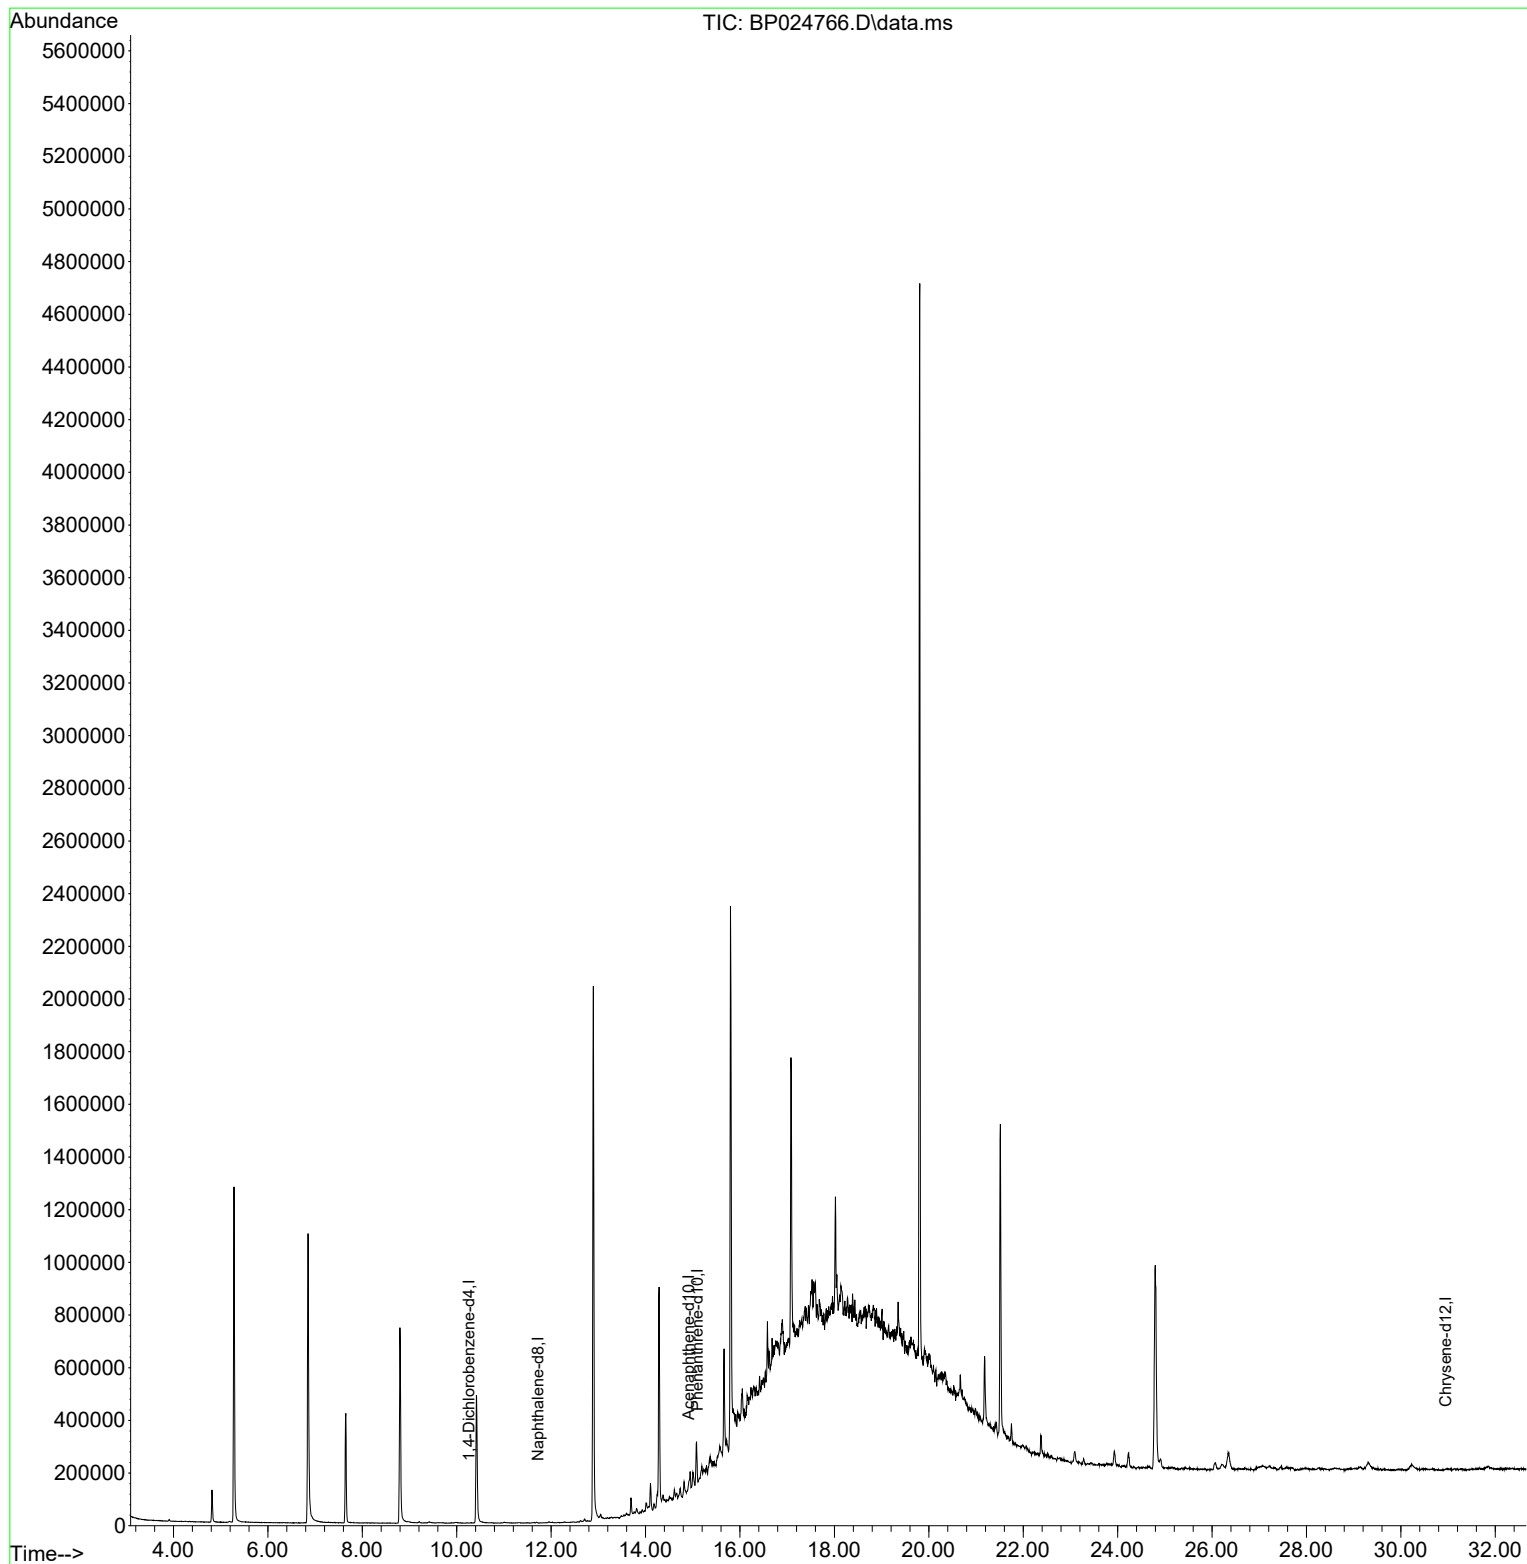


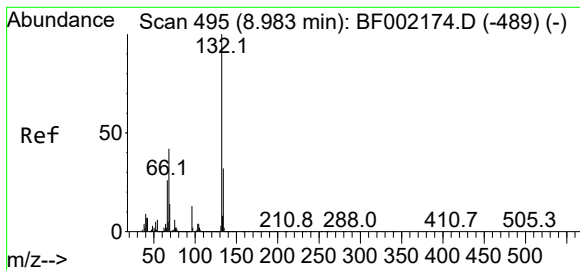

#5
DDE
Concen: Below Cal
RT: 10.452 min Scan# 11
Delta R.T. 0.012 min
Lab File: BP024766.D
Acq: 22 May 2025 19:45




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 3
Ion Ratio Lower Upper
246 100
248 0.0 1434.9 2152.3#
318 233.3 161.5 242.3
176 233.3 3844.2 5766.4#

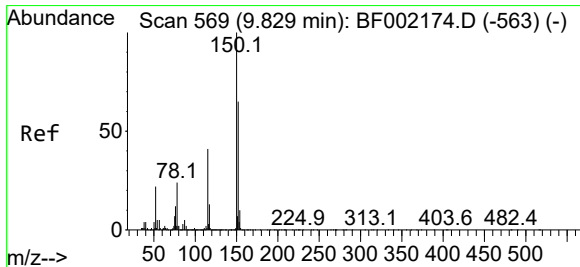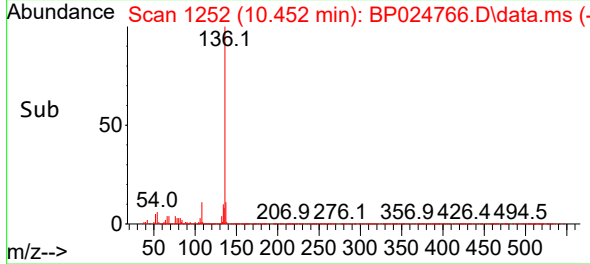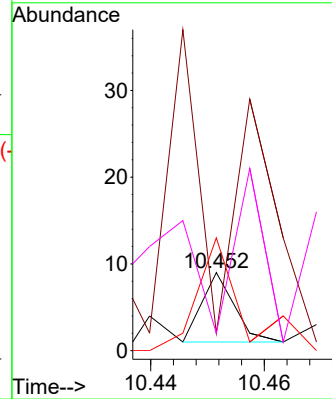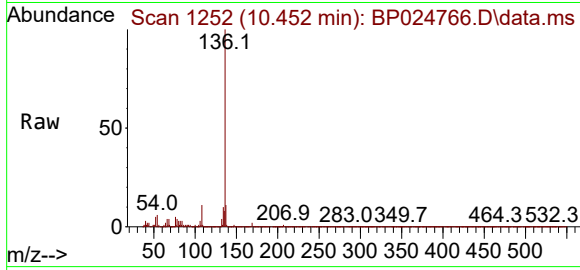

#6
DDD
Concen: Below Cal
RT: 10.828 min Scan# 1316
Delta R.T. -0.005 min
Lab File: BP024766.D
Acq: 22 May 2025 19:45


Tgt Ion:235 Resp: 34
Ion Ratio Lower Upper
235 100
237 14.7 4800.0 7200.0#
165 58.8 4800.0 7200.0#

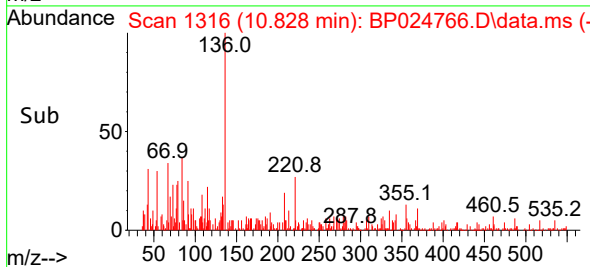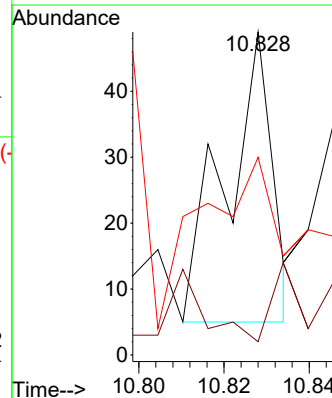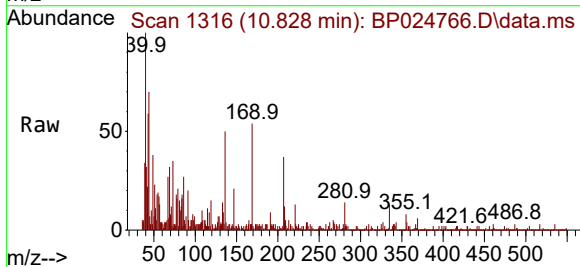

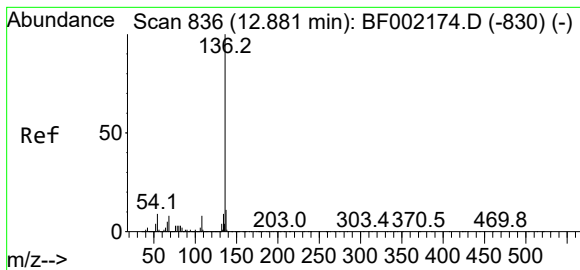

#7
DDT
Concen: Below Cal
RT: 11.204 min Scan# 11
Delta R.T. 0.012 min
Lab File: BP024766.D
Acq: 22 May 2025 19:45

Instrument :
BNA_P
ClientSampleId :

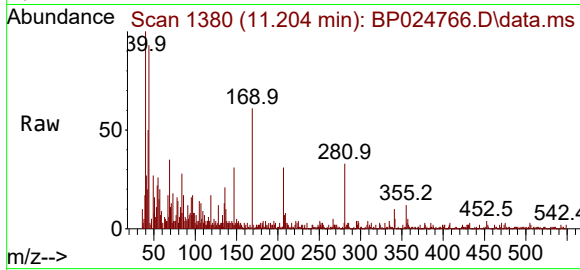

Tgt Ion: 235 Resp: 6
Ion Ratio Lower Upper
235 100
237 233.3 0.0 0.0#
165 0.0 0.2 0.2#

