

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024767.D
 Acq On : 22 May 2025 20:26
 Operator : RC/JU
 Sample : Q2088-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:58:04 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.281	152	81	40.000	ng	# 0.02
2) Naphthalene-d8	11.740	136	99	40.000	ng	# 0.02
3) Acenaphthene-d10	14.922	164	167	40.000	ng	# 0.01
4) Phenanthrene-d10	15.116	188	31	40.000	ng	# 0.02
8) Chrysene-d12	30.980	240	54	40.000	ng	# 0.05
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.463	246	5	N.D.		
6) DDD	10.840	235	5	N.D.		
7) DDT	11.222	235	19	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024767.D
Acq On : 22 May 2025 20:26
Operator : RC/JU
Sample : Q2088-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




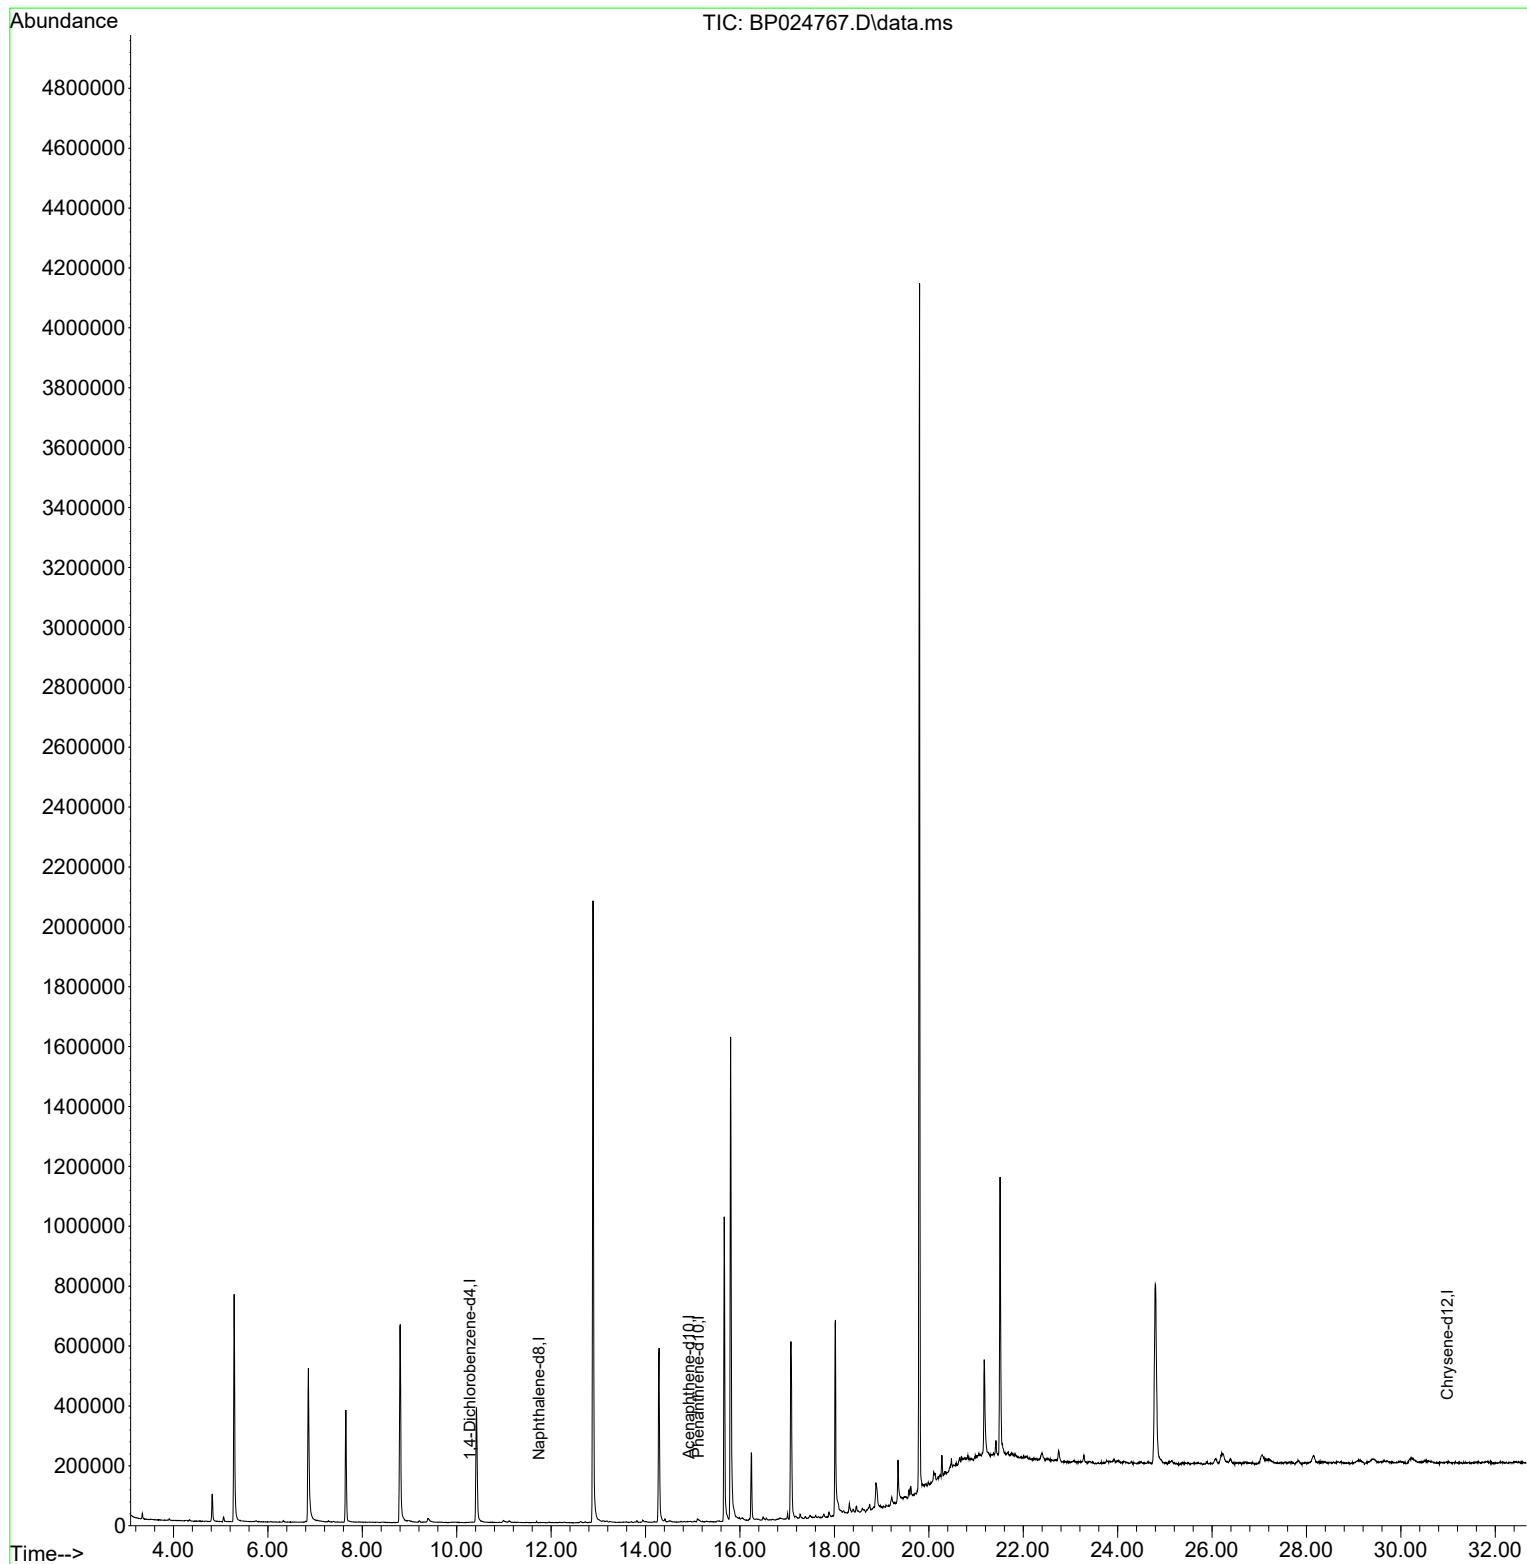


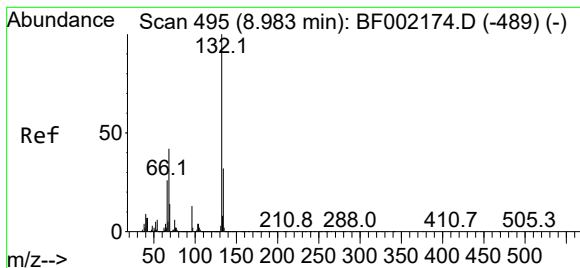

#5
DDE
Concen: Below Cal
RT: 10.463 min Scan# 11
Delta R.T. 0.024 min
Lab File: BP024767.D
Acq: 22 May 2025 20:26




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 5
Ion Ratio Lower Upper
246 100
248 280.0 1434.9 2152.3#
318 100.0 161.5 242.3#
176 640.0 3844.2 5766.4#

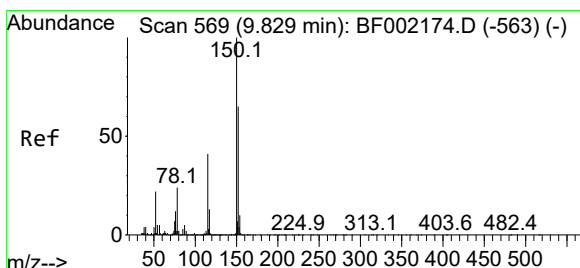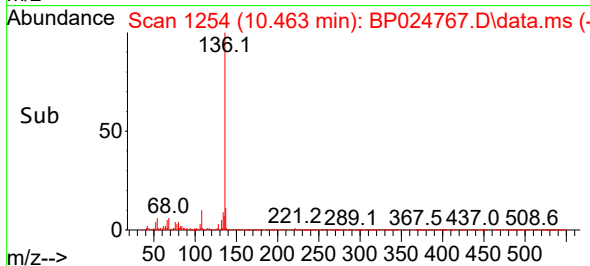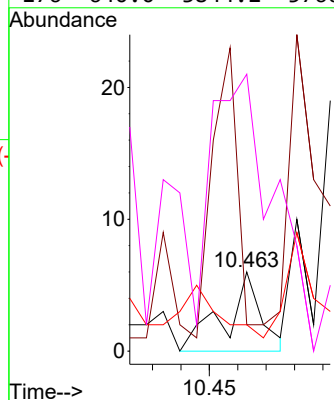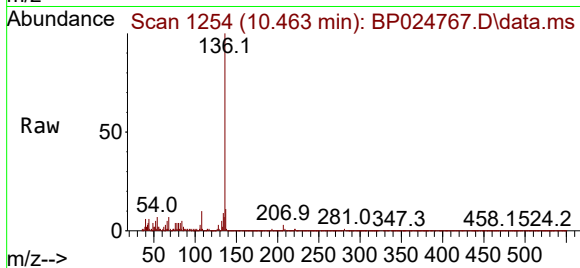

#6
DDD
Concen: Below Cal
RT: 10.840 min Scan# 1318
Delta R.T. 0.006 min
Lab File: BP024767.D
Acq: 22 May 2025 20:26


Tgt Ion:235 Resp: 5
Ion Ratio Lower Upper
235 100
237 640.0 4800.0 7200.0#
165 440.0 4800.0 7200.0#

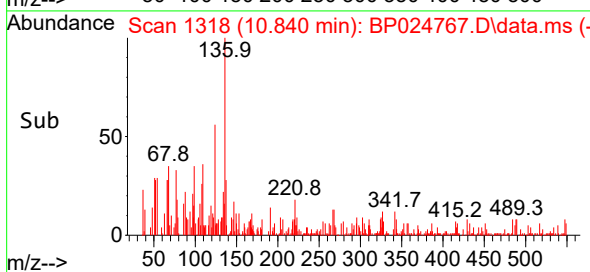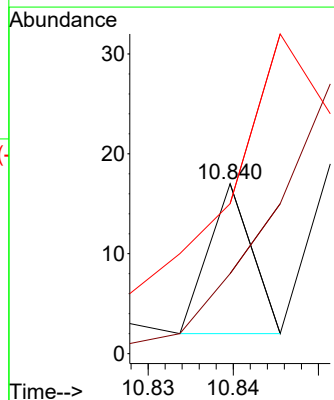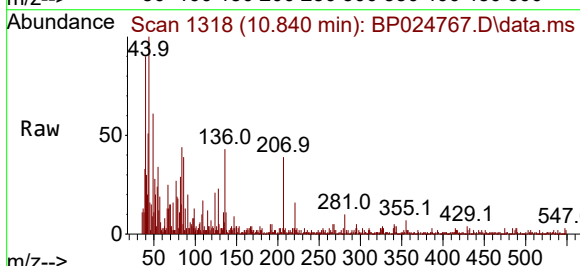

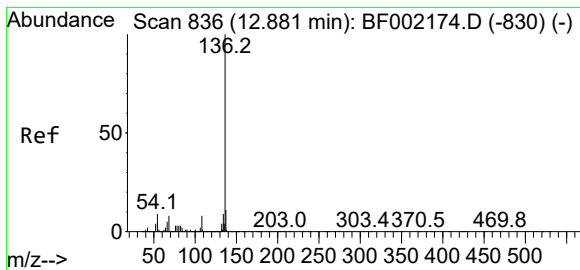

#7
DDT
Concen: Below Cal
RT: 11.222 min Scan# 11
Delta R.T. 0.030 min
Lab File: BP024767.D
Acq: 22 May 2025 20:26

Instrument :
BNA_P
ClientSampleId :

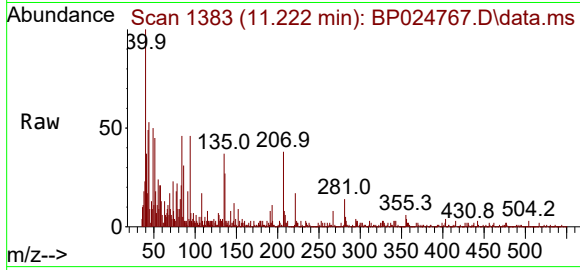

Tgt Ion: 235 Resp: 19
Ion Ratio Lower Upper
235 100
237 63.2 0.0 0.0#
165 321.1 0.2 0.2#

