

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024768.D
Acq On : 22 May 2025 21:07
Operator : RC/JU
Sample : Q23093-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.246	152	52	40.000	ng	#-0.02
2) Naphthalene-d8	11.693	136	126	40.000	ng	#-0.03
3) Acenaphthene-d10	14.798	164	10867	40.000	ng	#-0.11
4) Phenanthrene-d10	14.963	188	260	40.000	ng	#-0.13
8) Chrysene-d12	30.686	240	74	40.000	ng	#-0.24
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.328	246	10	N.D.		
6) DDD	10.740	235	14	N.D.		
7) DDT	11.093	235	4	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024768.D
Acq On : 22 May 2025 21:07
Operator : RC/JU
Sample : Q23093-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




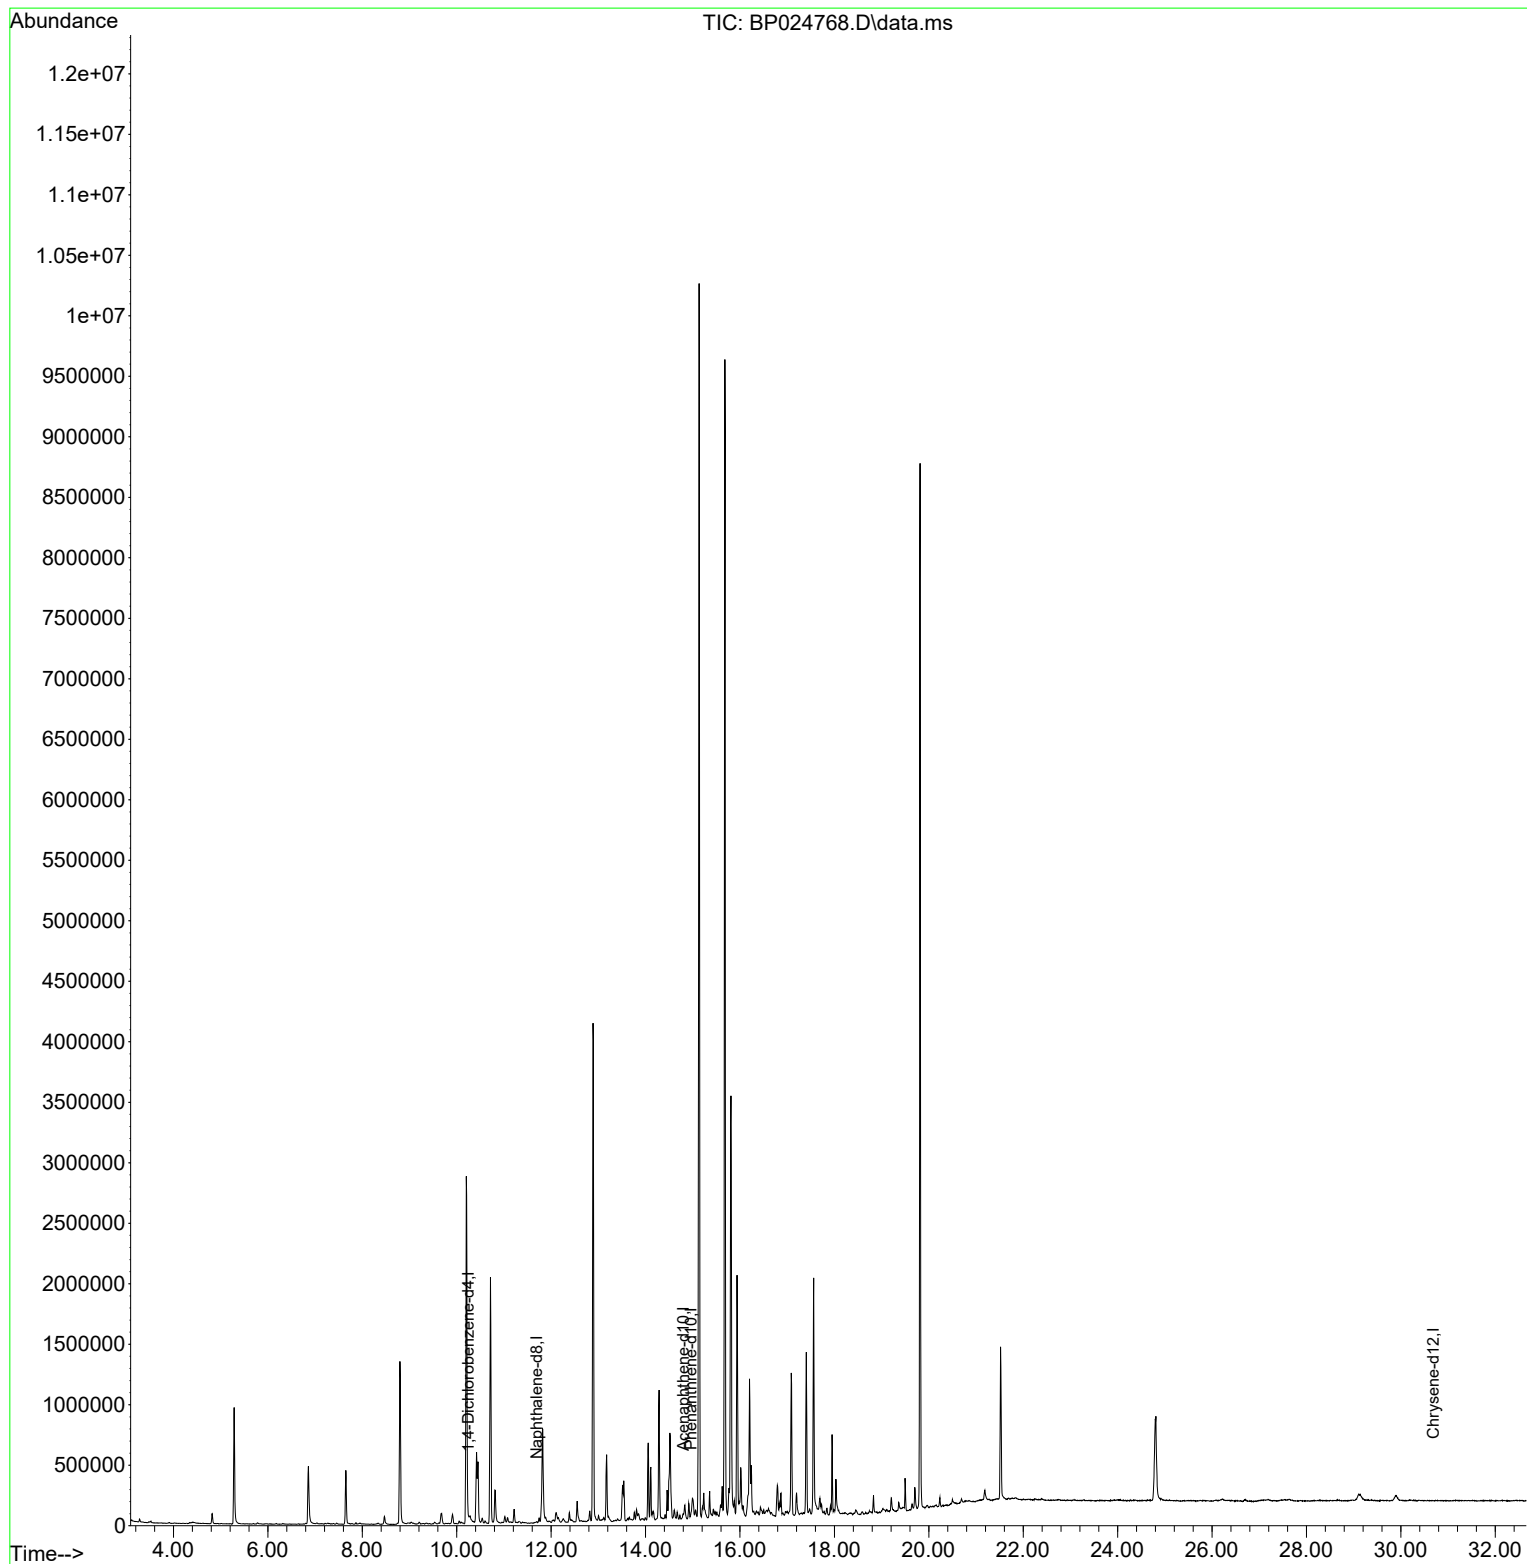


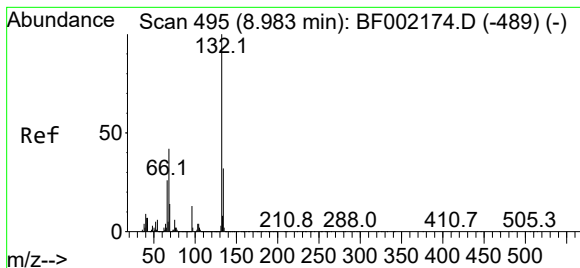

#5
DDE
Concen: Below Cal
RT: 10.328 min Scan# 11
Delta R.T. -0.111 min
Lab File: BP024768.D
Acq: 22 May 2025 21:07




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 10
Ion Ratio Lower Upper
246 100
248 60.0 1434.9 2152.3#
318 50.0 161.5 242.3#
176 50.0 3844.2 5766.4#

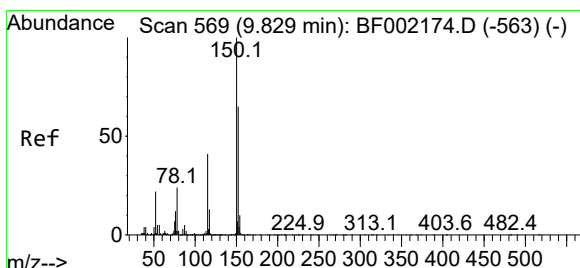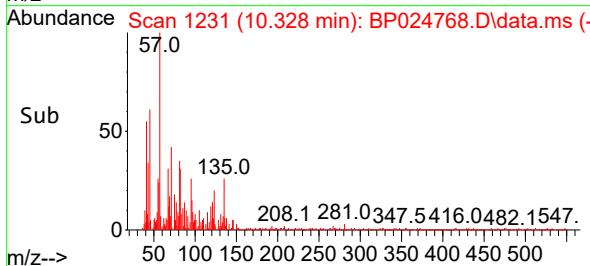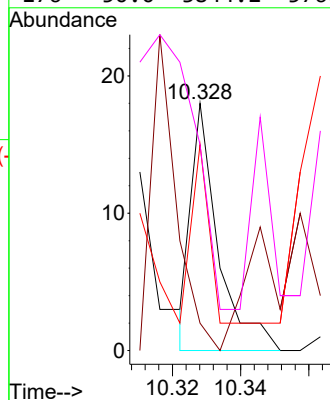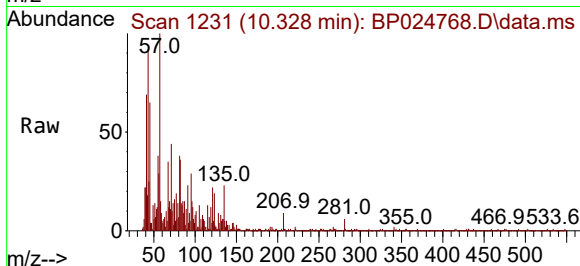

#6
DDD
Concen: Below Cal
RT: 10.740 min Scan# 1301
Delta R.T. -0.093 min
Lab File: BP024768.D
Acq: 22 May 2025 21:07


Tgt Ion:235 Resp: 14
Ion Ratio Lower Upper
235 100
237 50.0 4800.0 7200.0#
165 414.3 4800.0 7200.0#

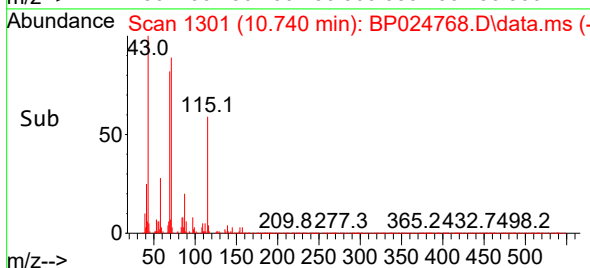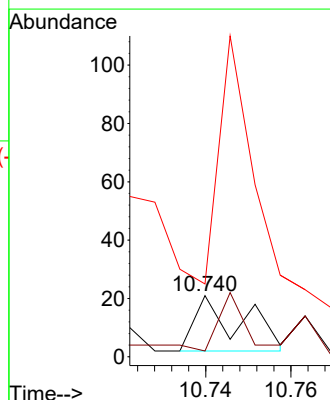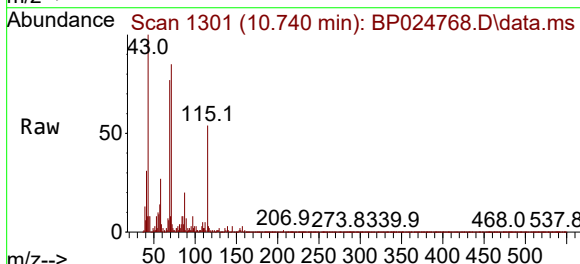

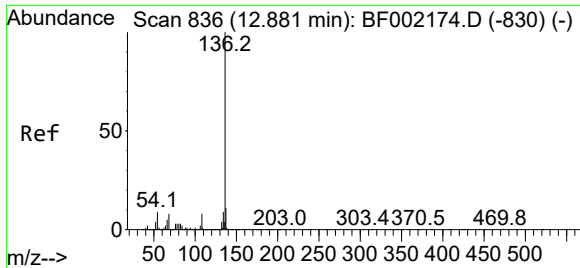

#7
DDT
Concen: Below Cal
RT: 11.093 min Scan# 11
Delta R.T. -0.099 min
Lab File: BP024768.D
Acq: 22 May 2025 21:07

Instrument :
BNA_P
ClientSampleId :

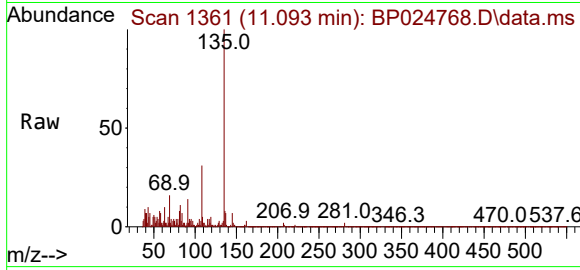

Tgt Ion:235 Resp: 4
Ion Ratio Lower Upper
235 100
237 0.0 0.0 0.0
165 675.0 0.2 0.2#

