

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024770.D
 Acq On : 22 May 2025 23:09
 Operator : RC/JU
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:58:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.251	152	17	40.000	ng	#-0.01
2) Naphthalene-d8	11.710	136	8	40.000	ng	#-0.01
3) Acenaphthene-d10	15.345	164	86467	40.000	ng	# 0.44
4) Phenanthrene-d10	15.545	188	22	40.000	ng	# 0.45
8) Chrysene-d12	31.868	240	70	40.000	ng	# 0.94
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.775	246	6	N.D.		
6) DDD	11.163	235	8	N.D.		
7) DDT	11.545	235	8	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024770.D
Acq On : 22 May 2025 23:09
Operator : RC/JU
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




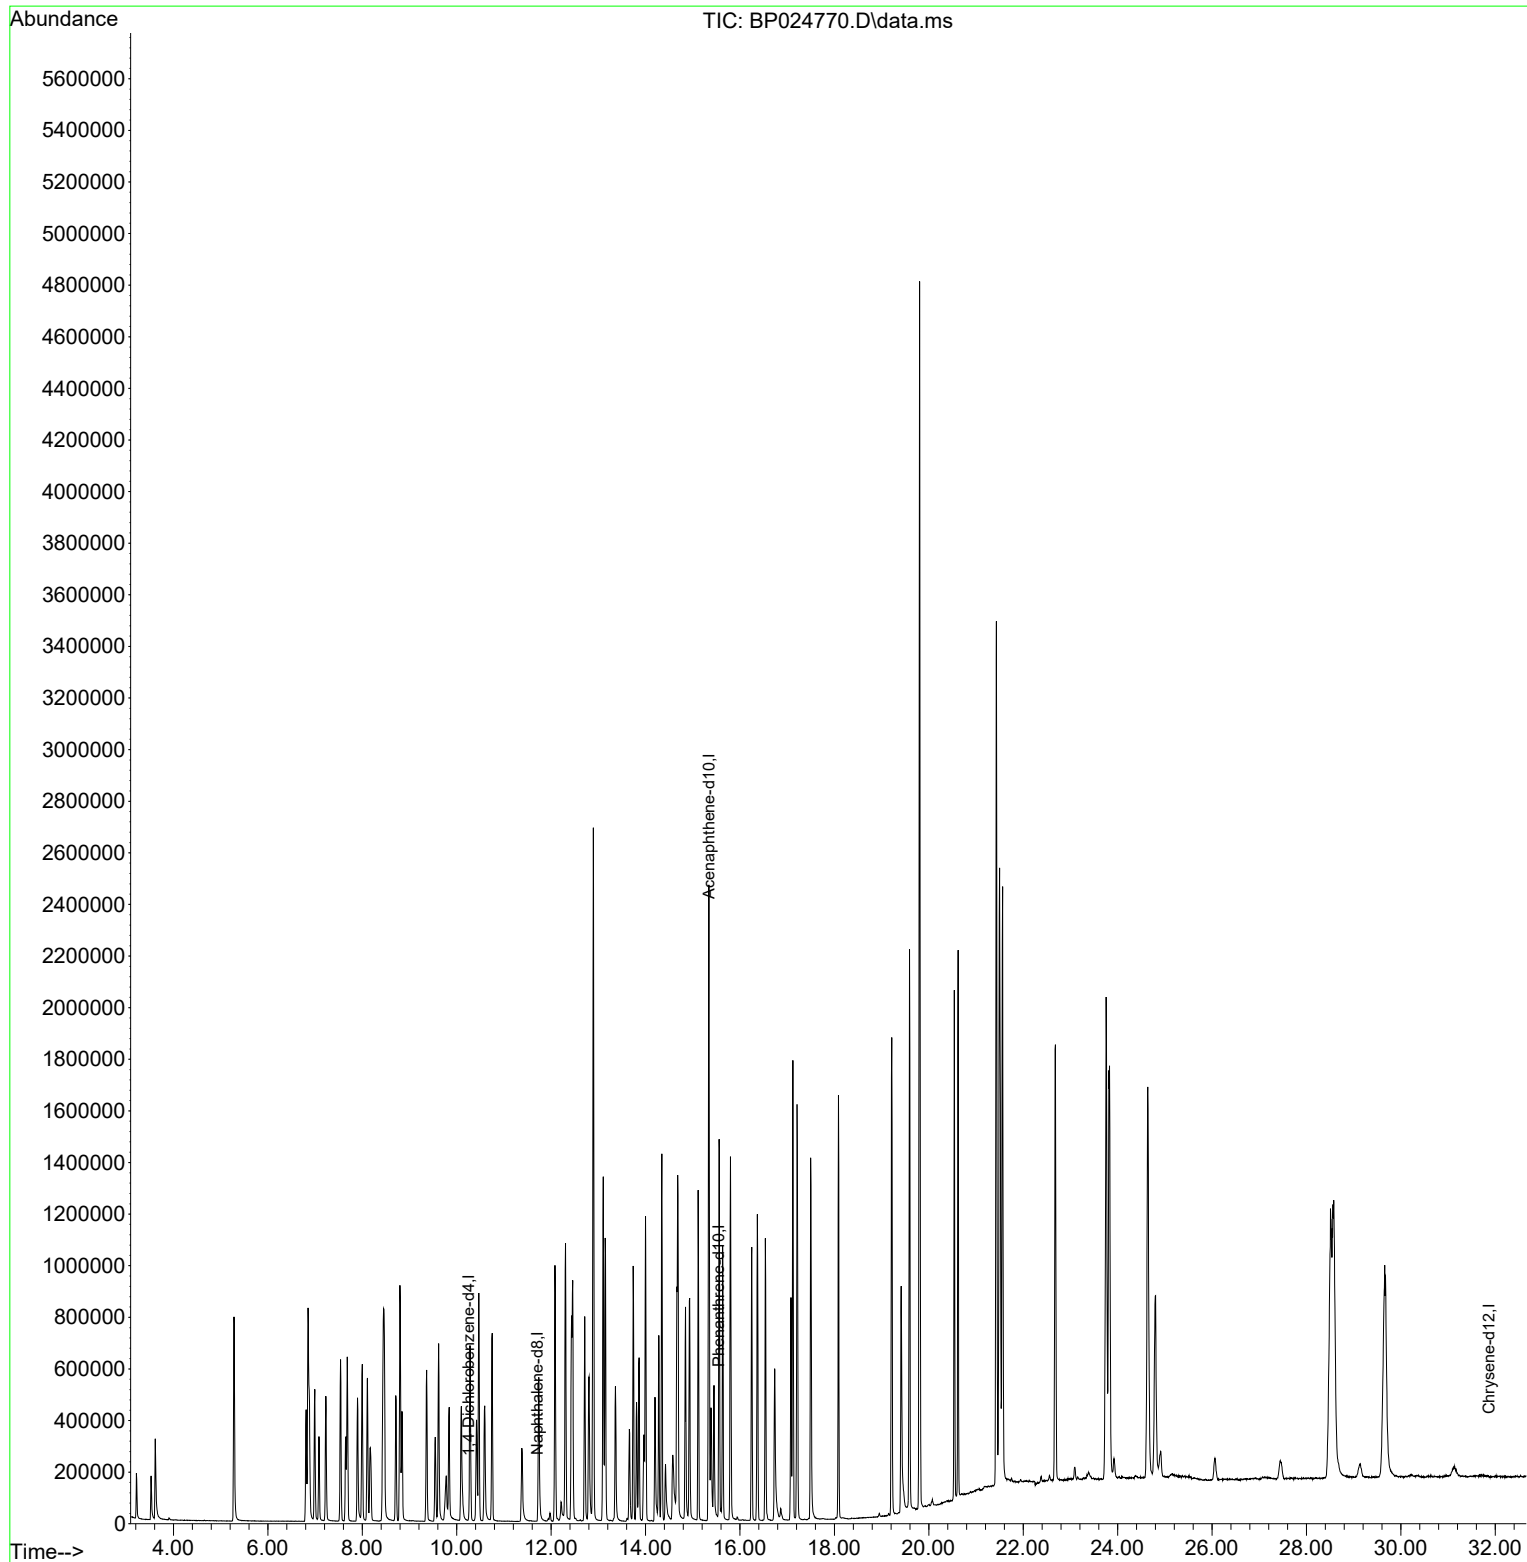


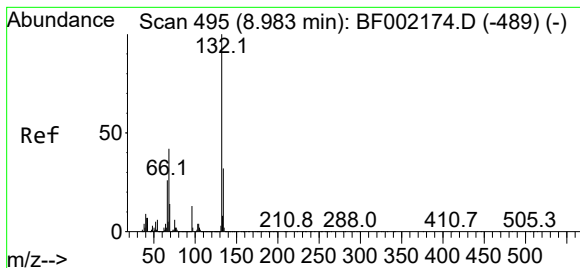

#5
DDE
Concen: Below Cal
RT: 10.775 min Scan# 11
Delta R.T. 0.336 min
Lab File: BP024770.D
Acq: 22 May 2025 23:09




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 6
Ion Ratio Lower Upper
246 100
248 183.3 1434.9 2152.3#
318 66.7 161.5 242.3#
176 183.3 3844.2 5766.4#

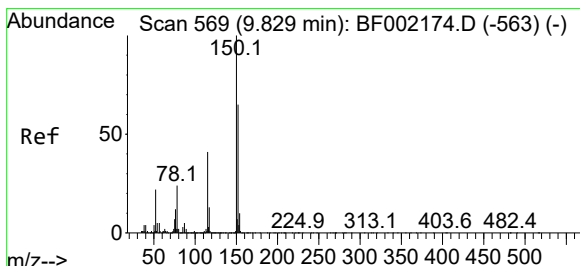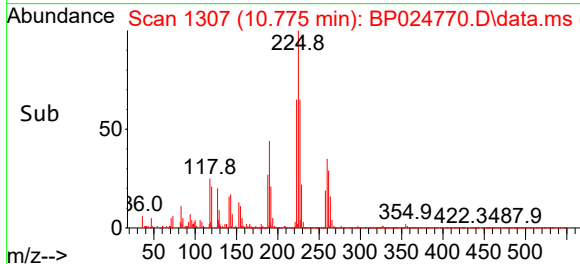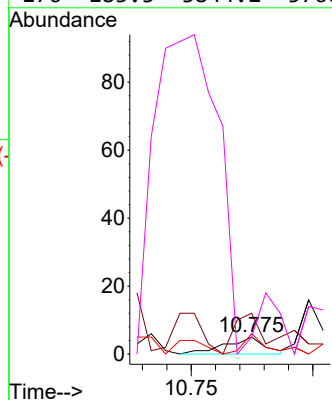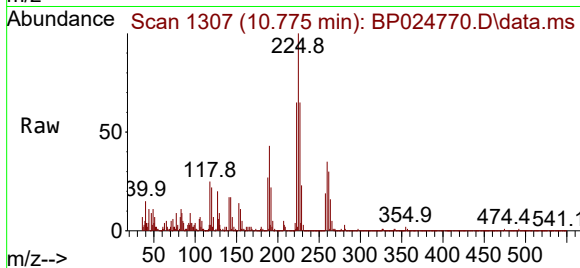

#6
DDD
Concen: Below Cal
RT: 11.163 min Scan# 1373
Delta R.T. 0.330 min
Lab File: BP024770.D
Acq: 22 May 2025 23:09


Tgt Ion:235 Resp: 8
Ion Ratio Lower Upper
235 100
237 237.5 4800.0 7200.0#
165 200.0 4800.0 7200.0#

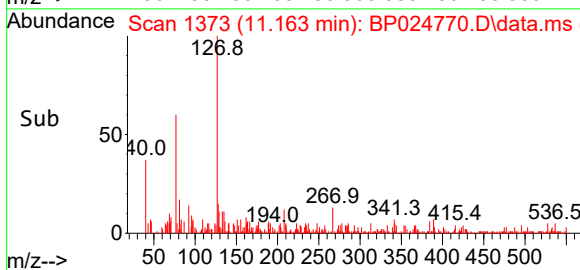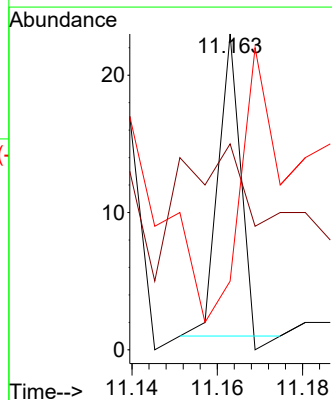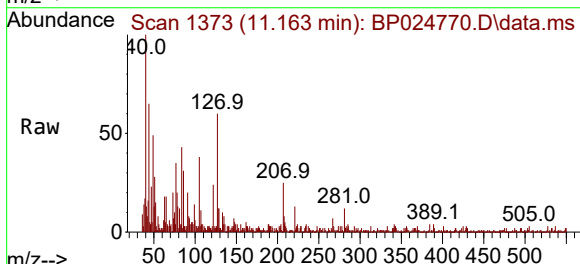

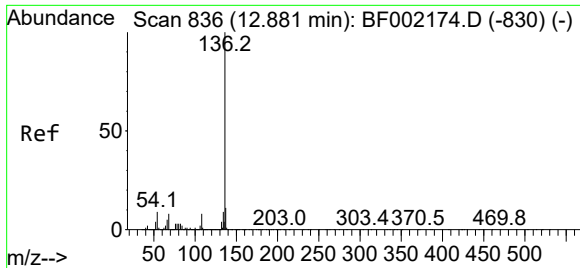

#7
DDT
Concen: Below Cal
RT: 11.545 min Scan# 14
Delta R.T. 0.353 min
Lab File: BP024770.D
Acq: 22 May 2025 23:09

Instrument :
BNA_P
ClientSampleId :

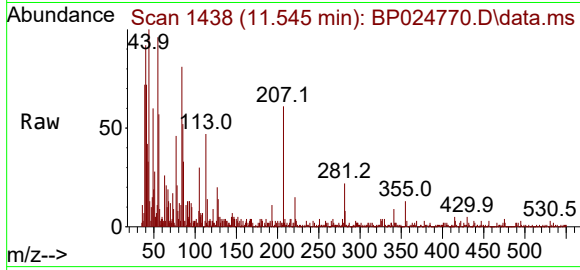

Tgt Ion:235 Resp: 8
Ion Ratio Lower Upper
235 100
237 187.5 0.0 0.0#
165 125.0 0.2 0.2#

