

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024771.D
 Acq On : 22 May 2025 23:50
 Operator : RC/JU
 Sample : PB168092TB
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:58:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.428	152	36	40.000	ng	0.17
2) Naphthalene-d8	11.892	136	21	40.000	ng	# 0.17
3) Acenaphthene-d10	15.151	164	28	40.000	ng	# 0.24
4) Phenanthrene-d10	15.328	188	5	40.000	ng	# 0.24
8) Chrysene-d12	31.433	240	27	40.000	ng	# 0.51
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.593	246	8	3.417	ng	# 1
6) DDD	11.010	235	6	N.D.		
7) DDT	11.381	235	27	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024771.D
Acq On : 22 May 2025 23:50
Operator : RC/JU
Sample : PB168092TB
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




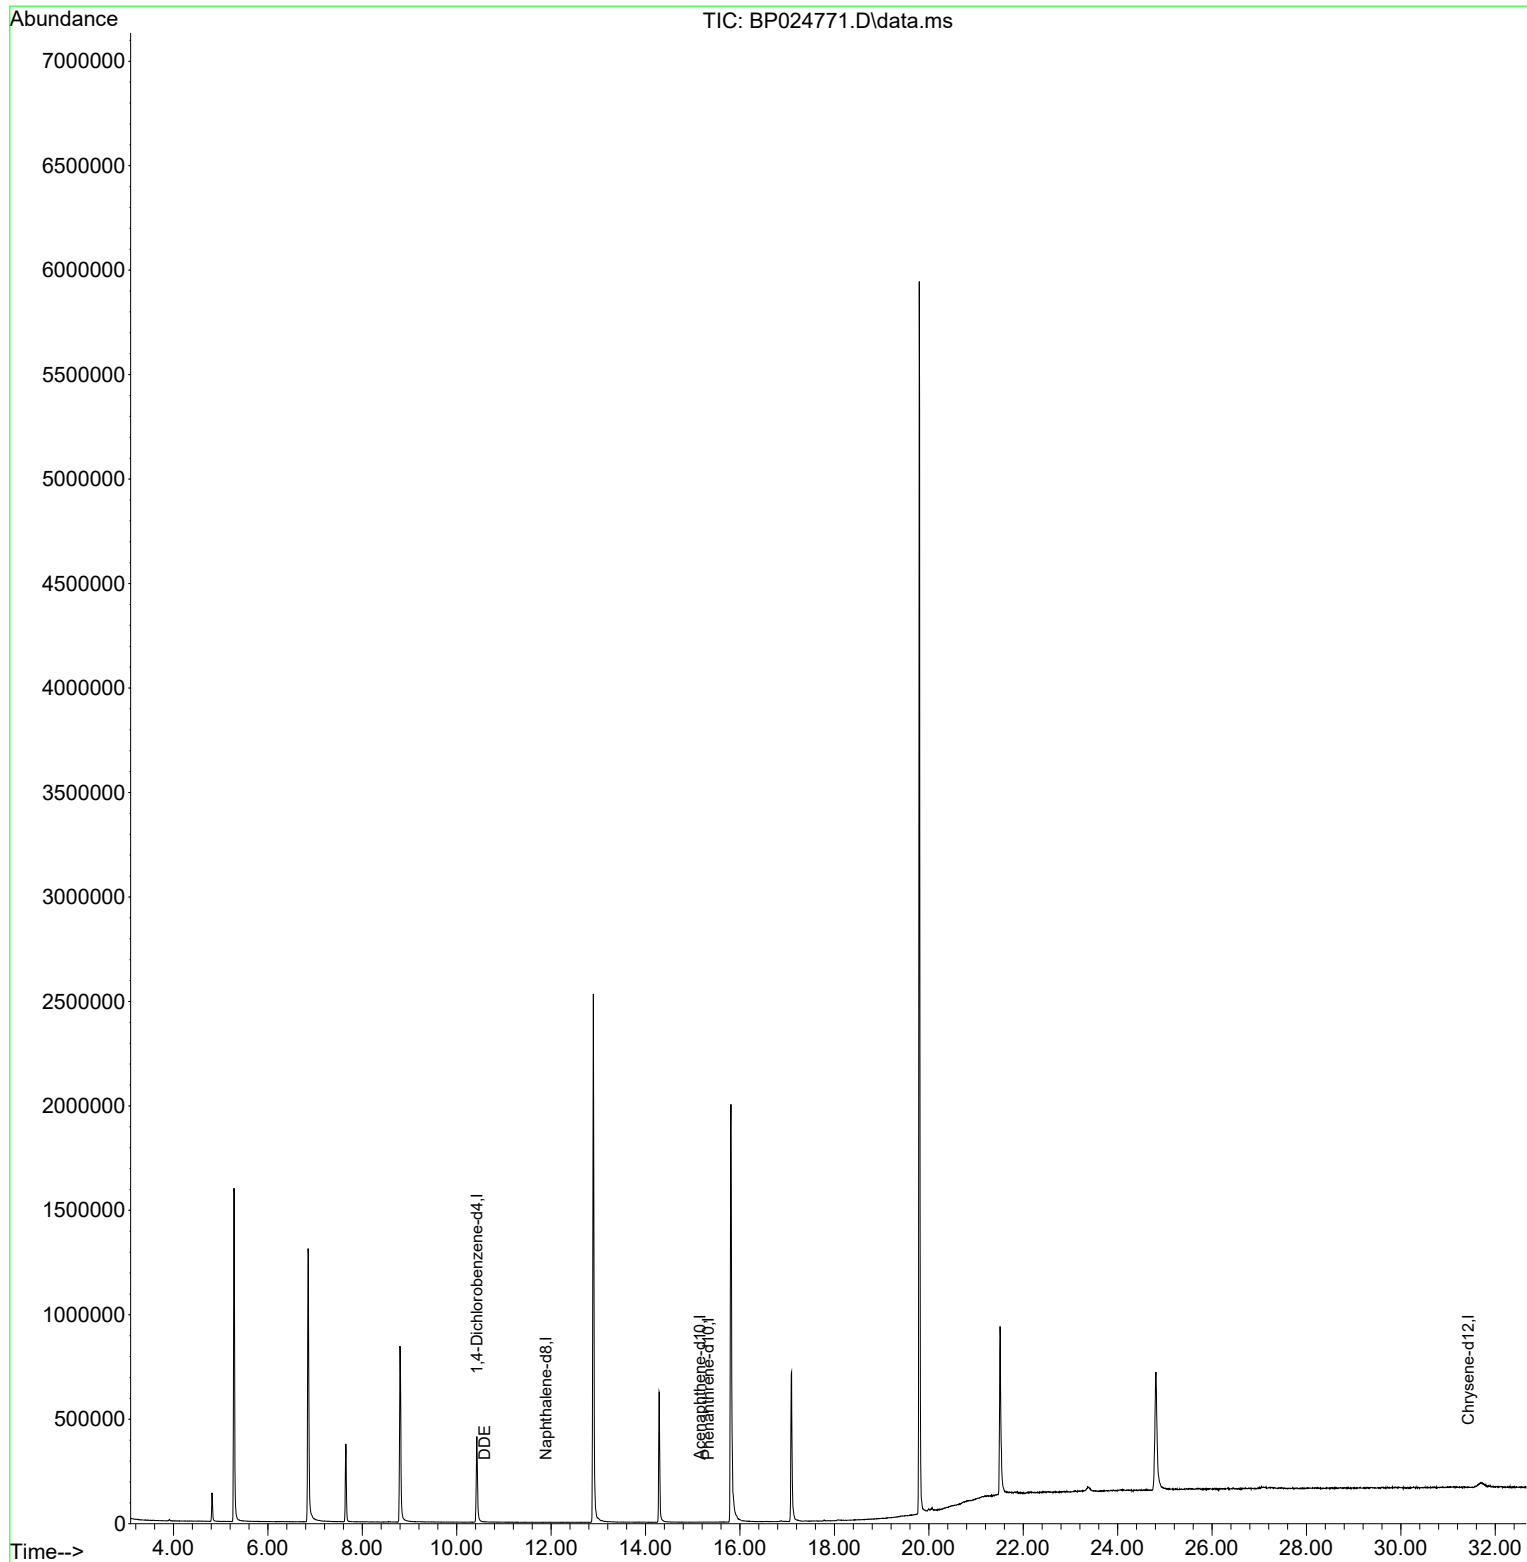


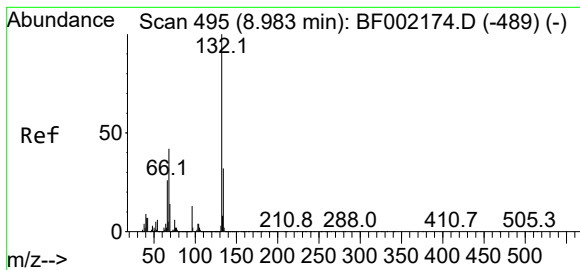

#5
DDE
Concen: 3.417 ng
RT: 10.593 min Scan# 11
Delta R.T. 0.153 min
Lab File: BP024771.D
Acq: 22 May 2025 23:50




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 8
Ion Ratio Lower Upper
246 100
248 87.5 1434.9 2152.3#
318 0.0 161.5 242.3#
176 200.0 3844.2 5766.4#

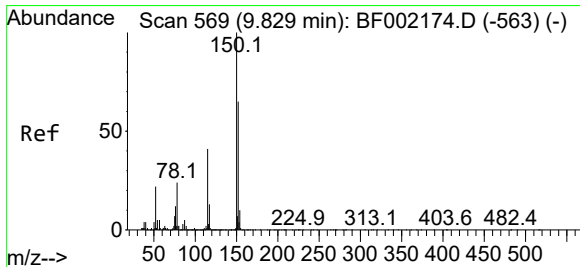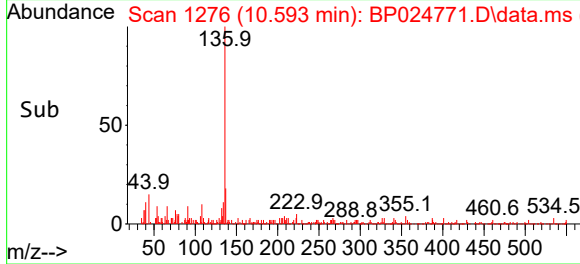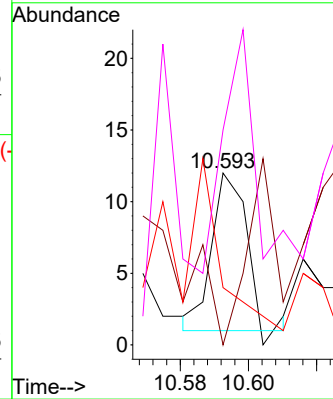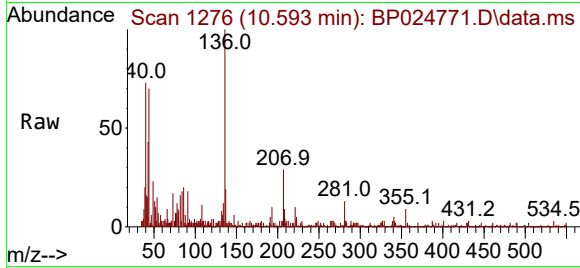

#6
DDD
Concen: Below Cal
RT: 11.010 min Scan# 1347
Delta R.T. 0.177 min
Lab File: BP024771.D
Acq: 22 May 2025 23:50


Tgt Ion:235 Resp: 6
Ion Ratio Lower Upper
235 100
237 233.3 4800.0 7200.0#
165 233.3 4800.0 7200.0#

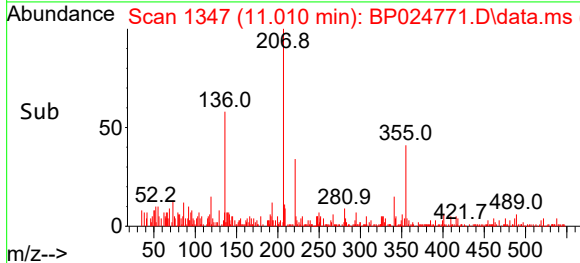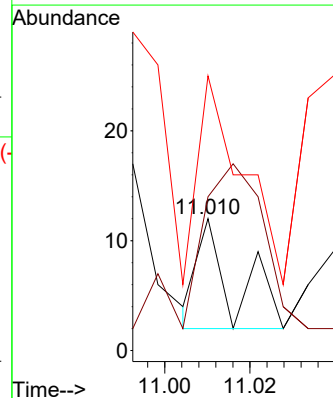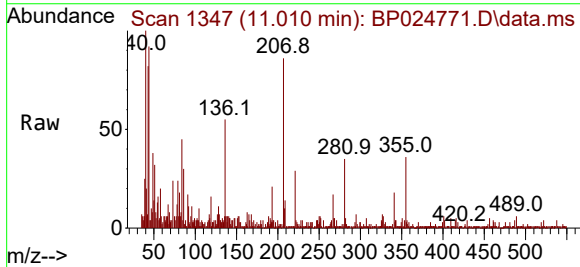

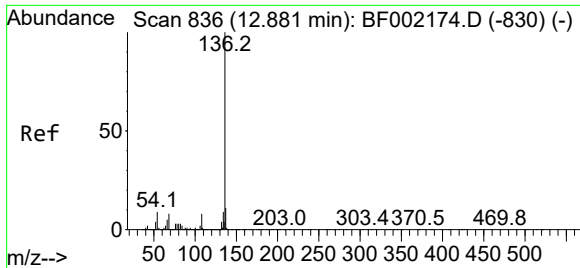

#7
DDT
Concen: Below Cal
RT: 11.381 min Scan# 14
Delta R.T. 0.189 min
Lab File: BP024771.D
Acq: 22 May 2025 23:50

Instrument :
BNA_P
ClientSampleId :

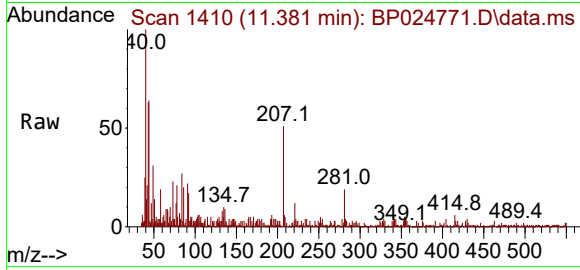

Tgt Ion: 235 Resp: 27
Ion Ratio Lower Upper
235 100
237 33.3 0.0 0.0#
165 0.0 0.2 0.2#

