

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024772.D
 Acq On : 23 May 2025 00:30
 Operator : RC/JU
 Sample : Q2078-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:58:30 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.257	152	16	40.000	ng	# 0.00
2) Naphthalene-d8	11.751	136	49	40.000	ng	# 0.03
3) Acenaphthene-d10	15.175	164	1857	40.000	ng	# 0.27
4) Phenanthrene-d10	15.339	188	27	40.000	ng	# 0.25
8) Chrysene-d12	31.444	240	33	40.000	ng	# 0.52
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.616	246	13	N.D.		
6) DDD	10.998	235	12	N.D.		
7) DDT	11.387	235	9	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024772.D
Acq On : 23 May 2025 00:30
Operator : RC/JU
Sample : Q2078-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




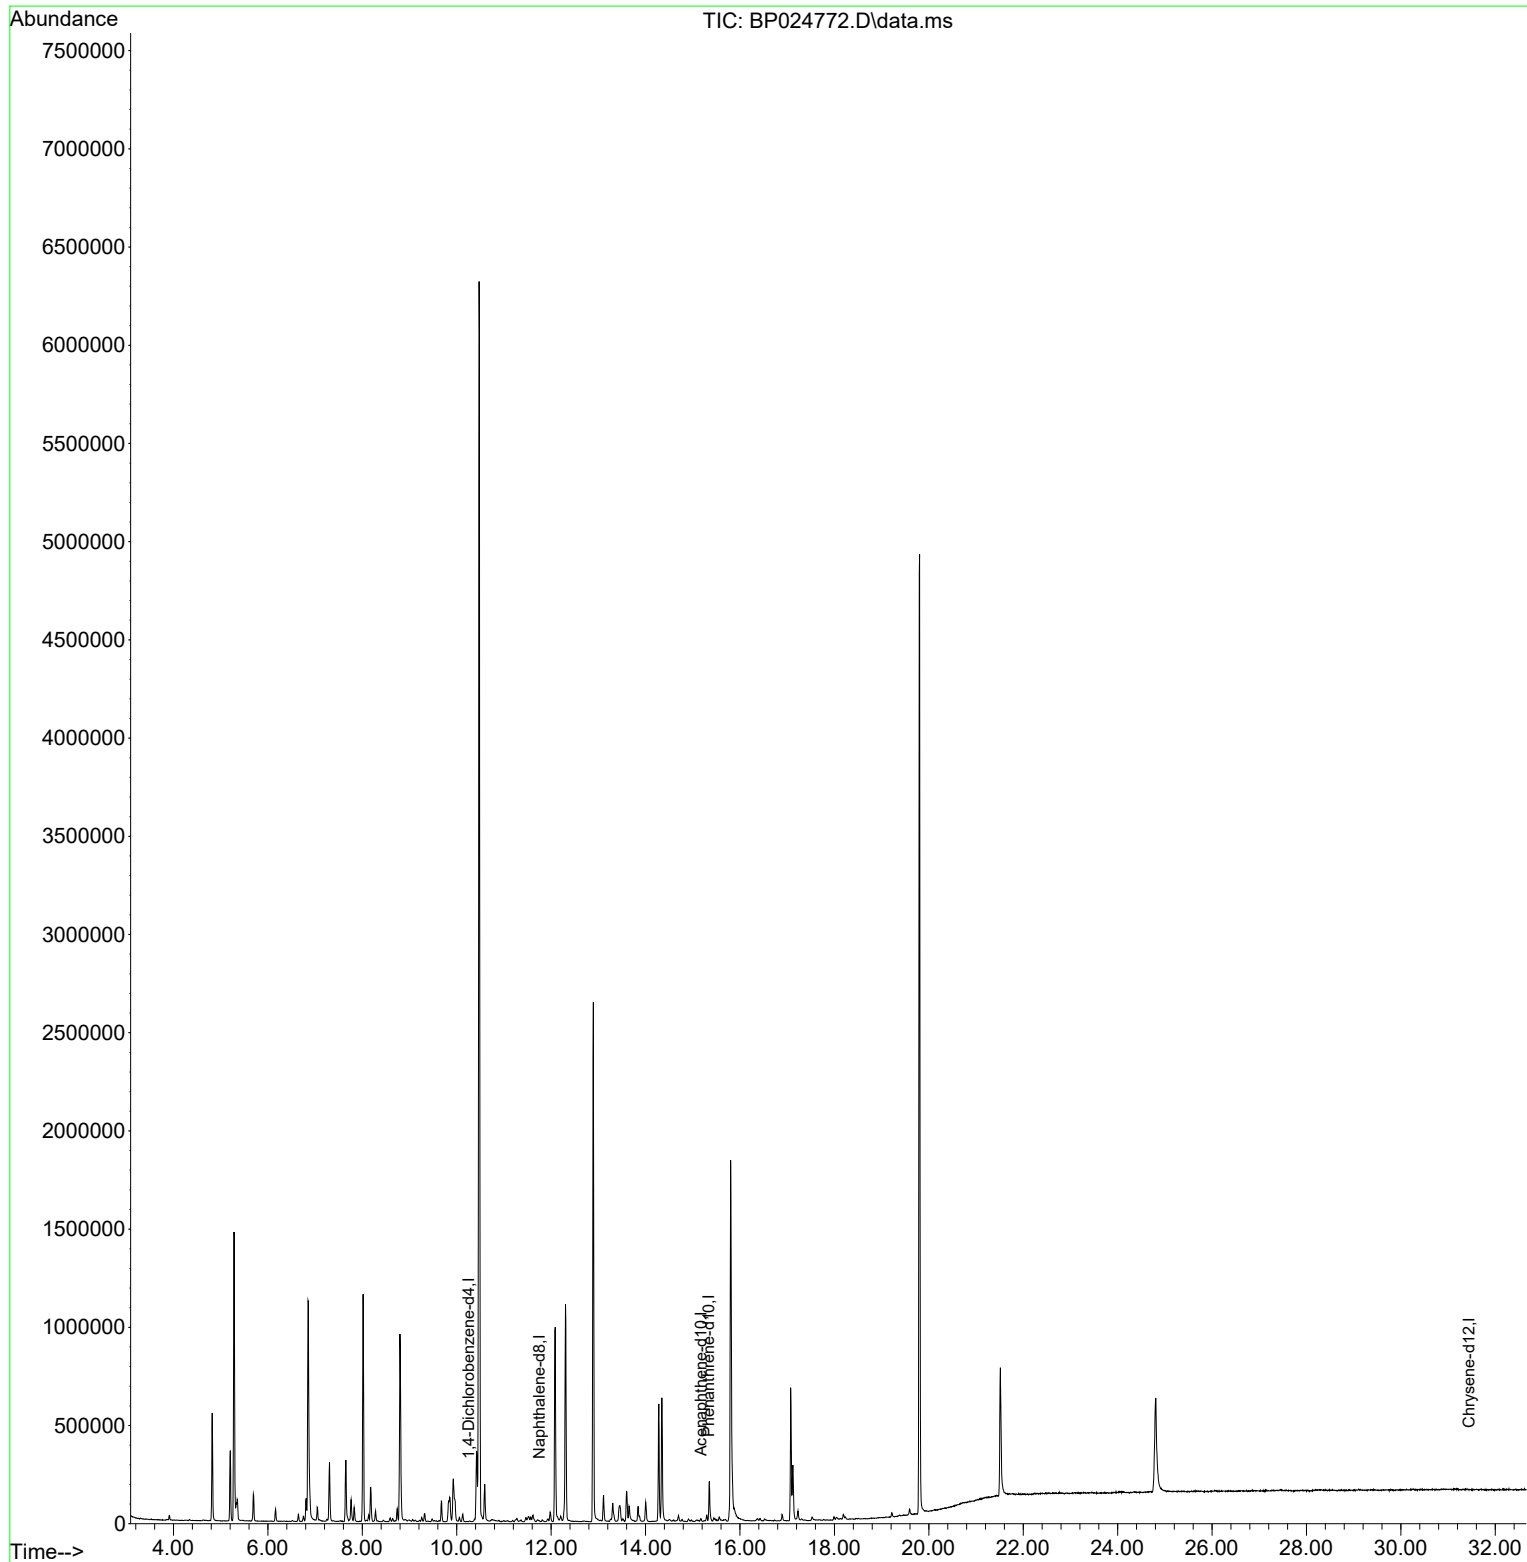


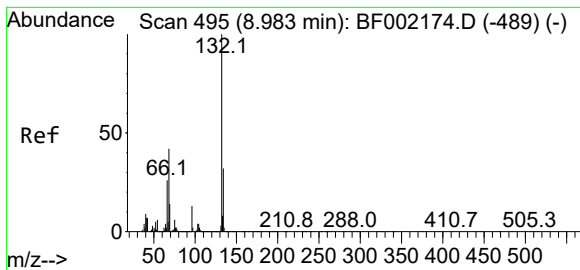

#5
DDE
Concen: Below Cal
RT: 10.616 min Scan# 13
Delta R.T. 0.177 min
Lab File: BP024772.D
Acq: 23 May 2025 00:30




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 13
Ion Ratio Lower Upper
246 100
248 38.5 1434.9 2152.3#
318 0.0 161.5 242.3#
176 0.0 3844.2 5766.4#

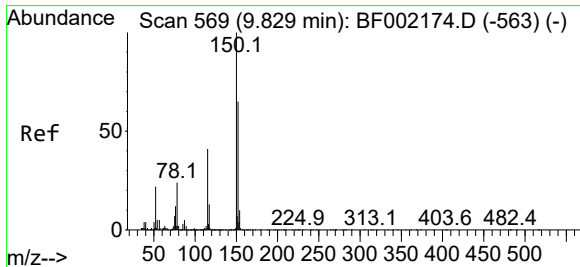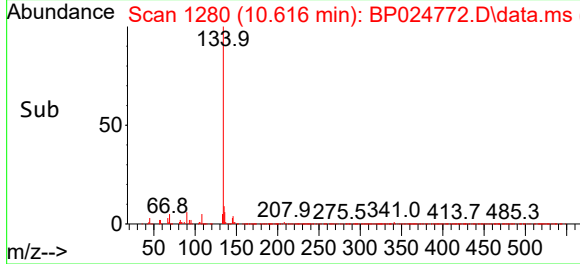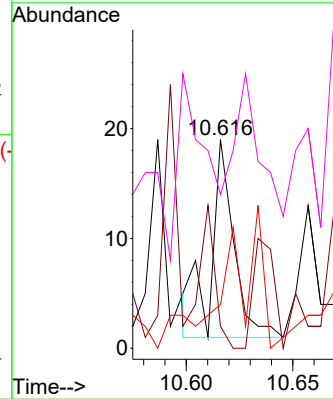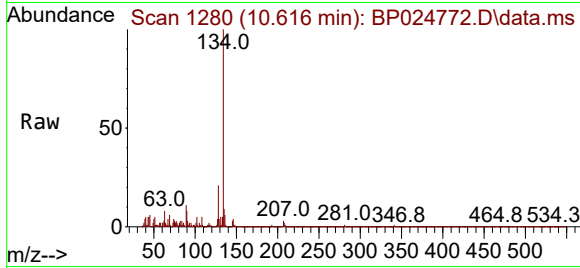

#6
DDD
Concen: Below Cal
RT: 10.998 min Scan# 1345
Delta R.T. 0.165 min
Lab File: BP024772.D
Acq: 23 May 2025 00:30


Tgt Ion:235 Resp: 12
Ion Ratio Lower Upper
235 100
237 66.7 4800.0 7200.0#
165 0.0 4800.0 7200.0#

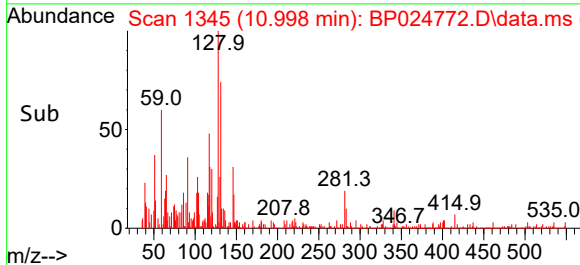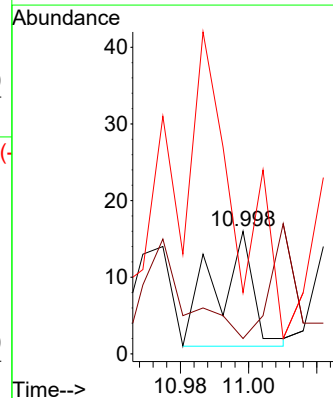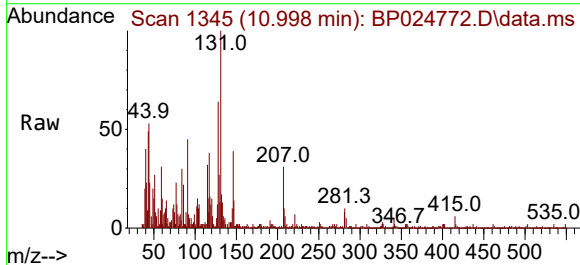

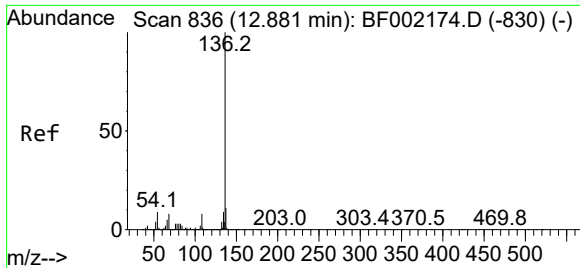

#7
DDT
Concen: Below Cal
RT: 11.387 min Scan# 14
Delta R.T. 0.195 min
Lab File: BP024772.D
Acq: 23 May 2025 00:30

Instrument :
BNA_P
ClientSampleId :

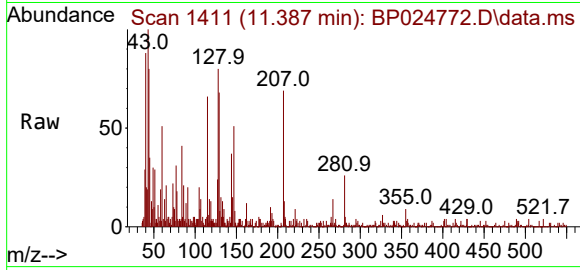

Tgt Ion: 235 Resp: 9
Ion Ratio Lower Upper
235 100
237 222.2 0.0 0.0#
165 0.0 0.2 0.2#

