

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024773.D
 Acq On : 23 May 2025 01:11
 Operator : RC/JU
 Sample : Q2078-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:58:36 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.258	152	13	40.000	ng	# 0.00
2) Naphthalene-d8	11.722	136	62	40.000	ng	# 0.00
3) Acenaphthene-d10	15.175	164	3614	40.000	ng	# 0.27
4) Phenanthrene-d10	15.363	188	7	40.000	ng	# 0.27
8) Chrysene-d12	31.462	240	28	40.000	ng	# 0.54
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.622	246	4	N.D.		
6) DDD	11.034	235	15	N.D.		
7) DDT	11.381	235	11	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024773.D
Acq On : 23 May 2025 01:11
Operator : RC/JU
Sample : Q2078-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




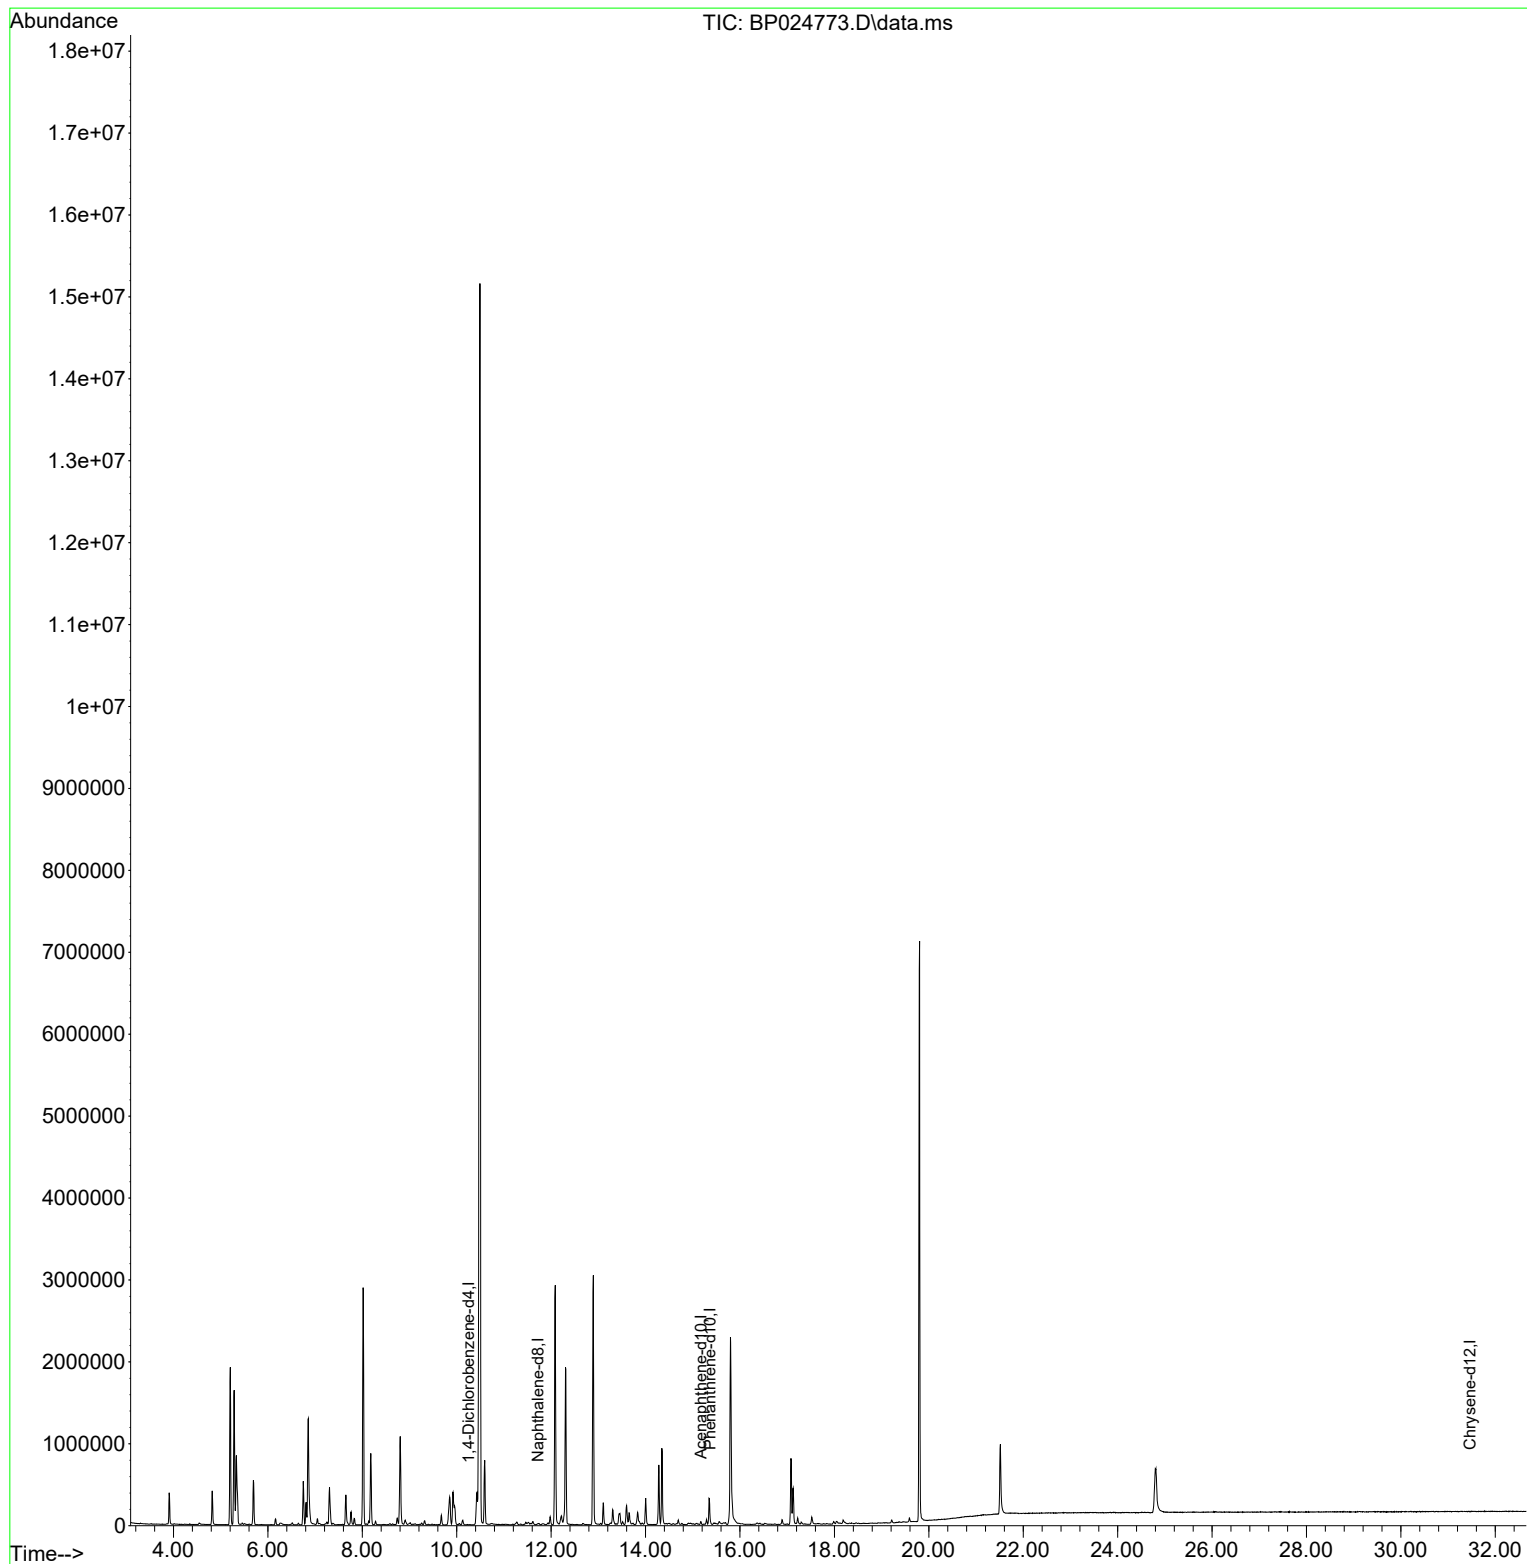


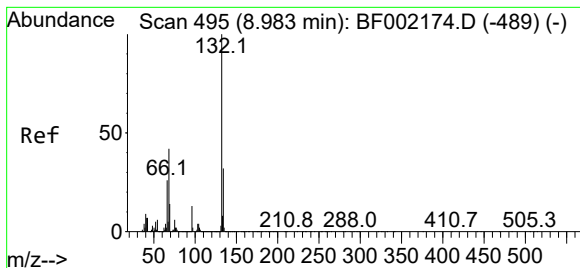

#5
DDE
Concen: Below Cal
RT: 10.622 min Scan# 131
Delta R.T. 0.183 min
Lab File: BP024773.D
Acq: 23 May 2025 01:11




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 4
Ion Ratio Lower Upper
246 100
248 250.0 1434.9 2152.3#
318 50.0 161.5 242.3#
176 0.0 3844.2 5766.4#

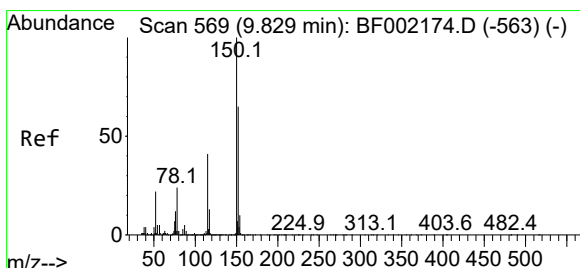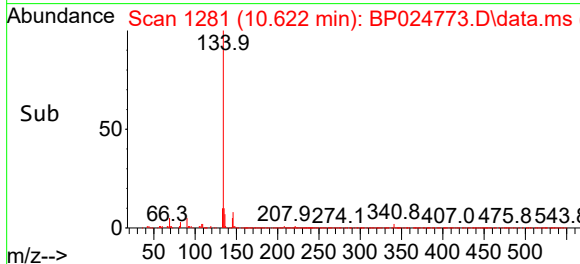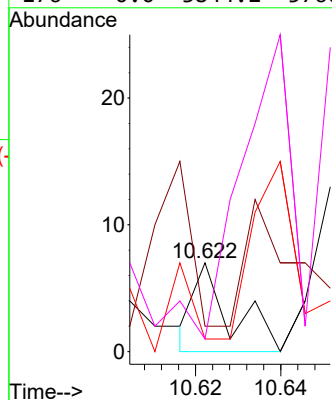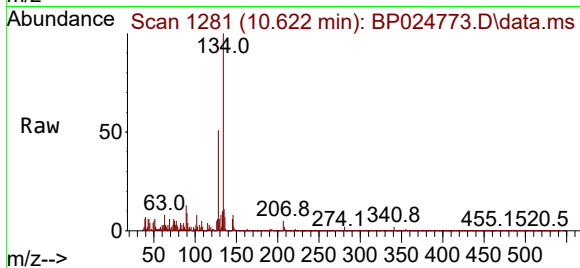

#6
DDD
Concen: Below Cal
RT: 11.034 min Scan# 1351
Delta R.T. 0.201 min
Lab File: BP024773.D
Acq: 23 May 2025 01:11


Tgt Ion:235 Resp: 15
Ion Ratio Lower Upper
235 100
237 60.0 4800.0 7200.0#
165 73.3 4800.0 7200.0#

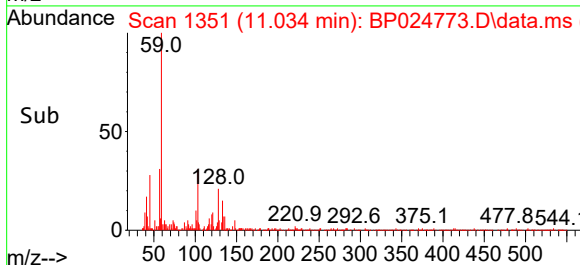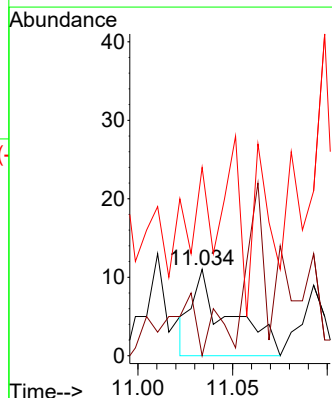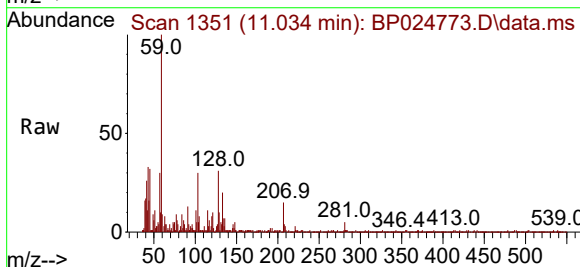

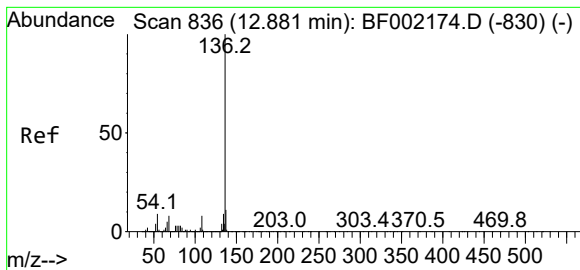

#7
DDT
Concen: Below Cal
RT: 11.381 min Scan# 14
Delta R.T. 0.189 min
Lab File: BP024773.D
Acq: 23 May 2025 01:11

Instrument :
BNA_P
ClientSampleId :

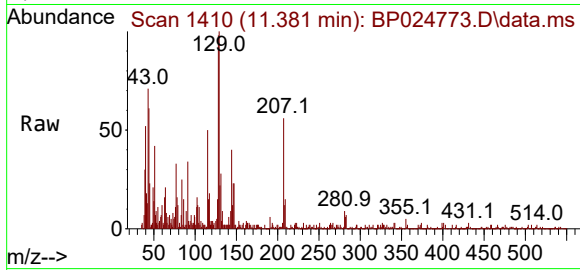

Tgt Ion:235 Resp: 11
Ion Ratio Lower Upper
235 100
237 209.1 0.0 0.0#
165 190.9 0.2 0.2#

