

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
 Data File : BP024775.D
 Acq On : 23 May 2025 02:32
 Operator : RC/JU
 Sample : Q2078-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: May 23 02:58:48 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	10.269	152	22	40.000	ng	# 0.00
2) Naphthalene-d8	11.751	136	105	40.000	ng	# 0.03
3) Acenaphthene-d10	15.175	164	1931	40.000	ng	# 0.27
4) Phenanthrene-d10	15.381	188	17	40.000	ng	# 0.29
8) Chrysene-d12	31.539	240	88	40.000	ng	# 0.61
9) Perylene-d12	0.000	264	0	0.000	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.646	246	10	N.D.		
6) DDD	11.057	235	19	N.D.		
7) DDT	11.410	235	15	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024775.D
Acq On : 23 May 2025 02:32
Operator : RC/JU
Sample : Q2078-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: May 23 02:58:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\BFDDTBREAKDOWN-8270.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration




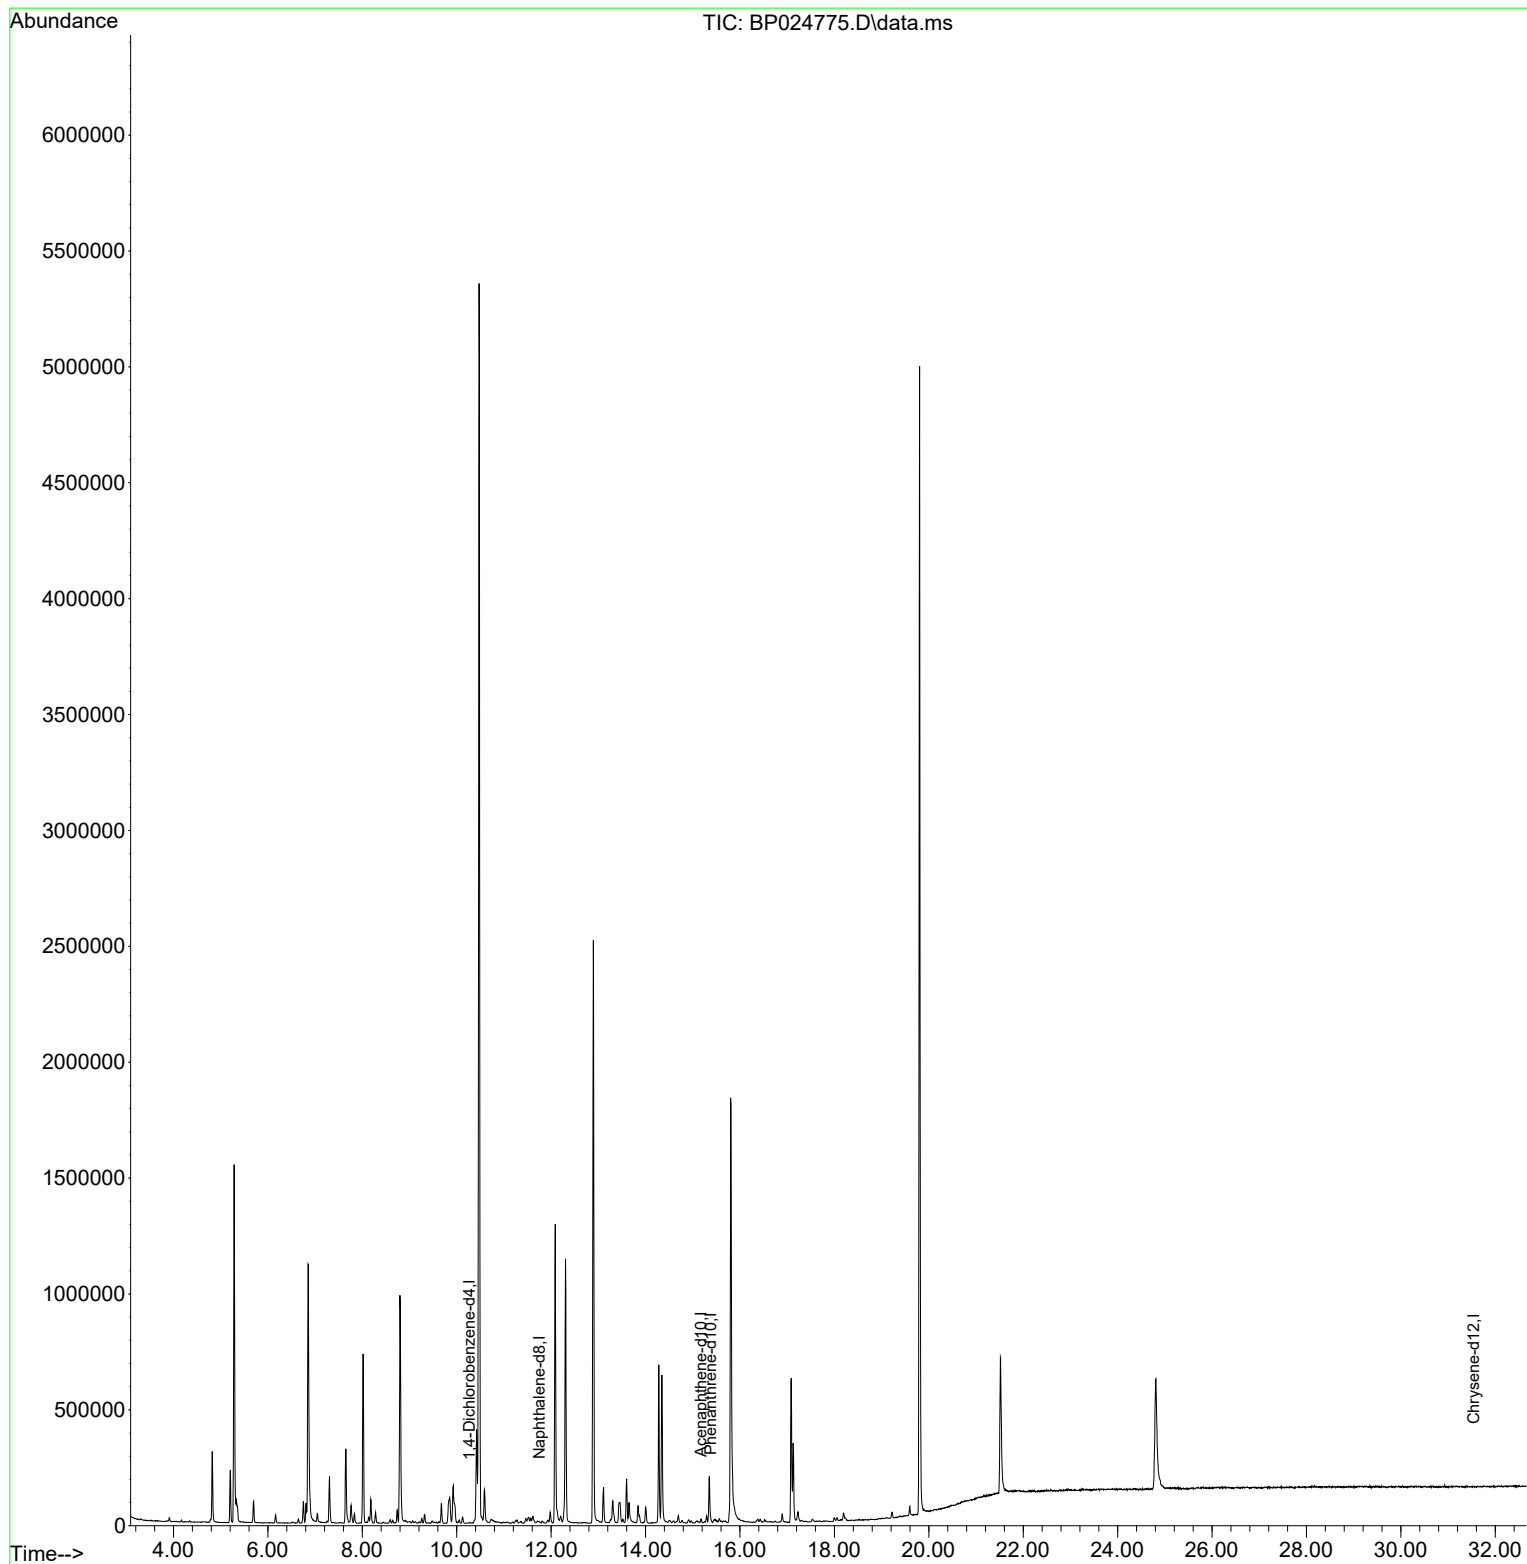


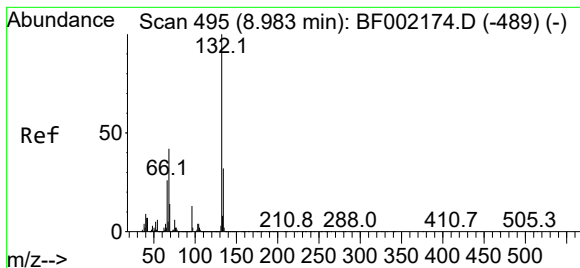

#5
DDE
Concen: Below Cal
RT: 10.646 min Scan# 11
Delta R.T. 0.206 min
Lab File: BP024775.D
Acq: 23 May 2025 02:32




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:246 Resp: 10
Ion Ratio Lower Upper
246 100
248 60.0 1434.9 2152.3#
318 60.0 161.5 242.3#
176 230.0 3844.2 5766.4#

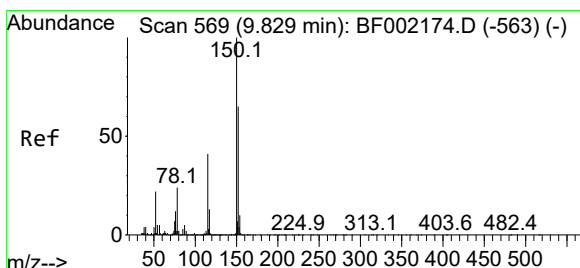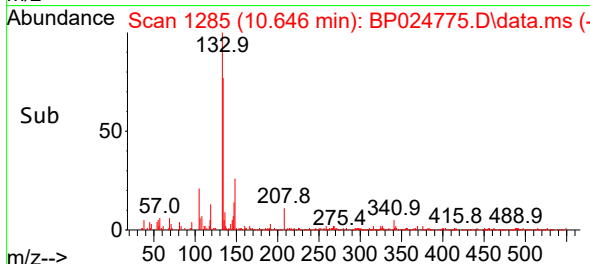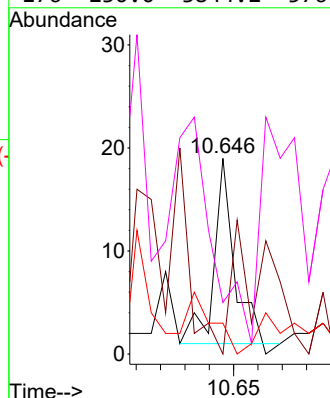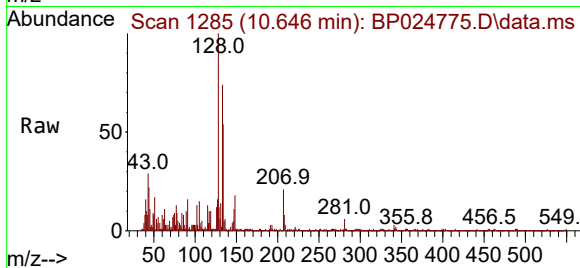

#6
DDD
Concen: Below Cal
RT: 11.057 min Scan# 1355
Delta R.T. 0.224 min
Lab File: BP024775.D
Acq: 23 May 2025 02:32


Tgt Ion:235 Resp: 19
Ion Ratio Lower Upper
235 100
237 0.0 4800.0 7200.0#
165 0.0 4800.0 7200.0#

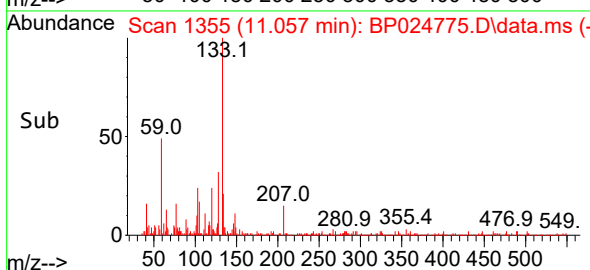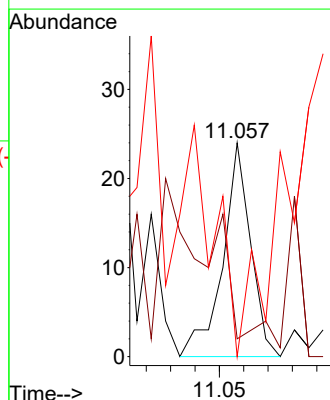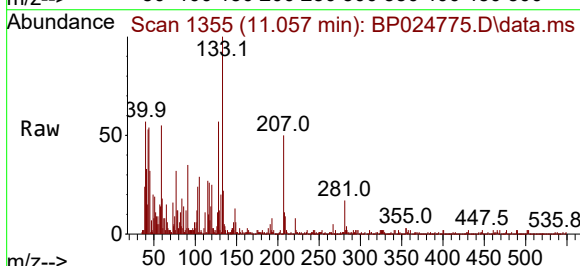

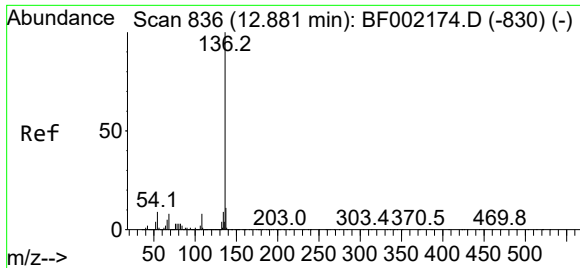

#7
DDT
Concen: Below Cal
RT: 11.410 min Scan# 14
Delta R.T. 0.218 min
Lab File: BP024775.D
Acq: 23 May 2025 02:32

Instrument :
BNA_P
ClientSampleId :

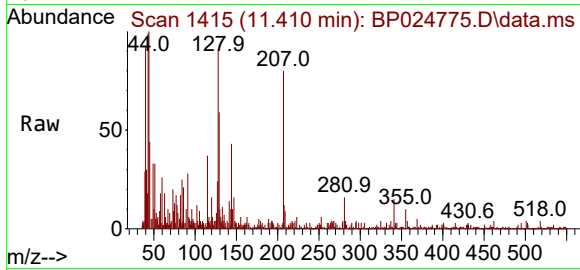

Tgt Ion:235 Resp: 15
Ion Ratio Lower Upper
235 100
237 80.0 0.0 0.0#
165 0.0 0.2 0.2#

