
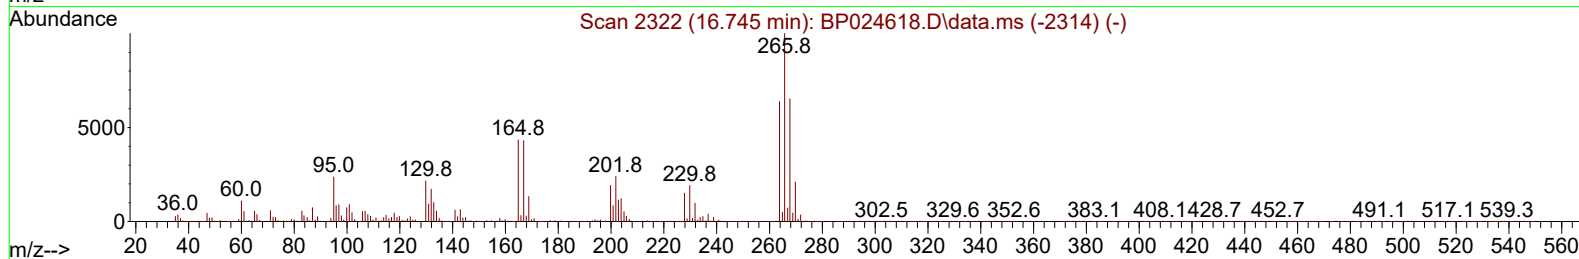
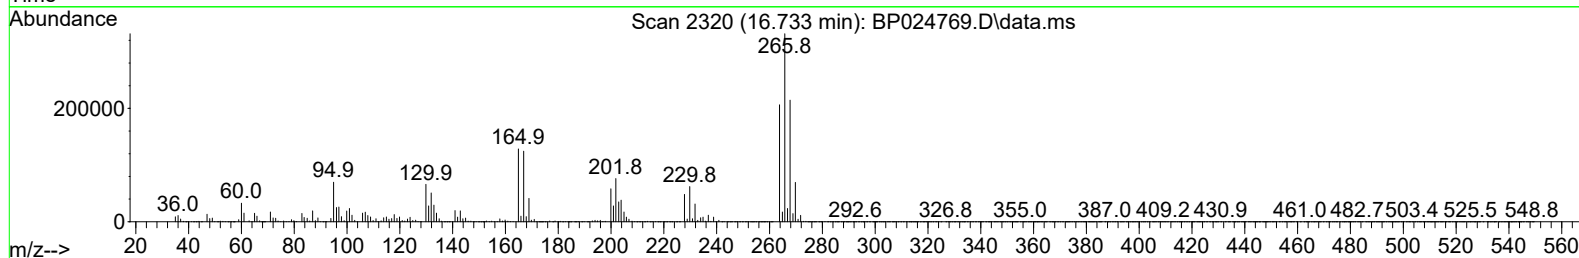


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024769.D
Acq On : 22 May 2025 22:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 02:32:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

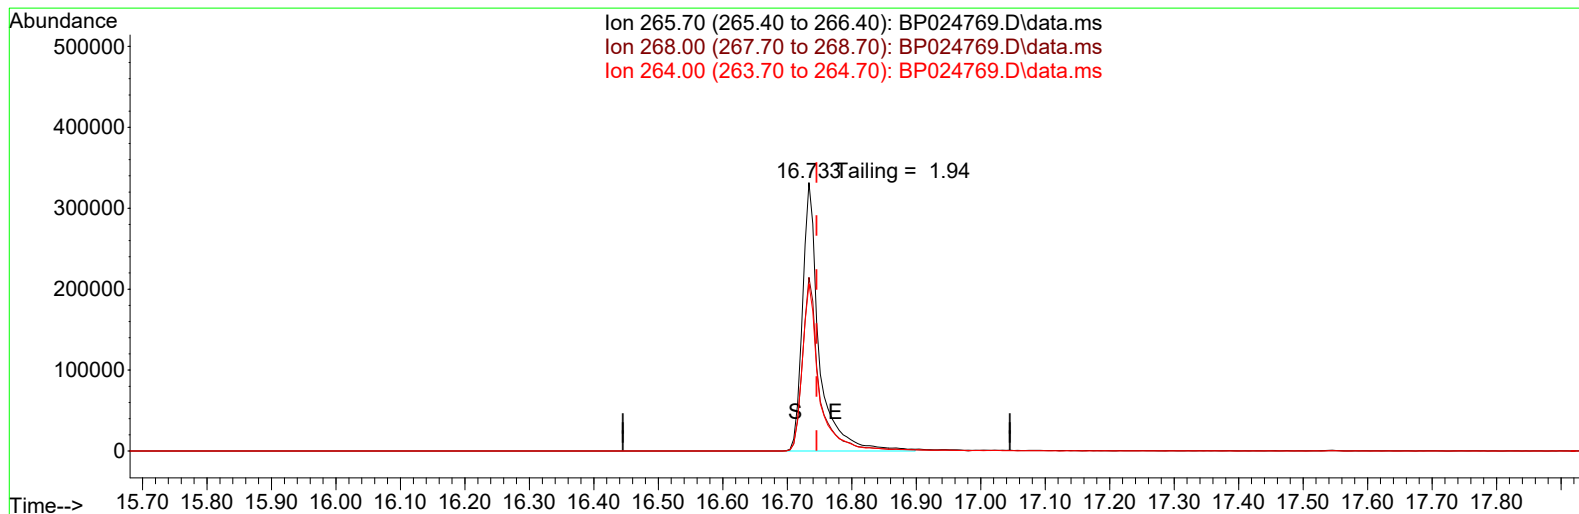

TIC: BP024769.D\data.ms

(70) Pentachlorophenol (C)




16.733min (-0.012) 149632.44 ng

response 601167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.69
264.00	63.90	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024769.D
Acq On : 22 May 2025 22:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 02:32:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

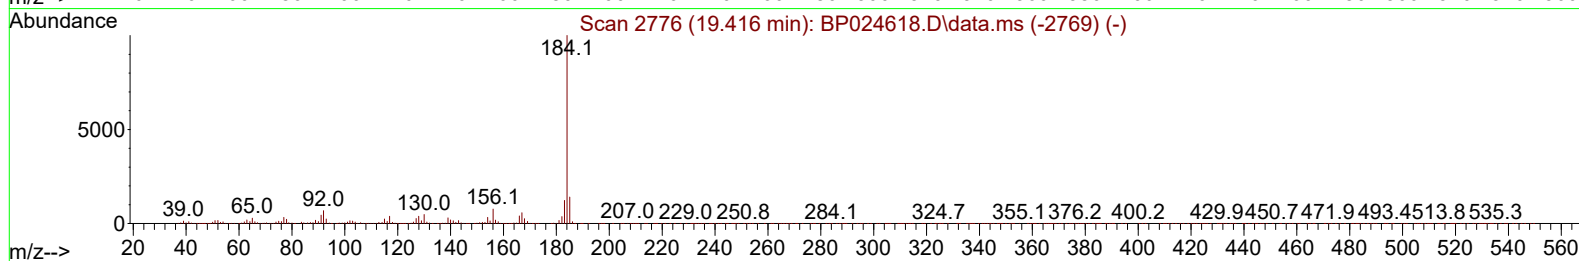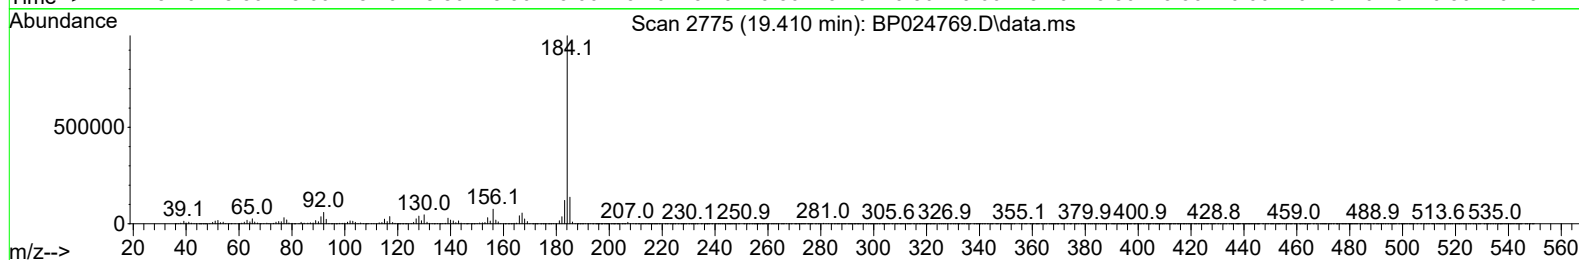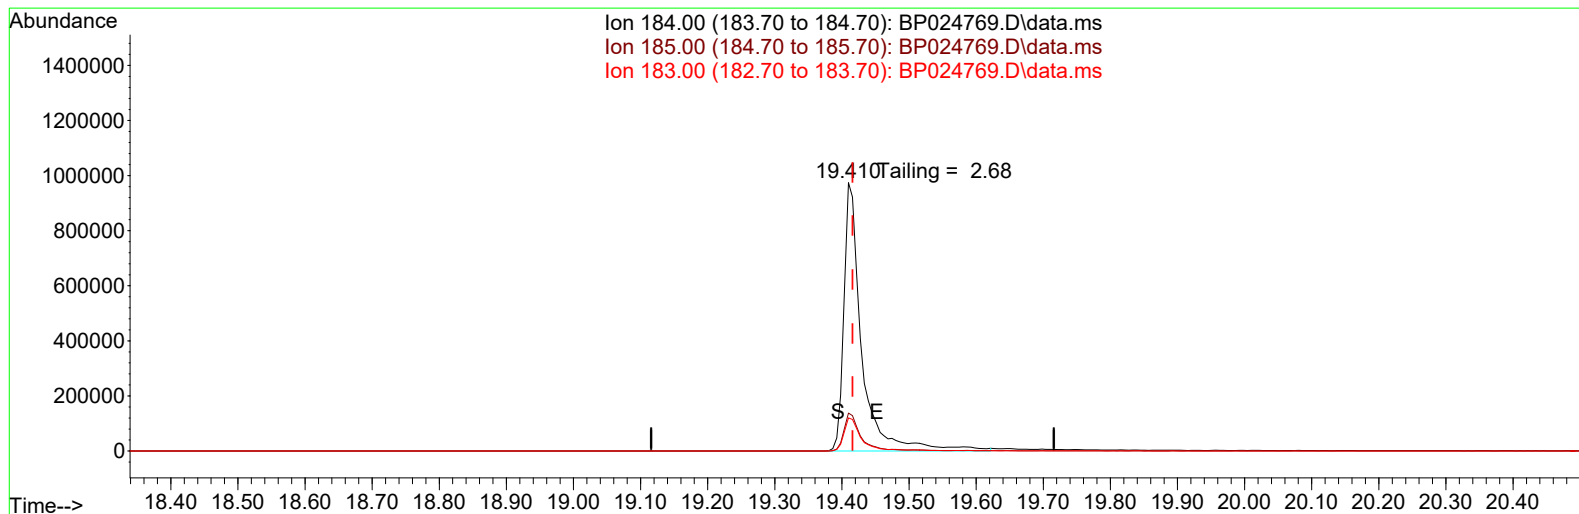

TIC: BP024769.D\data.ms

(77) Benzidine

19.410min (-0.006) 2086342.00 ng

response 1704705

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.14
183.00	12.30	12.39
0.00	0.00	0.00