
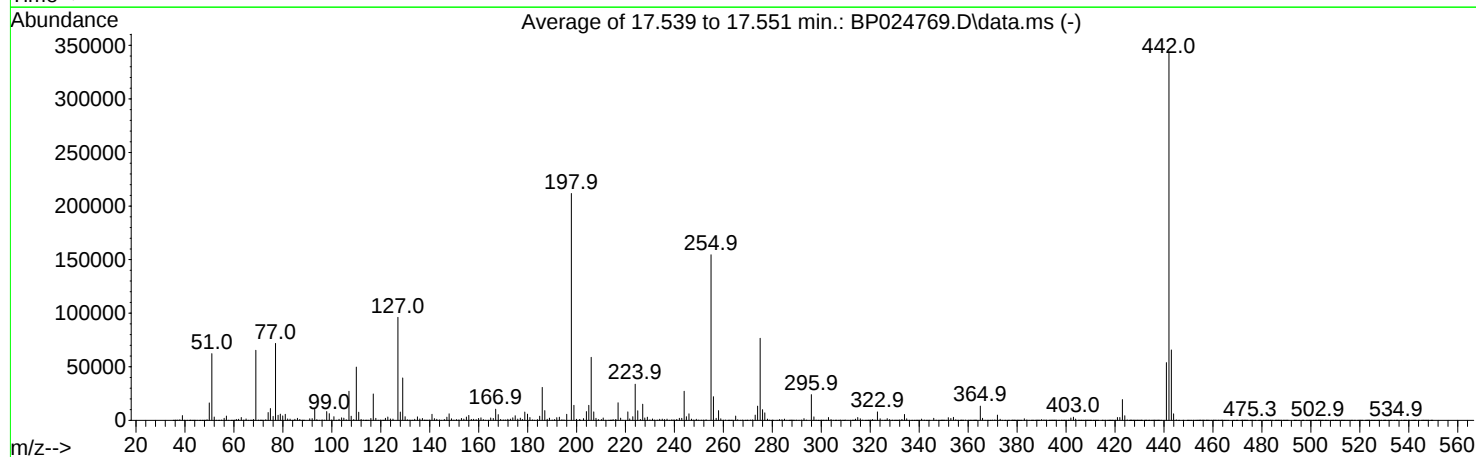


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024769.D
Acq On : 22 May 2025 22:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

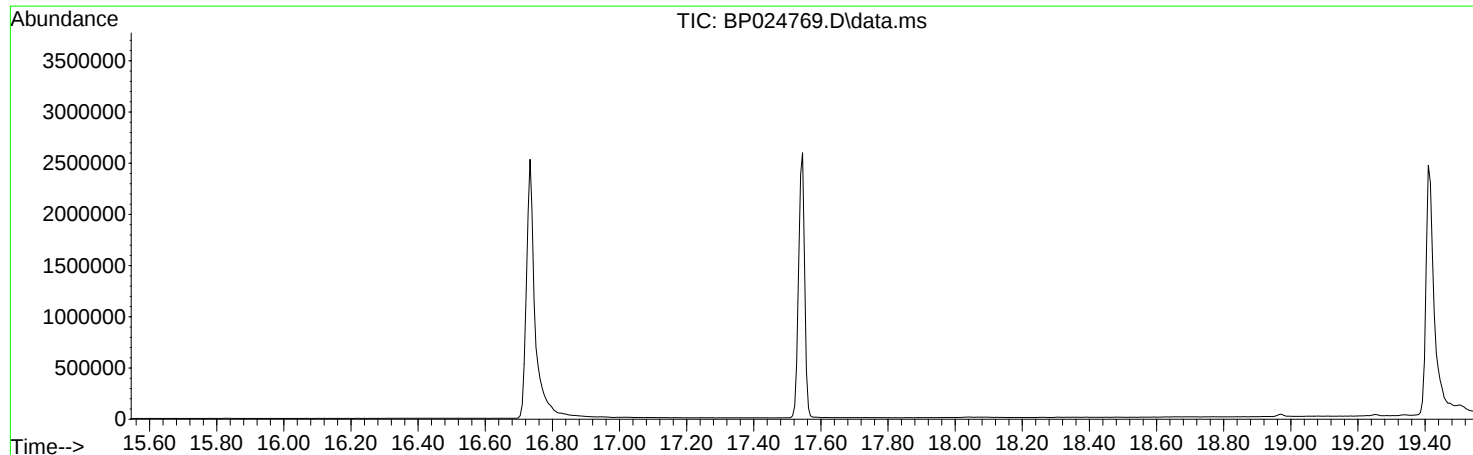




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	62211	PASS
68	69	0.00	2	1.3	861	PASS
69	198	0.00	100	30.9	65374	PASS
70	69	0.00	2	0.5	334	PASS
127	198	10	80	45.4	96107	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	211776	PASS
199	198	5	9	6.6	13998	PASS
275	198	10	60	36.2	76656	PASS
365	198	1	100	6.3	13312	PASS
441	198	0.01	100	25.5	53906	PASS
442	442	100	100	100.0	343309	PASS
443	442	15	24	19.1	65731	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024769.D
Acq On : 22 May 2025 22:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 23 02:32:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

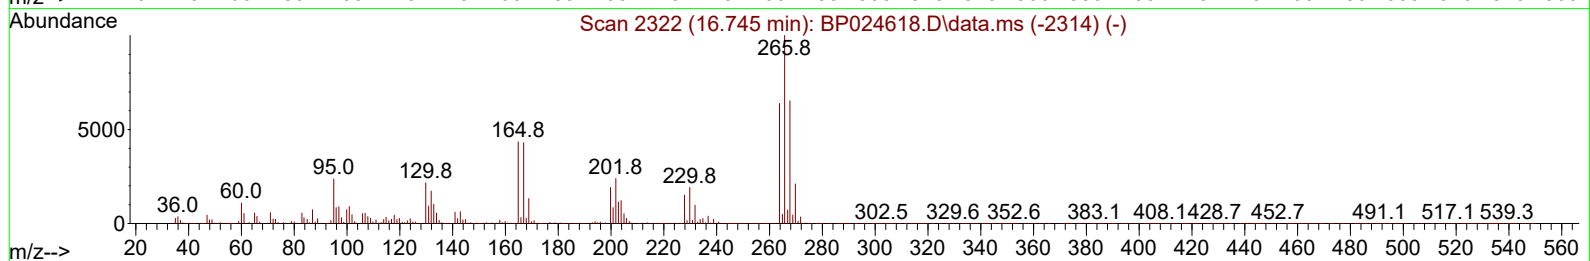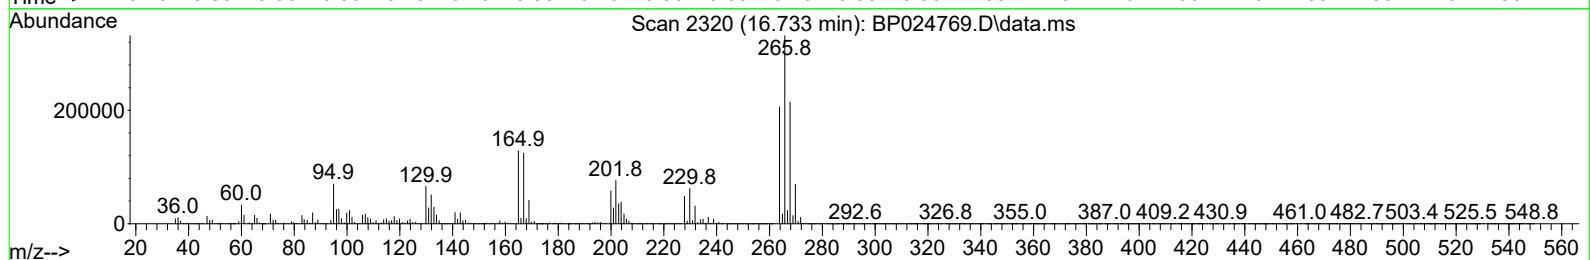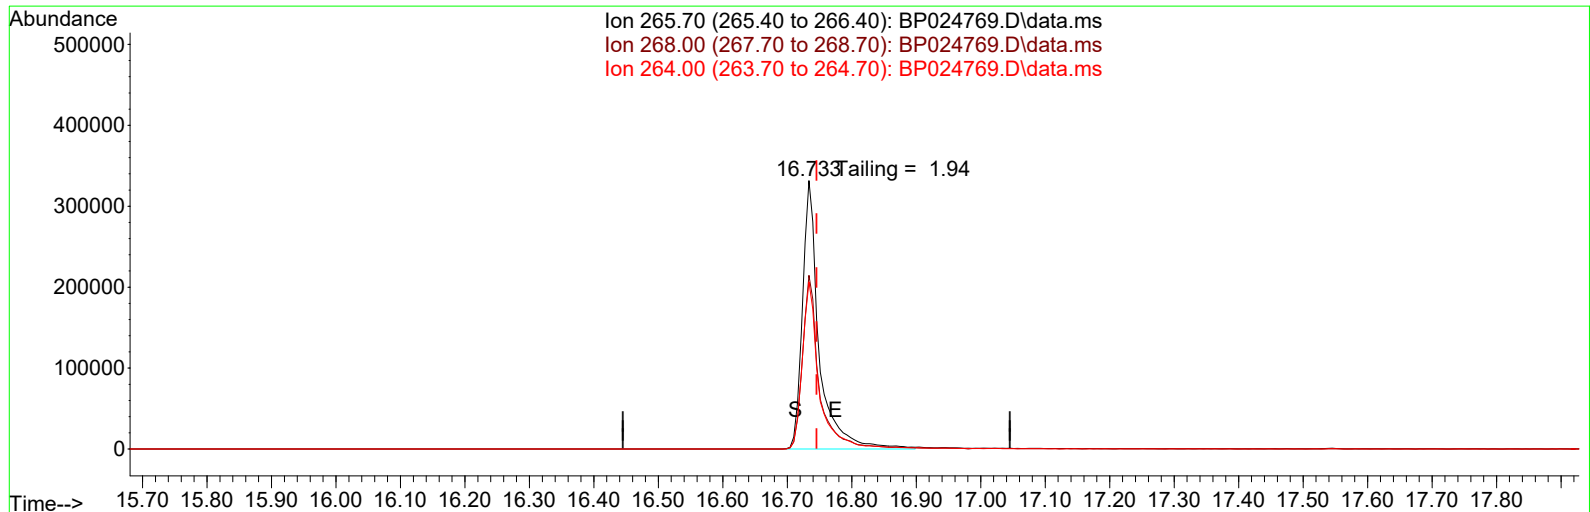

TIC: BP024769.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.012) 149632.44 ng




response 601167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.69
264.00	63.90	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024769.D
Acq On : 22 May 2025 22:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 23 02:32:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

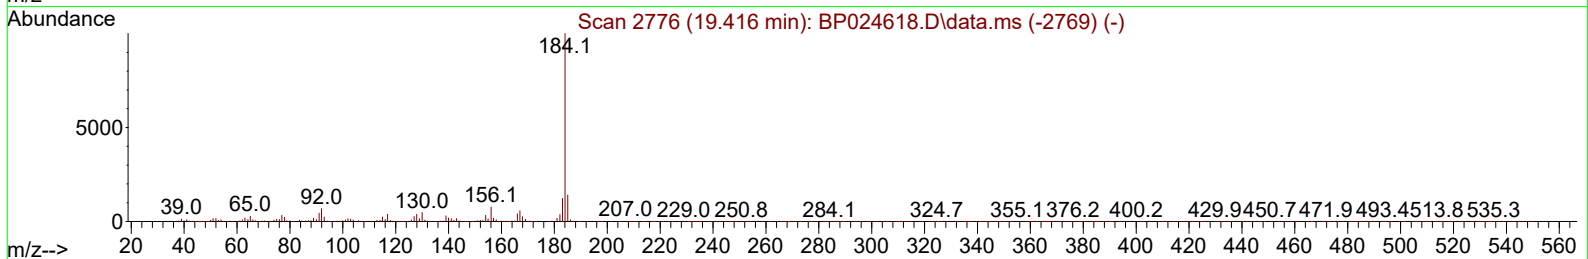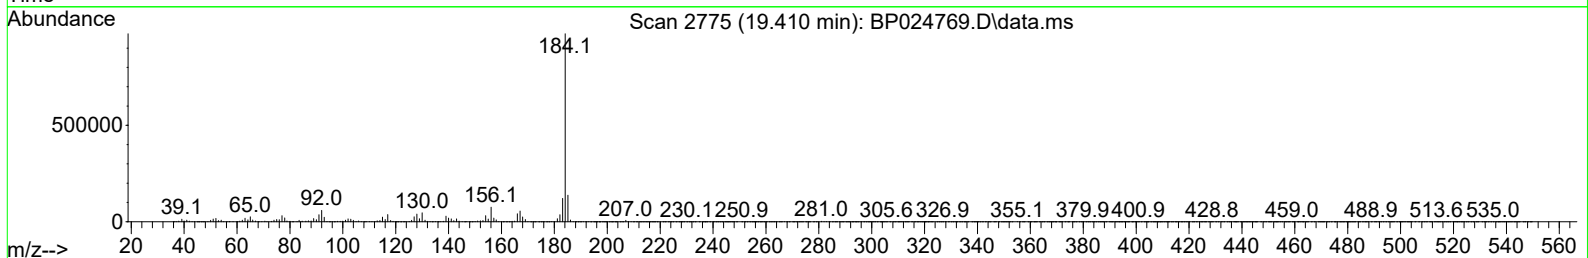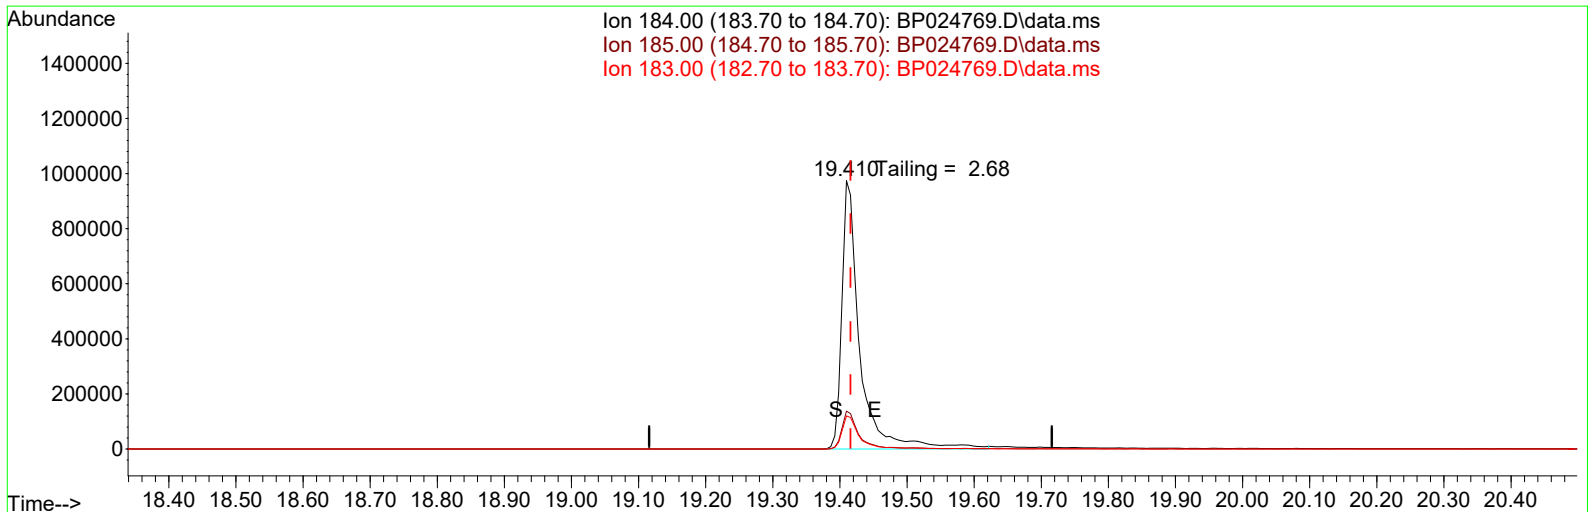

TIC: BP024769.D\data.ms

(77) Benzidine

19.410min (-0.006) 2086342.00 ng

response 1704705

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.14
183.00	12.30	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/22/2025	BNA_P	<u>BP024769.D</u>
Compound Name	Response	Retention Time
DDT	832087	20.692
DDD	19566	20.239
DDE	3224	19.716
	P	
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22790	854877	2.67

Instrument :
BNA_P
ClientSampleId :
DFTPP