




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010481.D
 Acq On : 23 May 2022 17:43
 Operator : CG/JU
 Sample : PB144963BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: May 23 23:20:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

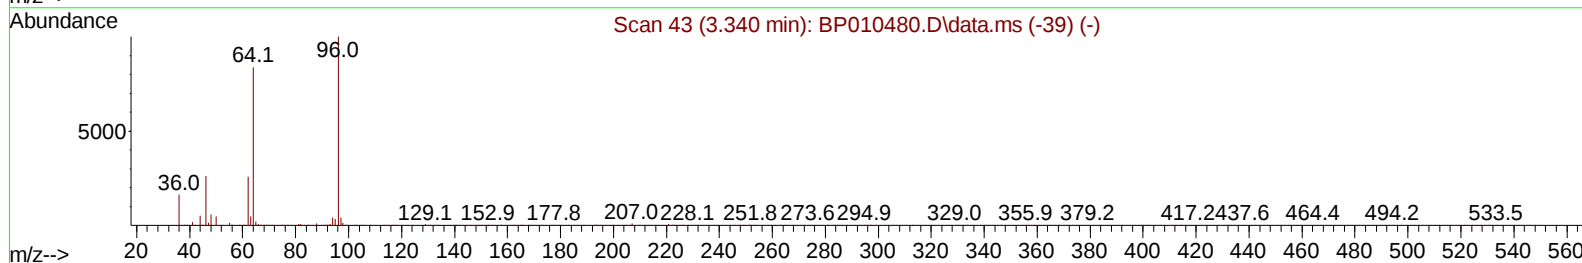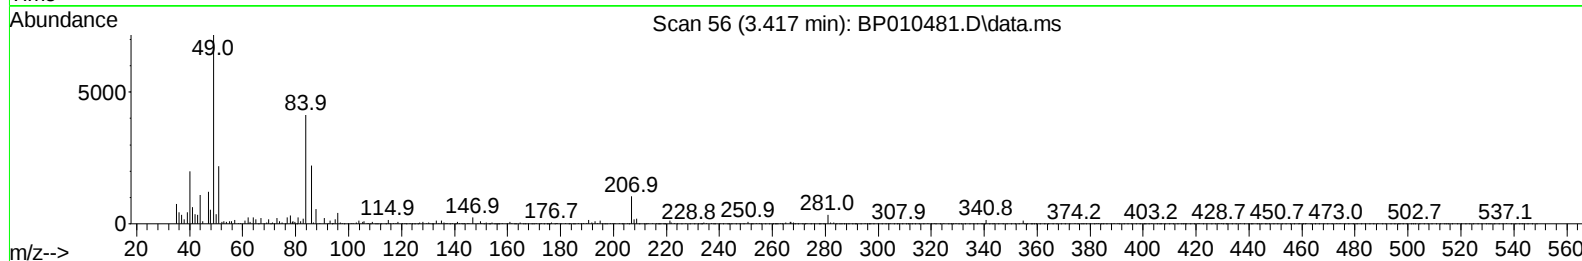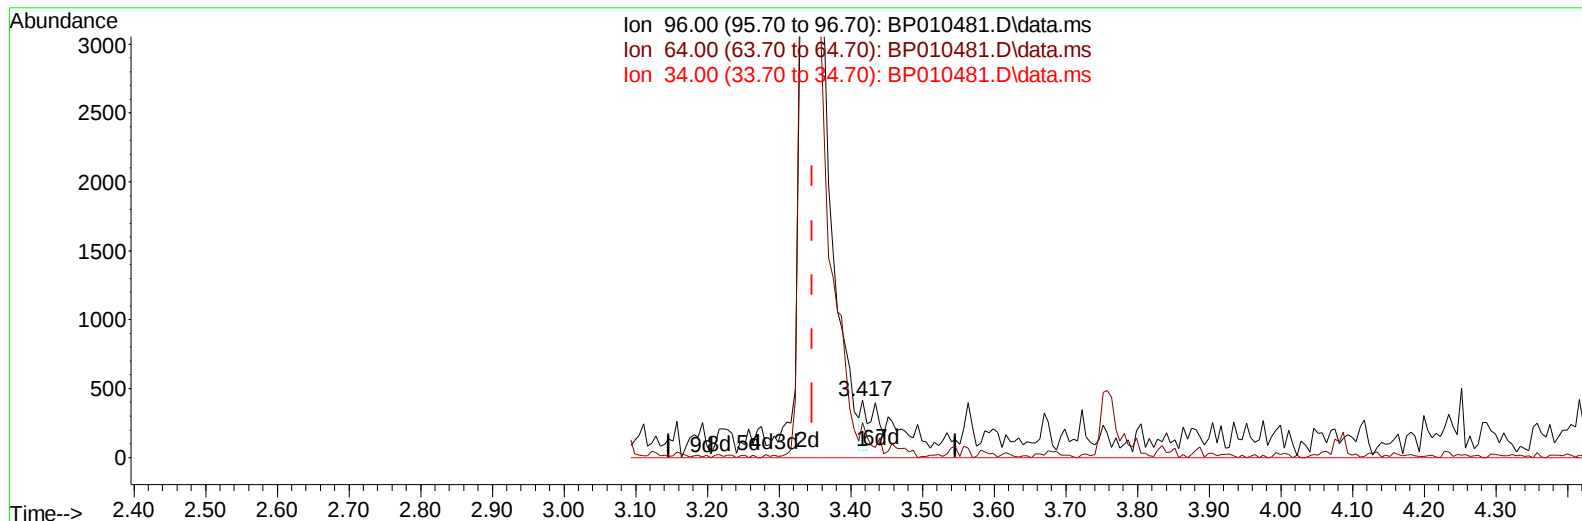

TIC: BP010481.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.417min (+ 0.071) 0.05 ng/uL

response 196

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	60.87
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010481.D
 Acq On : 23 May 2022 17:43
 Operator : CG/JU
 Sample : PB144963BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: May 23 23:20:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

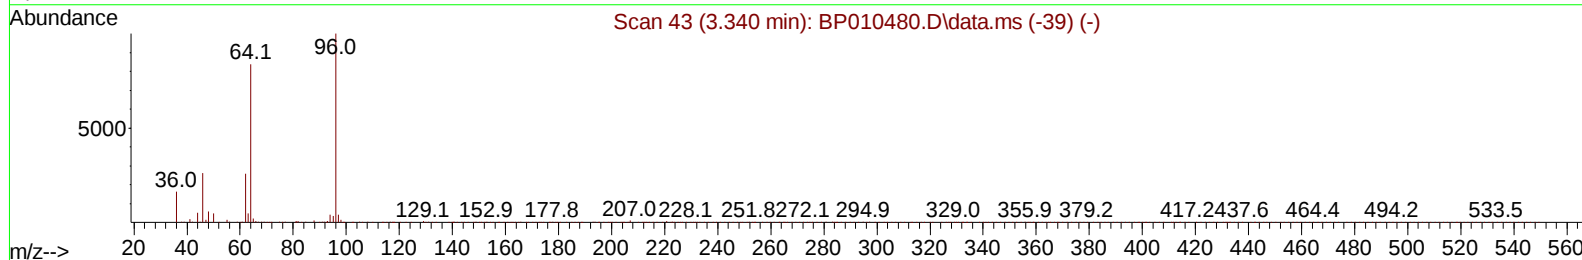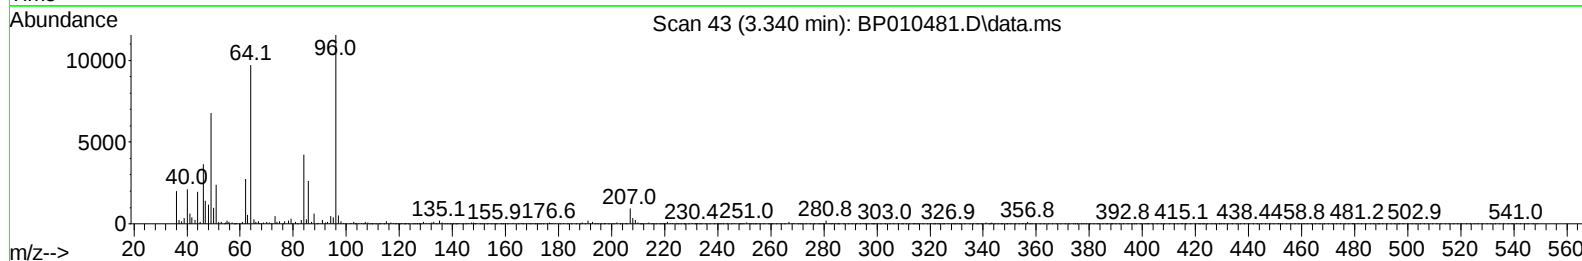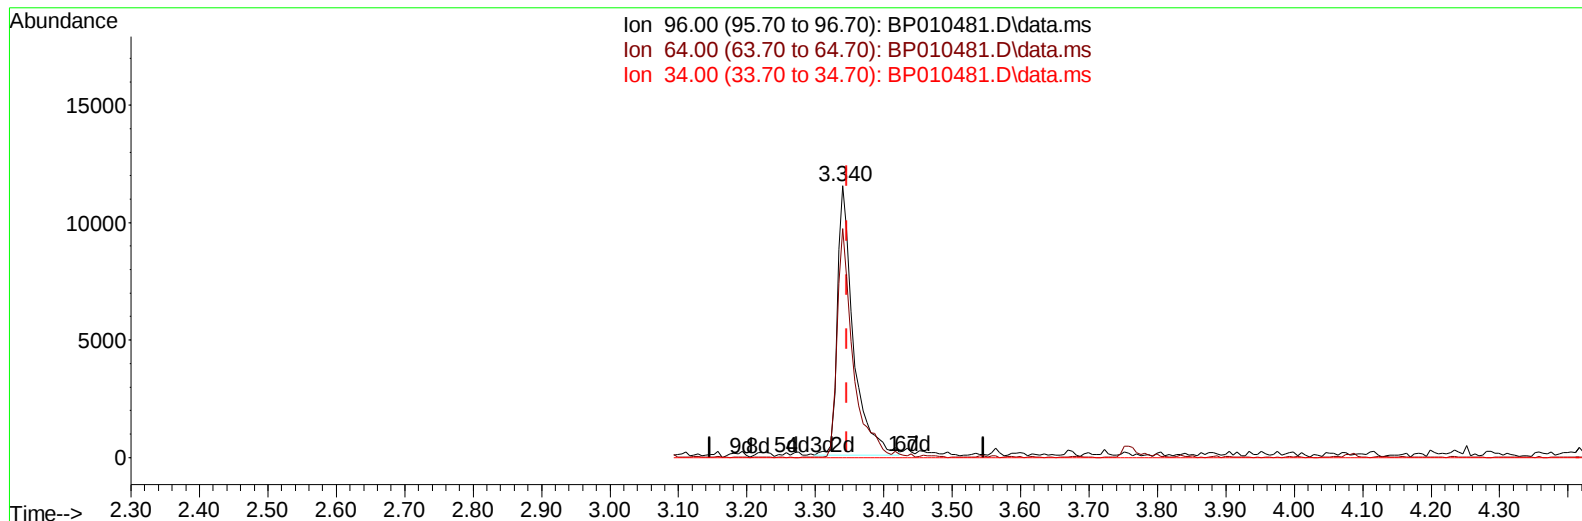

TIC: BP010481.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.006) 5.01 ng/uL m

response 18738

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	84.19#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010481.D
Acq On : 23 May 2022 17:43
Operator : CG/JU
Sample : PB144963BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Quant Time: May 23 23:20:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

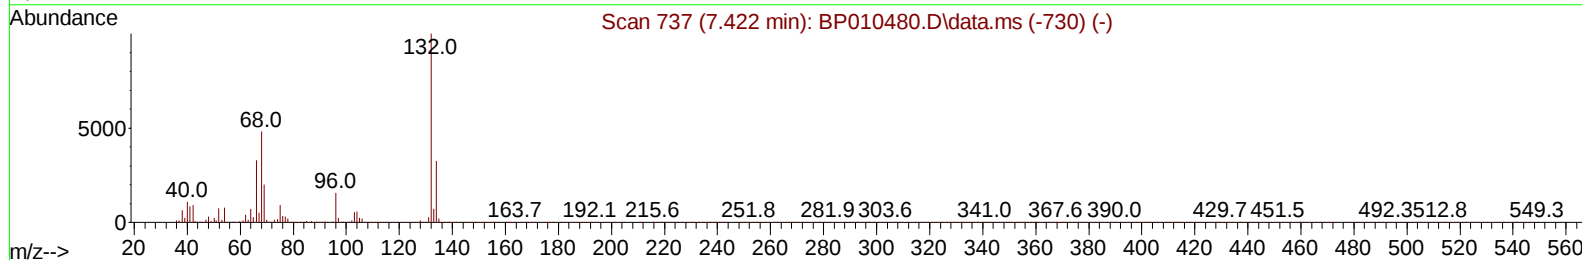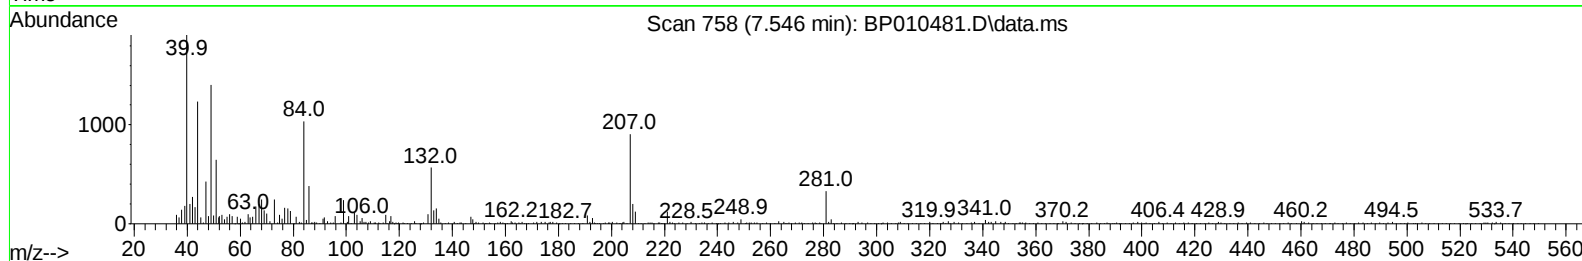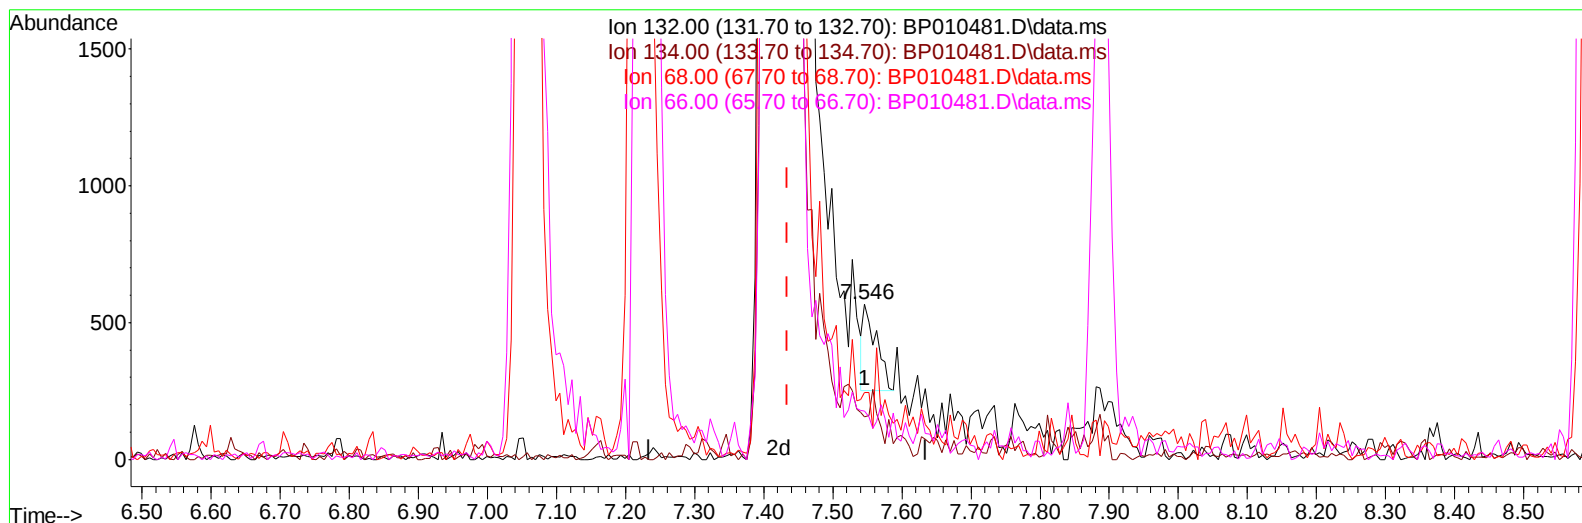

TIC: BP010481.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.546min (+ 0.112) 0.04 ng/u1

response 417

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	27.64
68.00	51.40	43.31
66.00	26.30	30.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010481.D
Acq On : 23 May 2022 17:43
Operator : CG/JU
Sample : PB144963BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 23 23:20:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

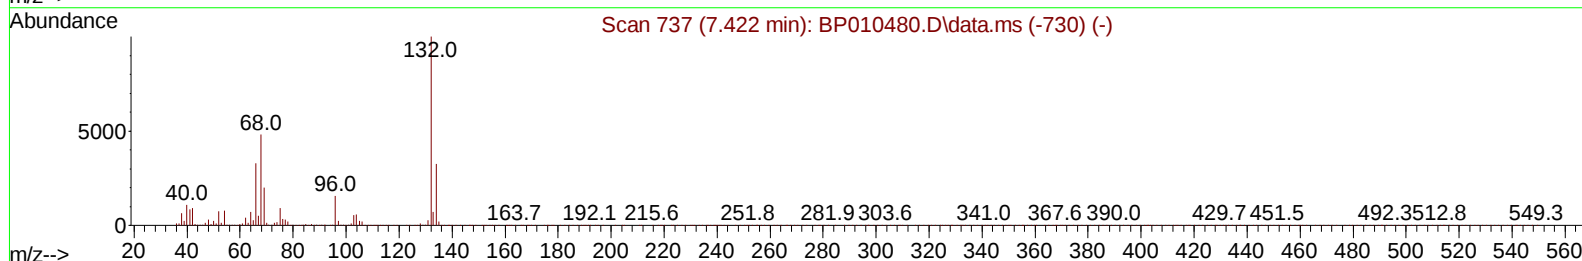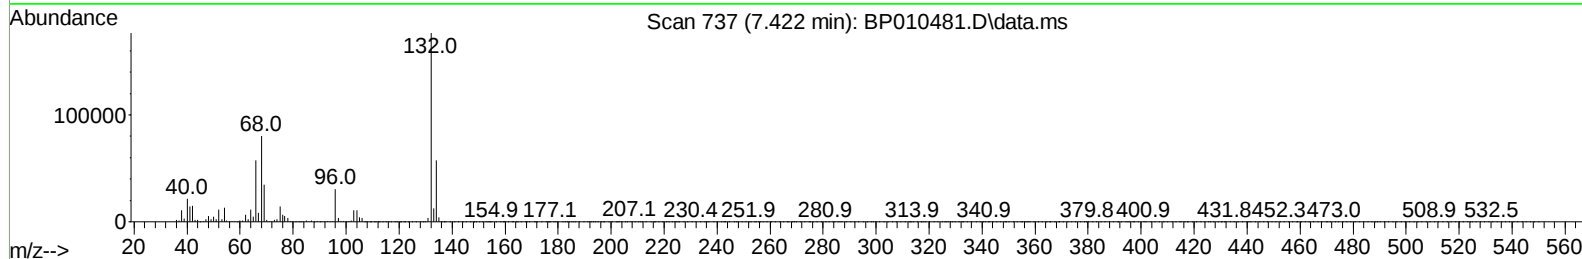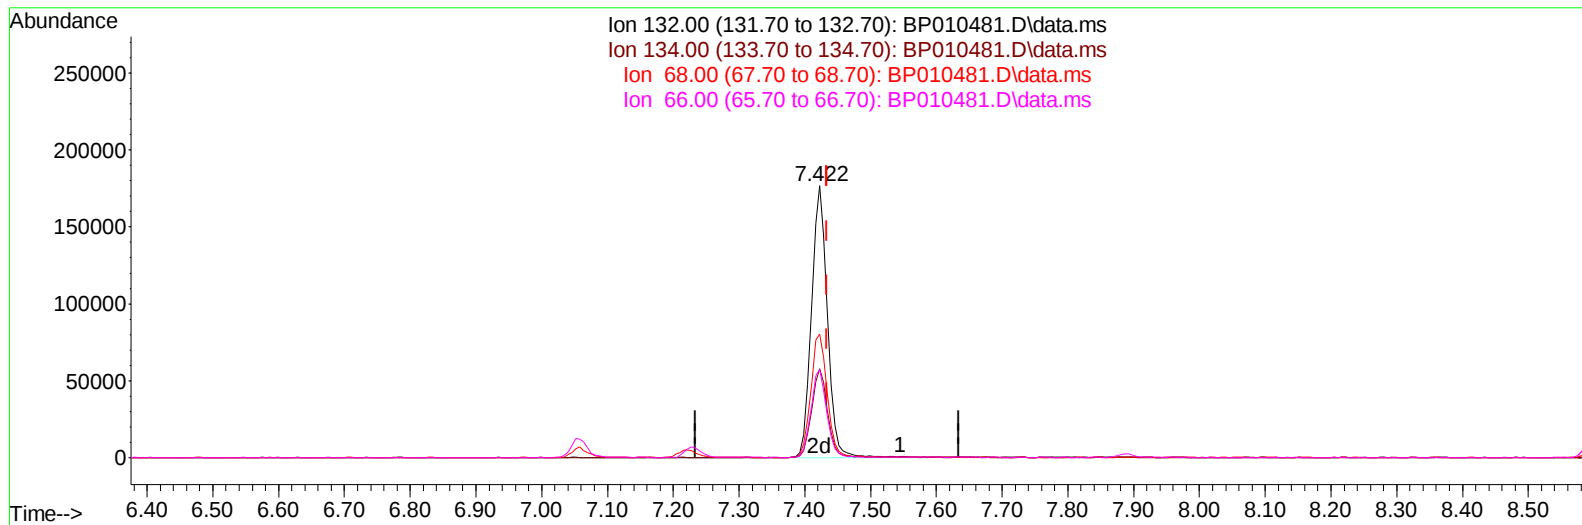

TIC: BP010481.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.422min (-0.012) 28.71 ng/u1 m

response 293966

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	32.71
68.00	51.40	45.43
66.00	26.30	32.46#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010481.D
 Acq On : 23 May 2022 17:43
 Operator : CG/JU
 Sample : PB144963BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: May 23 23:20:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

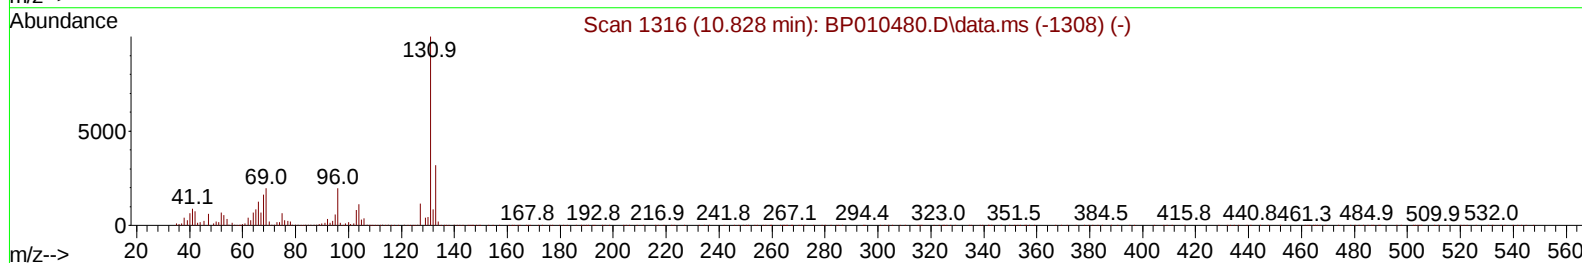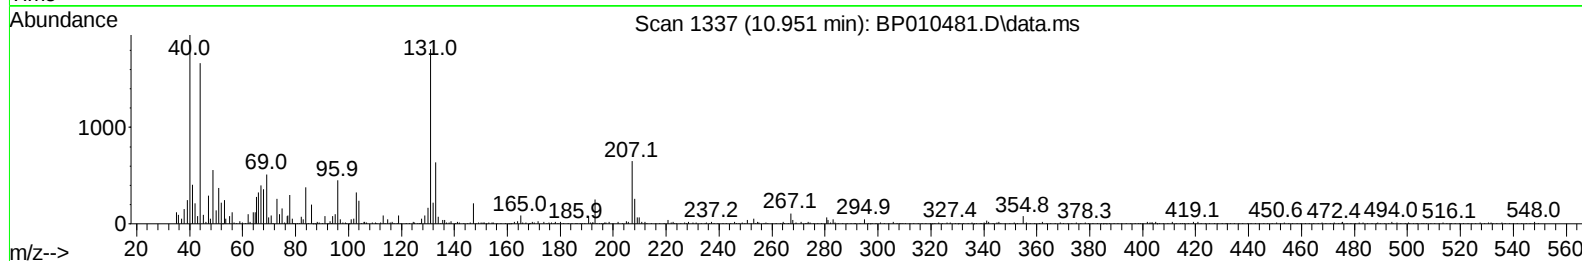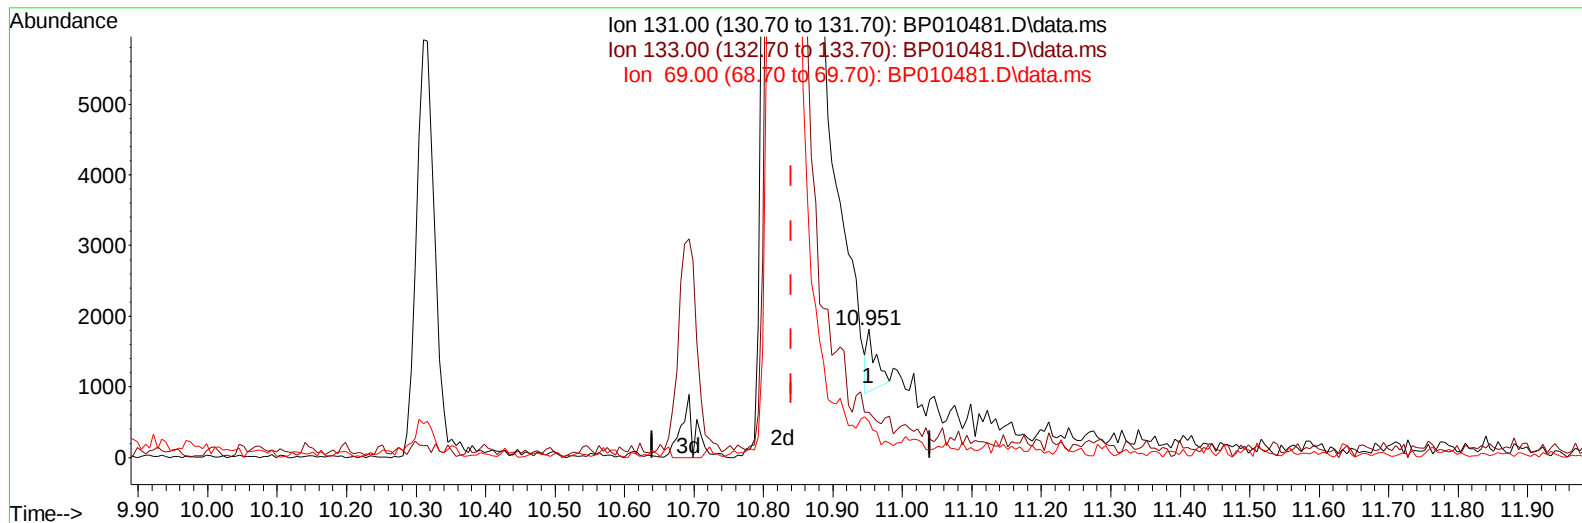

TIC: BP010481.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.951min (+ 0.112) 0.05 ng/u1

response 773

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	35.02
69.00	26.10	28.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010481.D
 Acq On : 23 May 2022 17:43
 Operator : CG/JU
 Sample : PB144963BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: May 23 23:20:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

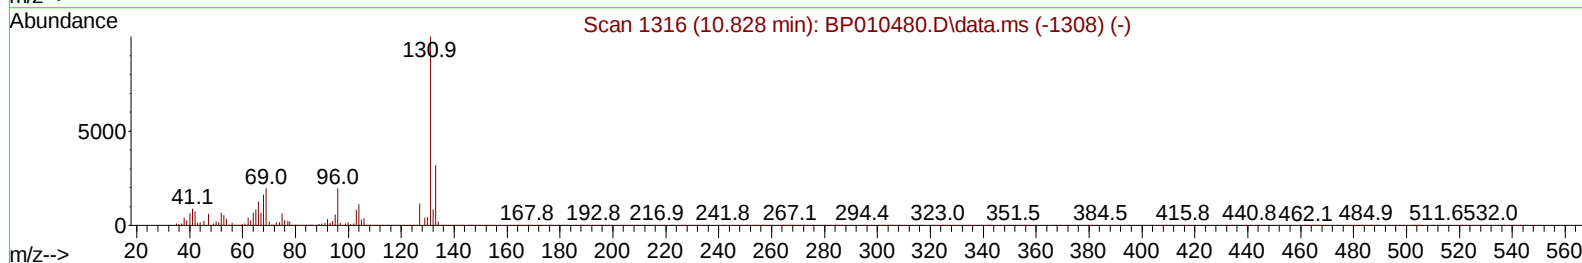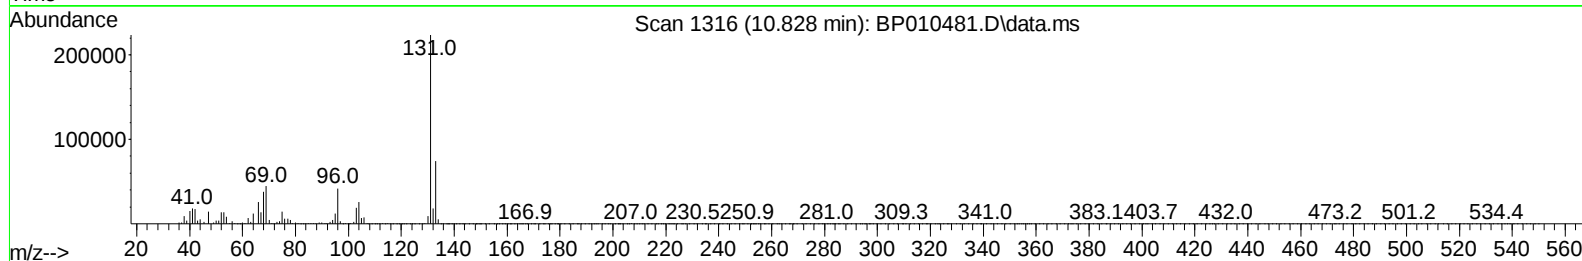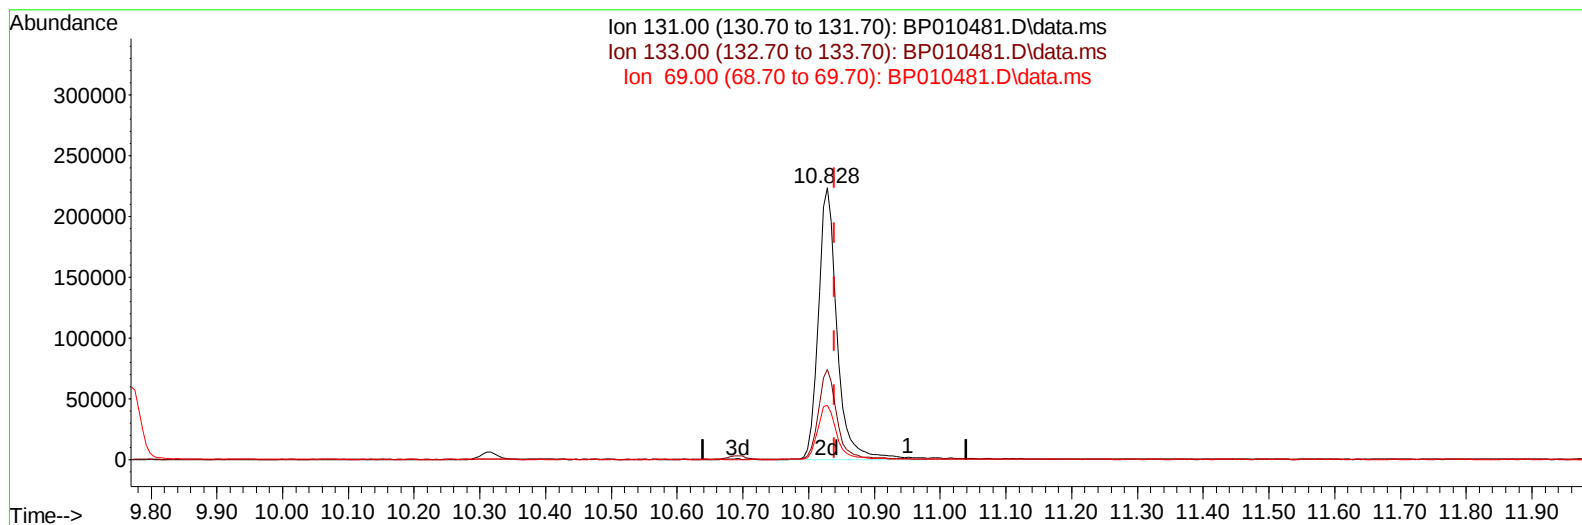

TIC: BP010481.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.828min (-0.012) 25.91 ng/ul m

response 438831

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	33.14
69.00	26.10	19.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010481.D
 Acq On : 23 May 2022 17:43
 Operator : CG/JU
 Sample : PB144963BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 23 23:20:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 13 15:04:31 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.887	152		159417	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.693	136		734494	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164		499136	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.275	188		1061699	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.357	240		926470	20.000	ng/ul	# 0.00
88) Perylene-d12	23.774	264		696912	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.340	96		18738m	5.010	ng/uL	0.00
4) Pyridine-d5	3.758	84		283616	26.707	ng/ul	0.00
7) Phenol-d5	7.058	99		360124	26.915	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67		251860	28.016	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.422	132		293966m	28.712	ng/ul	-0.01
15) 4-Methylphenol-d8	8.599	113		318004	27.966	ng/ul	-0.01
21) Nitrobenzene-d5	9.046	128		162735	28.628	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.769	143		174541	28.973	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.310	165		295931	25.980	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.828	131		438831m	25.910	ng/ul	-0.01
46) Dimethylphthalate-d6	13.934	166		1030548	28.023	ng/ul	0.00
49) Acenaphthylene-d8	14.216	160		1190745	28.071	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143		133573	20.406	ng/ul	0.00
60) Fluorene-d10	15.516	176		887264	27.733	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200		125925	20.280	ng/ul	0.00
73) Anthracene-d10	17.375	188		1390059	28.914	ng/ul	0.00
81) Pyrene-d10	19.604	212		1673722	34.017	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.621	264		1089374	31.130	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010481.D
Acq On : 23 May 2022 17:43
Operator : CG/JU
Sample : PB144963BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 23 23:20:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 13 15:04:31 2022
Response via : Initial Calibration

