




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010502.D
 Acq On : 24 May 2022 06:10
 Operator : CG/JU
 Sample : PB145034BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK034

Manual IntegrationsAPPROVED

Quant Time: May 24 07:01:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

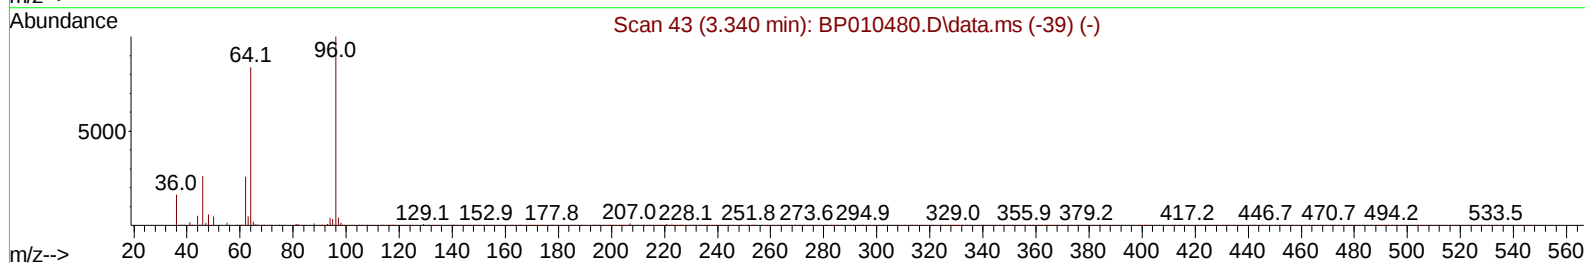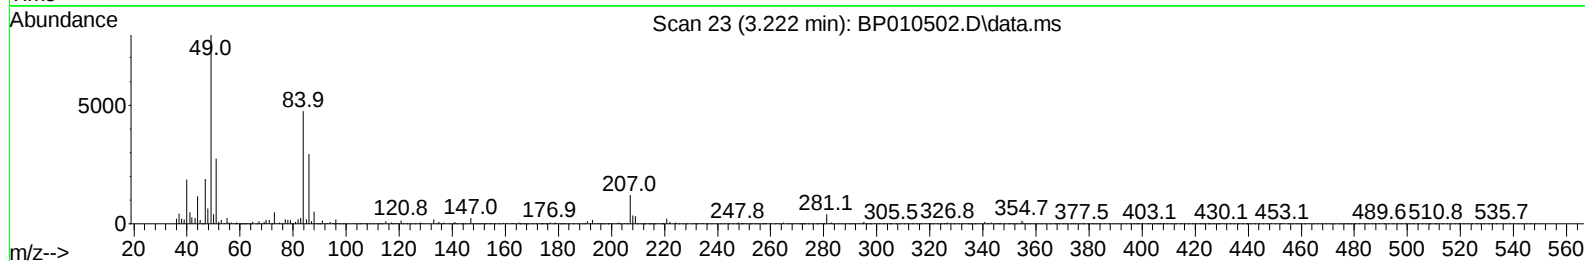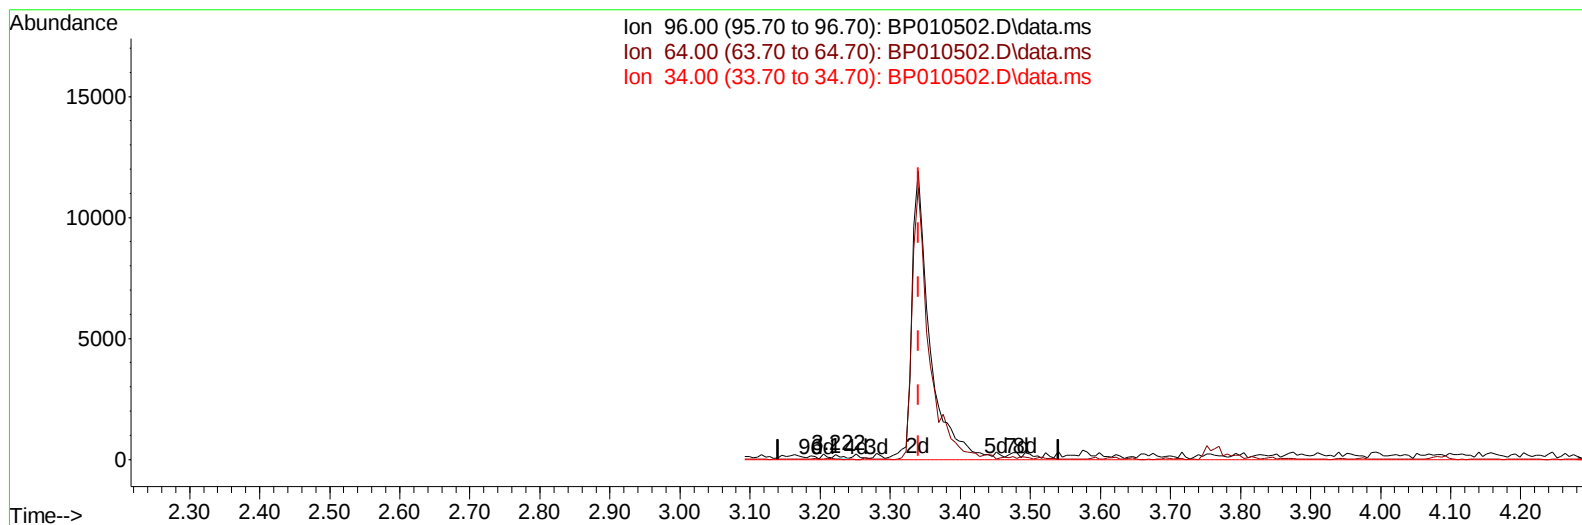

TIC: BP010502.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.222min (-0.118) 0.02 ng/uL

response 92

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	53.30
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010502.D
 Acq On : 24 May 2022 06:10
 Operator : CG/JU
 Sample : PB145034BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK034

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 07:01:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

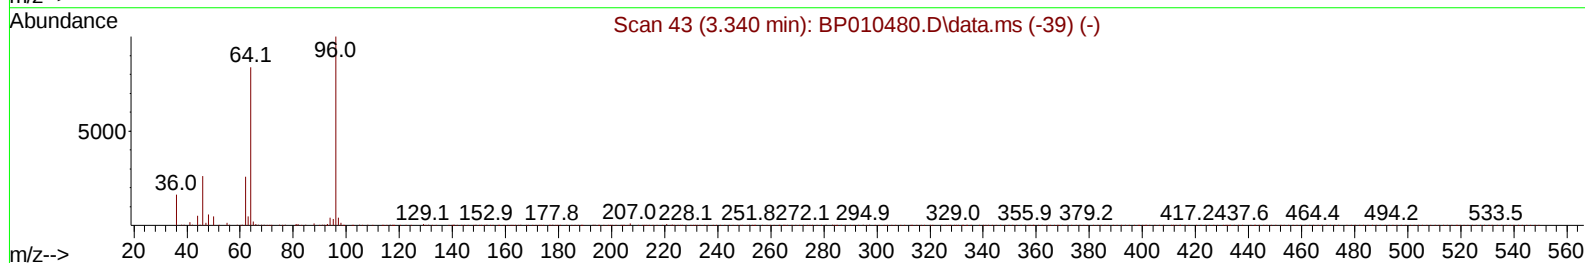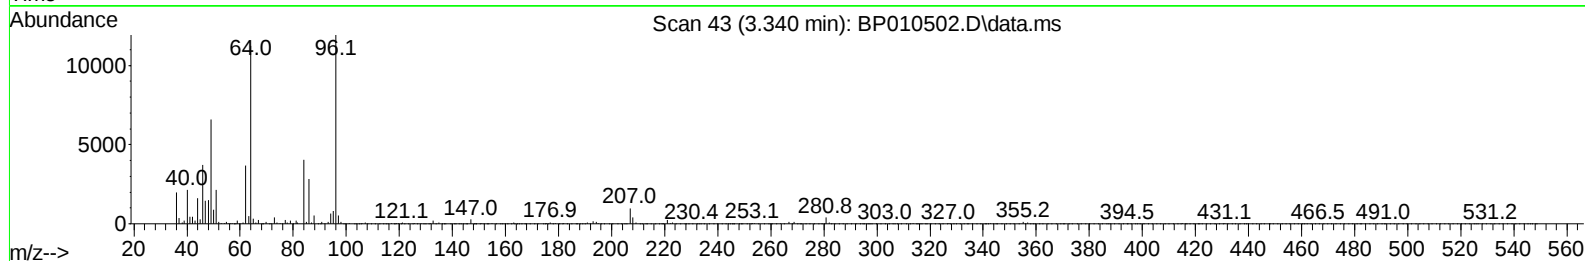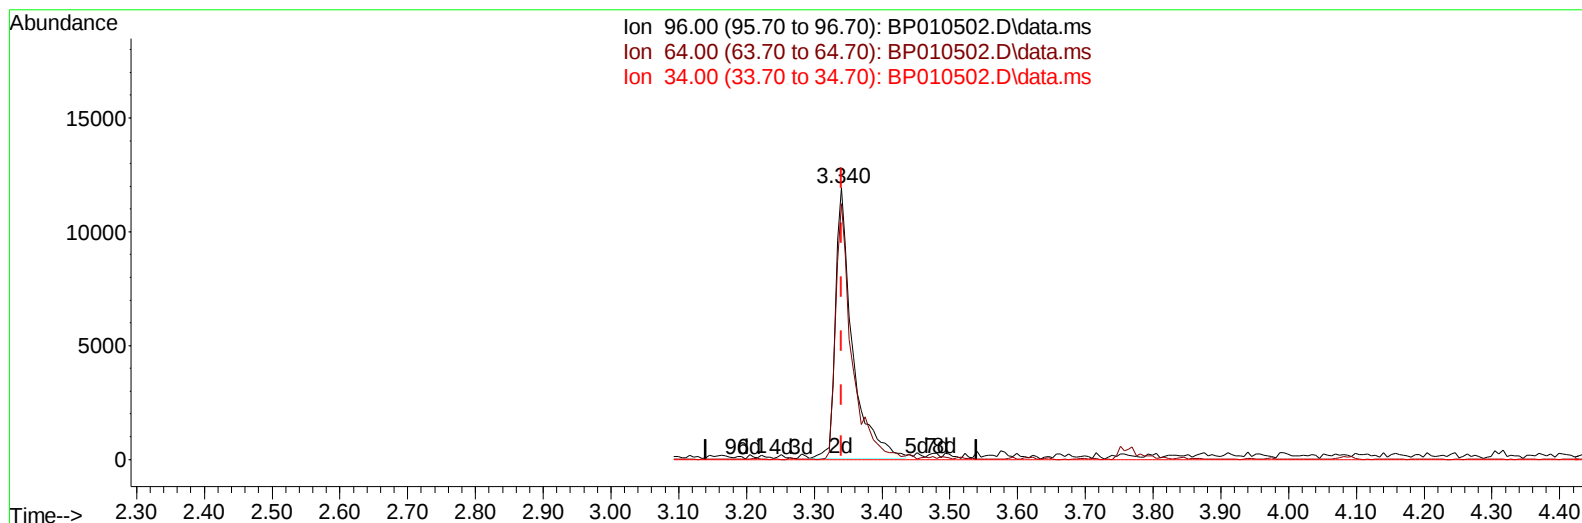

TIC: BP010502.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-0.000) 5.53 ng/uL m

response 20796

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	94.09#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 07:01:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

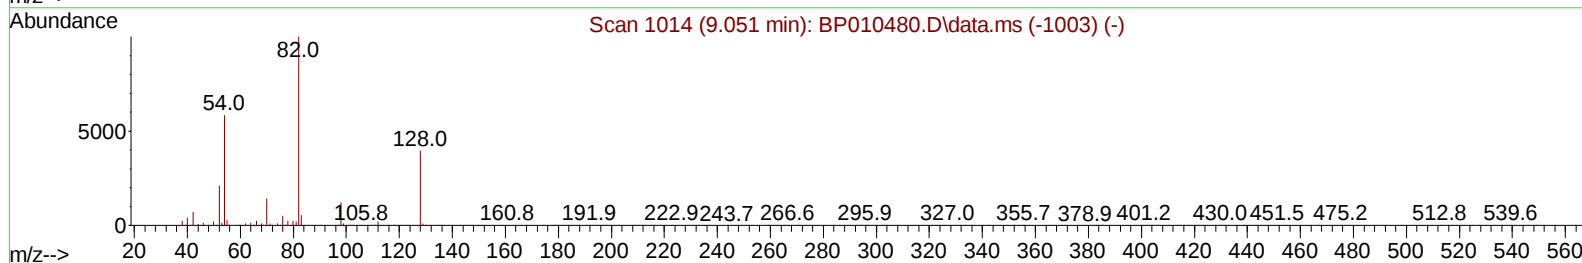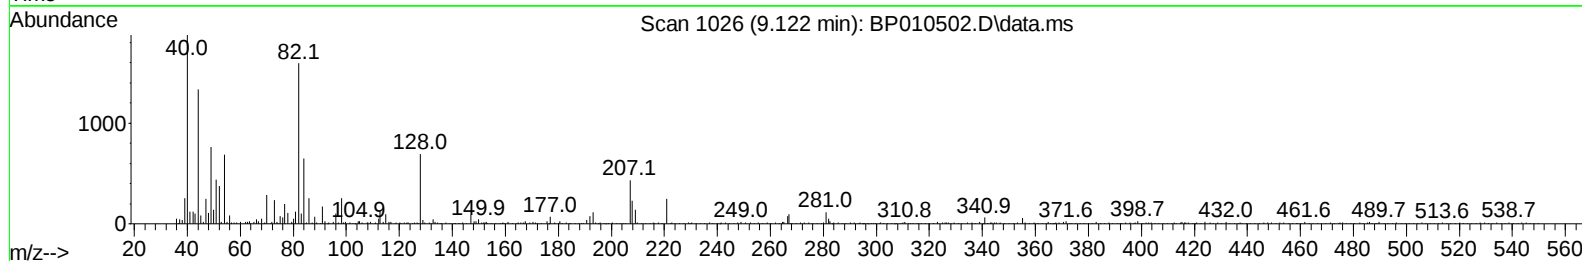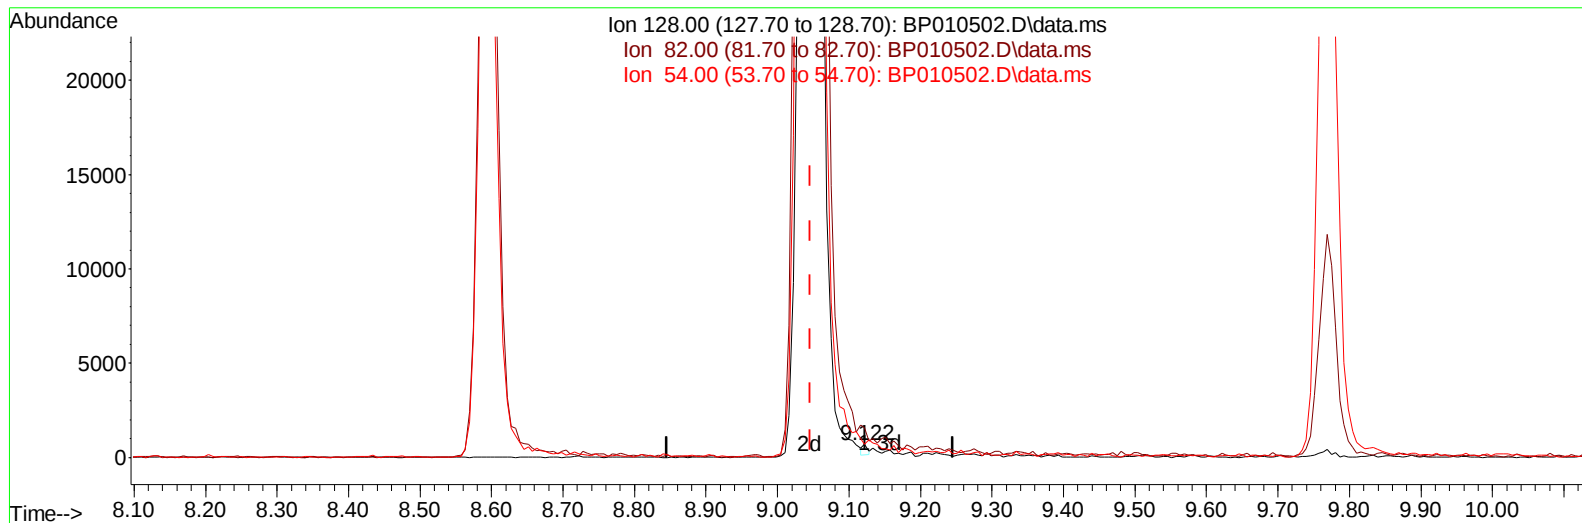

TIC: BP010502.D\data.ms

(21) Nitrobenzene-d5 (S)

9.122min (+ 0.076) 0.05 ng/u1

response 262

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	229.97
54.00	120.20	98.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 07:01:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

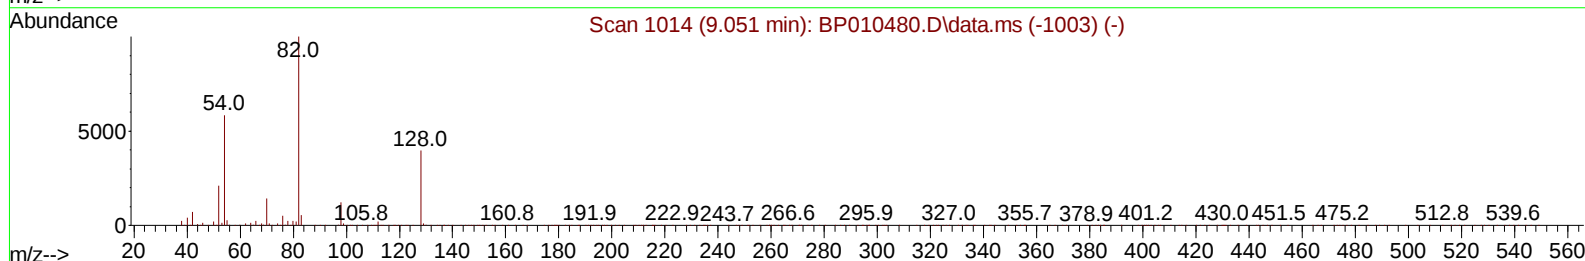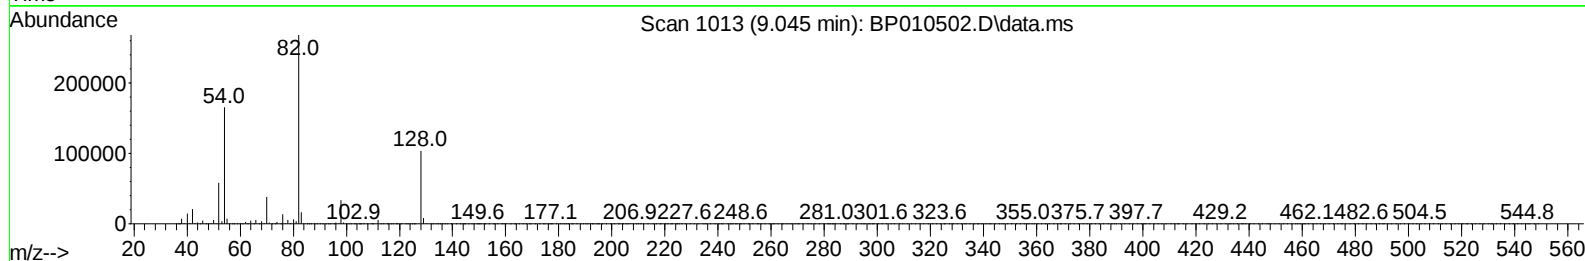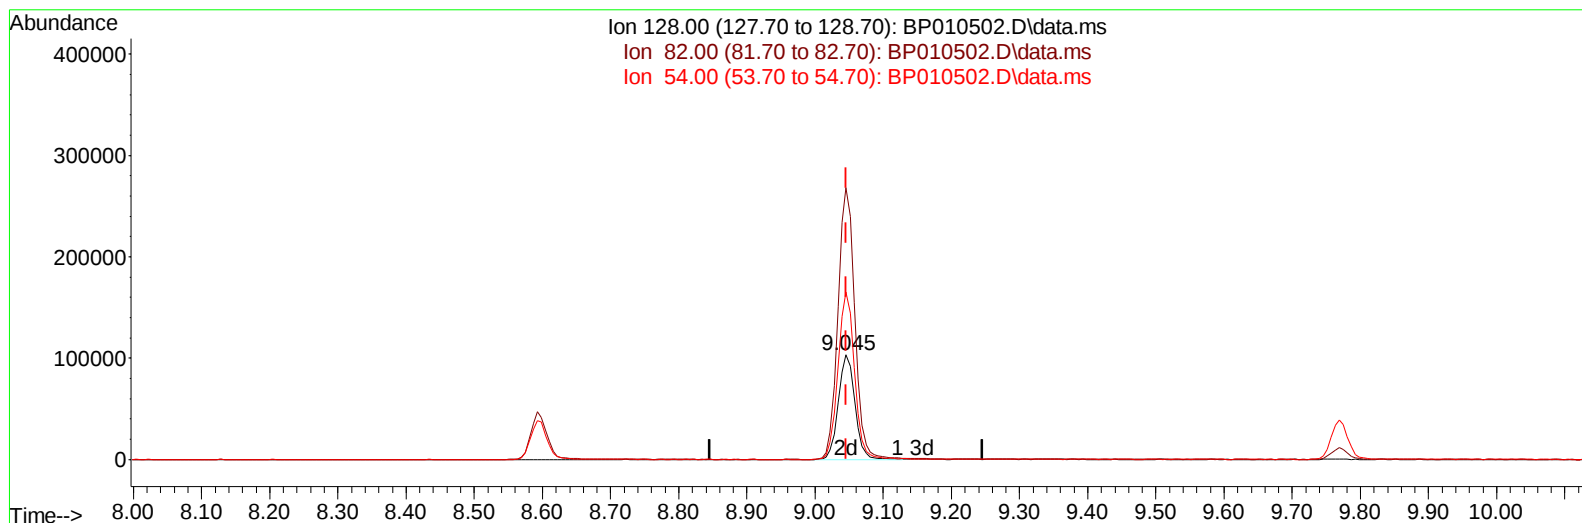

TIC: BP010502.D\data.ms

(21) Nitrobenzene-d5 (S)

9.045min (-0.000) 30.60 ng/u1 m

response 175575

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	258.80
54.00	120.20	159.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 07:01:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

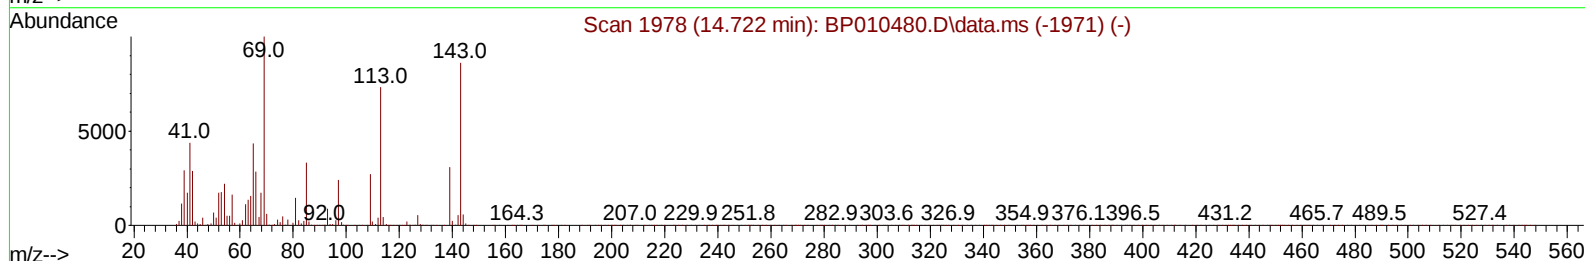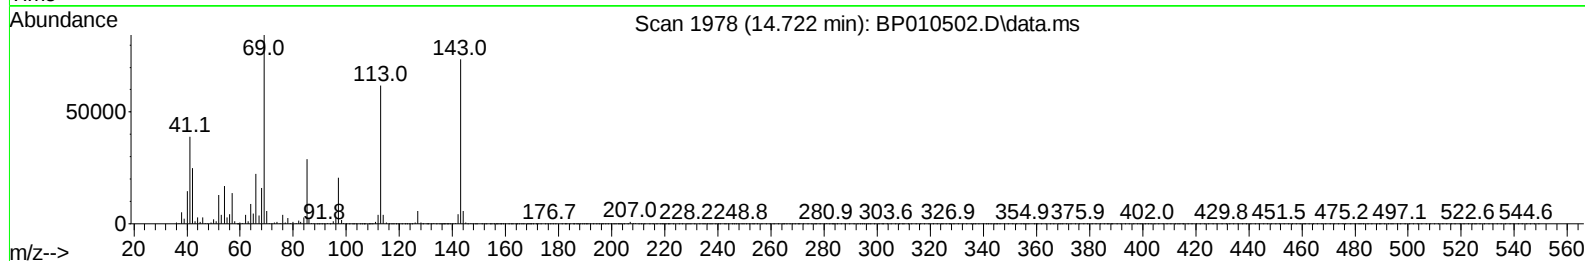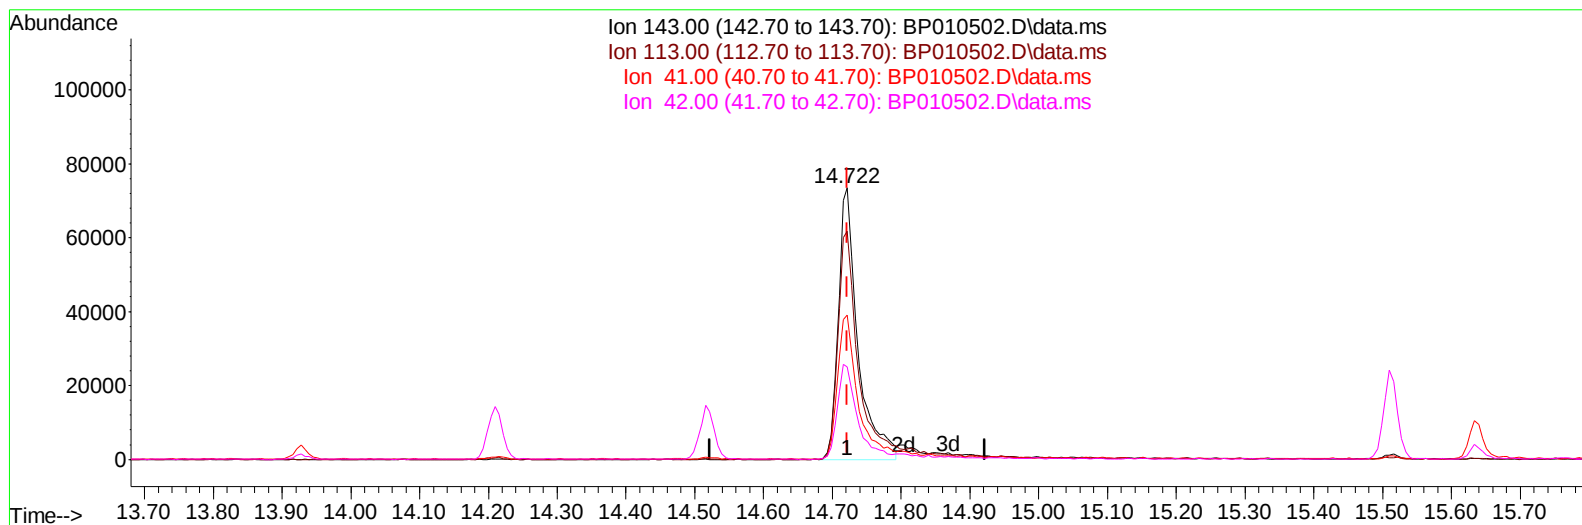

TIC: BP010502.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.722min (-0.000) 21.75 ng/u1****response 145323**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.09#
41.00	23.20	53.14#
42.00	18.00	34.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 07:01:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

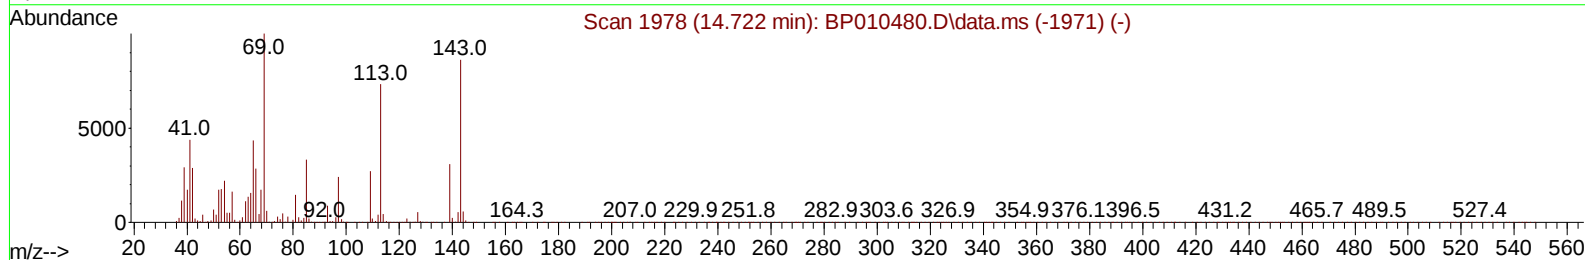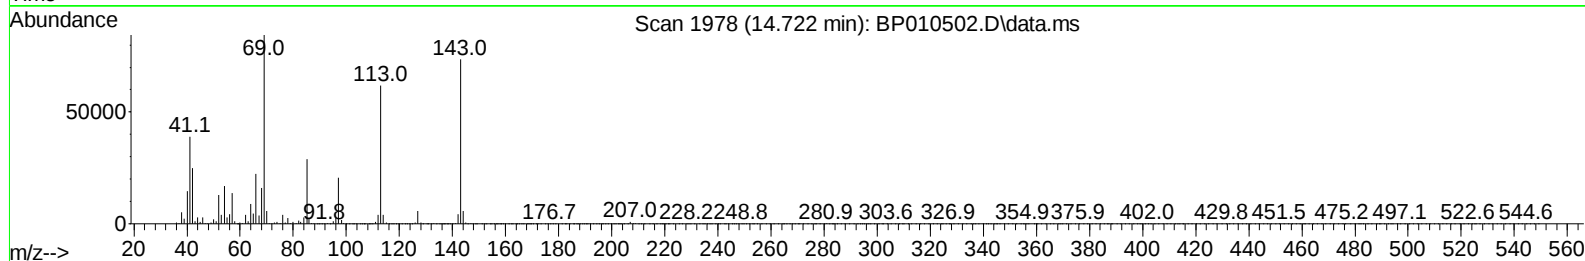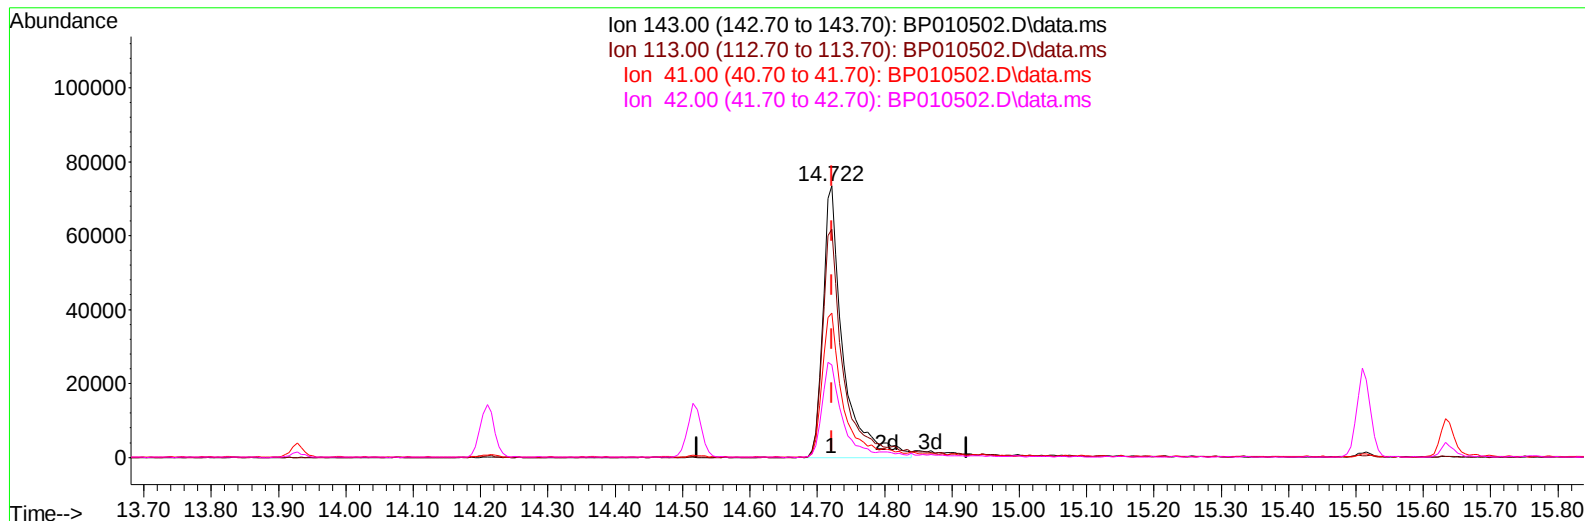

TIC: BP010502.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.722min (-0.000) 22.92 ng/ul m

response 153110

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	84.09#
41.00	23.20	53.14#
42.00	18.00	34.00#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010502.D
 Acq On : 24 May 2022 06:10
 Operator : CG/JU
 Sample : PB145034BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK034

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
 Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 07:01:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	160421	20.000	ng/ul	0.00
20) Naphthalene-d8	10.687	136	741436	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.516	164	509396	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.269	188	1076677	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.351	240	922045	20.000	ng/ul	# 0.00
88) Perylene-d12	23.774	264	714884	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	20796m	5.526	ng/uL	0.00
4) Pyridine-d5	3.757	84	316165	29.586	ng/ul	0.00
7) Phenol-d5	7.051	99	396933	29.480	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	272554	30.129	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	318648	30.928	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	345721	30.213	ng/ul	0.00
21) Nitrobenzene-d5	9.045	128	175575m	30.597	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	190335	31.299	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	333153	28.973	ng/ul	0.00
31) 4-Chloroaniline-d4	10.822	131	467019	27.316	ng/ul	0.00
46) Dimethylphthalate-d6	13.928	166	1161051	30.936	ng/ul	0.00
49) Acenaphthylene-d8	14.210	160	1336188	30.866	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	153110m	22.920	ng/ul	0.00
60) Fluorene-d10	15.510	176	996402	30.517	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.639	200	135608	21.536	ng/ul	0.00
73) Anthracene-d10	17.369	188	1603812	32.896	ng/ul	0.00
81) Pyrene-d10	19.604	212	1865658	38.100	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.615	264	1213372	33.802	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/24/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 07:01:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

