




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

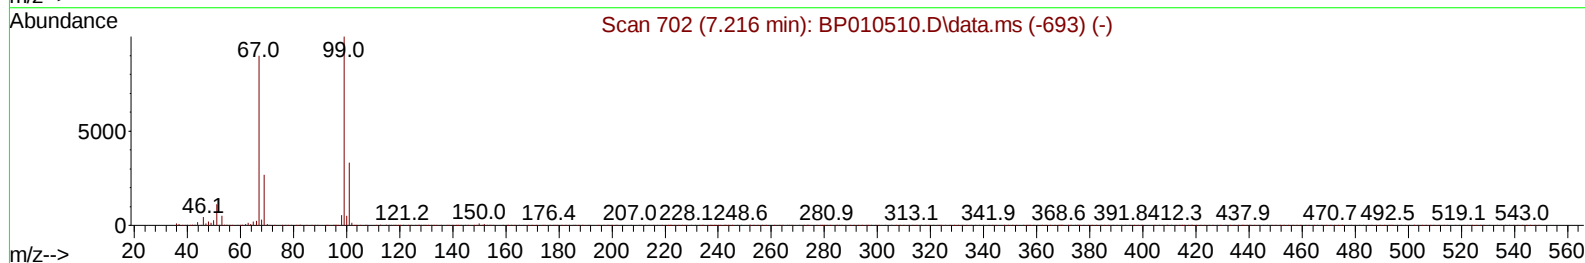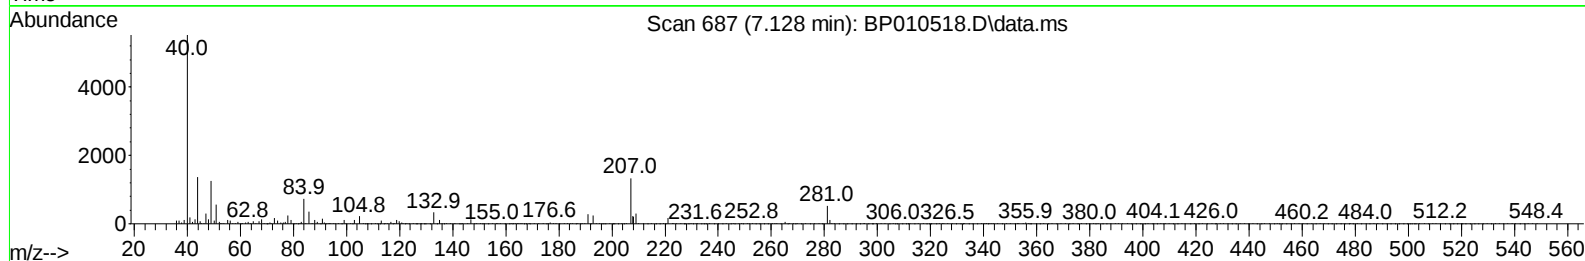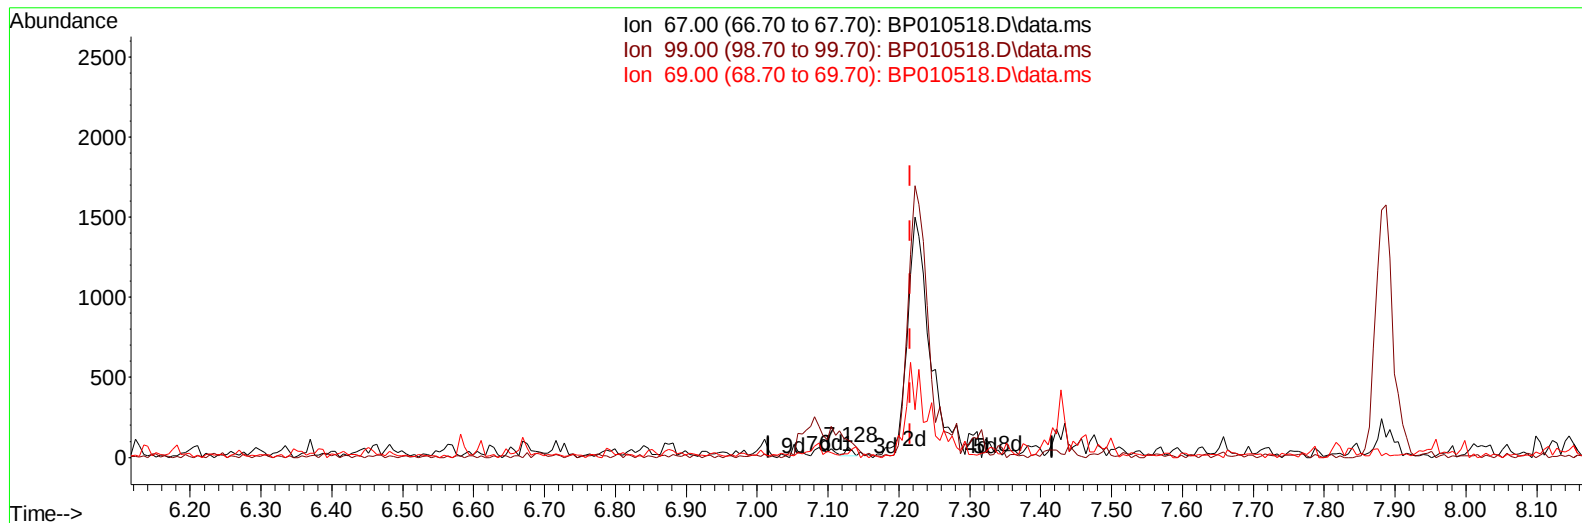

TIC: BP010518.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.128min (-0.088) 0.00 ng/u1

response	36	
Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	161.76
69.00	40.10	32.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

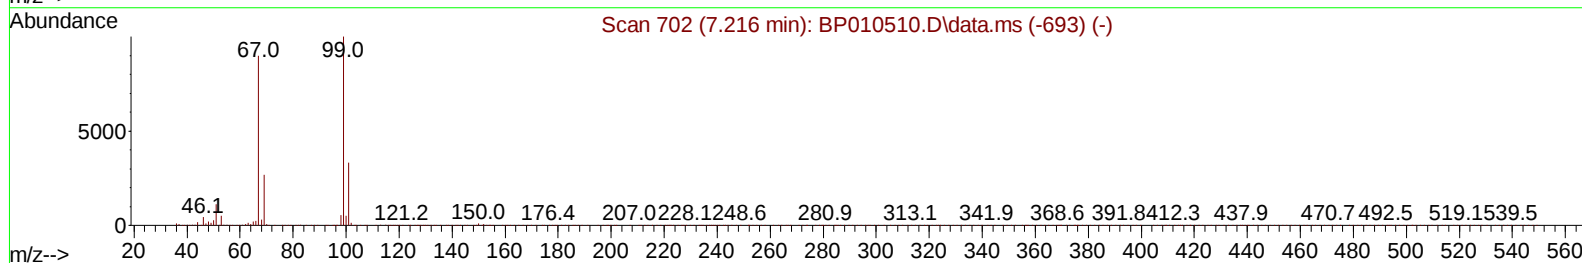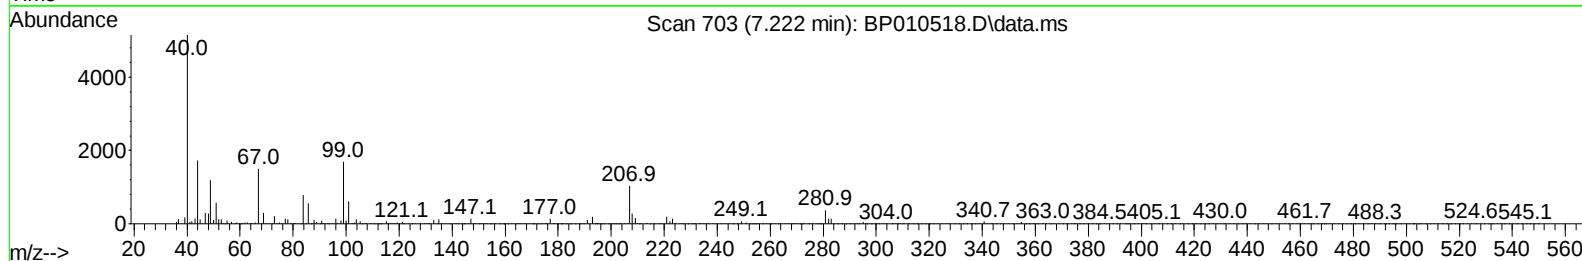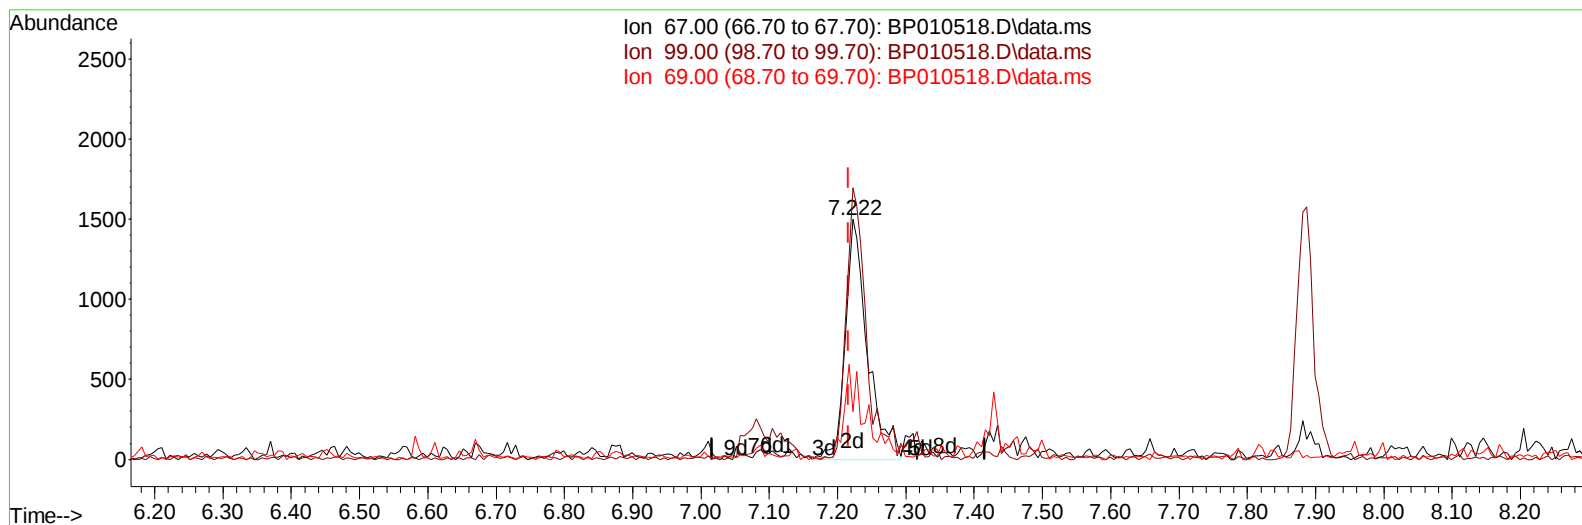

TIC: BP010518.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.222min (+ 0.006) 0.38 ng/ul m

response 3385

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	112.99#
69.00	40.10	19.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

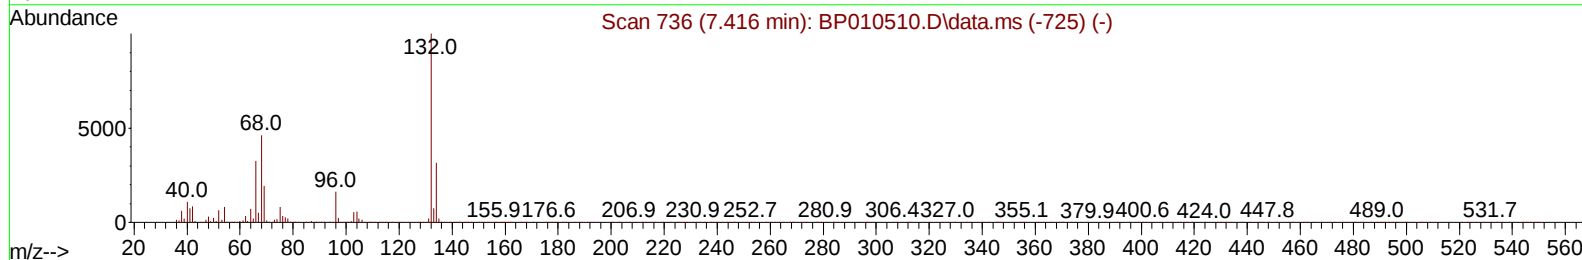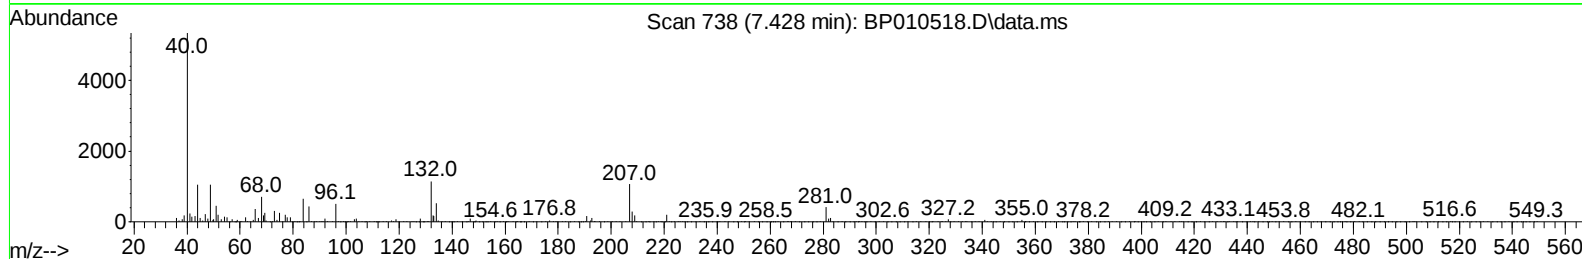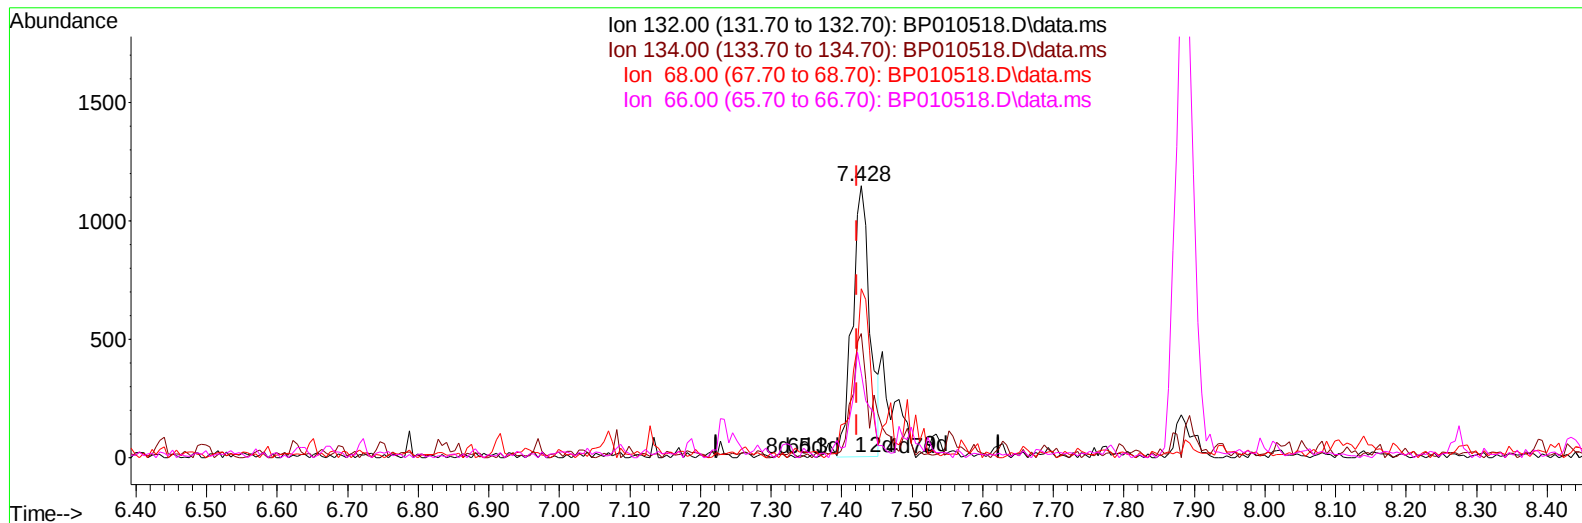

TIC: BP010518.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.428min (+ 0.006) 0.20 ng/u1

response 2001

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	45.68#
68.00	51.40	62.07#
66.00	26.30	30.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010518.D
Acq On : 24 May 2022 16:18
Operator : CG/JU
Sample : N2950-03DL2 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :Yogesh Patel 05/26/2022

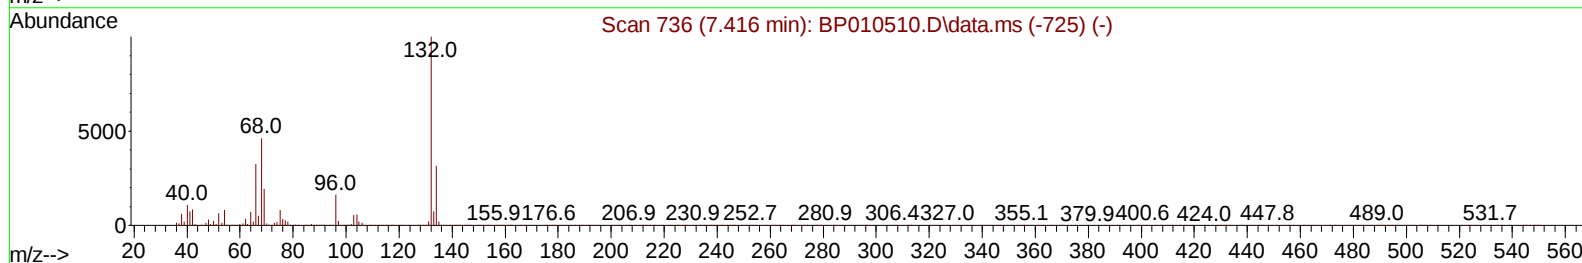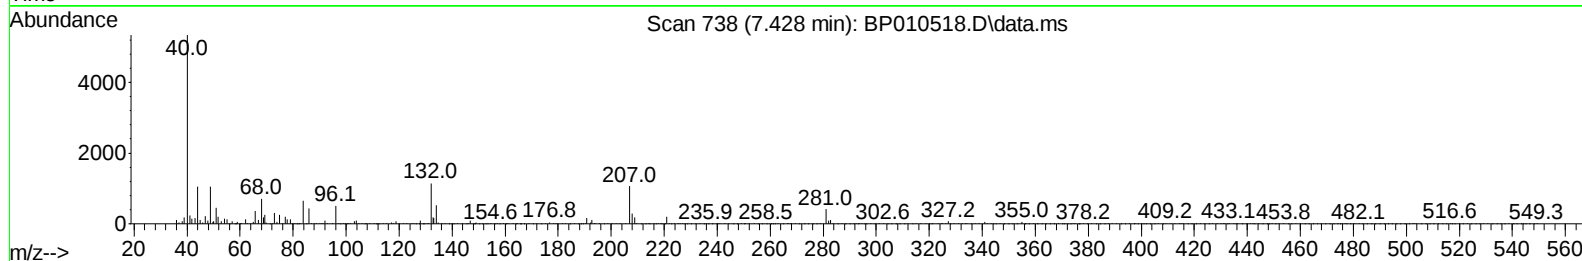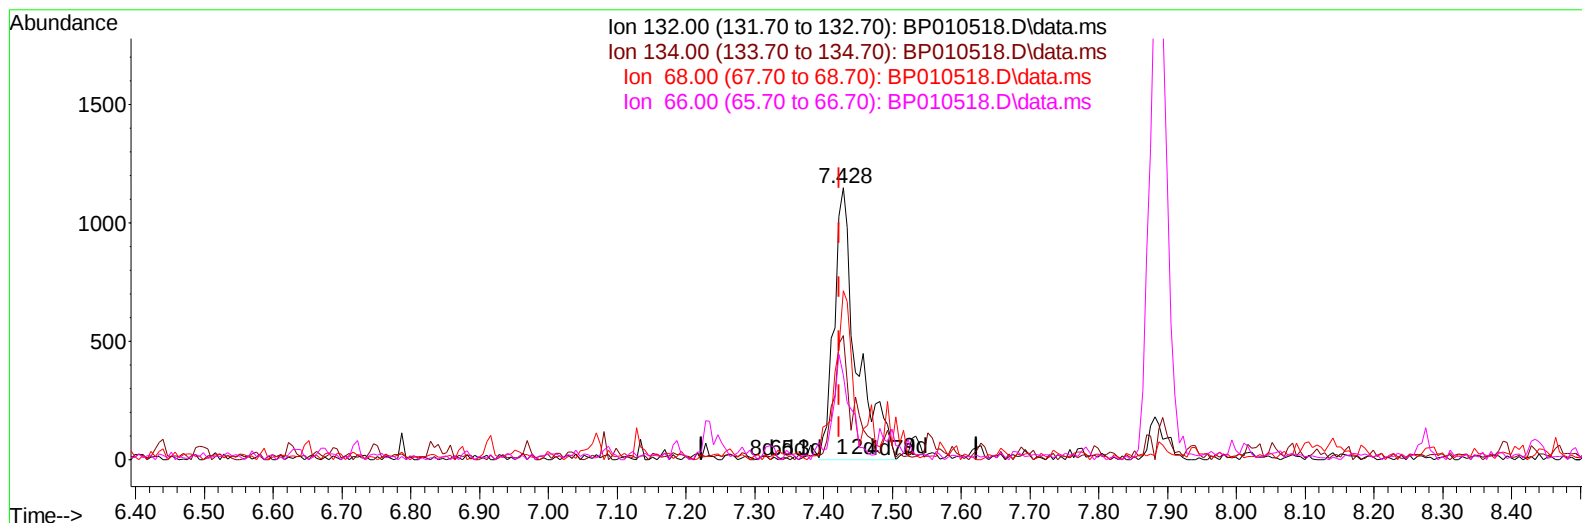

TIC: BP010518.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.428min (+ 0.006) 0.26 ng/ul m

response 2616

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	45.68#
68.00	51.40	62.07#
66.00	26.30	30.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

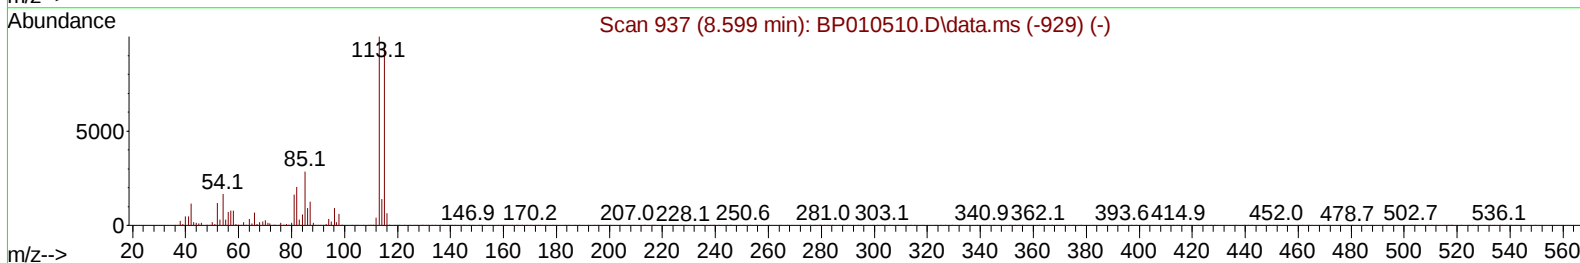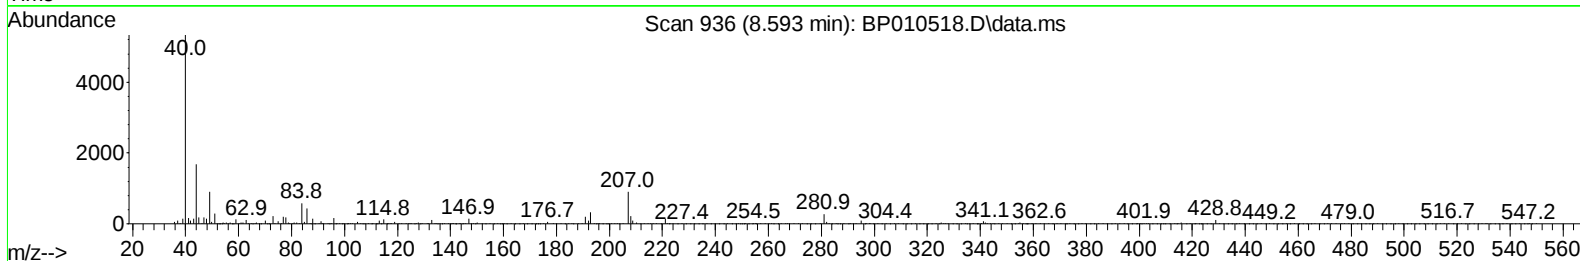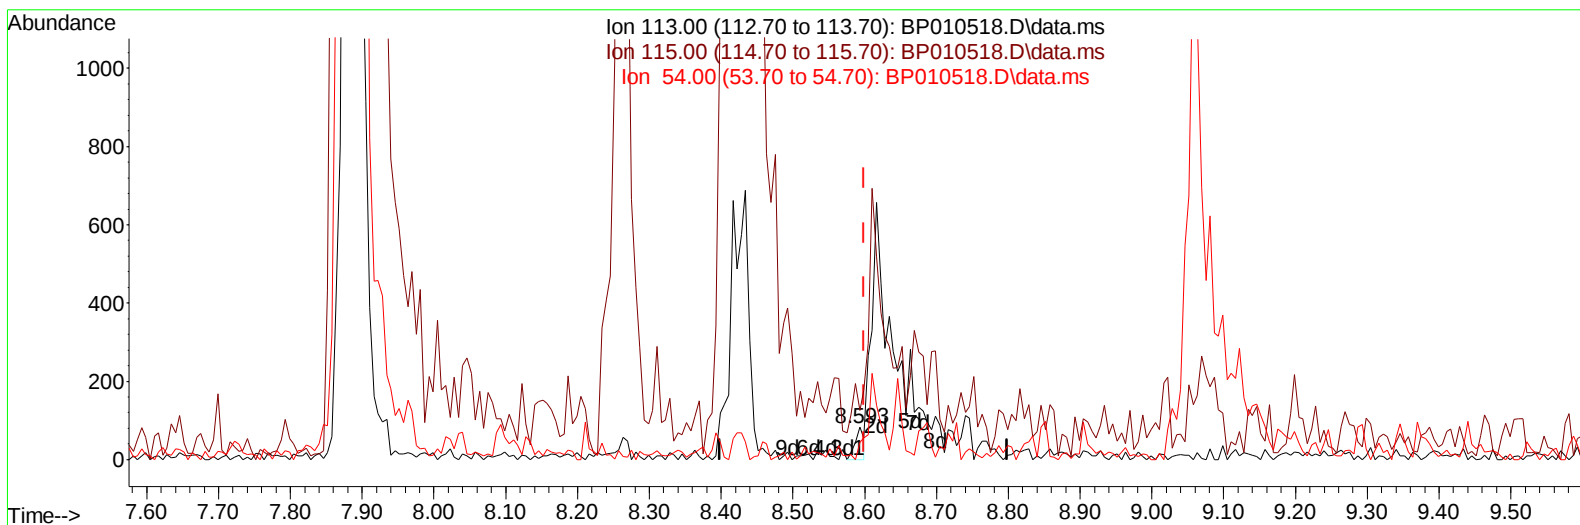

TIC: BP010518.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.593min (-0.006) 0.01 ng/u1

response 71

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	106.70	150.60#
54.00	4.50	81.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

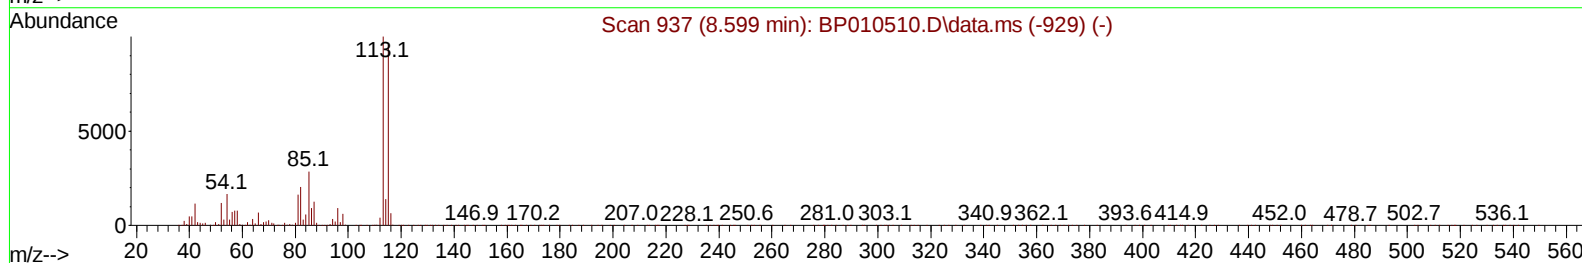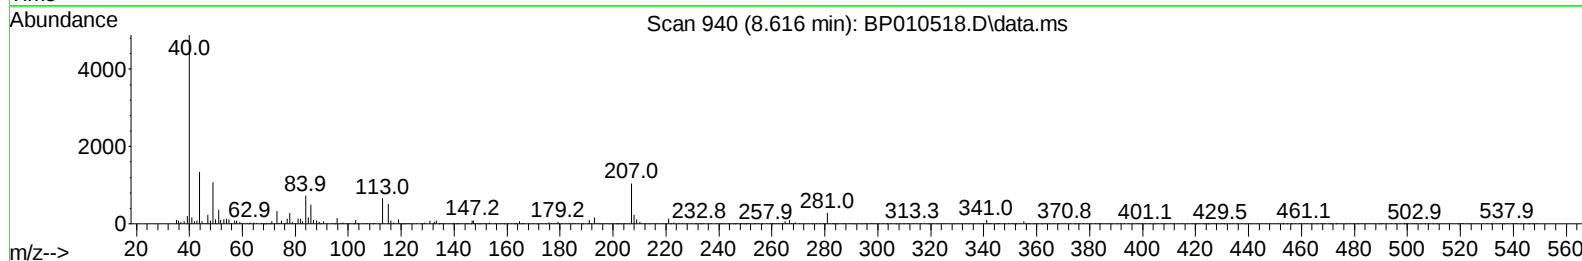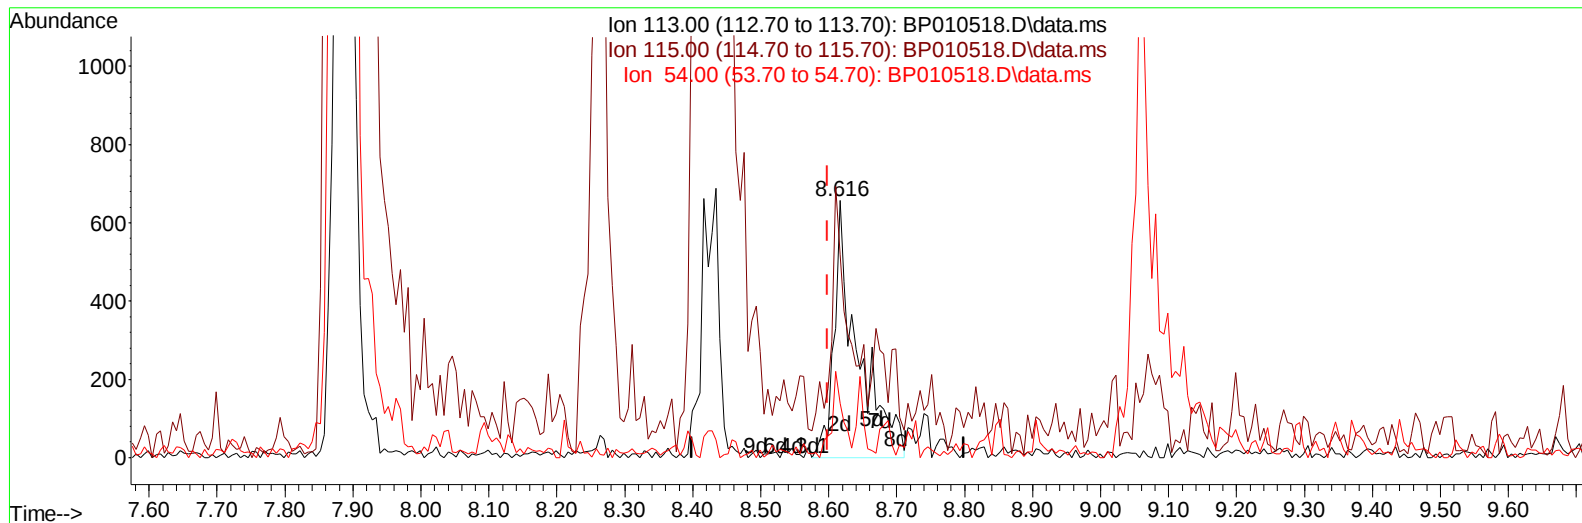

TIC: BP010518.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.616min (+ 0.018) 0.14 ng/ul m

response 1579

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	106.70	79.00#
54.00	4.50	21.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

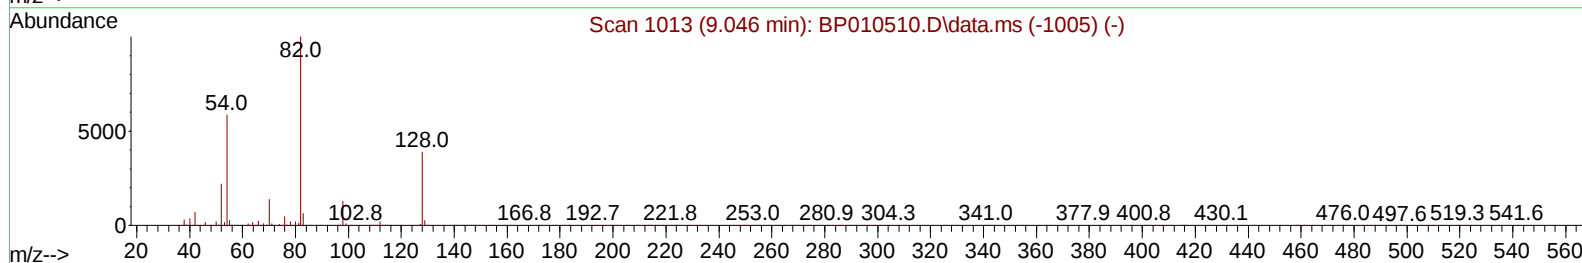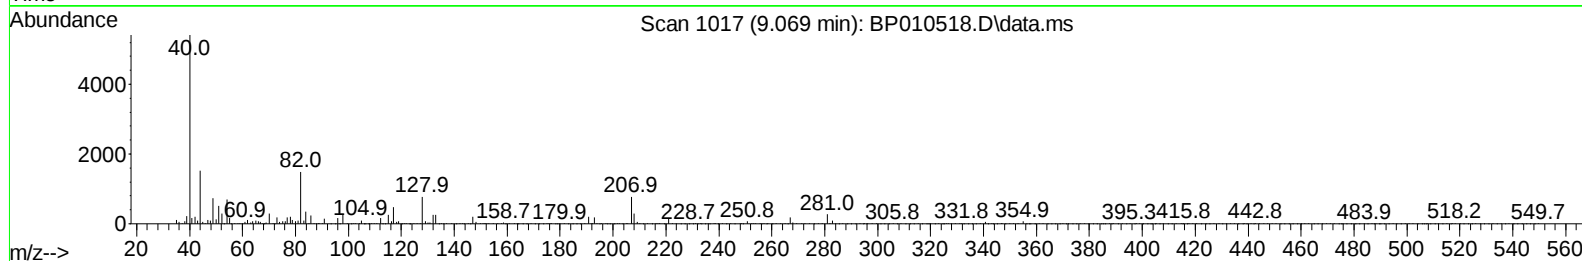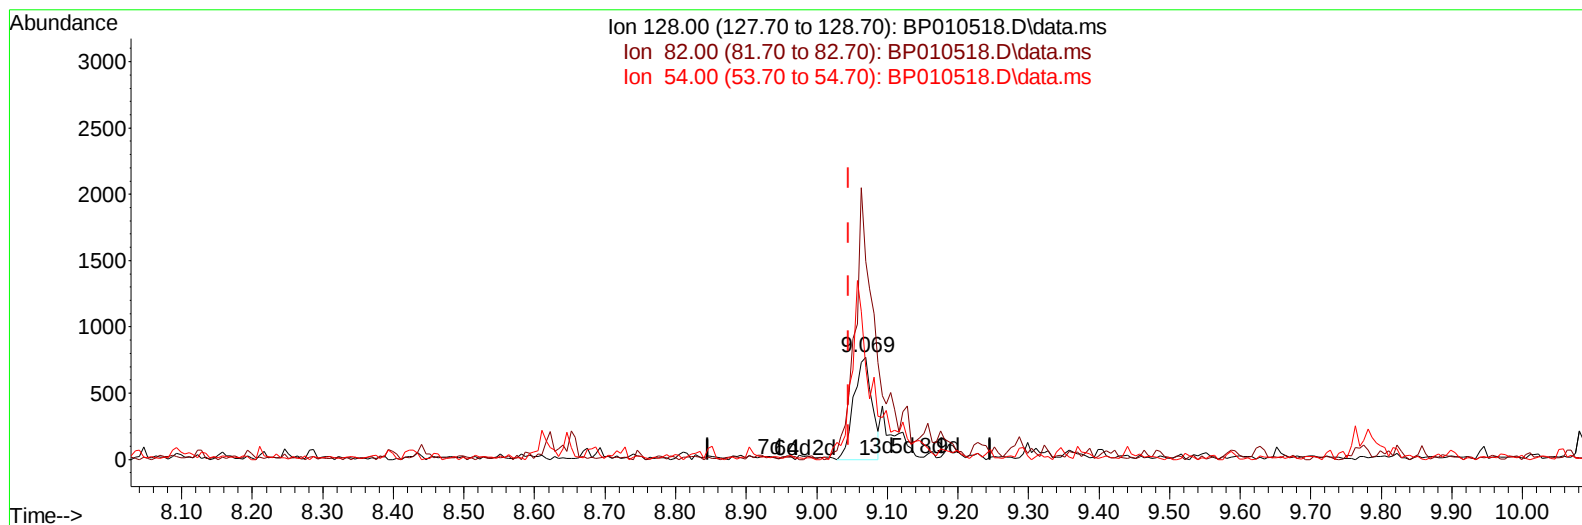

TIC: BP010518.D\data.ms

(21) Nitrobenzene-d5 (S)

9.069min (+ 0.024) 0.25 ng/u1

response 1394

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	193.90#
54.00	120.20	90.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

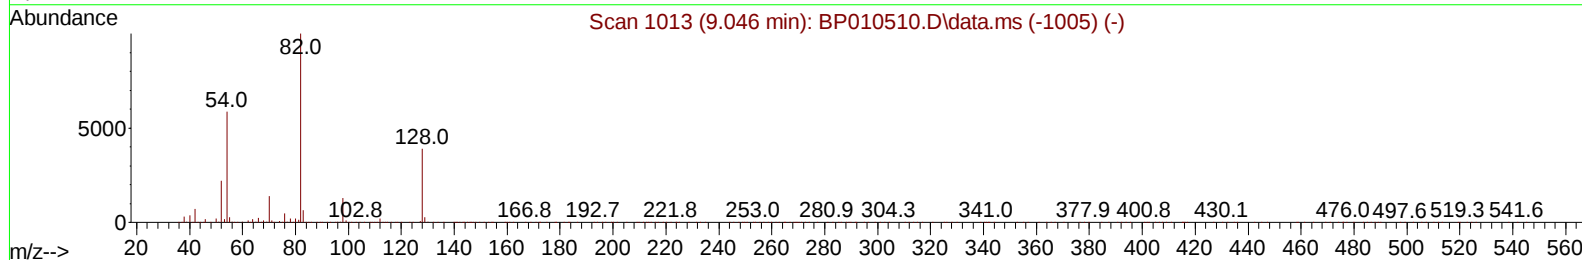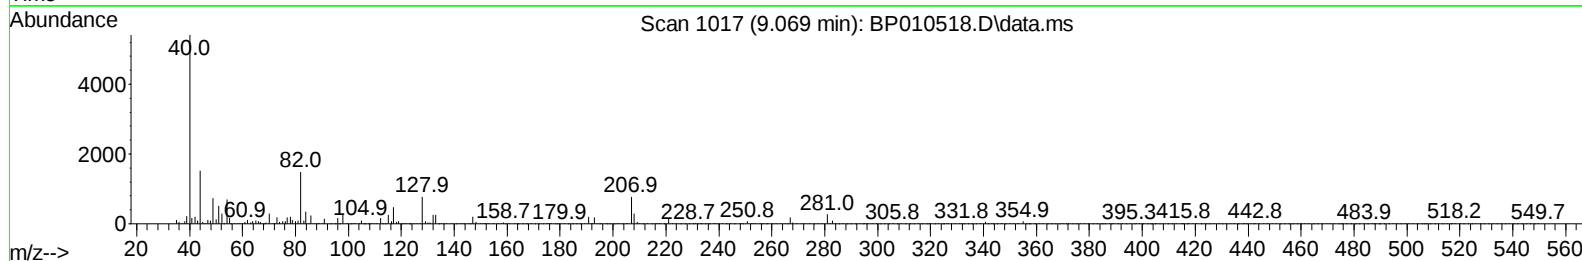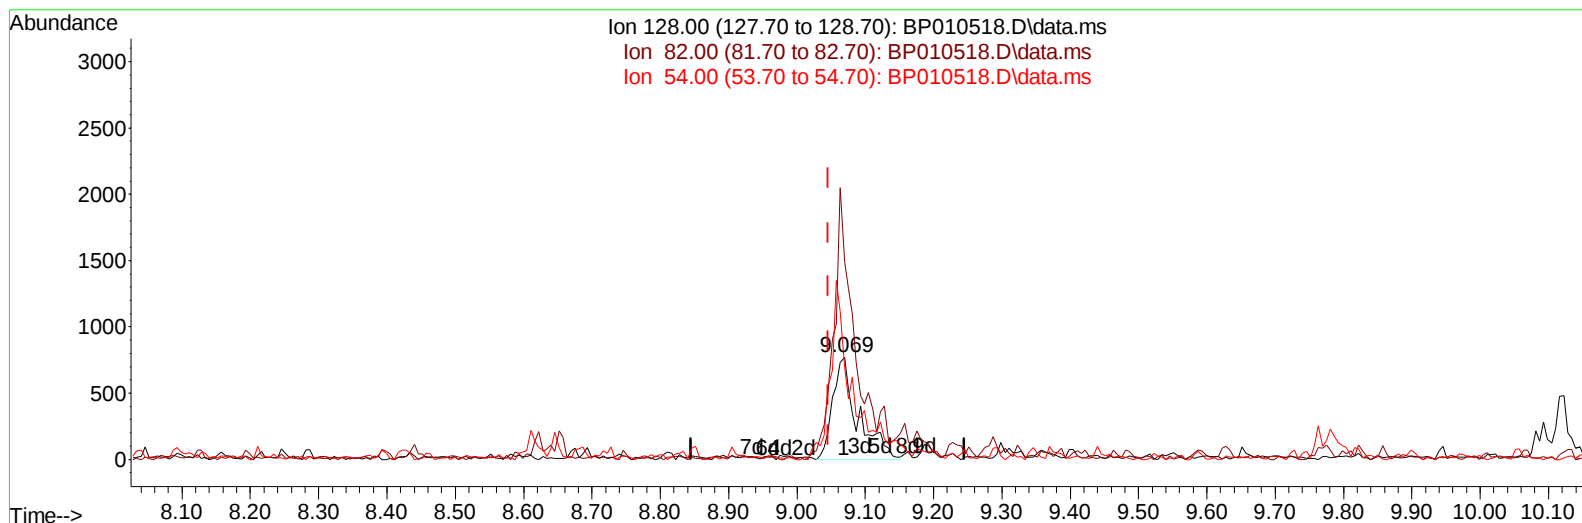

TIC: BP010518.D\data.ms

(21) Nitrobenzene-d5 (S)

9.069min (+ 0.024) 0.36 ng/ul m

response 1958

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	193.90#
54.00	120.20	90.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

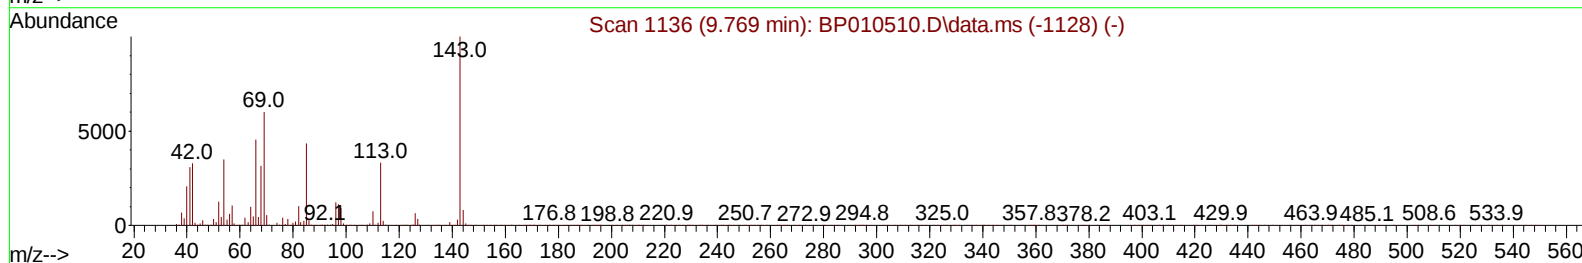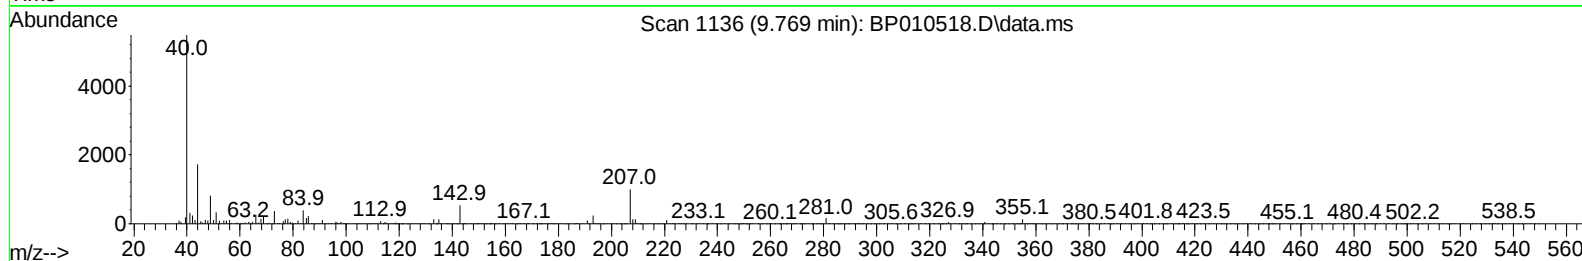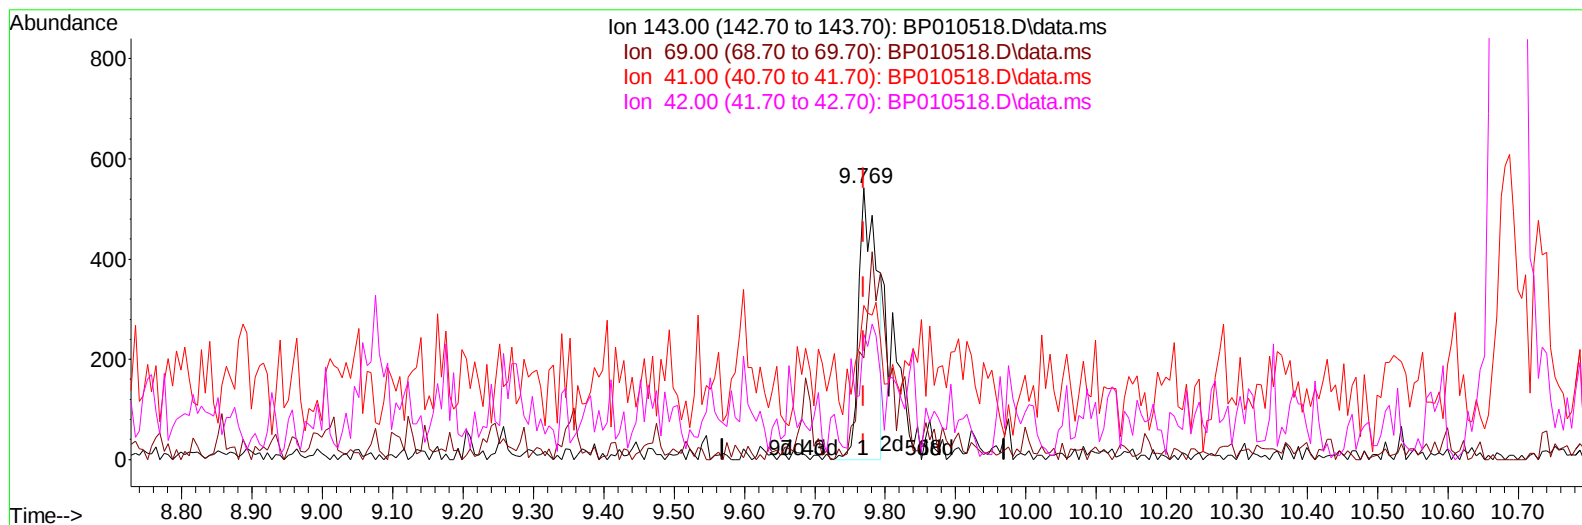

TIC: BP010518.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.769min (+ 0.000) 0.17 ng/u1

response 961

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	47.10	37.45#
41.00	16.70	56.64#
42.00	20.70	46.13#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010518.D
Acq On : 24 May 2022 16:18
Operator : CG/JU
Sample : N2950-03DL2 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :Yogesh Patel 05/26/2022

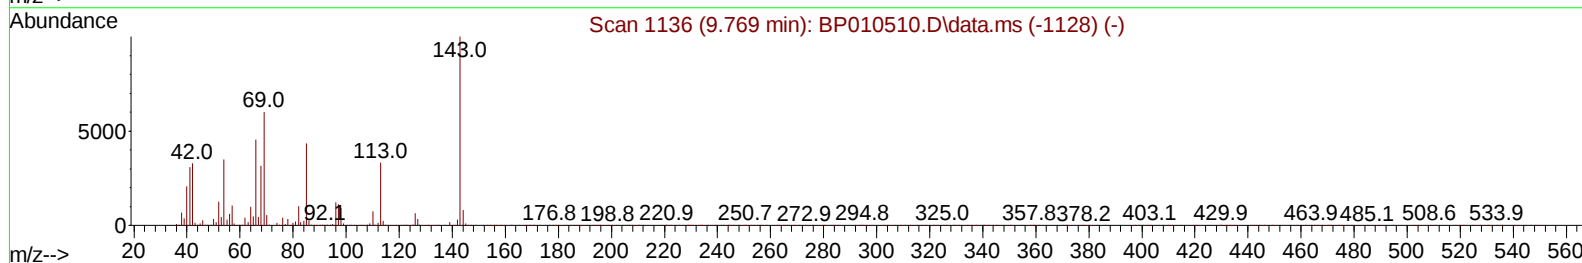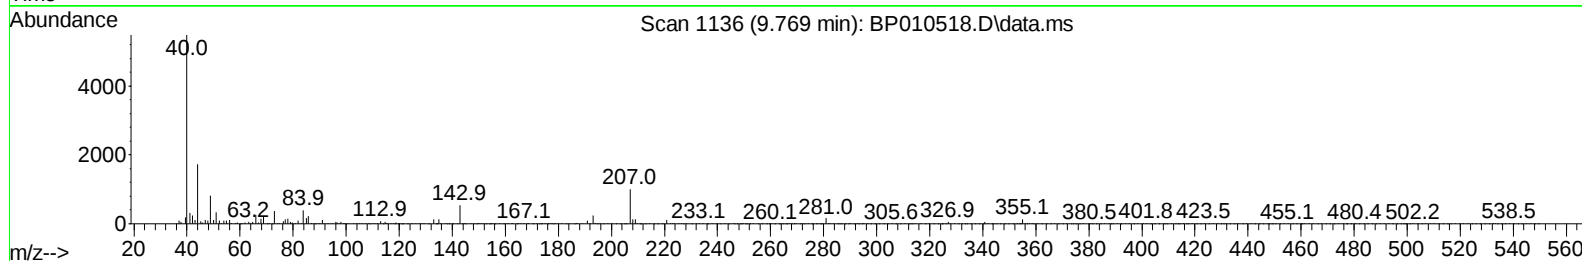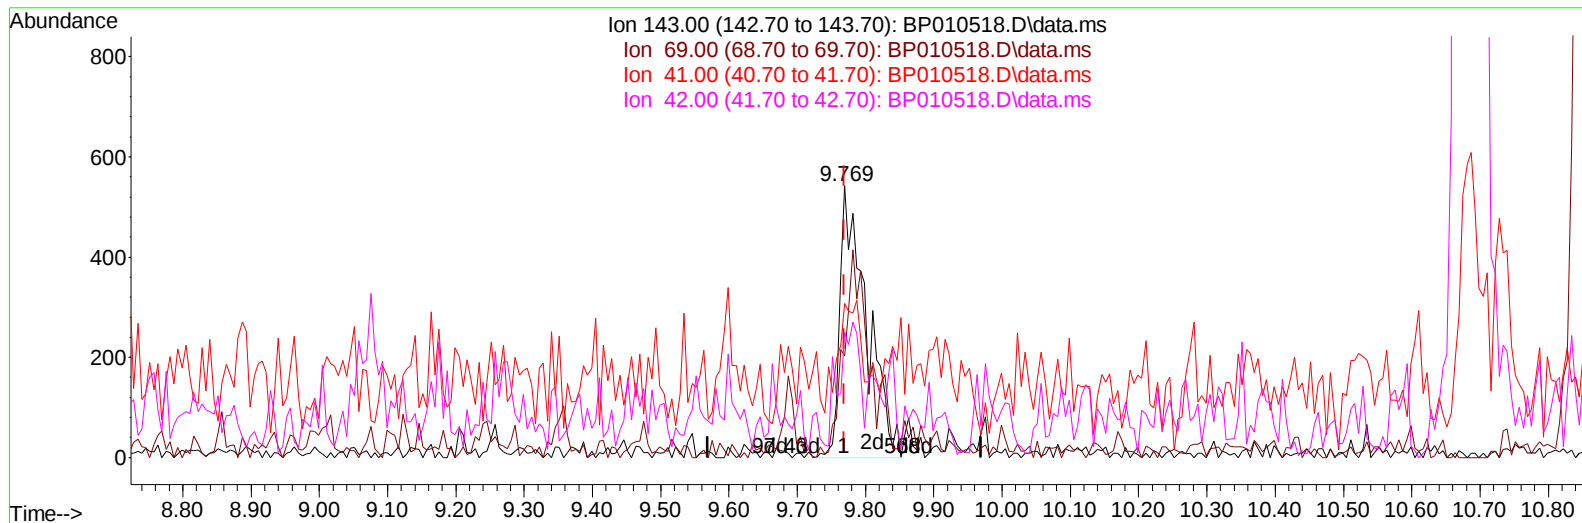

TIC: BP010518.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.769min (+ 0.000) 0.25 ng/ul m

response 1460

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	47.10	37.45#
41.00	16.70	56.64#
42.00	20.70	46.13#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010518.D
Acq On : 24 May 2022 16:18
Operator : CG/JU
Sample : N2950-03DL2 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :Yogesh Patel 05/26/2022

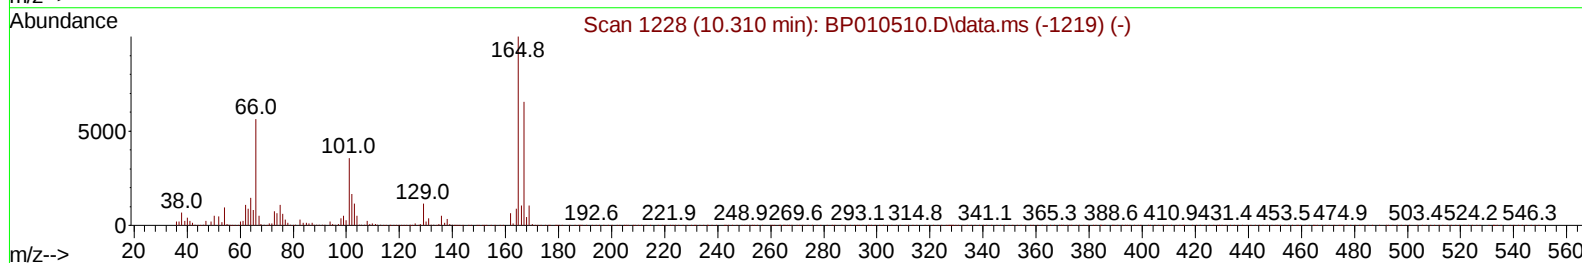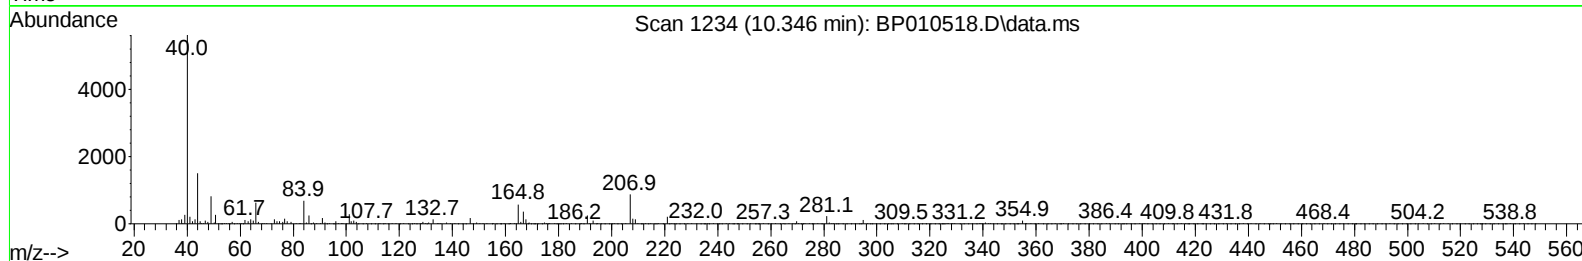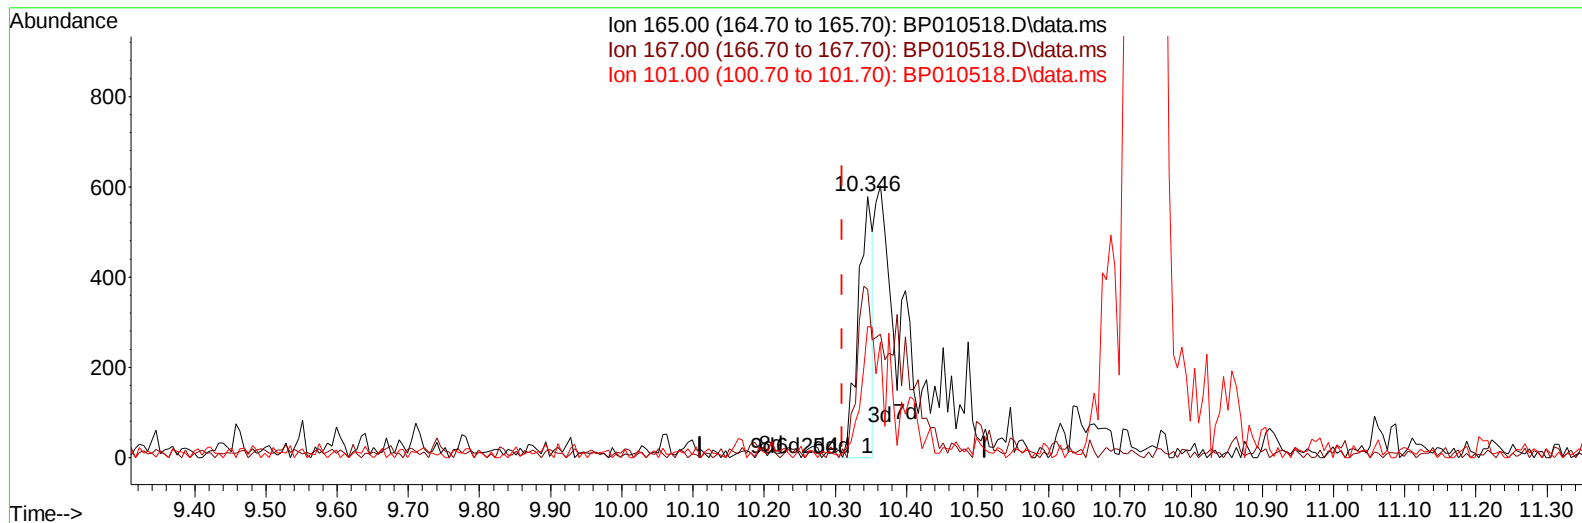

TIC: BP010518.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.346min (+ 0.035) 0.07 ng/u1

response 817

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	64.25
101.00	49.80	50.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

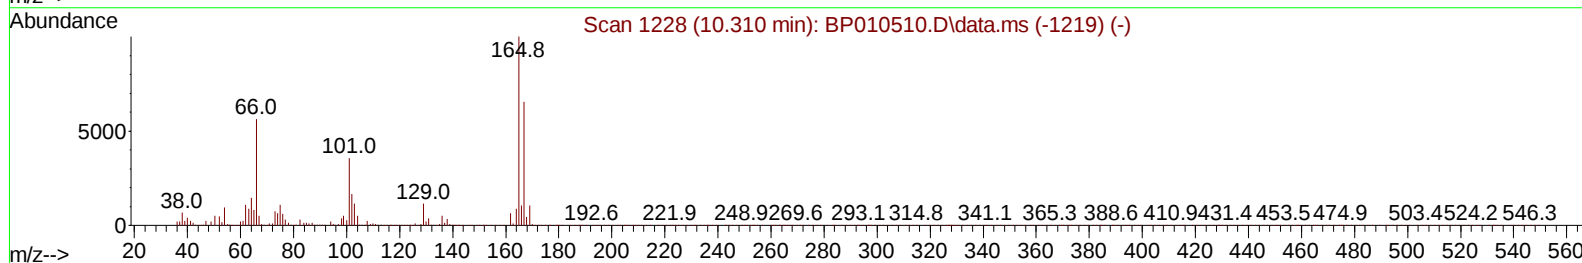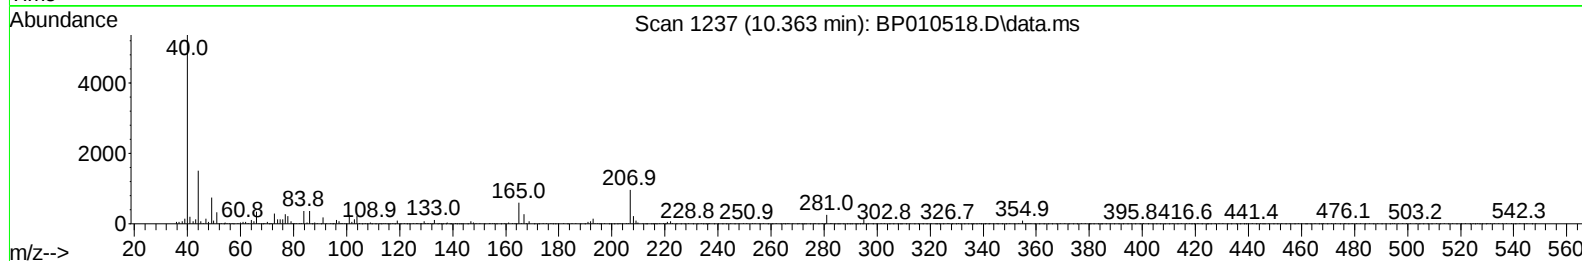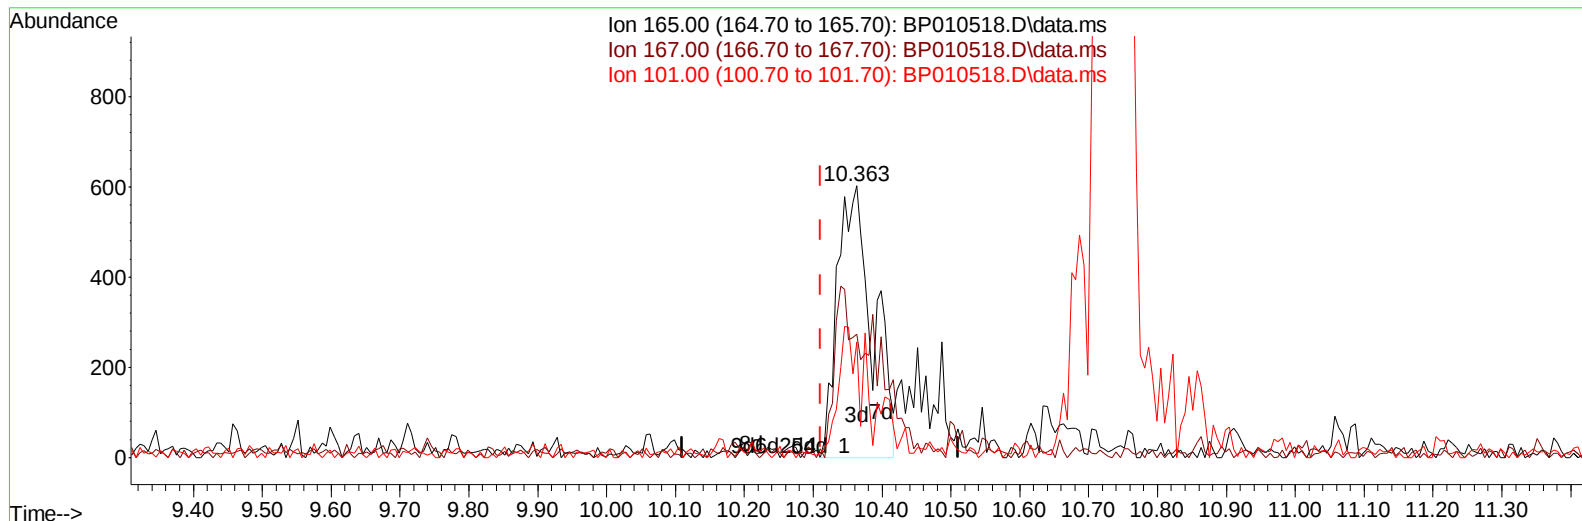

TIC: BP010518.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.363min (+ 0.053) 0.19 ng/ul m

response 2141

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	45.51#
101.00	49.80	42.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

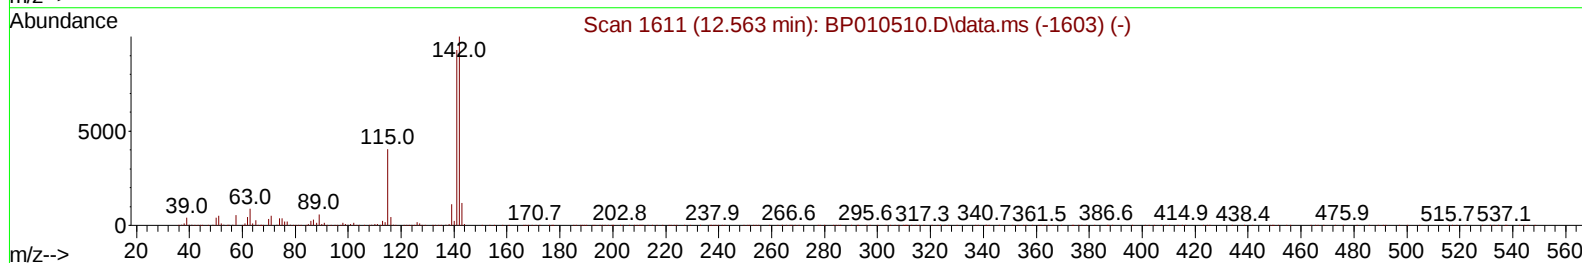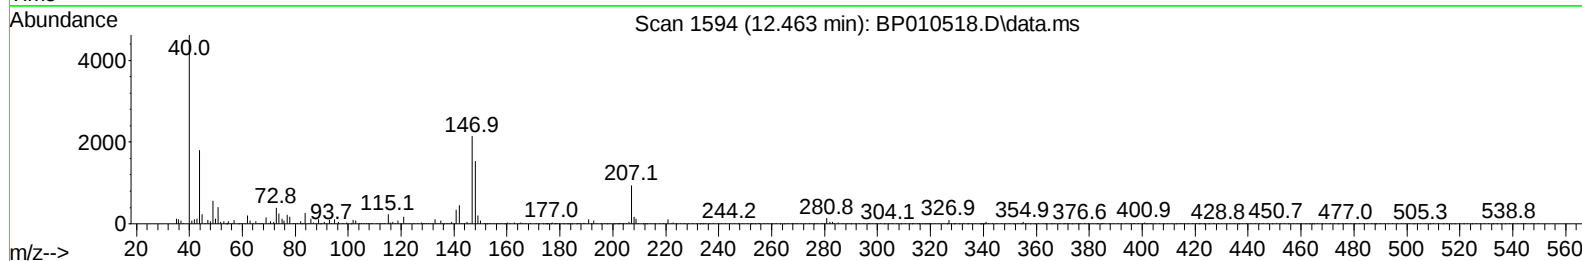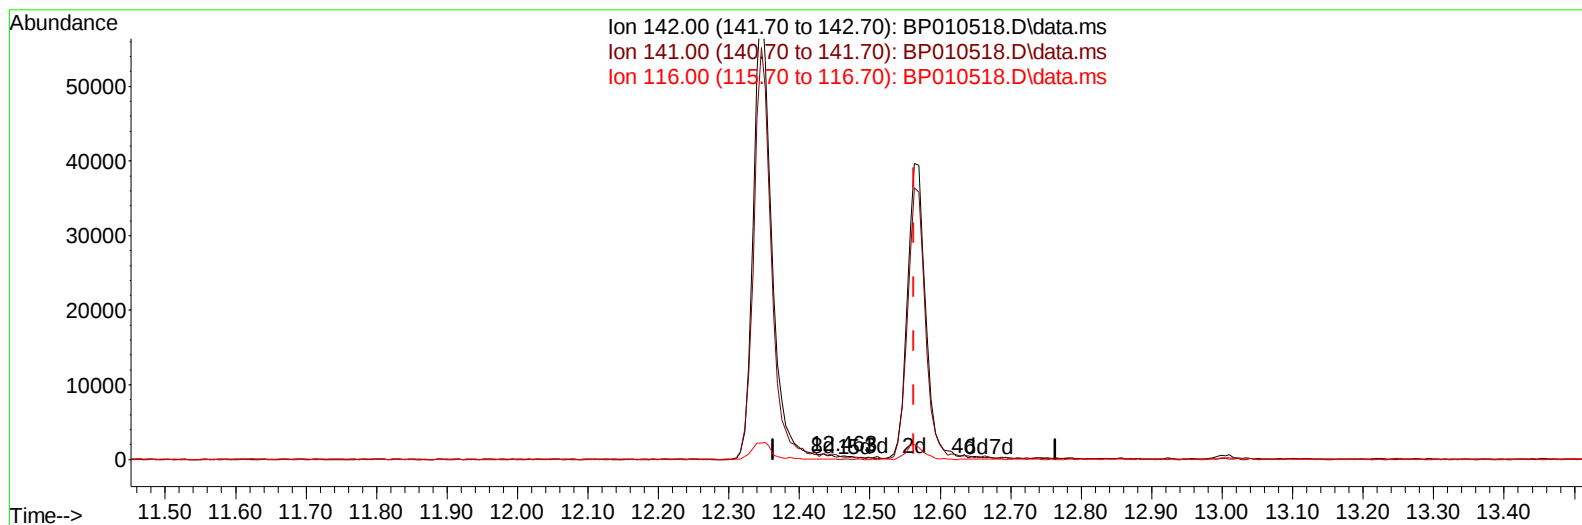

TIC: BP010518.D\data.ms

(37) 1-Methylnaphthalene

12.463min (-0.100) 0.02 ng/u1

response 403

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	87.30	76.65
116.00	7.00	5.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

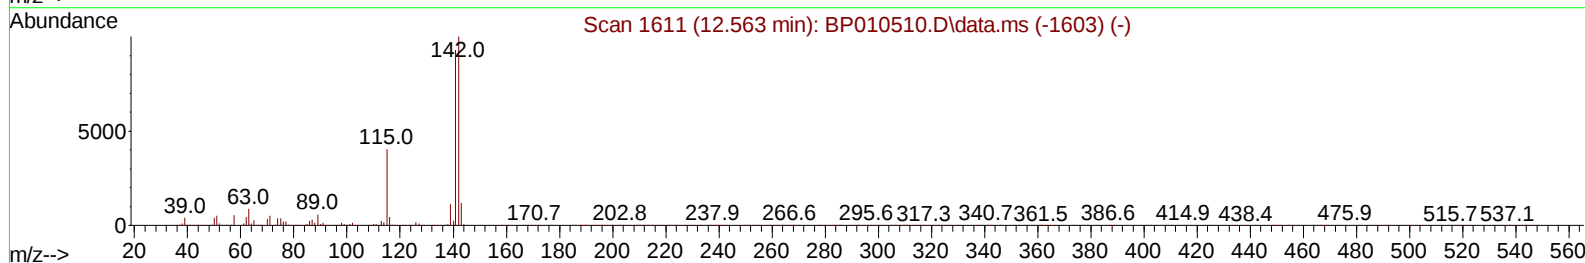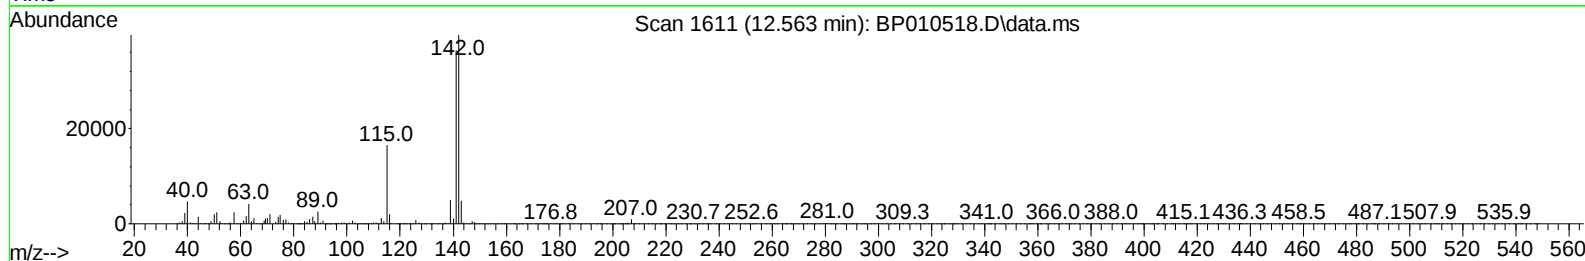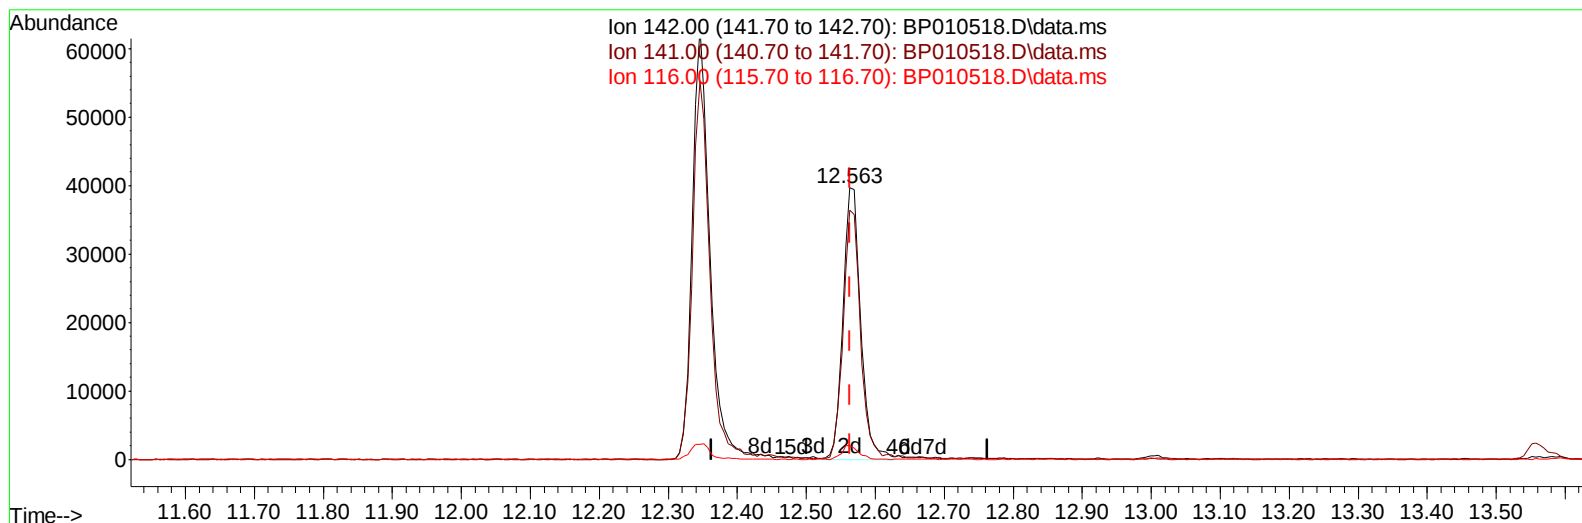

TIC: BP010518.D\data.ms

(37) 1-Methylnaphthalene

12.563min (+ 0.000) 2.68 ng/ul m

response 70978

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	87.30	91.75
116.00	7.00	5.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

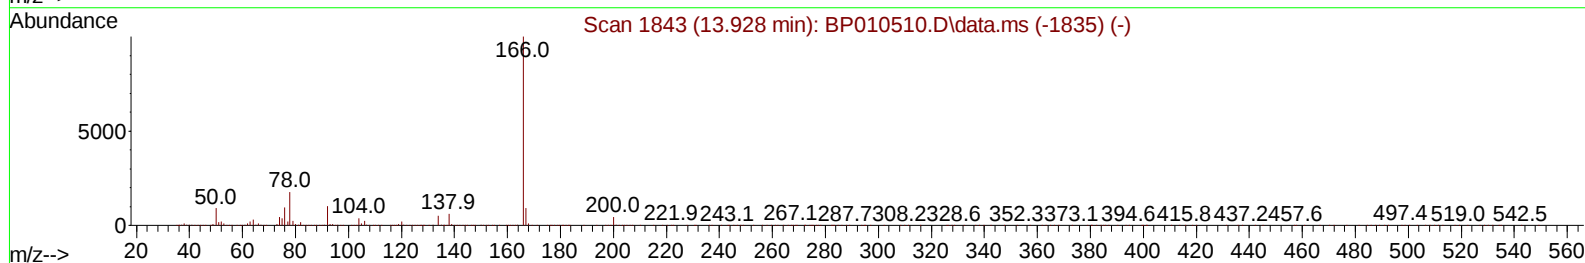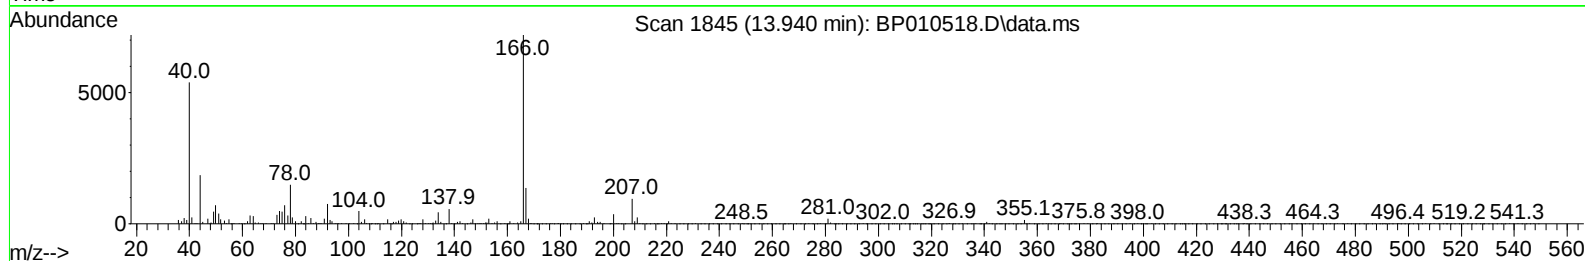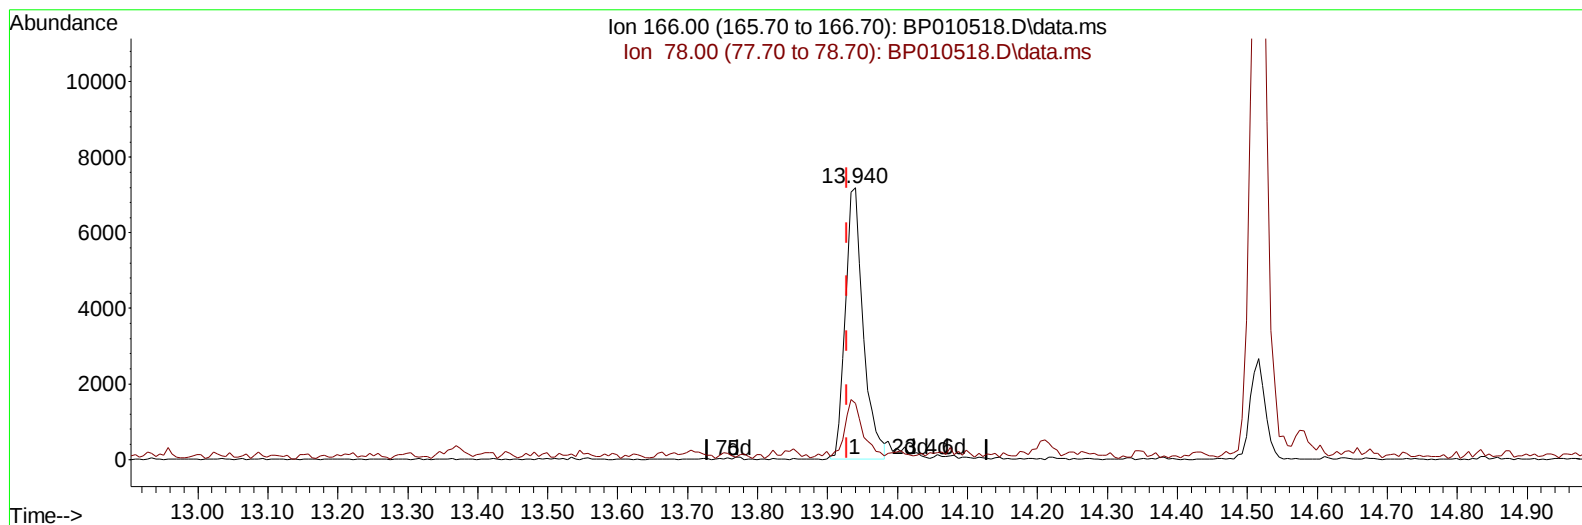

TIC: BP010518.D\data.ms

(46) Dimethylphthalate-d6 (S)

13.940min (+ 0.012) 0.35 ng/u1

response 12658

Ion	Exp%	Act%
166.00	100.00	100.00
78.00	18.50	20.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

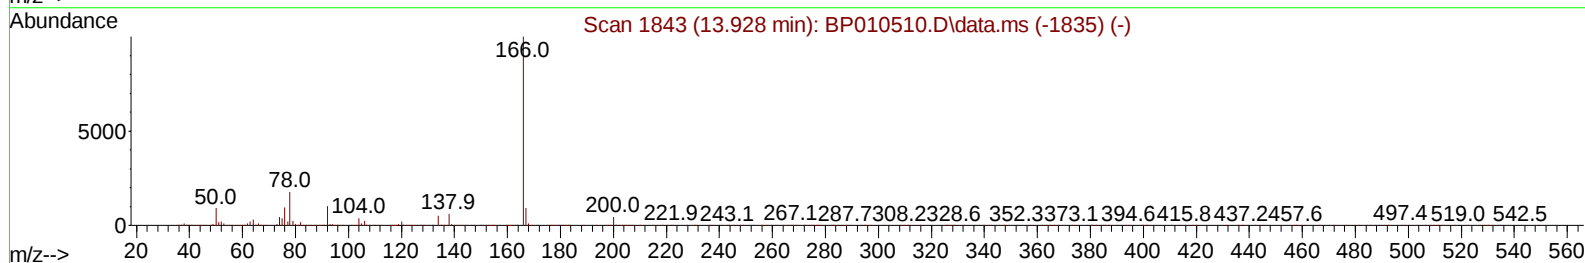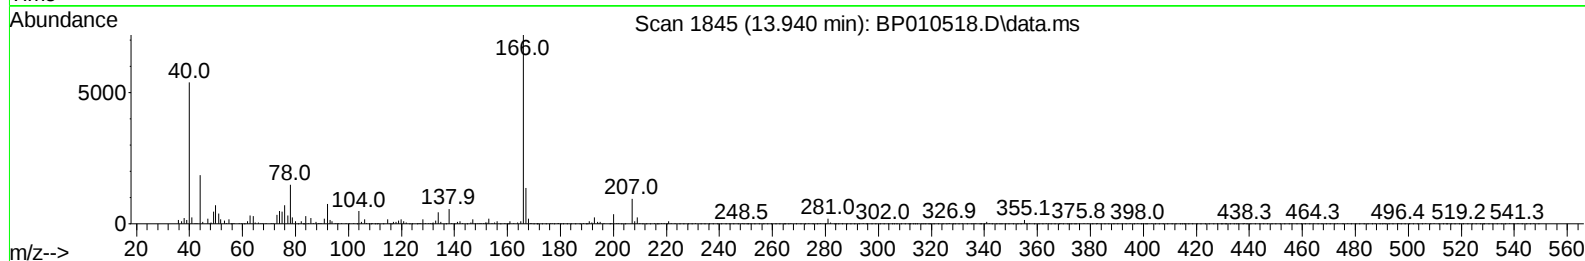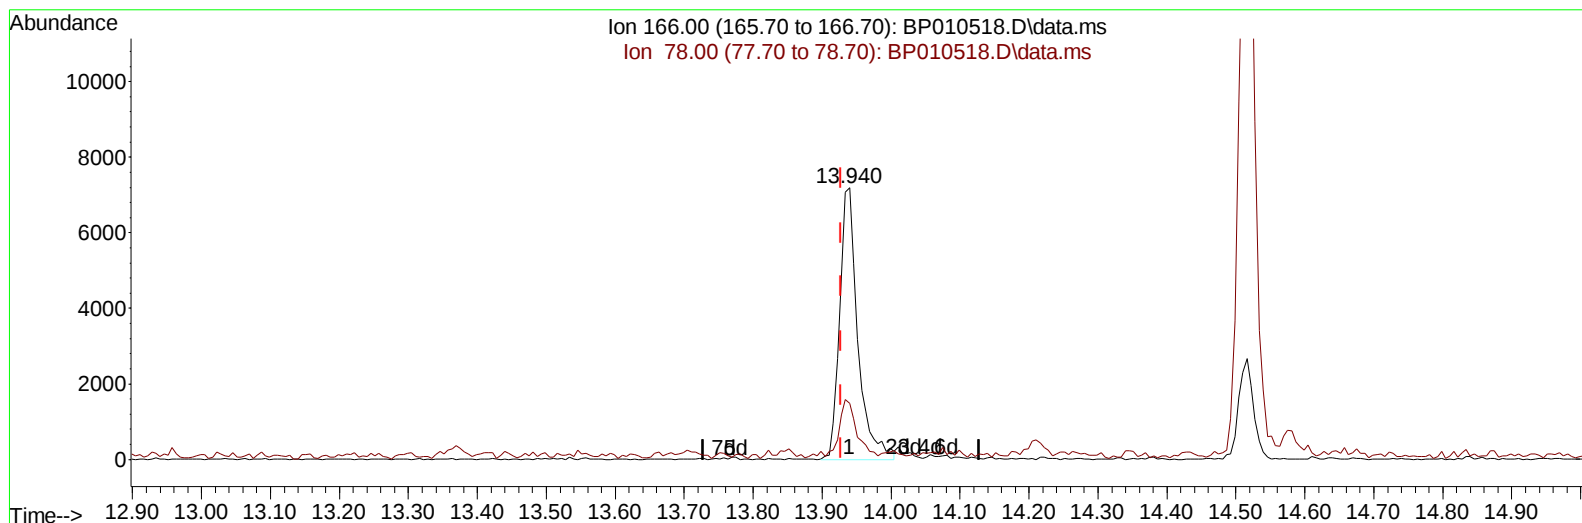

TIC: BP010518.D\data.ms

(46) Dimethylphthalate-d6 (S)

13.940min (+ 0.012) 0.37 ng/ul m

response 13184

Ion	Exp%	Act%
166.00	100.00	100.00
78.00	18.50	20.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

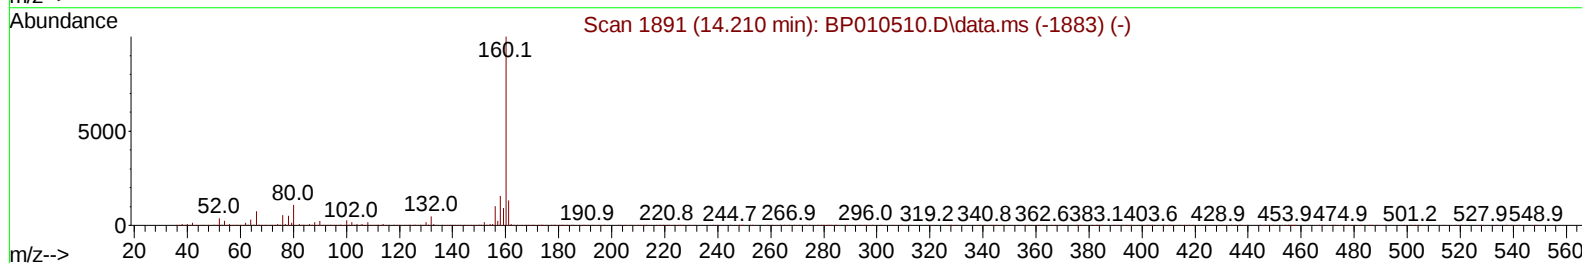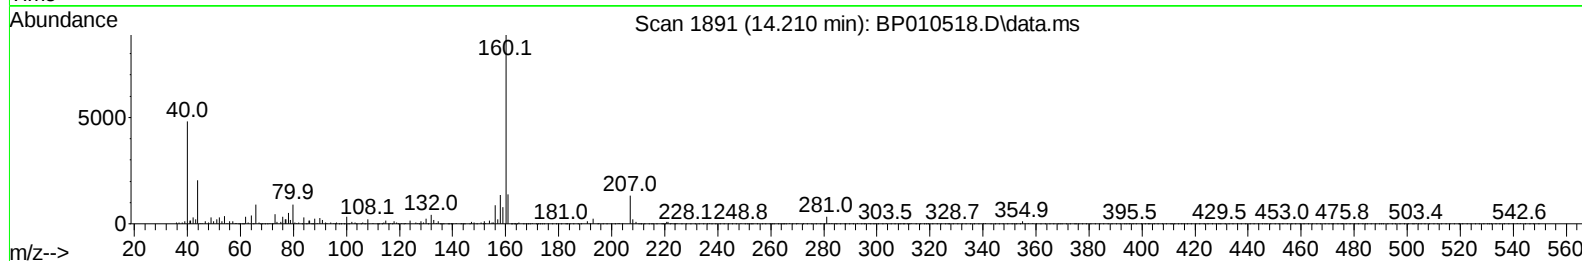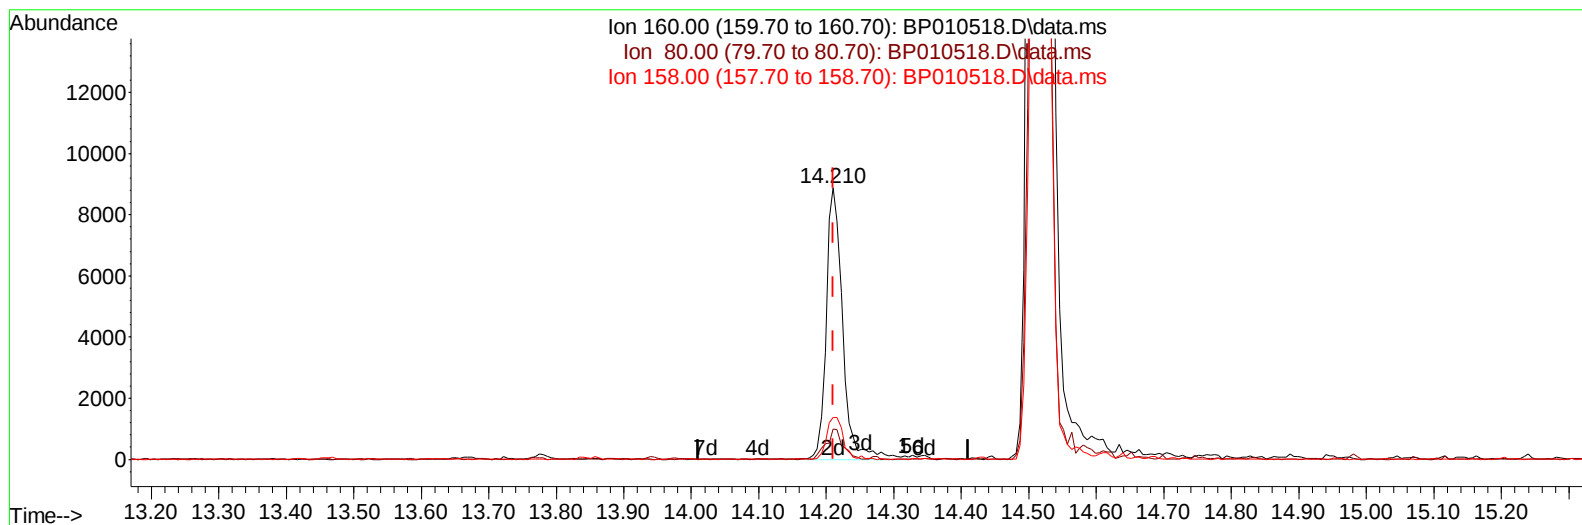

TIC: BP010518.D\data.ms

(49) Acenaphthylene-d8 (S)

14.210min (+ 0.000) 0.36 ng/ul m

response 15023

Ion	Exp%	Act%
160.00	100.00	100.00
80.00	17.00	10.34#
158.00	13.10	15.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

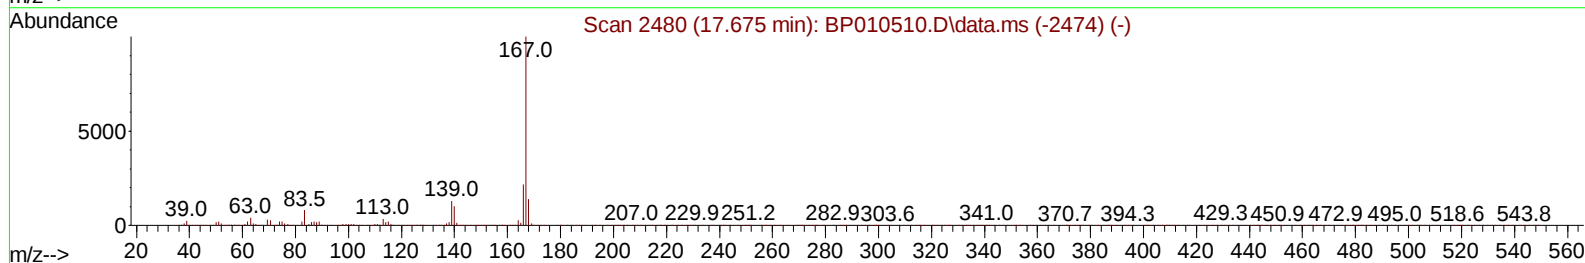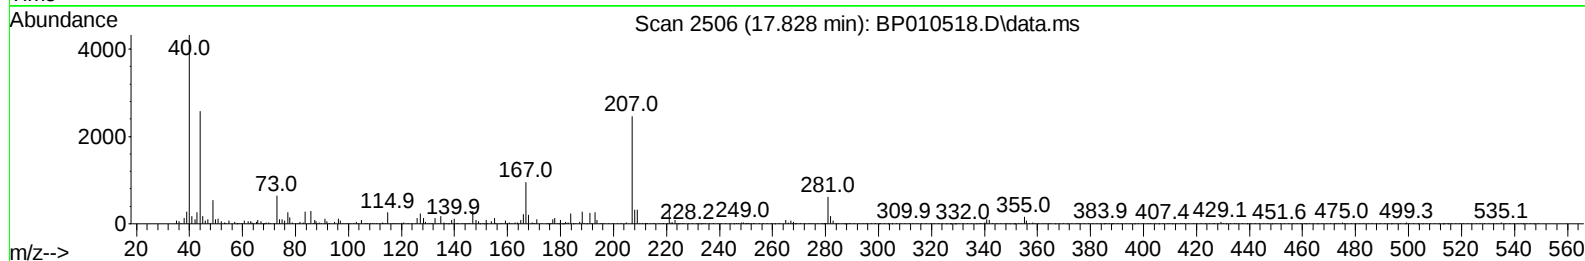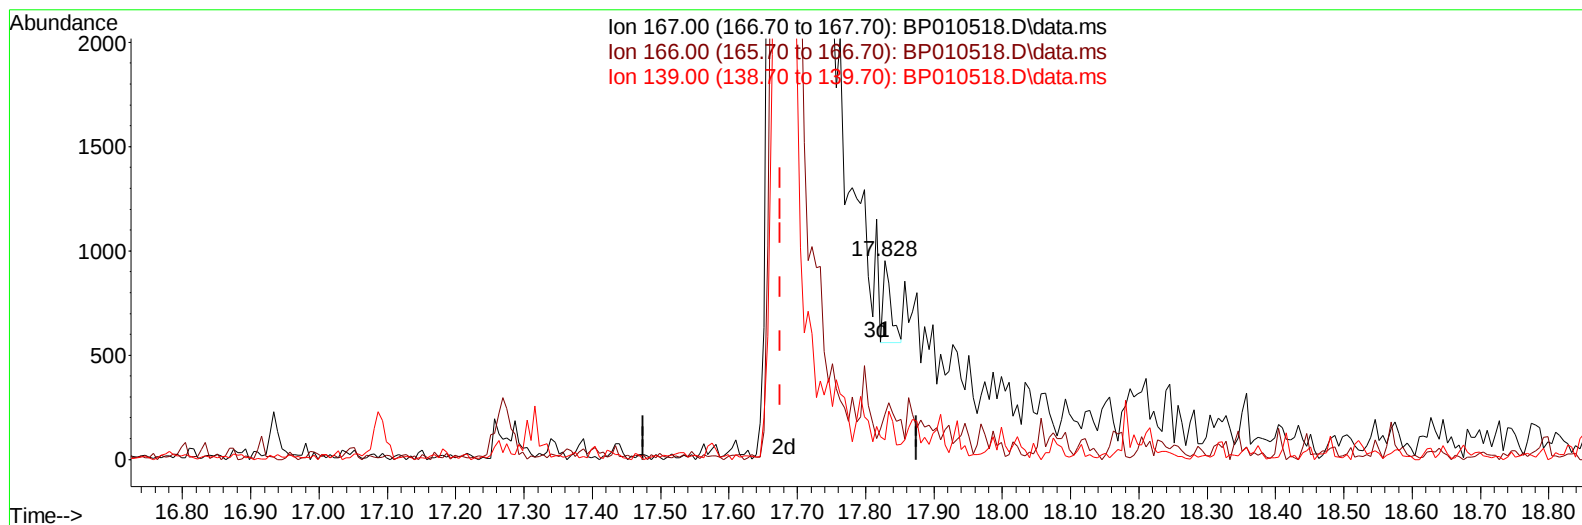

TIC: BP010518.D\data.ms

(77) Carbazole

17.828min (+ 0.153) 0.01 ng/u1

response 302

Ion	Exp%	Act%
167.00	100.00	100.00
166.00	19.80	22.77
139.00	10.40	9.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

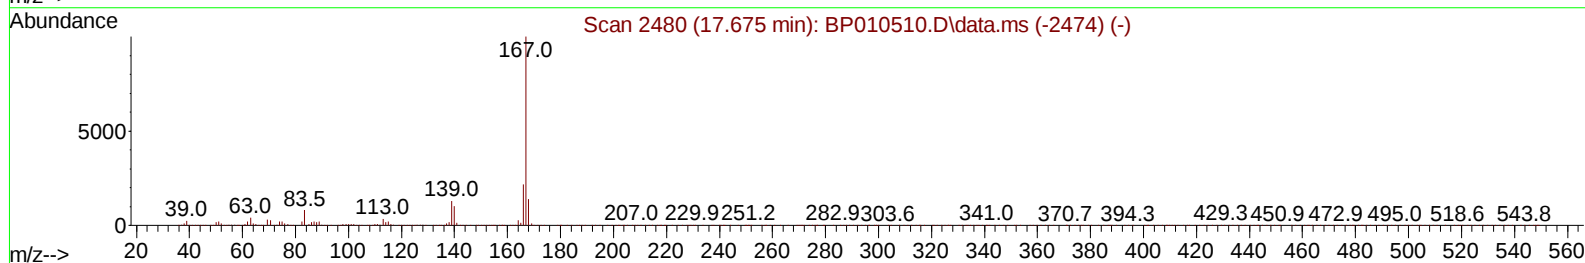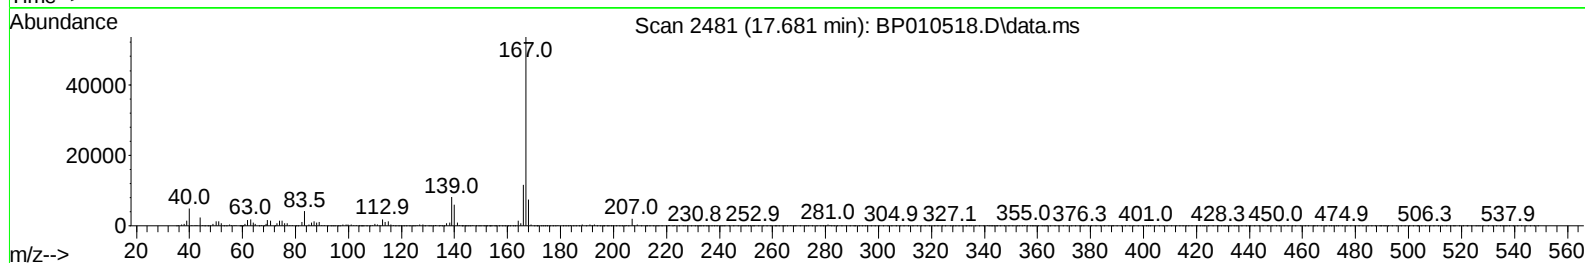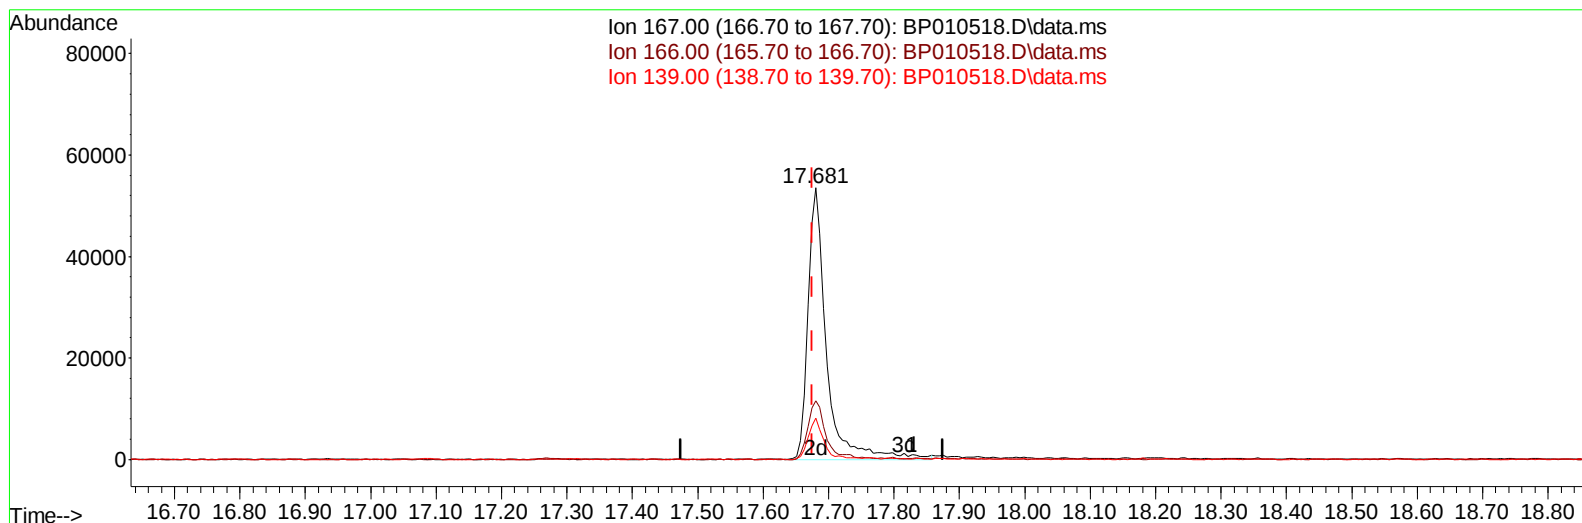

TIC: BP010518.D\data.ms

(77) Carbazole

17.681min (+ 0.006) 2.21 ng/ul m

response 105268

Ion	Exp%	Act%
167.00	100.00	100.00
166.00	19.80	21.59
139.00	10.40	15.21#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 24 05:50:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	156492	20.000	ng/ul	0.00
20) Naphthalene-d8	10.687	136	708809	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.516	164	486225	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.269	188	1012105	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.351	240	768552	20.000	ng/ul	# 0.00
88) Perylene-d12	23.774	264	625078	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	7.222	67	3385m	0.384	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	2616m	0.260	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113	1579m	0.141	ng/ul	0.02
21) Nitrobenzene-d5	9.069	128	1958m	0.357	ng/ul	0.02
24) 2-Nitrophenol-d4	9.769	143	1460m	0.251	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	2141m	0.195	ng/ul	0.05
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	13.940	166	13184m	0.368	ng/ul	0.01
49) Acenaphthylene-d8	14.210	160	15023m	0.364	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.516	176	12098	0.388	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.375	188	22822	0.498	ng/ul	0.00
81) Pyrene-d10	19.610	212	19667	0.482	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.616	264	10448	0.333	ng/ul	0.00
Target Compounds						
						Qvalue
30) Naphthalene	10.734	128	1364521	36.857	ng/ul	96
36) 2-Methylnaphthalene	12.346	142	110758	4.226	ng/ul	91
37) 1-Methylnaphthalene	12.563	142	70978m	2.682	ng/ul	
52) Acenaphthene	14.581	153	103015	3.533	ng/ul	98
56) Dibenzofuran	14.922	168	46915	1.098	ng/ul	99
77) Carbazole	17.681	167	105268m	2.211	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010518.D
Acq On : 24 May 2022 16:18
Operator : CG/JU
Sample : N2950-03DL2 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE9DL2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :Yogesh Patel 05/26/2022

Quant Time: May 24 23:17:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 24 05:50:40 2022
Response via : Initial Calibration

