

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010474.D
 Acq On : 23 May 2022 09:59
 Operator : CG/JU
 Sample : PB144961BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK961

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	52	rBV	35001	52605	1.16%	0.120%
2	3.757	111	114	136	rBV	448928	897496	19.85%	2.044%
3	4.087	166	170	178	rVB3	8974	18357	0.41%	0.042%
4	7.057	667	675	690	rBV	636977	1129846	24.99%	2.573%
5	7.222	697	703	718	rVB	526190	860500	19.03%	1.959%
6	7.428	730	738	748	rBV	667921	1142907	25.28%	2.602%
7	7.892	811	817	827	rBV	518601	840853	18.60%	1.915%
8	8.598	929	937	951	rBV	827980	1461609	32.33%	3.328%
9	9.051	1007	1014	1029	rBV	719033	1225097	27.10%	2.789%
10	9.775	1129	1137	1147	rBV	579784	1014299	22.43%	2.309%
11	10.316	1221	1229	1250	rBV	814983	1484423	32.83%	3.380%
12	10.692	1284	1293	1304	rBV	756253	1317965	29.15%	3.001%
13	10.828	1308	1316	1336	rBV	762052	1526968	33.77%	3.477%
14	12.286	1557	1564	1571	rBV3	12659	27804	0.61%	0.063%
15	13.933	1837	1844	1857	rBV	1596487	2283093	50.50%	5.198%
16	14.216	1885	1892	1908	rBV	1749190	2653129	58.68%	6.041%
17	14.521	1936	1944	1958	rBV	1195364	1831038	40.50%	4.169%
18	14.727	1972	1979	2006	rBV	448918	1029543	22.77%	2.344%
19	15.516	2106	2113	2129	rBV	2264263	3332628	73.71%	7.588%
20	15.645	2129	2135	2150	rVV	654988	998111	22.08%	2.273%
21	15.763	2150	2155	2165	rVB	27586	50018	1.11%	0.114%
22	16.304	2241	2247	2253	rVB6	8602	15622	0.35%	0.036%
23	17.274	2405	2412	2422	rBV	1495066	2240989	49.57%	5.103%
24	17.374	2423	2429	2445	rVV2	2512028	3731057	82.52%	8.495%
25	19.192	2733	2738	2742	rVB4	32735	46996	1.04%	0.107%
26	19.257	2745	2749	2756	rVB	30675	44199	0.98%	0.101%
27	19.609	2803	2809	2823	rBV	3336349	4521305	100.00%	10.295%
28	21.356	3101	3106	3117	rBV	1755627	2359503	52.19%	5.372%
29	23.627	3485	3492	3508	rVB2	1818565	3748828	82.91%	8.536%
30	23.786	3512	3519	3532	rVB2	976245	2031996	44.94%	4.627%




Sum of corrected areas: 43918784

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010474.D
Acq On : 23 May 2022 09:59
Operator : CG/JU
Sample : PB144961BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK961

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

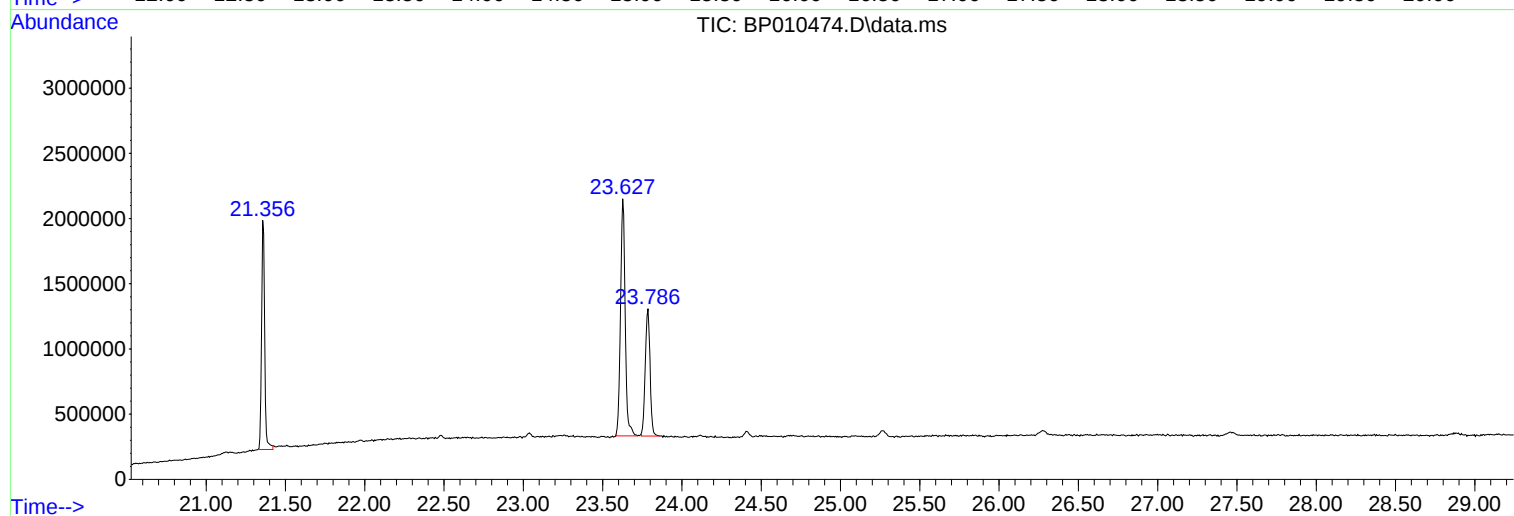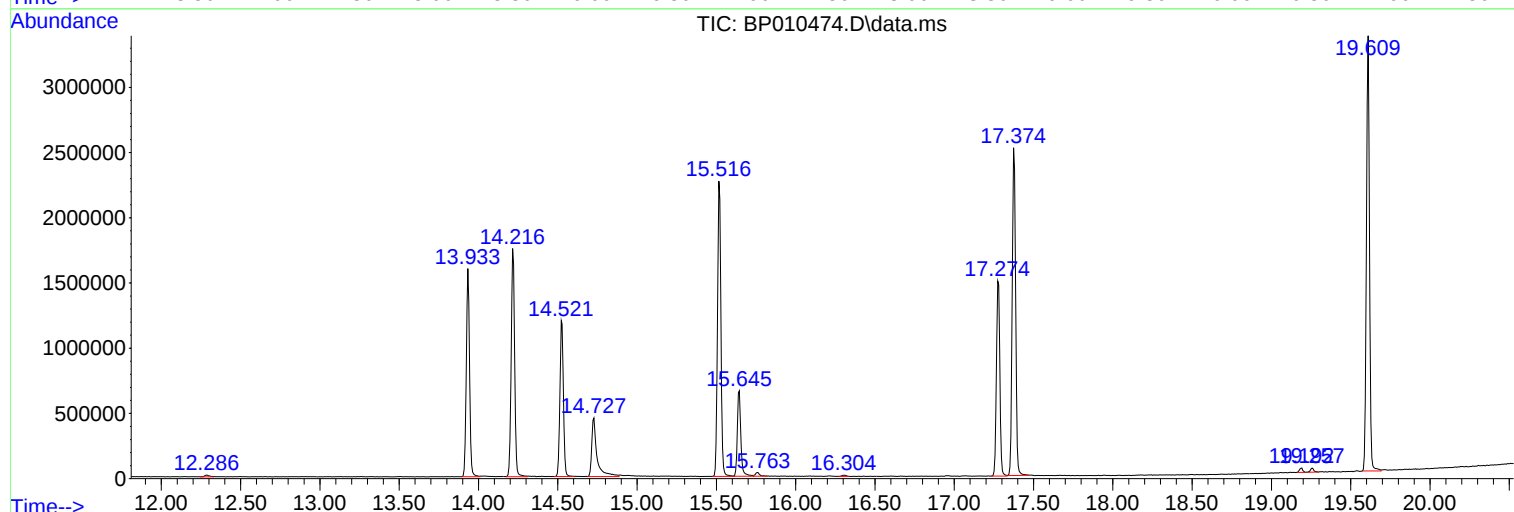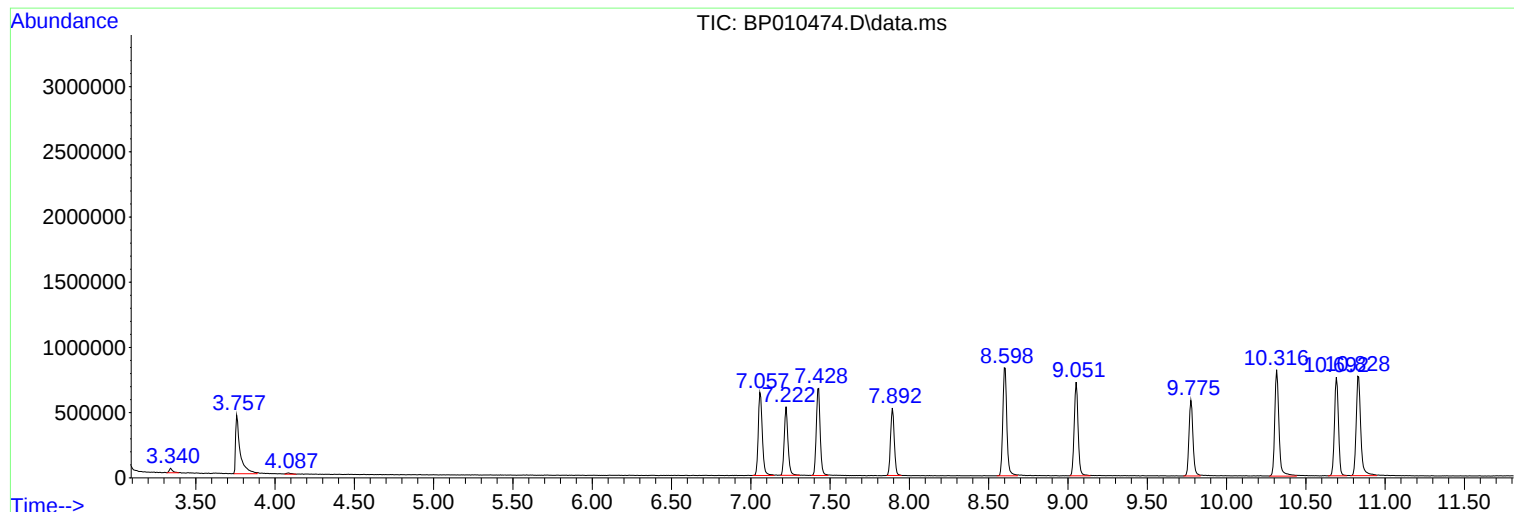

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010474.D
Acq On : 23 May 2022 09:59
Operator : CG/JU
Sample : PB144961BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK961

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010474.D
Acq On : 23 May 2022 09:59
Operator : CG/JU
Sample : PB144961BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK961

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------