

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010481.D
 Acq On : 23 May 2022 17:43
 Operator : CG/JU
 Sample : PB144963BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK963

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	50	rBV	32302	45039	1.04%	0.102%
2	3.758	111	114	136	rBV	478204	944475	21.88%	2.133%
3	4.081	165	169	174	rVB	10806	16411	0.38%	0.037%
4	7.058	667	675	688	rBV	660734	1141379	26.45%	2.578%
5	7.216	696	702	717	rVB	518469	870887	20.18%	1.967%
6	7.422	730	737	748	rBV	684930	1141984	26.46%	2.579%
7	7.887	809	816	826	rBV	606186	1011575	23.44%	2.284%
8	8.599	930	937	952	rBV	878394	1490136	34.53%	3.365%
9	9.046	1005	1013	1027	rBV	718697	1266466	29.34%	2.860%
10	9.769	1130	1136	1150	rBV	596667	1058573	24.53%	2.391%
11	10.310	1221	1228	1247	rBV	820504	1529302	35.43%	3.454%
12	10.687	1284	1292	1308	rBV	913150	1610841	37.32%	3.638%
13	10.828	1308	1316	1333	rBV	791489	1555529	36.04%	3.513%
14	12.293	1557	1565	1572	rBV4	12049	28215	0.65%	0.064%
15	12.363	1572	1577	1584	rVB10	2374	5960	0.14%	0.013%
16	12.575	1608	1613	1617	rBV7	4141	7026	0.16%	0.016%
17	12.981	1676	1682	1683	rBV6	4093	7412	0.17%	0.017%
18	13.804	1815	1822	1827	rBV6	2504	6144	0.14%	0.014%
19	13.934	1836	1844	1859	rBV	1576185	2346300	54.36%	5.299%
20	14.028	1859	1860	1868	rVB8	3792	7062	0.16%	0.016%
21	14.210	1884	1891	1905	rBV	1727903	2696990	62.49%	6.091%
22	14.522	1937	1944	1952	rBV	1487038	2203818	51.06%	4.977%
23	14.722	1971	1978	1995	rBV	438702	977242	22.64%	2.207%
24	15.157	2049	2052	2057	rBV7	3286	6001	0.14%	0.014%
25	15.345	2078	2084	2086	rBV6	4115	5846	0.14%	0.013%
26	15.516	2103	2113	2127	rBV	2358072	3394802	78.66%	7.666%
27	15.639	2128	2134	2145	rBV	626050	946152	21.92%	2.137%
28	15.757	2150	2154	2164	rVB4	29323	53653	1.24%	0.121%
29	16.304	2241	2247	2251	rBV4	9422	13353	0.31%	0.030%
30	16.581	2290	2294	2303	rBV4	4194	6722	0.16%	0.015%
31	16.757	2318	2324	2329	rBV10	3213	6187	0.14%	0.014%
32	16.951	2351	2357	2361	rBV9	6021	10212	0.24%	0.023%
33	17.063	2372	2376	2379	rVB6	3543	4900	0.11%	0.011%
34	17.275	2403	2412	2422	rBV	1871645	2635078	61.05%	5.951%
35	17.375	2422	2429	2445	rVV	2515194	3677504	85.21%	8.305%
36	18.233	2571	2575	2579	rVB5	5568	8132	0.19%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010481.D
Acq On : 23 May 2022 17:43
Operator : CG/JU
Sample : PB144963BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK963

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION

37	19.180	2732	2736	2741	rBV2	31220	48114	1.11%	0.109%
38	19.251	2744	2748	2752	rBV	27176	41237	0.96%	0.093%
39	19.604	2802	2808	2820	rBV	3123190	4315981	100.00%	9.747%
40	21.351	3100	3105	3117	rBV	1746571	2520534	58.40%	5.692%
41	23.621	3484	3491	3498	rBV2	1400066	2812816	65.17%	6.352%
42	23.774	3510	3517	3526	rBV2	882969	1805156	41.82%	4.077%




Sum of corrected areas: 44281146

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010481.D
Acq On : 23 May 2022 17:43
Operator : CG/JU
Sample : PB144963BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK963

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

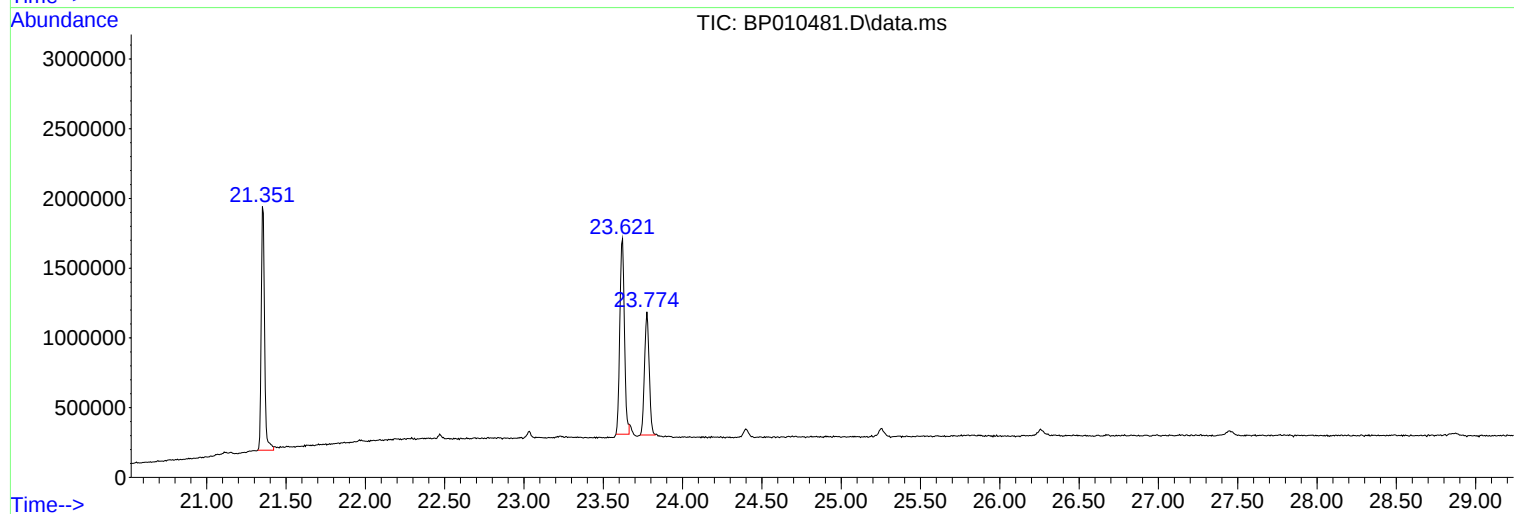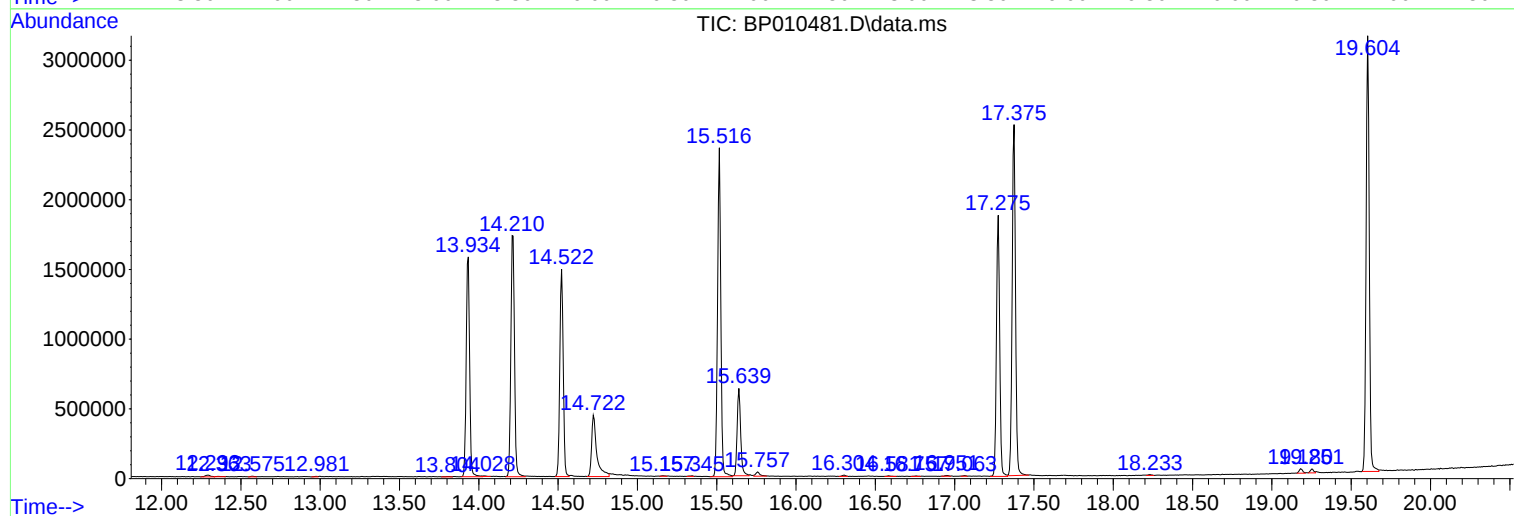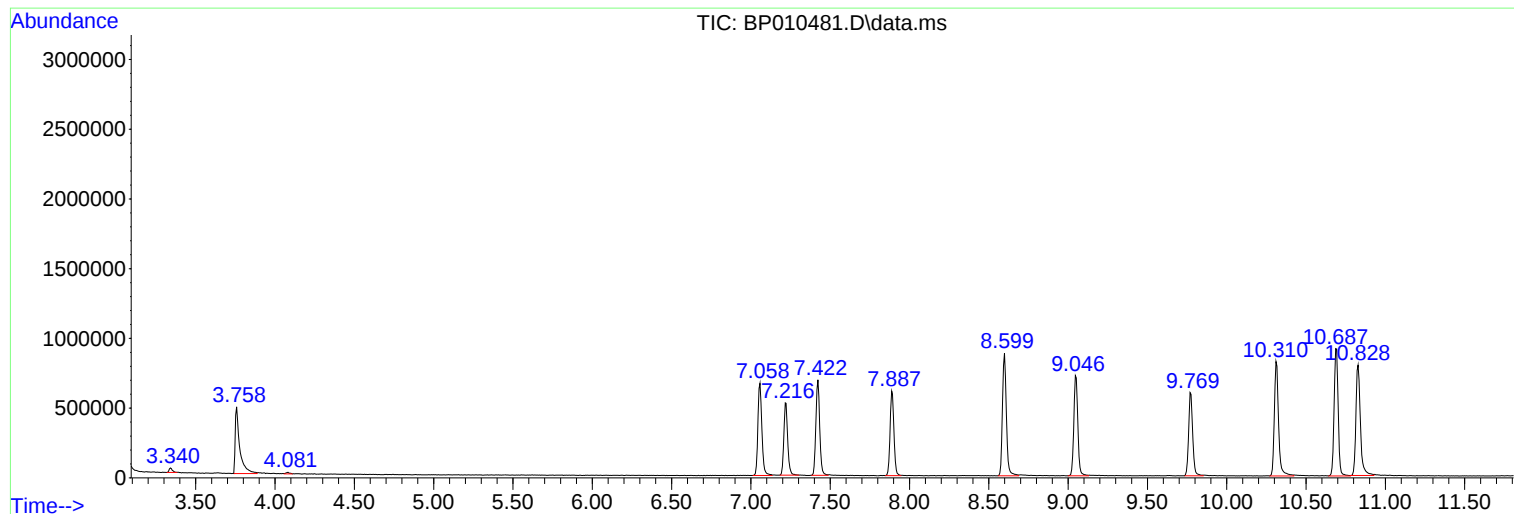

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010481.D
Acq On : 23 May 2022 17:43
Operator : CG/JU
Sample : PB144963BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK963

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010481.D
Acq On : 23 May 2022 17:43
Operator : CG/JU
Sample : PB144963BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK963

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------