

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010487.D
 Acq On : 23 May 2022 21:08
 Operator : CG/JU
 Sample : N2918-14DL 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.799	117	121	128	rBV6	9642	23311	0.79%	0.097%
2	3.981	149	152	153	rBV3	4944	5247	0.18%	0.022%
3	4.081	165	169	178	rVB2	12655	19910	0.68%	0.083%
4	5.022	324	329	332	rBV3	5718	9082	0.31%	0.038%
5	5.905	475	479	484	rVB	10998	15273	0.52%	0.064%
6	6.375	555	559	563	rBV6	3894	7501	0.25%	0.031%
7	7.063	668	676	681	rBV3	14013	29033	0.98%	0.121%
8	7.222	697	703	710	rBV	60486	106885	3.62%	0.447%
9	7.422	731	737	746	rBV	56818	105000	3.56%	0.439%
10	7.540	753	757	759	rBV5	2664	4310	0.15%	0.018%
11	7.611	762	769	778	rBV	33381	61200	2.08%	0.256%
12	7.887	808	816	828	rBV	648693	1102934	37.40%	4.611%
13	8.010	833	837	842	rVV6	7049	13507	0.46%	0.056%
14	8.063	844	846	852	rVB7	2663	4468	0.15%	0.019%
15	8.269	876	881	885	rBV7	2587	4320	0.15%	0.018%
16	8.428	903	908	913	rBV3	11060	19506	0.66%	0.082%
17	8.605	932	938	947	rBV2	39136	75719	2.57%	0.317%
18	8.740	953	961	971	rVB	53885	91980	3.12%	0.385%
19	8.999	1001	1005	1008	rBV4	5200	7527	0.26%	0.031%
20	9.052	1008	1014	1025	rVB2	77800	158373	5.37%	0.662%
21	9.252	1040	1048	1056	rVB6	10469	21096	0.72%	0.088%
22	9.375	1061	1069	1074	rVV2	17400	37180	1.26%	0.155%
23	9.440	1075	1080	1084	rVB3	8447	12948	0.44%	0.054%
24	9.528	1090	1095	1099	rVV8	2324	3762	0.13%	0.016%
25	9.581	1099	1104	1109	rVB8	3221	6640	0.23%	0.028%
26	9.775	1129	1137	1145	rBV	58948	112335	3.81%	0.470%
27	9.834	1145	1147	1151	rVB5	3422	4281	0.15%	0.018%
28	9.940	1160	1165	1166	rBV5	3320	3747	0.13%	0.016%
29	9.969	1167	1170	1173	rVB5	3332	4385	0.15%	0.018%
30	10.093	1187	1191	1198	rVB10	6694	12225	0.41%	0.051%
31	10.322	1224	1230	1239	rBV2	71185	153447	5.20%	0.642%
32	10.393	1239	1242	1248	rVB8	5238	9071	0.31%	0.038%
33	10.610	1272	1279	1282	rBV9	4508	8713	0.30%	0.036%
34	10.687	1284	1292	1296	rVV	1019933	1747374	59.26%	7.305%
35	10.740	1296	1301	1311	rVV	1699610	2891235	98.05%	12.087%
36	10.857	1311	1321	1333	rVB2	225001	507123	17.20%	2.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010487.D
 Acq On : 23 May 2022 21:08
 Operator : CG/JU
 Sample : N2918-14DL 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	10.987	1340	1343	1349	rVB8	3059	5921	0.20%	0.025%
38	11.804	1474	1482	1489	rBV3	26157	50013	1.70%	0.209%
39	12.246	1550	1557	1562	rBV	18250	35626	1.21%	0.149%
40	12.351	1568	1575	1583	rBV	120969	212396	7.20%	0.888%

41	12.463	1590	1594	1595	rBV3	5384	4578	0.16%	0.019%
42	12.569	1601	1612	1620	rBV	104678	189555	6.43%	0.792%
43	12.734	1636	1640	1646	rVB7	6385	12857	0.44%	0.054%
44	13.010	1680	1687	1692	rBV7	11125	30136	1.02%	0.126%
45	13.134	1703	1708	1712	rVB8	3147	4332	0.15%	0.018%

46	13.251	1723	1728	1731	rBV7	6295	10552	0.36%	0.044%
47	13.357	1740	1746	1754	rBV	60022	101822	3.45%	0.426%
48	13.563	1777	1781	1782	rBV3	4437	5769	0.20%	0.024%
49	13.581	1782	1784	1792	rVB9	9128	14583	0.49%	0.061%
50	13.704	1798	1805	1811	rVB8	13468	28765	0.98%	0.120%

51	13.775	1811	1817	1820	rBV8	2934	5283	0.18%	0.022%
52	13.845	1821	1829	1834	rVV4	14645	29333	0.99%	0.123%
53	13.934	1834	1844	1854	rVV	216923	339311	11.51%	1.419%
54	14.004	1854	1856	1861	rVV6	3606	5641	0.19%	0.024%
55	14.081	1865	1869	1872	rVV5	7367	10278	0.35%	0.043%

56	14.104	1872	1873	1879	rVB6	4037	4830	0.16%	0.020%
57	14.210	1884	1891	1905	rBV	217544	391309	13.27%	1.636%
58	14.340	1911	1913	1919	rVB7	3077	5395	0.18%	0.023%
59	14.422	1925	1927	1932	rVB6	3337	4764	0.16%	0.020%
60	14.522	1934	1944	1950	rBV	1661055	2471771	83.83%	10.333%

61	14.581	1950	1954	1961	rVV	164588	263004	8.92%	1.100%
62	14.651	1961	1966	1976	rVB	148920	240997	8.17%	1.008%
63	14.798	1988	1991	1996	rVB5	8492	11513	0.39%	0.048%
64	14.922	2006	2012	2020	rVB	157529	241223	8.18%	1.008%
65	15.075	2029	2038	2044	rBV	62348	110948	3.76%	0.464%

66	15.116	2044	2045	2048	rVV3	7523	9250	0.31%	0.039%
67	15.151	2048	2051	2058	rVB4	21791	34143	1.16%	0.143%
68	15.469	2100	2105	2106	rBV5	2734	3625	0.12%	0.015%
69	15.516	2106	2113	2118	rBV	305346	467857	15.87%	1.956%
70	15.569	2118	2122	2130	rVB2	66850	114661	3.89%	0.479%

71	15.651	2130	2136	2143	rBV5	54393	123334	4.18%	0.516%
72	15.728	2145	2149	2158	rVB4	19536	44021	1.49%	0.184%
73	15.869	2170	2173	2178	rVB6	13485	20514	0.70%	0.086%
74	15.969	2187	2190	2191	rBV3	4050	4404	0.15%	0.018%
75	16.010	2194	2197	2207	rVB4	17259	32253	1.09%	0.135%

76	16.134	2210	2218	2220	rVB9	5081	8690	0.29%	0.036%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010487.D
 Acq On : 23 May 2022 21:08
 Operator : CG/JU
 Sample : N2918-14DL 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTH3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

77	16.204	2225	2230	2231	rBV5	6572	9332	0.32%	0.039%
78	16.245	2231	2237	2243	rBV2	85312	151077	5.12%	0.632%
79	16.428	2260	2268	2270	rBV9	10064	18074	0.61%	0.076%
80	16.539	2284	2287	2293	rVB3	9922	15232	0.52%	0.064%
81	16.775	2321	2327	2329	rBV6	6372	11218	0.38%	0.047%
82	16.892	2340	2347	2349	rBV2	51394	79515	2.70%	0.332%
83	16.928	2349	2353	2364	rVB	119833	200106	6.79%	0.837%
84	17.063	2373	2376	2377	rBV3	4566	5789	0.20%	0.024%
85	17.092	2377	2381	2385	rVB	16446	24182	0.82%	0.101%
86	17.269	2401	2411	2417	rBV	1953736	2948652	100.00%	12.327%
87	17.316	2417	2419	2423	rVV	111291	129621	4.40%	0.542%
88	17.369	2423	2428	2438	rVV2	338619	538727	18.27%	2.252%
89	17.469	2442	2445	2450	rBV7	5732	11990	0.41%	0.050%
90	17.522	2450	2454	2459	rVB8	8138	14723	0.50%	0.062%
91	17.675	2474	2480	2493	rBV	697265	1014824	34.42%	4.243%
92	17.881	2513	2515	2516	rBV2	6307	5382	0.18%	0.022%
93	18.028	2536	2540	2544	rBV7	5437	10621	0.36%	0.044%
94	18.186	2559	2567	2571	rBV6	19761	37236	1.26%	0.156%
95	18.557	2628	2630	2634	rVB4	9361	10931	0.37%	0.046%
96	18.663	2646	2648	2652	rVB5	7701	7949	0.27%	0.033%
97	19.604	2803	2808	2818	rBV	464447	596440	20.23%	2.493%
98	21.357	3101	3106	3119	rBV	2023665	2702612	91.66%	11.299%
99	23.621	3486	3491	3496	rBV	147529	290203	9.84%	1.213%
100	23.774	3511	3517	3525	rVB2	969429	1979664	67.14%	8.276%



Sum of corrected areas: 23920005

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010487.D
Acq On : 23 May 2022 21:08
Operator : CG/JU
Sample : N2918-14DL 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

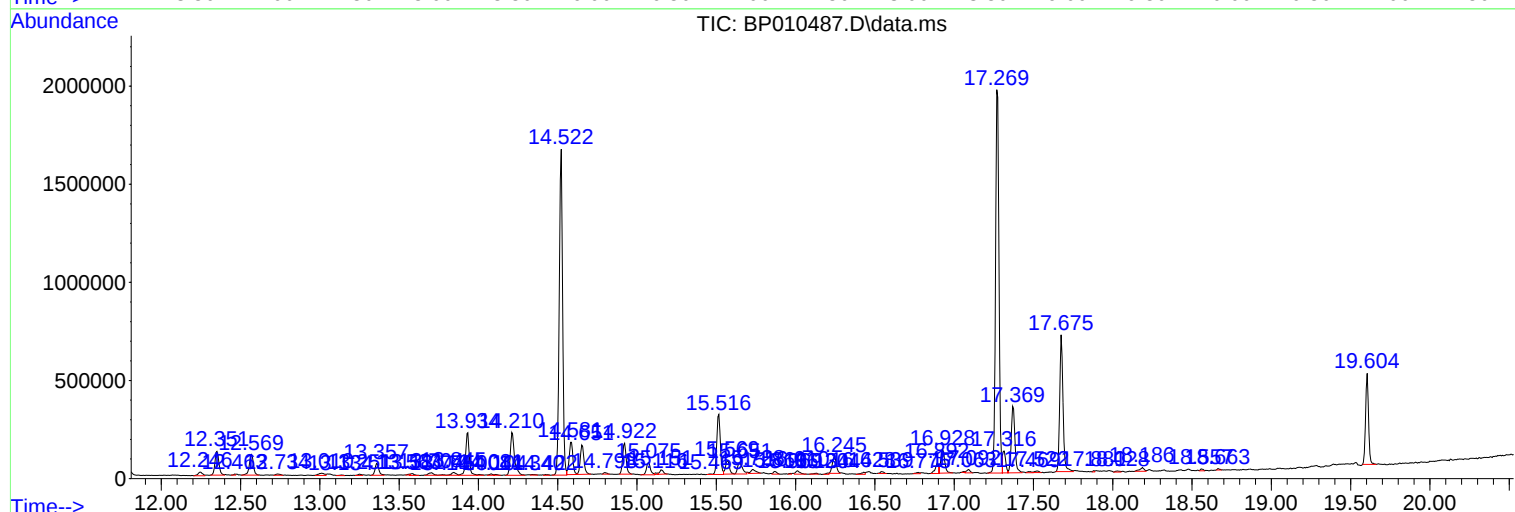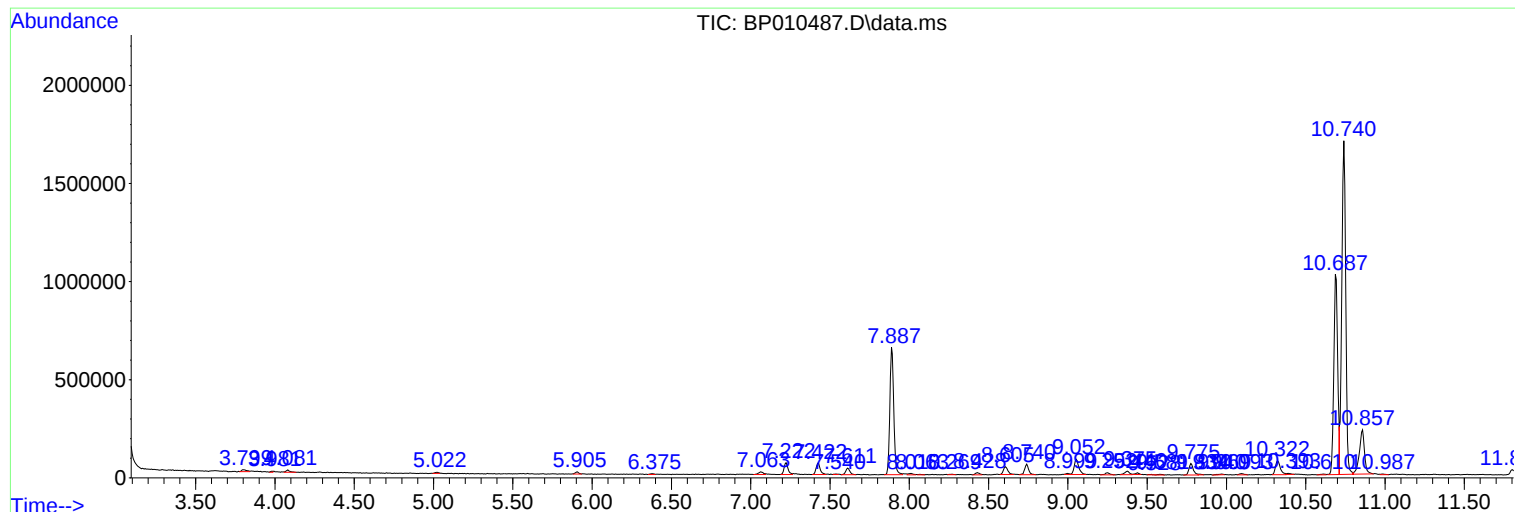

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010487.D
Acq On : 23 May 2022 21:08
Operator : CG/JU
Sample : N2918-14DL 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010487.D
Acq On : 23 May 2022 21:08
Operator : CG/JU
Sample : N2918-14DL 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTH3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------