

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010489.D
 Acq On : 23 May 2022 22:16
 Operator : CG/JU
 Sample : N2955-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rBV	23867	34812	0.77%	0.089%
2	3.776	114	117	127	rBV	55621	129404	2.85%	0.330%
3	3.981	149	152	164	rVV2	15354	33596	0.74%	0.086%
4	4.081	166	169	176	rVB3	10559	18049	0.40%	0.046%
5	4.446	227	231	239	rVB7	10602	18834	0.41%	0.048%
6	4.805	290	292	299	rBV7	2723	5309	0.12%	0.014%
7	5.011	321	327	328	rBV4	4864	7518	0.17%	0.019%
8	5.428	394	398	402	rVB7	4123	6741	0.15%	0.017%
9	5.599	423	427	432	rVB6	4314	7760	0.17%	0.020%
10	7.058	668	675	687	rBV	113274	214647	4.73%	0.547%
11	7.216	696	702	716	rBV	470497	785240	17.29%	2.001%
12	7.422	729	737	750	rBV	462010	789802	17.39%	2.012%
13	7.522	750	754	756	rVB5	3179	4818	0.11%	0.012%
14	7.887	809	816	824	rBV	502169	838318	18.46%	2.136%
15	7.958	824	828	837	rVB	60898	97832	2.15%	0.249%
16	8.599	928	937	947	rBV	387604	655438	14.43%	1.670%
17	8.716	955	957	965	rVB5	7260	10585	0.23%	0.027%
18	8.987	997	1003	1007	rBV3	11482	19491	0.43%	0.050%
19	9.046	1007	1013	1025	rVV	649640	1147550	25.27%	2.924%
20	9.134	1026	1028	1032	rVB5	3463	5008	0.11%	0.013%
21	9.222	1039	1043	1048	rVB6	5839	11742	0.26%	0.030%
22	9.769	1127	1136	1149	rBV	469501	842673	18.56%	2.147%
23	9.940	1159	1165	1176	rVB2	51509	120845	2.66%	0.308%
24	10.187	1200	1207	1218	rBV	44723	94633	2.08%	0.241%
25	10.310	1221	1228	1247	rBV	670508	1247198	27.47%	3.177%
26	10.475	1253	1256	1260	rVB6	7693	10380	0.23%	0.026%
27	10.687	1284	1292	1308	rBV	764953	1336270	29.43%	3.404%
28	10.828	1308	1316	1340	rBV	532245	1062478	23.40%	2.707%
29	12.116	1528	1535	1540	rBV8	5914	12810	0.28%	0.033%
30	12.281	1557	1563	1570	rBV3	12715	26753	0.59%	0.068%
31	12.746	1639	1642	1647	rBV5	3095	5505	0.12%	0.014%
32	12.893	1661	1667	1670	rBV8	3506	6387	0.14%	0.016%
33	13.140	1704	1709	1713	rBV5	7084	10754	0.24%	0.027%
34	13.363	1741	1747	1753	rBV8	4146	7687	0.17%	0.020%
35	13.504	1762	1771	1773	rBV10	3720	7744	0.17%	0.020%
36	13.757	1808	1814	1818	rBV8	5994	12551	0.28%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010489.D
 Acq On : 23 May 2022 22:16
 Operator : CG/JU
 Sample : N2955-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.846	1825	1829	1835	rVB8	3399	5990	0.13%	0.015%
38	13.928	1835	1843	1856	rBV	1516940	2212883	48.73%	5.638%
39	14.210	1883	1891	1910	rBV	1626044	2518975	55.47%	6.418%
40	14.522	1935	1944	1953	rBV	1311798	1919335	42.27%	4.890%
41	14.604	1953	1958	1967	rVB2	28855	45051	0.99%	0.115%
42	14.746	1975	1982	1996	rBV4	29133	105068	2.31%	0.268%
43	14.951	2013	2017	2023	rVB9	5267	8633	0.19%	0.022%
44	15.198	2055	2059	2064	rBV2	12481	17238	0.38%	0.044%
45	15.328	2077	2081	2088	rVB5	7567	13202	0.29%	0.034%
46	15.516	2105	2113	2126	rBV	2189815	3231400	71.16%	8.233%
47	15.640	2128	2134	2149	rVV	296001	484882	10.68%	1.235%
48	15.757	2149	2154	2159	rVV2	31056	56021	1.23%	0.143%
49	15.810	2159	2163	2170	rVV7	14193	22992	0.51%	0.059%
50	15.887	2171	2176	2183	rVB3	9018	15504	0.34%	0.039%
51	16.087	2203	2210	2211	rBV7	4437	6057	0.13%	0.015%
52	16.216	2226	2232	2236	rBV9	3180	8279	0.18%	0.021%
53	16.298	2239	2246	2251	rBV7	9330	16695	0.37%	0.043%
54	16.869	2337	2343	2346	rBV6	6171	9796	0.22%	0.025%
55	16.945	2354	2356	2359	rBV4	5753	6055	0.13%	0.015%
56	17.063	2371	2376	2379	rVB6	3967	7309	0.16%	0.019%
57	17.269	2402	2411	2421	rBV	1572146	2267960	49.95%	5.778%
58	17.369	2422	2428	2443	rVV2	2610319	3817753	84.07%	9.726%
59	17.563	2457	2461	2466	rVB2	8284	11042	0.24%	0.028%
60	17.939	2519	2525	2532	rBV	368085	440109	9.69%	1.121%
61	18.045	2539	2543	2548	rBV6	3692	7402	0.16%	0.019%
62	18.228	2570	2574	2578	rBV	15797	20984	0.46%	0.053%
63	18.404	2600	2604	2608	rBV6	4602	6379	0.14%	0.016%
64	18.645	2641	2645	2647	rBV4	3928	6413	0.14%	0.016%
65	19.181	2732	2736	2741	rBV2	36682	49185	1.08%	0.125%
66	19.251	2744	2748	2753	rVV2	28632	42560	0.94%	0.108%
67	19.533	2793	2796	2800	rVB4	10255	9913	0.22%	0.025%
68	19.604	2802	2808	2824	rVV	3383443	4540894	100.00%	11.569%
69	21.351	3100	3105	3119	rBV	1636769	2367028	52.13%	6.030%
70	23.616	3483	3490	3504	rVB2	1570525	3425881	75.45%	8.728%
71	23.774	3510	3517	3531	rVB2	902729	1879265	41.39%	4.788%


Sum of corrected areas: 39251295

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010489.D
Acq On : 23 May 2022 22:16
Operator : CG/JU
Sample : N2955-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

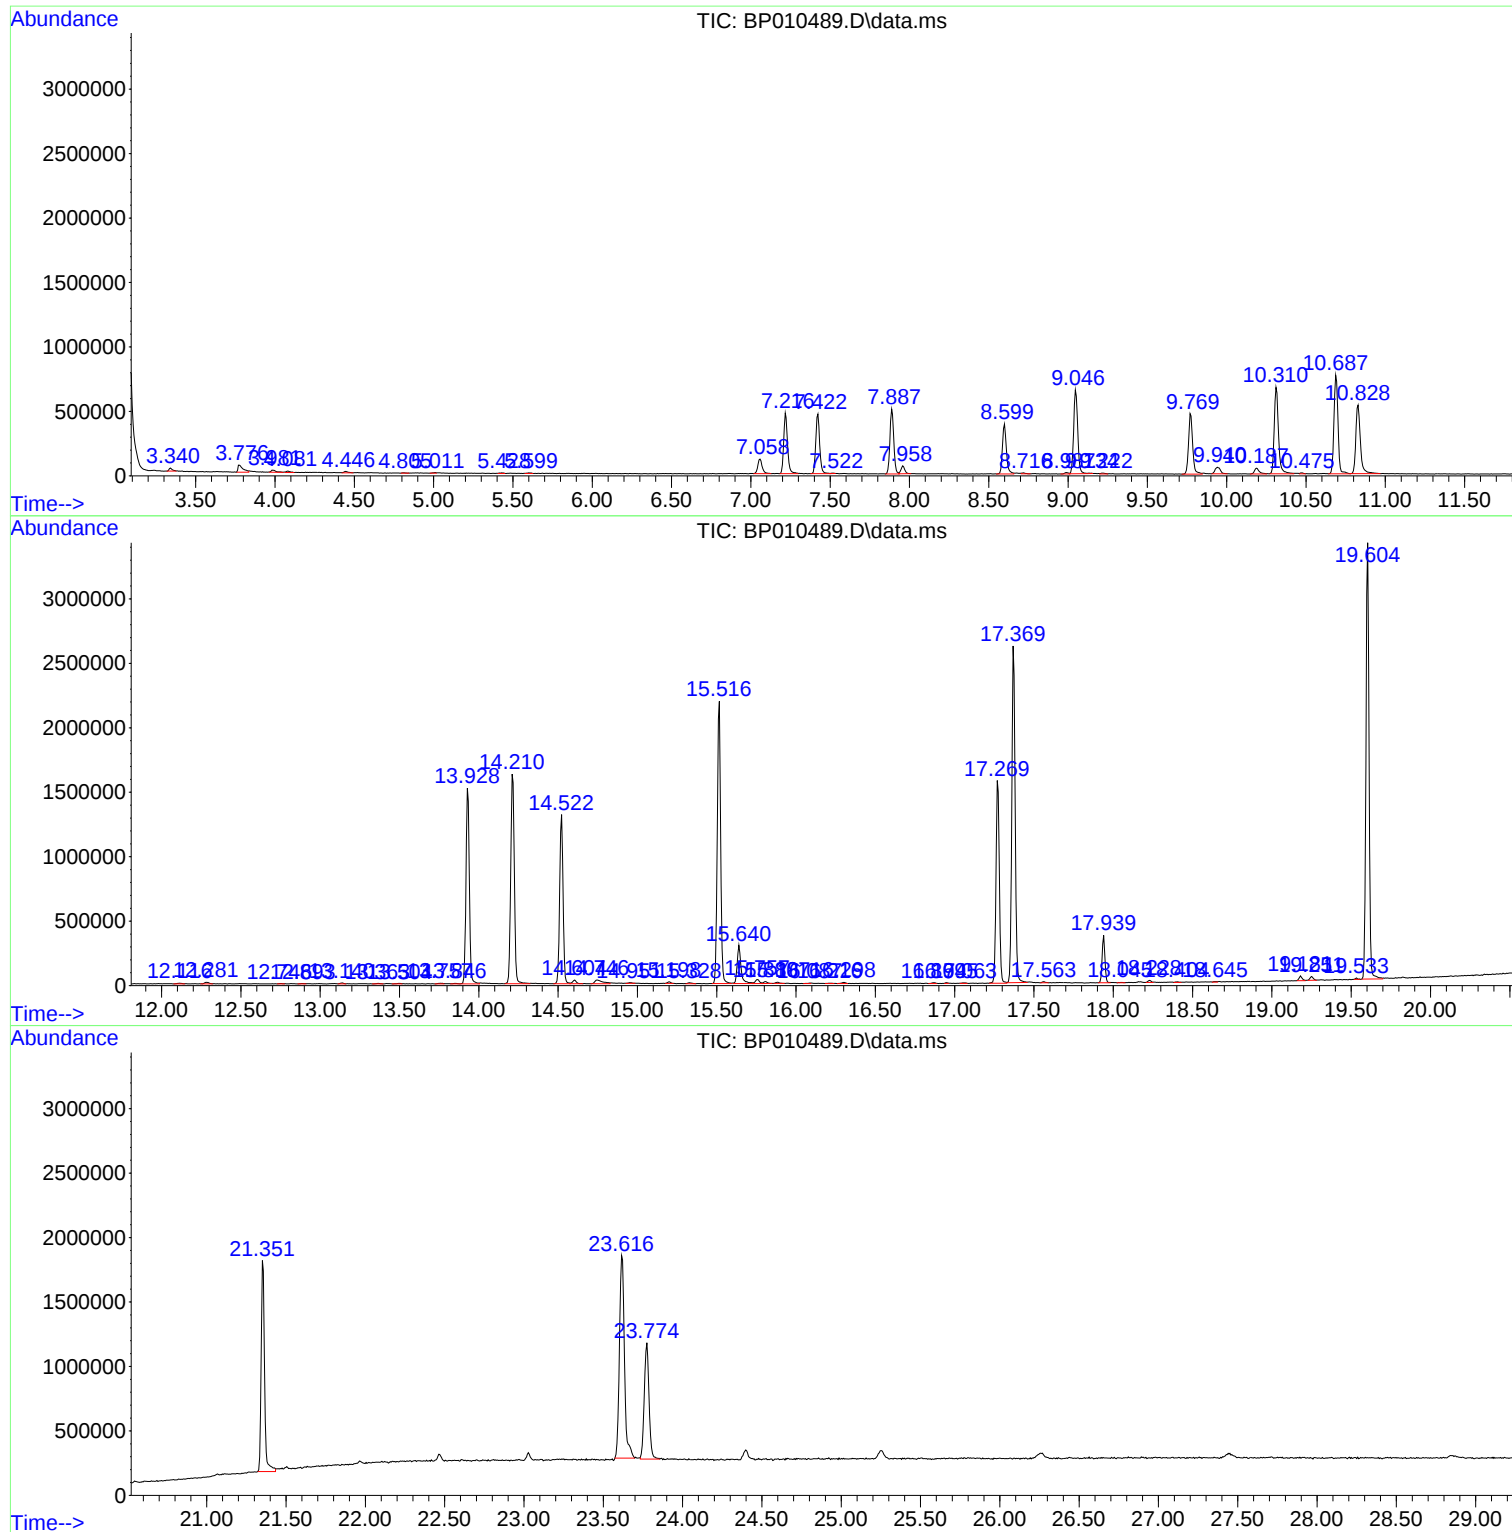

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010489.D
Acq On : 23 May 2022 22:16
Operator : CG/JU
Sample : N2955-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010489.D
Acq On : 23 May 2022 22:16
Operator : CG/JU
Sample : N2955-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc