

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010492.D
 Acq On : 23 May 2022 23:58
 Operator : CG/JU
 Sample : N2918-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rBV	33245	46136	0.75%	0.090%
2	3.770	112	116	133	rBV	96884	219072	3.54%	0.428%
3	3.987	148	153	158	rBV	20941	33705	0.54%	0.066%
4	4.075	165	168	175	rVB3	9067	15483	0.25%	0.030%
5	5.005	321	326	338	rVB	204069	316507	5.11%	0.619%
6	5.599	425	427	433	rVB4	5148	6743	0.11%	0.013%
7	7.052	667	674	684	rBV	151168	280268	4.53%	0.548%
8	7.216	695	702	714	rBV	638785	1064387	17.20%	2.080%
9	7.422	729	737	747	rBV	602126	1026659	16.59%	2.007%
10	7.722	784	788	794	rVB8	3536	7763	0.13%	0.015%
11	7.887	808	816	826	rBV	568961	947100	15.30%	1.851%
12	8.599	929	937	952	rBV	494631	886064	14.32%	1.732%
13	9.046	1006	1013	1031	rBV	916009	1576197	25.47%	3.081%
14	9.487	1083	1088	1093	rBV6	6456	9291	0.15%	0.018%
15	9.769	1129	1136	1150	rBV	734379	1260164	20.36%	2.463%
16	9.863	1150	1152	1159	rVB8	3773	6401	0.10%	0.013%
17	10.310	1220	1228	1242	rBV	941838	1703777	27.53%	3.330%
18	10.687	1283	1292	1307	rBV	876662	1475569	23.84%	2.884%
19	10.828	1307	1316	1335	rBV	860430	1692232	27.34%	3.308%
20	11.516	1428	1433	1436	rBV6	3792	6929	0.11%	0.014%
21	11.987	1507	1513	1517	rBV5	6281	11010	0.18%	0.022%
22	12.281	1558	1563	1572	rVB2	16890	32722	0.53%	0.064%
23	13.357	1739	1746	1754	rVB9	6226	13755	0.22%	0.027%
24	13.928	1837	1843	1853	rBV	2251337	3252392	52.55%	6.357%
25	14.210	1882	1891	1906	rBV	2349439	3630528	58.66%	7.096%
26	14.522	1937	1944	1954	rBV	1368149	2031388	32.82%	3.971%
27	14.734	1974	1980	1994	rBV	74426	209350	3.38%	0.409%
28	14.945	2010	2016	2022	rVB10	9371	19664	0.32%	0.038%
29	15.181	2048	2056	2062	rBV10	6194	14813	0.24%	0.029%
30	15.269	2066	2071	2077	rVV3	15738	28016	0.45%	0.055%
31	15.322	2077	2080	2085	rVV3	7982	15607	0.25%	0.031%
32	15.516	2105	2113	2127	rBV	3238428	4734503	76.49%	9.254%
33	15.640	2127	2134	2147	rVV	934877	1408431	22.76%	2.753%
34	15.757	2149	2154	2160	rVB	36966	61170	0.99%	0.120%
35	15.875	2169	2174	2178	rBV8	3421	6859	0.11%	0.013%
36	16.304	2242	2247	2252	rVB5	14794	22922	0.37%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010492.D
 Acq On : 23 May 2022 23:58
 Operator : CG/JU
 Sample : N2918-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	16.951	2352	2357	2362	rBV6	8236	13602	0.22%	0.027%
38	17.039	2367	2372	2375	rBV7	6002	8681	0.14%	0.017%
39	17.269	2402	2411	2422	rBV	1665538	2446476	39.53%	4.782%
40	17.375	2422	2429	2444	rVV	3535503	5260542	84.99%	10.282%
41	17.475	2444	2446	2449	rVB4	6442	6747	0.11%	0.013%
42	17.563	2458	2461	2463	rBV4	5987	6665	0.11%	0.013%
43	17.775	2495	2497	2503	rVB7	5655	6312	0.10%	0.012%
44	17.939	2522	2525	2531	rVB8	17975	25573	0.41%	0.050%
45	18.039	2539	2542	2545	rBV5	4768	6568	0.11%	0.013%
46	18.157	2557	2562	2569	rBV3	34797	57961	0.94%	0.113%
47	18.228	2571	2574	2580	rVB2	10898	15927	0.26%	0.031%
48	18.445	2609	2611	2616	rVB5	5032	6528	0.11%	0.013%
49	18.892	2681	2687	2693	rBV9	13301	27216	0.44%	0.053%
50	19.181	2732	2736	2743	rVB3	45768	68346	1.10%	0.134%
51	19.251	2743	2748	2759	rBV	45461	82800	1.34%	0.162%
52	19.386	2768	2771	2773	rBV4	14619	14963	0.24%	0.029%
53	19.604	2802	2808	2822	rBV	4643064	6189418	100.00%	12.098%
54	21.063	3053	3056	3061	rBV5	52886	79055	1.28%	0.155%
55	21.351	3100	3105	3116	rBV	1696469	2365045	38.21%	4.623%
56	23.622	3483	3491	3506	rVV	2125652	4527153	73.14%	8.849%
57	23.774	3510	3517	3530	rVB2	896583	1871472	30.24%	3.658%




Sum of corrected areas: 51160627

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010492.D
Acq On : 23 May 2022 23:58
Operator : CG/JU
Sample : N2918-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

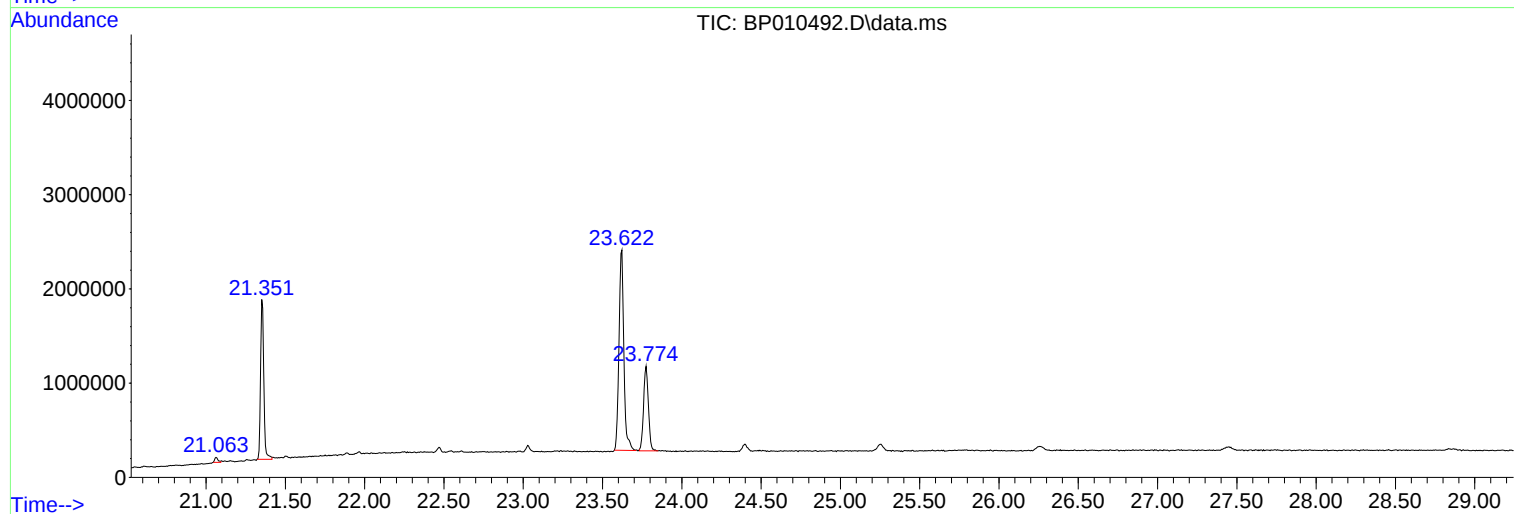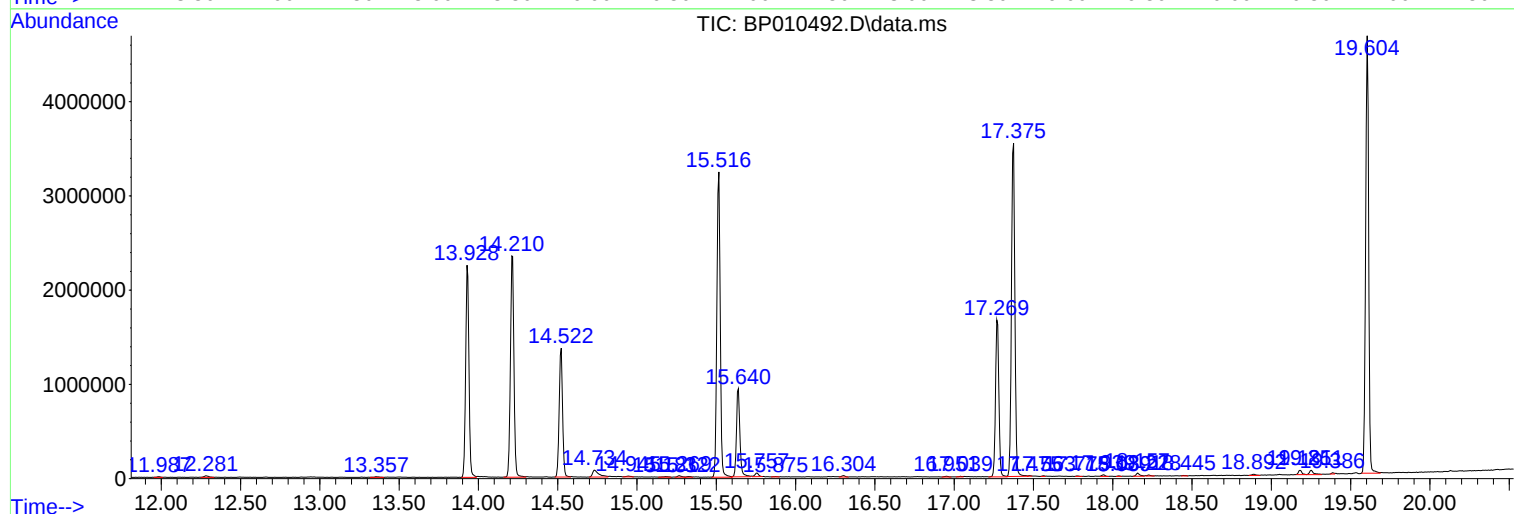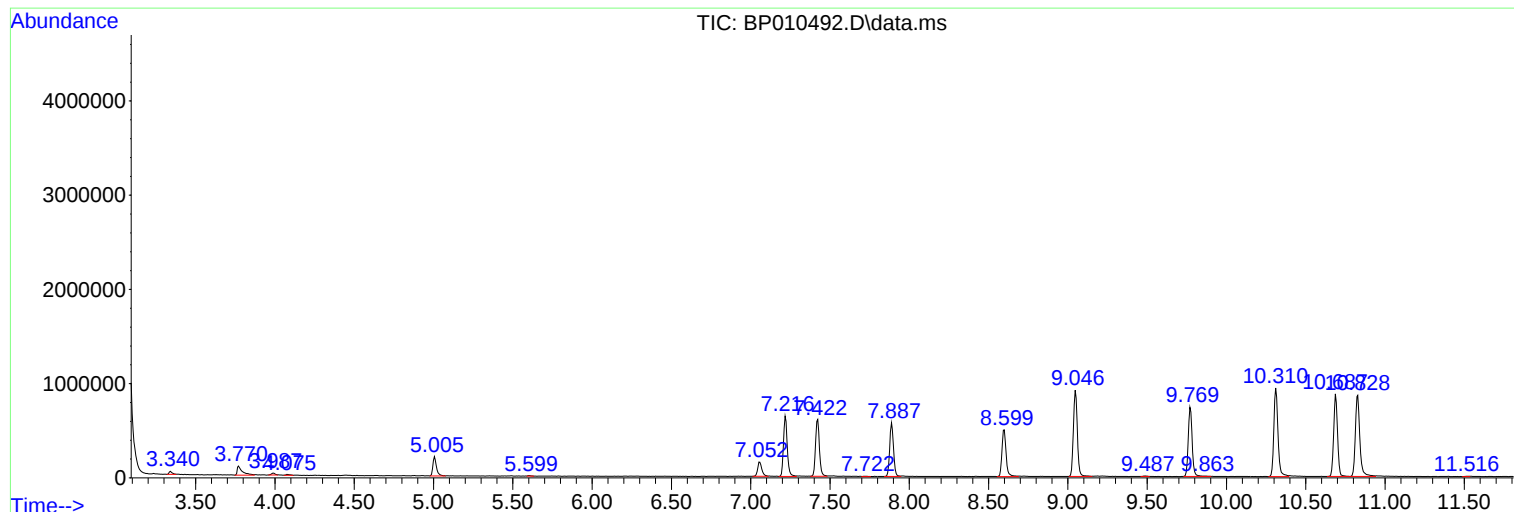

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010492.D
Acq On : 23 May 2022 23:58
Operator : CG/JU
Sample : N2918-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.005	6.68 ng/ul	316507	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
3	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	39		
4	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	38		
5	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36		

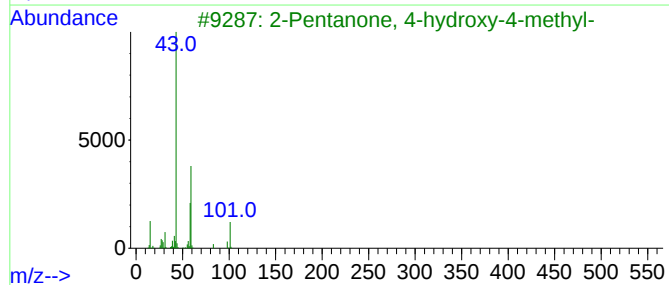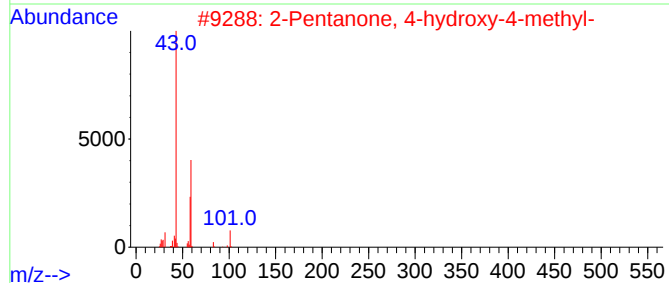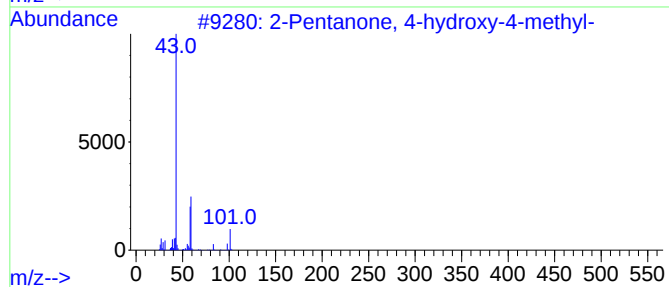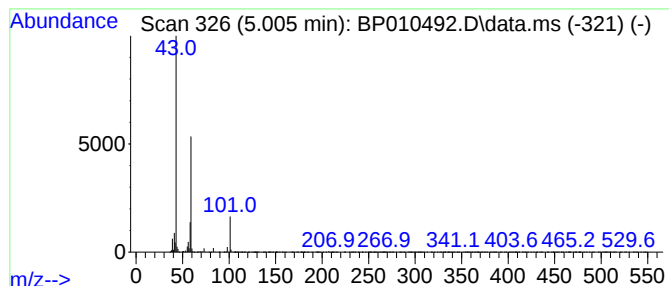

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010492.D
Acq On : 23 May 2022 23:58
Operator : CG/JU
Sample : N2918-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.005	6.7	ng/ul	316507	1	7.887	947100	20.0