

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010495.D
 Acq On : 24 May 2022 01:40
 Operator : CG/JU
 Sample : N2950-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	55	rVB	30474	50618	0.92%	0.108%
2	3.770	113	116	132	rBV	78609	171949	3.14%	0.368%
3	3.987	148	153	157	rBV2	22778	37576	0.69%	0.080%
4	4.081	165	169	173	rVB3	10659	18048	0.33%	0.039%
5	4.999	321	325	330	rBV4	5831	8702	0.16%	0.019%
6	5.181	351	356	362	rVB8	8493	14446	0.26%	0.031%
7	5.605	422	428	432	rBV3	5672	8545	0.16%	0.018%
8	7.058	667	675	683	rBV	142573	257916	4.71%	0.552%
9	7.217	695	702	714	rBV	563726	946594	17.27%	2.024%
10	7.422	730	737	749	rBV	551383	935210	17.07%	2.000%
11	7.887	809	816	828	rBV	625411	1040987	19.00%	2.226%
12	8.428	904	908	914	rVB9	4148	6953	0.13%	0.015%
13	8.599	930	937	951	rBV	449991	789381	14.40%	1.688%
14	9.046	1003	1013	1024	rBV	787066	1358389	24.79%	2.905%
15	9.487	1082	1088	1093	rBV4	9116	16729	0.31%	0.036%
16	9.769	1129	1136	1151	rBV	639723	1106634	20.19%	2.367%
17	10.310	1219	1228	1242	rBV	805893	1471390	26.85%	3.147%
18	10.687	1284	1292	1307	rBV	955908	1652348	30.15%	3.534%
19	10.828	1307	1316	1337	rBV	684985	1345997	24.56%	2.878%
20	11.981	1507	1512	1518	rVB2	21784	38112	0.70%	0.082%
21	12.122	1529	1536	1540	rBV10	4118	9891	0.18%	0.021%
22	12.281	1558	1563	1572	rVB3	12964	25027	0.46%	0.054%
23	12.893	1663	1667	1669	rBV5	3600	6033	0.11%	0.013%
24	13.357	1742	1746	1751	rVB6	6365	10036	0.18%	0.021%
25	13.928	1836	1843	1860	rBV	1893486	2695130	49.18%	5.764%
26	14.040	1860	1862	1868	rVB7	3800	5886	0.11%	0.013%
27	14.210	1884	1891	1905	rBV	2005165	2983895	54.45%	6.381%
28	14.422	1924	1927	1933	rVB6	7638	11409	0.21%	0.024%
29	14.522	1933	1944	1953	rBV	1523082	2283355	41.67%	4.883%
30	14.734	1974	1980	1997	rBV2	61212	196099	3.58%	0.419%
31	14.946	2010	2016	2023	rVB2	9652	17760	0.32%	0.038%
32	15.181	2049	2056	2062	rVB2	4831	11022	0.20%	0.024%
33	15.269	2067	2071	2076	rVV2	9659	15885	0.29%	0.034%
34	15.334	2076	2082	2086	rVV8	5208	11295	0.21%	0.024%
35	15.375	2086	2089	2097	rVB5	8513	13929	0.25%	0.030%
36	15.516	2105	2113	2127	rBV	2597365	4031154	73.56%	8.621%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010495.D
 Acq On : 24 May 2022 01:40
 Operator : CG/JU
 Sample : N2950-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	15.634	2127	2133	2147	rVV	848285	1300197	23.73%	2.781%
38	15.751	2149	2153	2160	rVB2	30664	55076	1.01%	0.118%
39	16.240	2233	2236	2242	rVB4	8416	10867	0.20%	0.023%
40	16.304	2242	2247	2250	rVB5	9992	15811	0.29%	0.034%
41	16.493	2274	2279	2283	rBV3	6879	10978	0.20%	0.023%
42	16.775	2322	2327	2331	rBV8	3244	6921	0.13%	0.015%
43	16.945	2350	2356	2363	rBV8	8305	16271	0.30%	0.035%
44	17.034	2368	2371	2375	rBV3	9803	14332	0.26%	0.031%
45	17.269	2404	2411	2421	rBV	1904608	2722085	49.67%	5.821%
46	17.369	2421	2428	2443	rVV	3296182	4752440	86.72%	10.163%
47	17.563	2458	2461	2465	rBV6	5578	9782	0.18%	0.021%
48	17.775	2494	2497	2502	rBV7	7365	10009	0.18%	0.021%
49	17.939	2521	2525	2532	rVB6	16270	23099	0.42%	0.049%
50	18.157	2558	2562	2571	rBV3	40126	73536	1.34%	0.157%
51	18.228	2571	2574	2578	rVB4	7337	11892	0.22%	0.025%
52	18.445	2607	2611	2614	rBV4	9723	10838	0.20%	0.023%
53	19.045	2710	2713	2716	rBV5	9018	13871	0.25%	0.030%
54	19.181	2732	2736	2742	rBV2	44918	59747	1.09%	0.128%
55	19.251	2744	2748	2755	rVV	37688	52147	0.95%	0.112%
56	19.386	2768	2771	2775	rBV6	15399	22966	0.42%	0.049%
57	19.534	2792	2796	2800	rBV7	14798	19259	0.35%	0.041%
58	19.604	2802	2808	2821	rBV	4110768	5480072	100.00%	11.719%
59	21.063	3053	3056	3061	rBV5	57498	75614	1.38%	0.162%
60	21.351	3100	3105	3118	rBV	1813148	2601530	47.47%	5.563%
61	23.616	3483	3490	3504	rBV2	1781402	3812374	69.57%	8.153%
62	23.774	3510	3517	3527	rVB2	936700	1974849	36.04%	4.223%




Sum of corrected areas: 46760893

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010495.D
Acq On : 24 May 2022 01:40
Operator : CG/JU
Sample : N2950-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

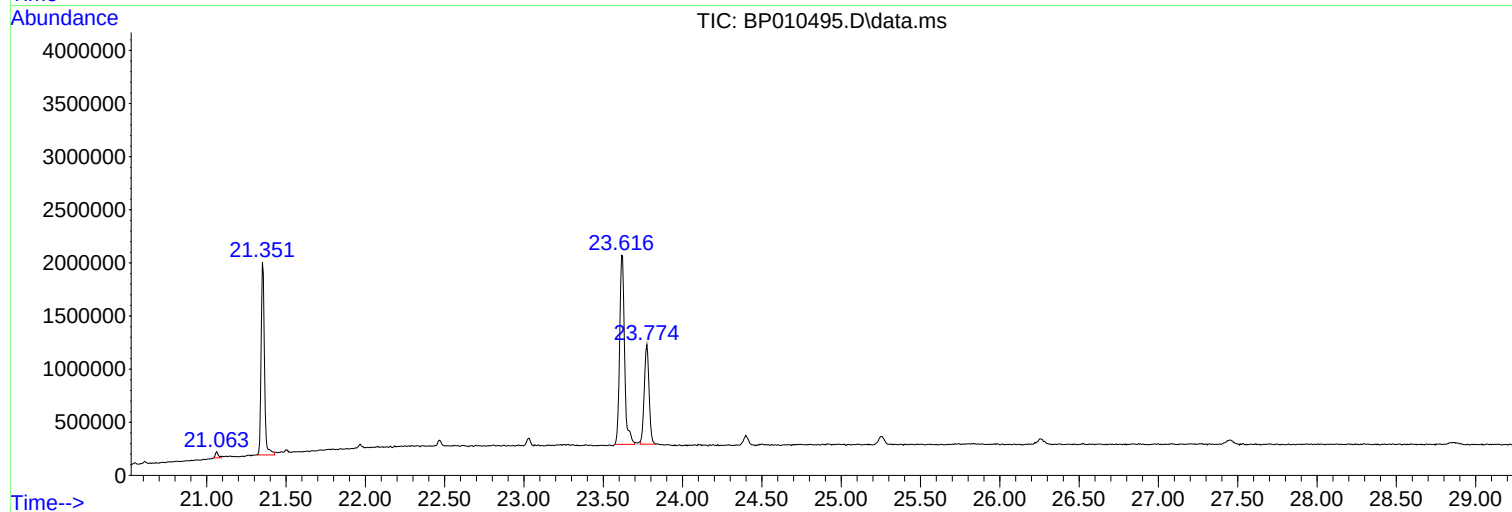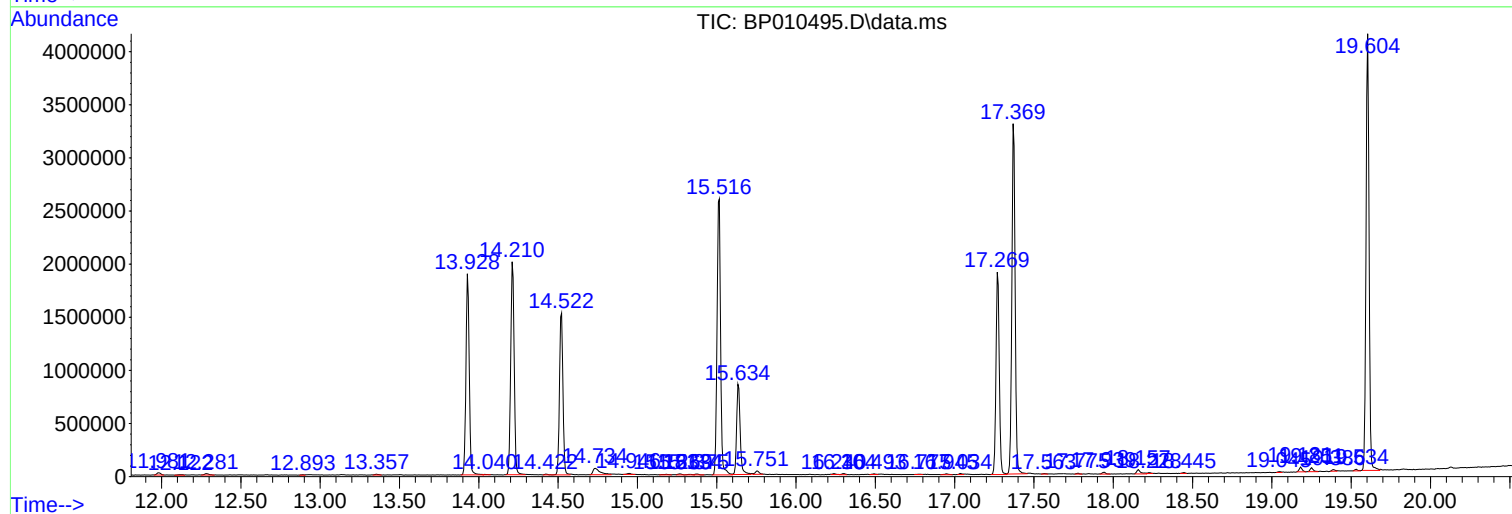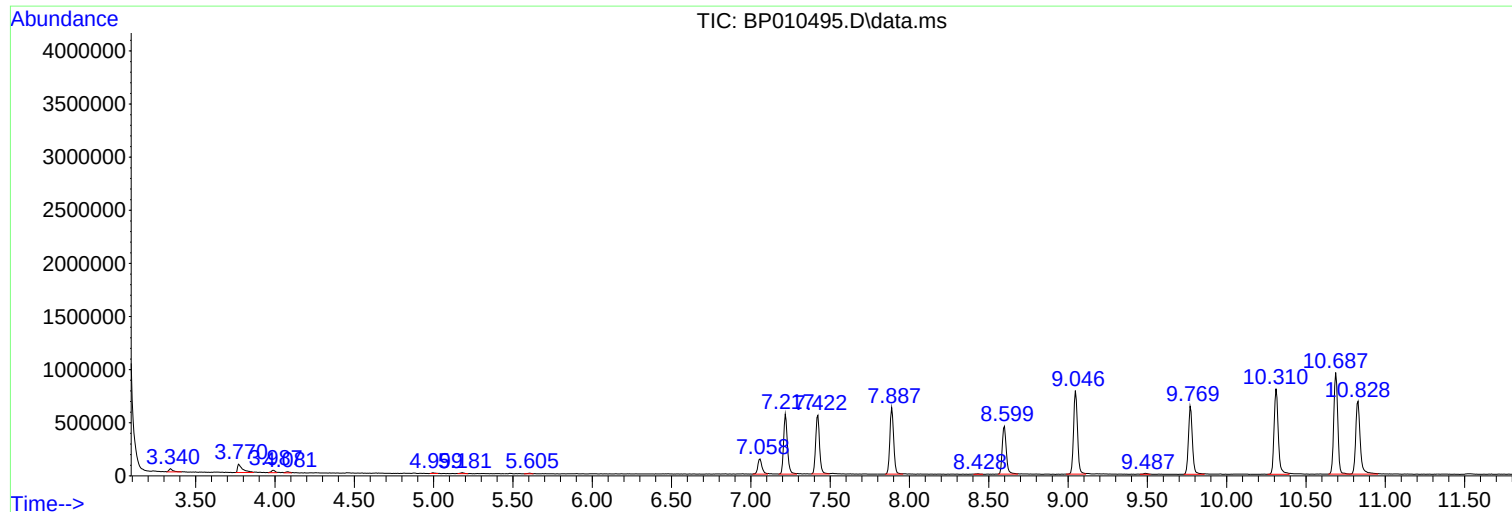

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010495.D
Acq On : 24 May 2022 01:40
Operator : CG/JU
Sample : N2950-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010495.D
Acq On : 24 May 2022 01:40
Operator : CG/JU
Sample : N2950-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc