

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010496.D
 Acq On : 24 May 2022 02:13
 Operator : CG/JU
 Sample : N2950-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	23	25	29	rVB5	8993	9750	0.17%	0.021%
2	3.340	40	43	50	rVB	26787	35911	0.64%	0.077%
3	3.775	113	117	129	rBV	59139	134690	2.40%	0.288%
4	3.987	149	153	160	rBV	26039	43507	0.78%	0.093%
5	4.081	165	169	180	rVB	25212	46342	0.83%	0.099%
6	4.634	258	263	268	rVB6	4405	8262	0.15%	0.018%
7	4.875	300	304	309	rBV6	5877	9049	0.16%	0.019%
8	5.005	322	326	331	rVB2	6666	10599	0.19%	0.023%
9	5.175	351	355	359	rBV4	5897	11392	0.20%	0.024%
10	5.399	390	393	398	rBV6	4097	5811	0.10%	0.012%
11	5.534	411	416	423	rBV3	11191	24275	0.43%	0.052%
12	5.605	425	428	432	rVB3	5216	5770	0.10%	0.012%
13	5.905	474	479	484	rVB4	8988	14924	0.27%	0.032%
14	6.975	658	661	668	rVB7	5031	8497	0.15%	0.018%
15	7.058	668	675	689	rBV	158793	302254	5.39%	0.646%
16	7.216	694	702	710	rBV	618886	1004604	17.91%	2.146%
17	7.422	727	737	747	rBV	605751	1024605	18.27%	2.189%
18	7.516	750	753	754	rVV3	8010	9745	0.17%	0.021%
19	7.540	754	757	764	rVB4	11220	18471	0.33%	0.039%
20	7.887	808	816	827	rBV	599882	990561	17.66%	2.116%
21	8.434	905	909	914	rBV8	3563	7147	0.13%	0.015%
22	8.593	930	936	951	rBV	482489	847788	15.12%	1.811%
23	9.046	1003	1013	1024	rBV	828956	1458553	26.00%	3.115%
24	9.175	1031	1035	1039	rBV4	5275	8594	0.15%	0.018%
25	9.487	1082	1088	1092	rBV3	8213	12072	0.22%	0.026%
26	9.769	1128	1136	1150	rBV	670116	1183752	21.10%	2.528%
27	10.310	1219	1228	1245	rBV	884001	1587258	28.30%	3.390%
28	10.687	1284	1292	1308	rVB	886416	1522918	27.15%	3.253%
29	10.828	1308	1316	1334	rBV	541376	1114408	19.87%	2.380%
30	11.516	1426	1433	1443	rBV10	11324	31456	0.56%	0.067%
31	11.981	1507	1512	1518	rBV	18084	31273	0.56%	0.067%
32	12.128	1532	1537	1542	rVB8	4407	6663	0.12%	0.014%
33	12.281	1551	1563	1569	rBV3	15085	31424	0.56%	0.067%
34	12.493	1592	1599	1601	rBV7	3654	6473	0.12%	0.014%
35	13.351	1742	1745	1750	rVB6	5897	10070	0.18%	0.022%
36	13.834	1820	1827	1829	rBV7	4395	7332	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010496.D
 Acq On : 24 May 2022 02:13
 Operator : CG/JU
 Sample : N2950-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.928	1836	1843	1858	rBV	2033721	2853692	50.88%	6.095%
38	14.210	1881	1891	1907	rBV	2079007	3143819	56.05%	6.715%
39	14.428	1924	1928	1932	rVB3	9892	12525	0.22%	0.027%
40	14.516	1936	1943	1952	rBV	1325911	2053547	36.61%	4.386%
41	14.657	1963	1967	1969	rBV5	5176	6334	0.11%	0.014%
42	14.728	1974	1979	1988	rBV	77909	186712	3.33%	0.399%
43	14.934	2010	2014	2020	rVB9	6618	12644	0.23%	0.027%
44	15.269	2063	2071	2076	rBV	13516	25722	0.46%	0.055%
45	15.334	2076	2082	2084	rBV3	6372	11678	0.21%	0.025%
46	15.375	2086	2089	2093	rVB2	12793	15703	0.28%	0.034%
47	15.516	2102	2113	2119	rBV	2779520	4120354	73.46%	8.801%
48	15.634	2127	2133	2149	rBV	946466	1393174	24.84%	2.976%
49	15.757	2149	2154	2163	rVB2	36278	68300	1.22%	0.146%
50	15.881	2171	2175	2178	rVB6	4163	7071	0.13%	0.015%
51	16.204	2226	2230	2231	rBV4	5359	6413	0.11%	0.014%
52	16.239	2232	2236	2243	rVV2	20118	37332	0.67%	0.080%
53	16.298	2243	2246	2253	rVB5	16418	25854	0.46%	0.055%
54	16.816	2331	2334	2338	rVB6	4605	7106	0.13%	0.015%
55	16.945	2353	2356	2361	rVB7	7010	8867	0.16%	0.019%
56	17.034	2367	2371	2377	rBV3	15043	25370	0.45%	0.054%
57	17.086	2378	2380	2385	rVB6	6042	6510	0.12%	0.014%
58	17.269	2405	2411	2421	rBV	1677573	2435656	43.42%	5.203%
59	17.375	2421	2429	2443	rVV	3333331	4880983	87.02%	10.426%
60	17.775	2492	2497	2503	rBV2	18608	27306	0.49%	0.058%
61	17.939	2521	2525	2530	rBV6	22195	28678	0.51%	0.061%
62	18.157	2557	2562	2568	rBV	56217	87689	1.56%	0.187%
63	18.228	2571	2574	2577	rVB4	10766	14450	0.26%	0.031%
64	18.445	2607	2611	2615	rBV	16587	17967	0.32%	0.038%
65	18.633	2639	2643	2646	rBV6	5727	9595	0.17%	0.020%
66	19.051	2711	2714	2718	rBV6	12012	14543	0.26%	0.031%
67	19.180	2732	2736	2742	rBV2	48416	69773	1.24%	0.149%
68	19.251	2744	2748	2754	rVV	43791	58880	1.05%	0.126%
69	19.386	2768	2771	2776	rBV6	27485	39569	0.71%	0.085%
70	19.533	2793	2796	2800	rVB6	12816	16746	0.30%	0.036%
71	19.604	2802	2808	2822	rBV	4369870	5608914	100.00%	11.981%
72	21.063	3052	3056	3062	rBV3	91932	159866	2.85%	0.341%
73	21.351	3100	3105	3119	rBV	1603695	2231644	39.79%	4.767%
74	23.616	3483	3490	3508	rVV2	1772206	3785439	67.49%	8.086%
75	23.774	3510	3517	3529	rVB2	786824	1714021	30.56%	3.661%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010496.D
Acq On : 24 May 2022 02:13
Operator : CG/JU
Sample : N2950-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46816646

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010496.D
Acq On : 24 May 2022 02:13
Operator : CG/JU
Sample : N2950-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

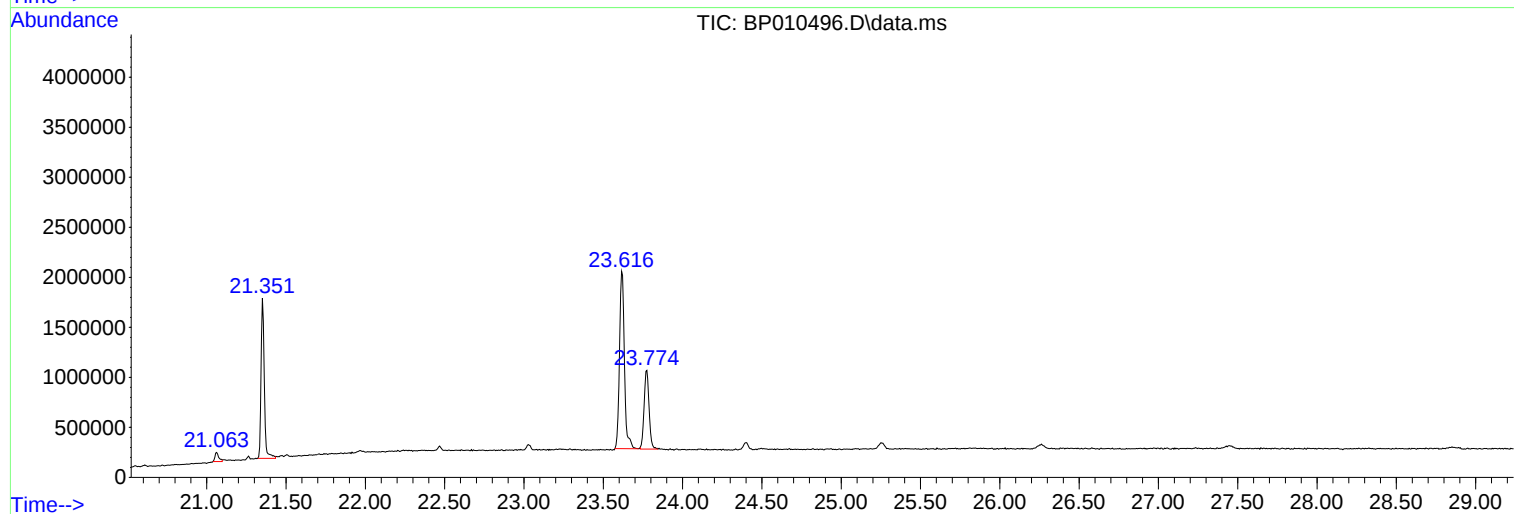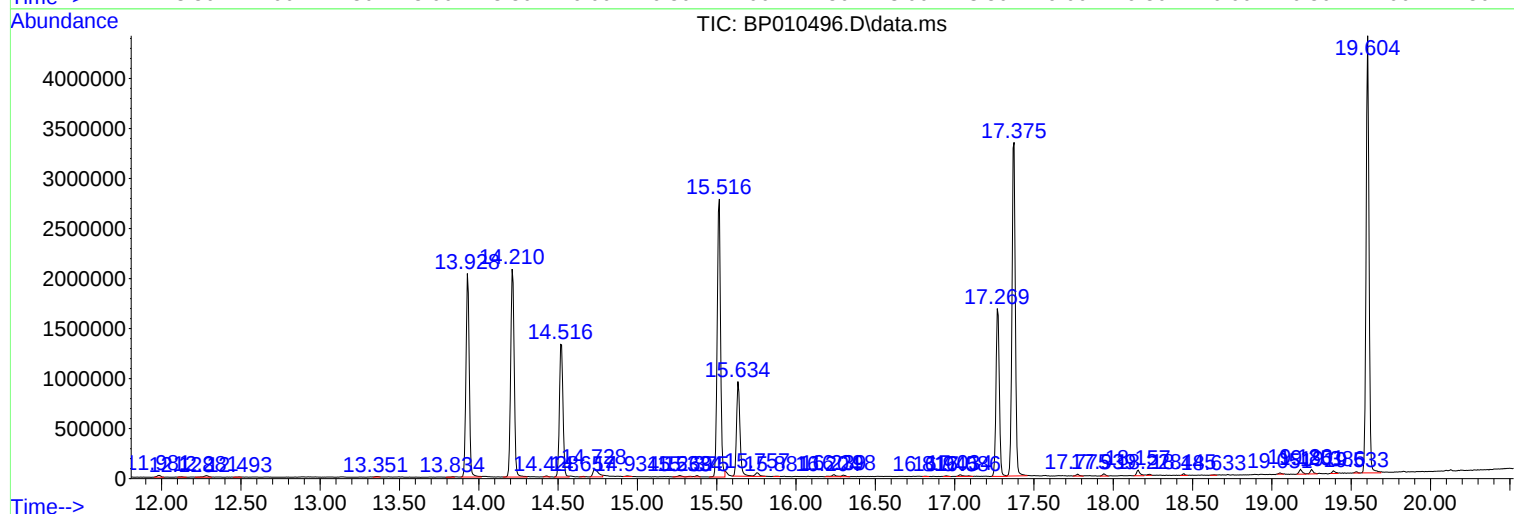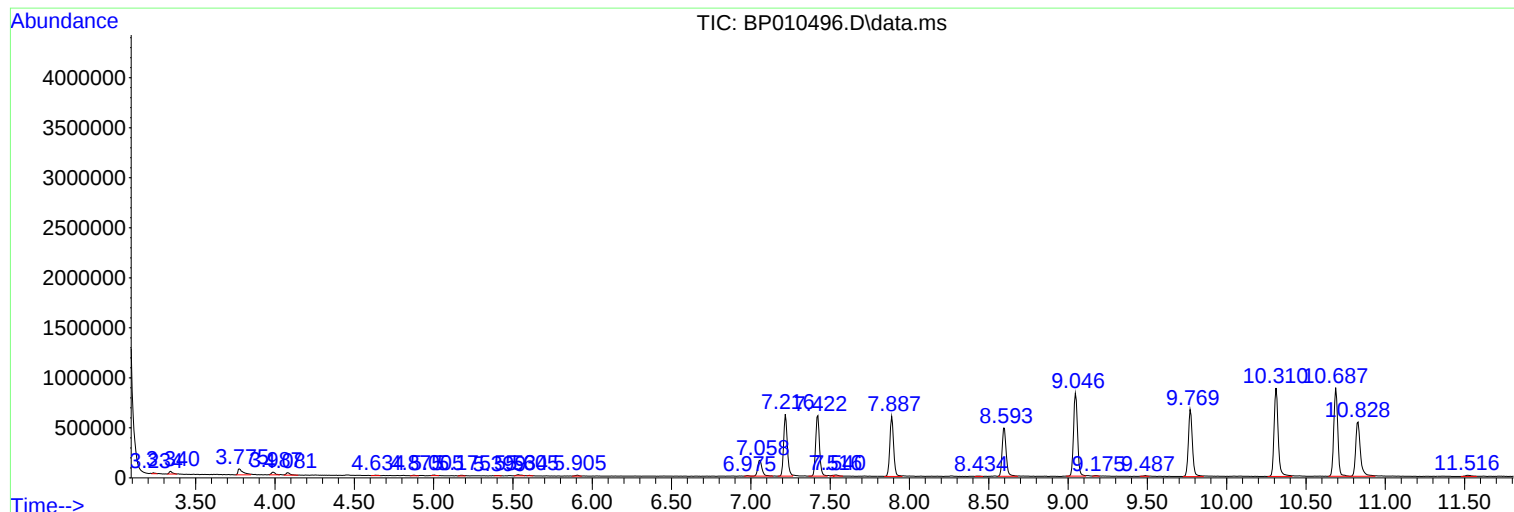

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010496.D
Acq On : 24 May 2022 02:13
Operator : CG/JU
Sample : N2950-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010496.D
Acq On : 24 May 2022 02:13
Operator : CG/JU
Sample : N2950-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc