

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010502.D
 Acq On : 24 May 2022 06:10
 Operator : CG/JU
 Sample : PB145034BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK034

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	40	43	54	rVB	38641	67954	1.39%	0.139%
2	3.752	110	113	136	rBV	517325	1064733	21.82%	2.171%
3	4.081	166	169	174	rVB2	8902	11817	0.24%	0.024%
4	7.051	668	674	690	rBV	747564	1281890	26.28%	2.614%
5	7.216	696	702	715	rVB	585035	953978	19.55%	1.945%
6	7.416	730	736	747	rBV	755940	1272731	26.09%	2.595%
7	7.887	806	816	825	rBV	636855	1036883	21.25%	2.114%
8	8.593	929	936	948	rBV	967492	1657399	33.97%	3.380%
9	9.045	1005	1013	1027	rBV	827364	1424614	29.20%	2.905%
10	9.769	1129	1136	1149	rBV	693264	1197449	24.54%	2.442%
11	10.310	1220	1228	1245	rBV	950441	1710283	35.06%	3.488%
12	10.687	1284	1292	1305	rBV	944076	1631340	33.44%	3.327%
13	10.822	1308	1315	1340	rBV	882961	1748017	35.83%	3.565%
14	12.286	1556	1564	1572	rBV3	12773	30523	0.63%	0.062%
15	13.928	1835	1843	1856	rBV	1885848	2671255	54.75%	5.447%
16	14.039	1860	1862	1870	rVB8	4430	9022	0.18%	0.018%
17	14.210	1884	1891	1905	rBV	2027114	3026151	62.03%	6.171%
18	14.516	1936	1943	1954	rBV	1471482	2255932	46.24%	4.600%
19	14.722	1970	1978	2010	rBV	536778	1225967	25.13%	2.500%
20	14.945	2012	2016	2022	rVB9	6066	12764	0.26%	0.026%
21	15.510	2105	2112	2126	rBV	2597282	3803377	77.96%	7.756%
22	15.633	2128	2133	2149	rVV	704635	1090044	22.34%	2.223%
23	15.751	2149	2153	2165	rVB3	31283	59292	1.22%	0.121%
24	16.298	2242	2246	2251	rVB5	10848	15423	0.32%	0.031%
25	16.945	2353	2356	2362	rVB7	5320	7452	0.15%	0.015%
26	17.063	2371	2376	2380	rBV7	4689	8350	0.17%	0.017%
27	17.269	2405	2411	2421	rBV	1844730	2699792	55.34%	5.505%
28	17.369	2421	2428	2445	rVV2	2876204	4234275	86.79%	8.635%
29	18.163	2559	2563	2568	rBV8	6613	12840	0.26%	0.026%
30	19.180	2732	2736	2740	rVB2	32880	44743	0.92%	0.091%
31	19.251	2743	2748	2754	rBV	33967	49692	1.02%	0.101%
32	19.533	2794	2796	2799	rVB3	8023	5874	0.12%	0.012%
33	19.604	2801	2808	2821	rBV	3685666	4878658	100.00%	9.949%
34	21.351	3100	3105	3119	rBV	1835178	2543698	52.14%	5.187%
35	23.615	3483	3490	3508	rVB2	1588217	3338384	68.43%	6.808%
36	23.774	3510	3517	3530	rVB2	918008	1955887	40.09%	3.988%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Title : SVOA CALIBRATION




Sum of corrected areas: 49038483

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

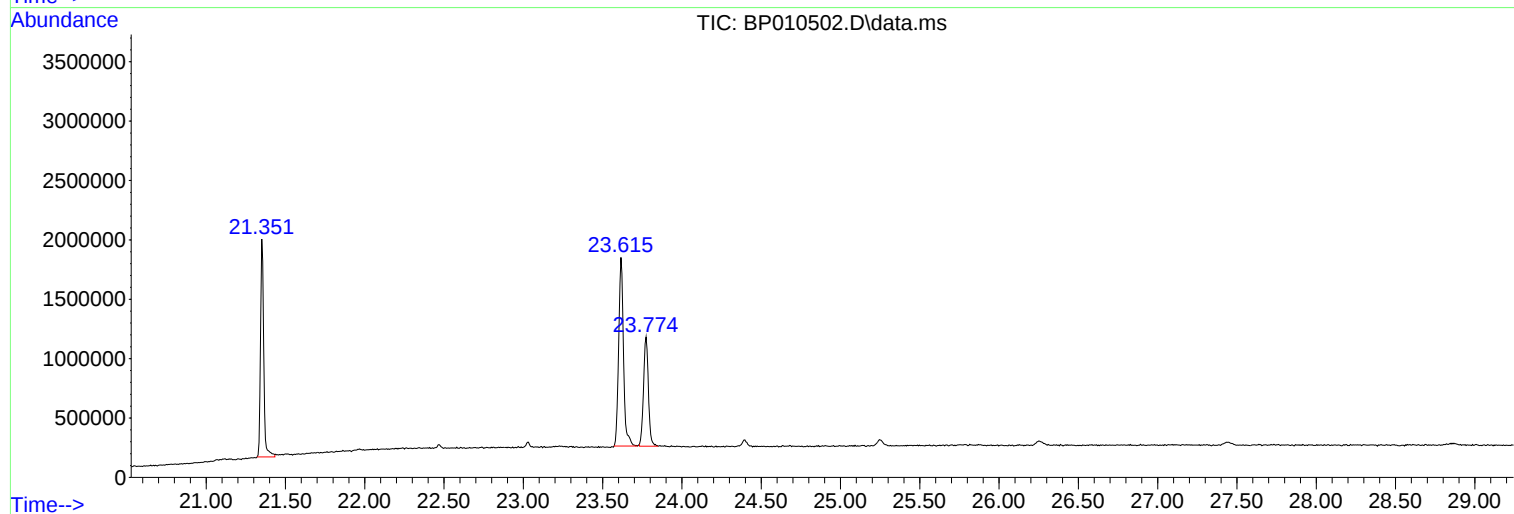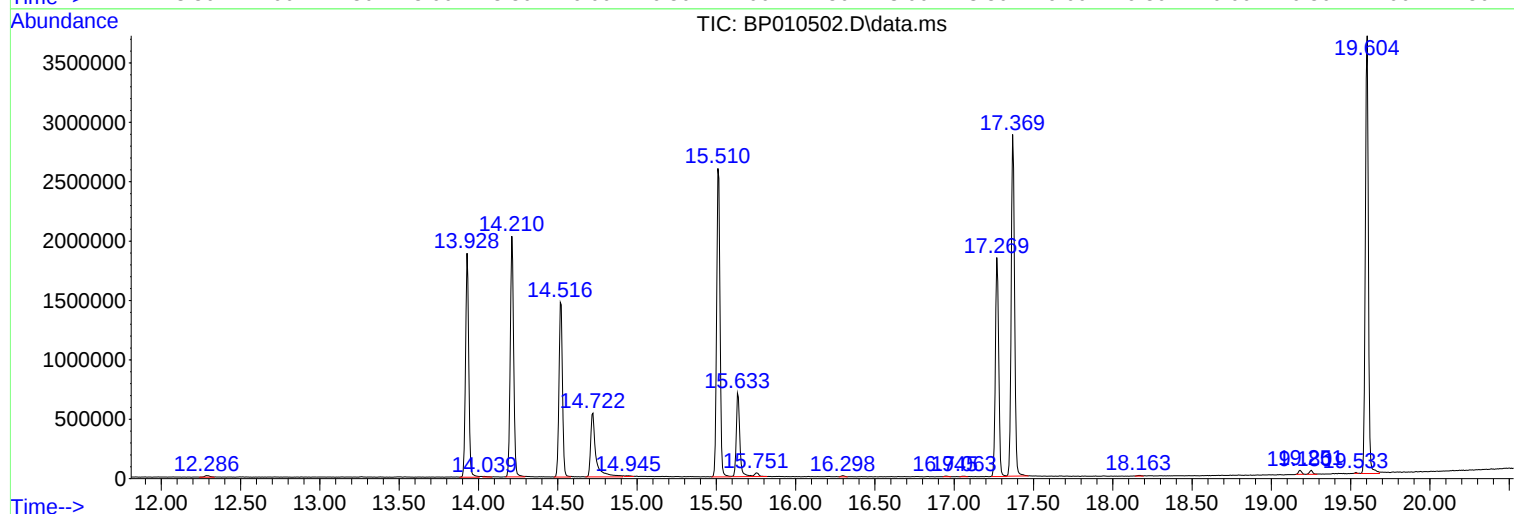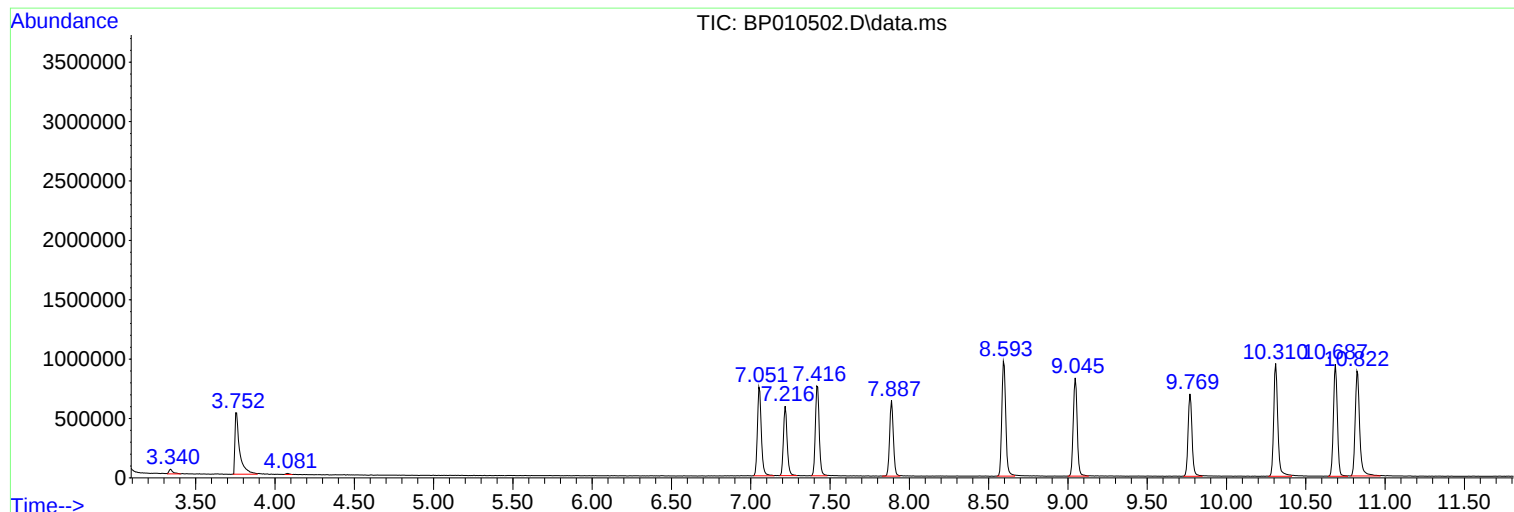

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010502.D
Acq On : 24 May 2022 06:10
Operator : CG/JU
Sample : PB145034BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------