

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.705	103	105	107	rBV3	3355	3665	0.12%	0.022%
2	3.981	150	152	158	rBV7	3345	6921	0.23%	0.041%
3	4.081	165	169	175	rBV3	8982	14172	0.47%	0.085%
4	4.240	194	196	198	rBV3	2552	3187	0.11%	0.019%
5	6.711	613	616	618	rBV3	2162	3046	0.10%	0.018%
6	7.228	699	704	706	rBV5	4935	7472	0.25%	0.045%
7	7.434	733	739	742	rBV8	4633	7409	0.25%	0.044%
8	7.540	751	757	764	rVB10	5289	10381	0.34%	0.062%
9	7.887	808	816	831	rBV	580683	1009930	33.56%	6.051%
10	7.999	833	835	840	rVV6	4976	7149	0.24%	0.043%
11	8.122	853	856	858	rBV4	2016	3039	0.10%	0.018%
12	8.264	873	880	886	rVV2	17456	32118	1.07%	0.192%
13	8.428	901	908	917	rBV	55430	106968	3.55%	0.641%
14	8.622	933	941	944	rBV10	3092	5657	0.19%	0.034%
15	9.016	1005	1008	1012	rVB6	2267	3499	0.12%	0.021%
16	9.069	1012	1017	1023	rBV9	6968	17558	0.58%	0.105%
17	9.369	1062	1068	1075	rVB9	7072	16079	0.53%	0.096%
18	9.781	1132	1138	1144	rBV9	4165	9386	0.31%	0.056%
19	9.940	1161	1165	1172	rVV9	3222	5740	0.19%	0.034%
20	10.093	1186	1191	1200	rVB7	7573	18726	0.62%	0.112%
21	10.193	1205	1208	1212	rVV6	4511	7558	0.25%	0.045%
22	10.346	1227	1234	1236	rBV7	3540	7283	0.24%	0.044%
23	10.387	1239	1241	1249	rVB9	3729	5825	0.19%	0.035%
24	10.610	1274	1279	1281	rBV5	2195	3450	0.11%	0.021%
25	10.687	1284	1292	1296	rVV	895399	1610252	53.51%	9.648%
26	10.734	1296	1300	1314	rVV	1774430	3009307	100.00%	18.031%
27	10.852	1314	1320	1329	rVB	75905	141663	4.71%	0.849%
28	11.322	1397	1400	1403	rBV4	2478	3719	0.12%	0.022%
29	11.475	1422	1426	1431	rVB8	2456	3352	0.11%	0.020%
30	11.793	1475	1480	1483	rBV6	3586	5364	0.18%	0.032%
31	11.975	1506	1511	1514	rBV7	2792	4017	0.13%	0.024%
32	12.240	1552	1556	1561	rBV4	7647	12001	0.40%	0.072%
33	12.346	1566	1574	1588	rBV	224472	404739	13.45%	2.425%
34	12.452	1590	1592	1593	rBV2	4699	3928	0.13%	0.024%
35	12.469	1593	1595	1601	rVB4	7010	10594	0.35%	0.063%
36	12.563	1601	1611	1619	rBV	146335	267071	8.87%	1.600%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010518.D
 Acq On : 24 May 2022 16:18
 Operator : CG/JU
 Sample : N2950-03DL2 100X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTE9DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	13.357	1740	1746	1752	rBV2	35617	65633	2.18%	0.393%
38	13.399	1752	1753	1756	rVV3	4298	3570	0.12%	0.021%
39	13.557	1776	1780	1783	rBV4	7013	11021	0.37%	0.066%
40	13.699	1796	1804	1805	rBV6	9575	16921	0.56%	0.101%
41	13.840	1823	1828	1835	rBV3	15090	31548	1.05%	0.189%
42	13.898	1835	1838	1841	rVV4	10136	16225	0.54%	0.097%
43	13.940	1841	1845	1854	rVB	18934	34319	1.14%	0.206%
44	14.075	1865	1868	1871	rBV4	4702	6438	0.21%	0.039%
45	14.210	1887	1891	1895	rBV2	21414	37946	1.26%	0.227%
46	14.516	1934	1943	1949	rBV	1426422	2158714	71.73%	12.934%
47	14.581	1949	1954	1962	rVV	271174	423445	14.07%	2.537%
48	14.657	1962	1967	1981	rVB	47861	95298	3.17%	0.571%
49	14.834	1989	1997	1999	rBV8	5680	10412	0.35%	0.062%
50	14.922	2004	2012	2016	rBV	67371	120581	4.01%	0.722%
51	15.087	2036	2040	2048	rVB9	3650	7534	0.25%	0.045%
52	15.328	2076	2081	2083	rBV6	1718	3075	0.10%	0.018%
53	15.516	2108	2113	2118	rVV2	29518	49976	1.66%	0.299%
54	15.569	2118	2122	2134	rVB2	68337	111396	3.70%	0.667%
55	15.693	2134	2143	2146	rBV10	6275	15352	0.51%	0.092%
56	15.881	2173	2175	2179	rVB5	3618	3613	0.12%	0.022%
57	16.016	2195	2198	2204	rVB7	5213	8581	0.29%	0.051%
58	16.245	2233	2237	2238	rVV4	5112	4671	0.16%	0.028%
59	16.263	2238	2240	2243	rVB4	5074	5051	0.17%	0.030%
60	16.940	2352	2355	2361	rBV8	5932	10289	0.34%	0.062%
61	17.063	2372	2376	2377	rBV4	3898	4886	0.16%	0.029%
62	17.269	2404	2411	2423	rBV	1685671	2557165	84.98%	15.322%
63	17.375	2425	2429	2438	rVB	31125	59683	1.98%	0.358%
64	17.681	2474	2481	2494	rBV	128783	241485	8.02%	1.447%
65	17.992	2530	2534	2535	rBV4	2727	3521	0.12%	0.021%
66	18.192	2564	2568	2572	rVB6	6946	10727	0.36%	0.064%
67	18.381	2596	2600	2601	rBV4	3563	4080	0.14%	0.024%
68	19.604	2804	2808	2813	rBV2	33774	53182	1.77%	0.319%
69	21.351	3100	3105	3118	rBV	1544571	2136508	71.00%	12.801%
70	23.774	3510	3517	3526	rBV2	737738	1574874	52.33%	9.436%




Sum of corrected areas: 16689945

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010518.D
Acq On : 24 May 2022 16:18
Operator : CG/JU
Sample : N2950-03DL2 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE9DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

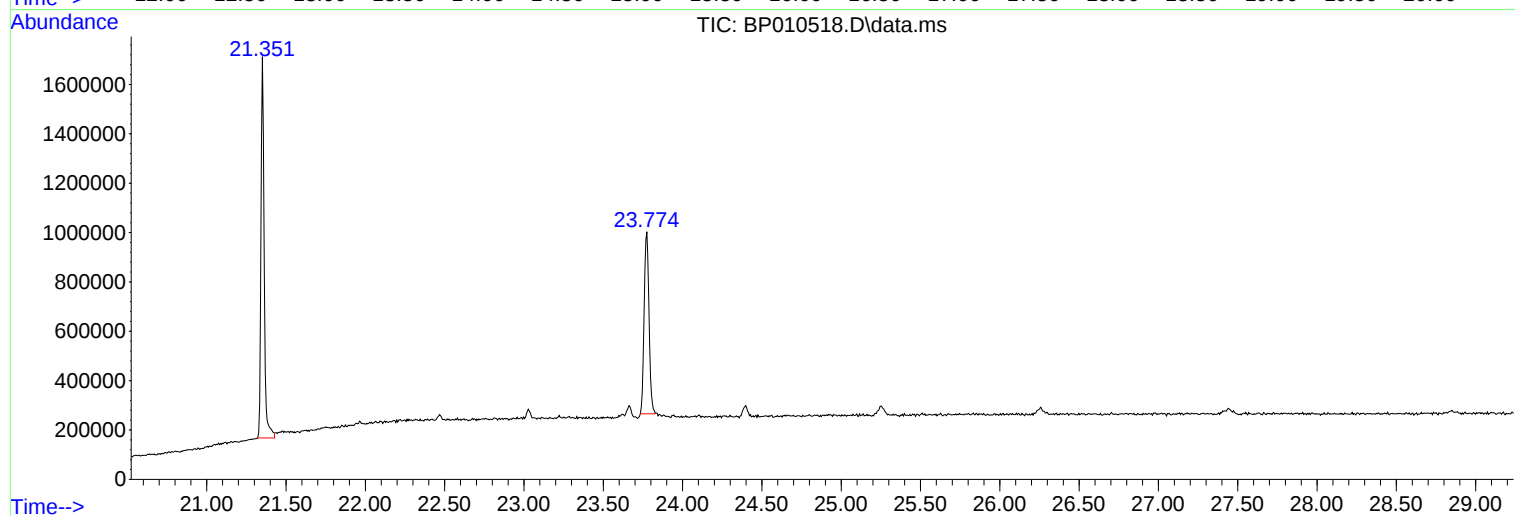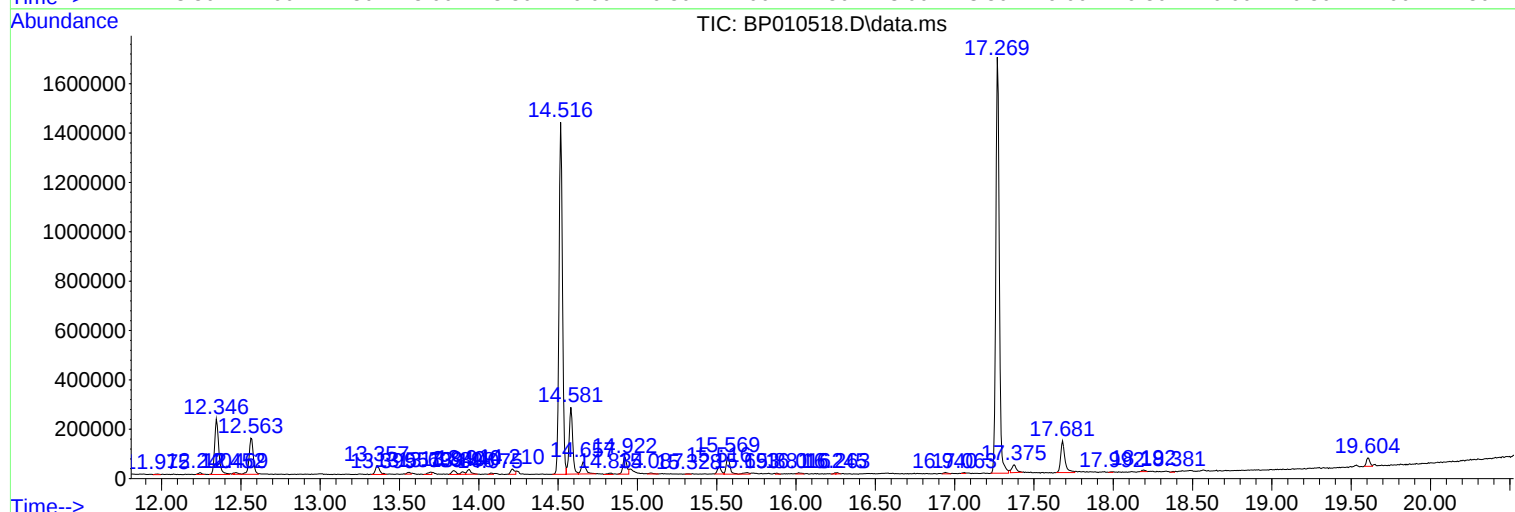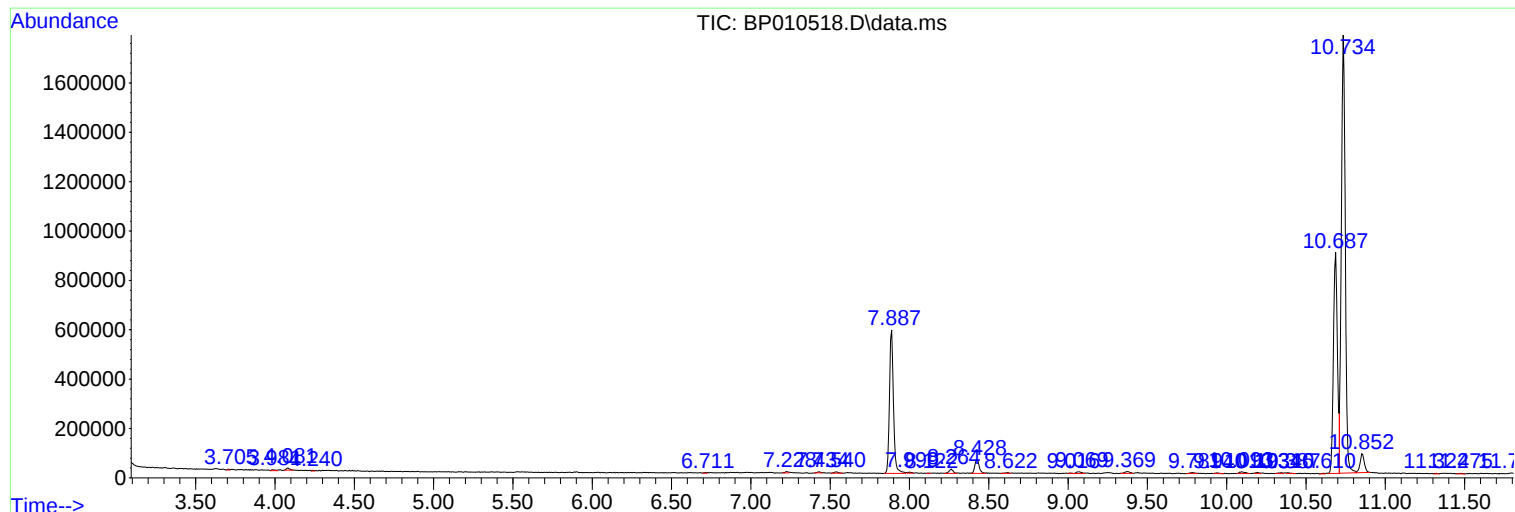

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010518.D
Acq On : 24 May 2022 16:18
Operator : CG/JU
Sample : N2950-03DL2 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE9DL2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.428	2.12 ng/ul	106968	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indene	116	C9H8	000095-13-6	94
2			Benzene, 1,2-propadienyl-	116	C9H8	002327-99-3	91
3			Indene	116	C9H8	000095-13-6	91
4			Benzene, 1-propynyl-	116	C9H8	000673-32-5	91
5			Benzene, 1-propynyl-	116	C9H8	000673-32-5	91

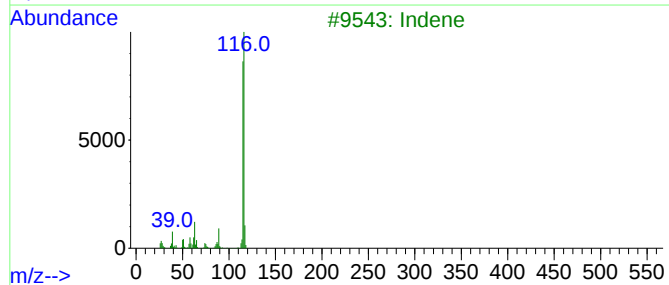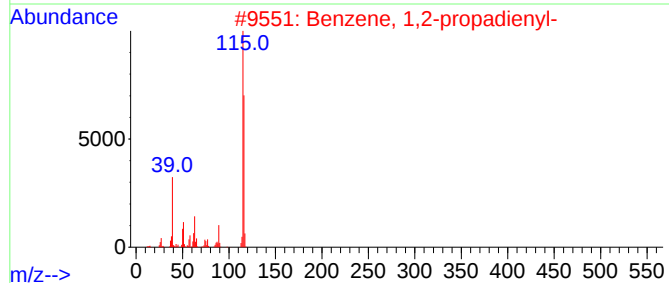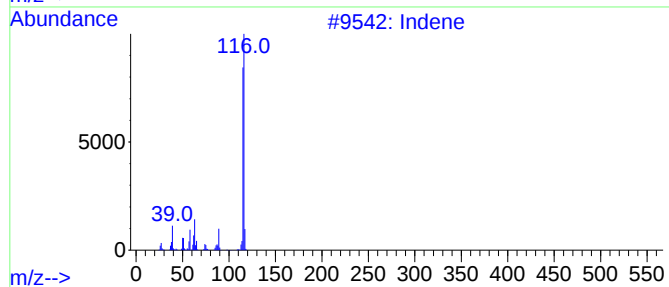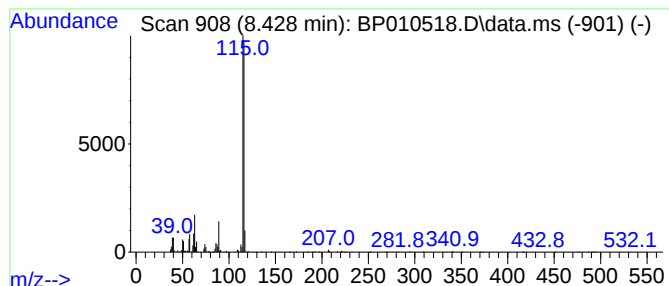

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010518.D
Acq On : 24 May 2022 16:18
Operator : CG/JU
Sample : N2950-03DL2 100X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTE9DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indene	8.428	2.1	ng/ul	106968	1	7.887	1009930	20.0