

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010524.D
 Acq On : 24 May 2022 19:41
 Operator : CG/JU
 Sample : N2950-06
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rVB	22886	34099	0.67%	0.079%
2	3.611	87	89	92	rBV4	4276	6210	0.12%	0.014%
3	3.769	113	116	123	rBV	82436	155453	3.05%	0.361%
4	3.987	147	153	158	rBV	19779	34630	0.68%	0.080%
5	4.075	165	168	174	rVB4	8138	13082	0.26%	0.030%
6	4.999	321	325	332	rBV6	6989	12589	0.25%	0.029%
7	5.605	423	428	434	rBV4	4958	9413	0.18%	0.022%
8	7.052	666	674	692	rBV	133559	251051	4.92%	0.583%
9	7.216	695	702	714	rBV	530224	875730	17.17%	2.032%
10	7.416	728	736	750	rBV	528436	893717	17.52%	2.074%
11	7.887	808	816	824	rBV	518248	881380	17.28%	2.046%
12	8.263	872	880	885	rVB2	14425	27926	0.55%	0.065%
13	8.428	903	908	912	rVB3	6807	10961	0.21%	0.025%
14	8.593	929	936	953	rBV	440050	759195	14.88%	1.762%
15	9.046	1004	1013	1030	rBV	745864	1303918	25.56%	3.026%
16	9.481	1084	1087	1093	rVB7	4689	7377	0.14%	0.017%
17	9.769	1128	1136	1150	rBV	598055	1039729	20.38%	2.413%
18	10.310	1219	1228	1248	rBV	751367	1431603	28.06%	3.323%
19	10.687	1283	1292	1298	rBV	813331	1404706	27.54%	3.260%
20	10.822	1307	1315	1333	rBV	653956	1332123	26.11%	3.092%
21	11.522	1429	1434	1437	rBV6	3667	8208	0.16%	0.019%
22	11.792	1474	1480	1482	rBV7	2840	5437	0.11%	0.013%
23	11.981	1508	1512	1518	rVB4	9473	14456	0.28%	0.034%
24	12.281	1558	1563	1569	rVB4	11579	23259	0.46%	0.054%
25	12.569	1607	1612	1617	rVB3	11630	20897	0.41%	0.048%
26	12.887	1657	1666	1671	rBV10	4615	9661	0.19%	0.022%
27	13.057	1689	1695	1699	rVB9	2412	5119	0.10%	0.012%
28	13.351	1736	1745	1754	rVB9	3740	10155	0.20%	0.024%
29	13.498	1764	1770	1776	rBV10	4746	9413	0.18%	0.022%
30	13.845	1824	1829	1834	rVB9	4065	6109	0.12%	0.014%
31	13.928	1836	1843	1856	rBV	1784046	2548347	49.95%	5.914%
32	14.210	1881	1891	1908	rBV	1900574	2857044	56.01%	6.631%
33	14.516	1935	1943	1950	rBV	1358258	1940235	38.03%	4.503%
34	14.581	1950	1954	1960	rVB	55218	80976	1.59%	0.188%
35	14.657	1963	1967	1971	rVB4	4825	6392	0.13%	0.015%
36	14.734	1974	1980	1987	rBV3	45253	119529	2.34%	0.277%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010524.D
 Acq On : 24 May 2022 19:41
 Operator : CG/JU
 Sample : N2950-06
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	14.922	2006	2012	2023	rVB	44195	81972	1.61%	0.190%
38	15.263	2065	2070	2075	rVV6	5071	10226	0.20%	0.024%
39	15.322	2075	2080	2082	rVV4	5994	8171	0.16%	0.019%
40	15.510	2105	2112	2118	rBV	2572444	3723277	72.99%	8.641%
41	15.557	2118	2120	2126	rVV3	46747	77593	1.52%	0.180%
42	15.633	2127	2133	2147	rVV	618315	957092	18.76%	2.221%
43	15.751	2149	2153	2161	rVB2	32055	52481	1.03%	0.122%
44	15.875	2170	2174	2179	rVB7	5036	8918	0.17%	0.021%
45	16.204	2225	2230	2232	rBV6	4184	6029	0.12%	0.014%
46	16.233	2232	2235	2242	rVV8	9355	21107	0.41%	0.049%
47	16.298	2242	2246	2249	rVV5	10675	17456	0.34%	0.041%
48	16.775	2323	2327	2330	rBV4	4764	7022	0.14%	0.016%
49	16.922	2349	2352	2354	rBV4	3903	5151	0.10%	0.012%
50	16.945	2354	2356	2360	rVB4	6956	9406	0.18%	0.022%
51	17.086	2375	2380	2387	rVB5	7868	15706	0.31%	0.036%
52	17.269	2404	2411	2417	rVV	1656877	2355619	46.18%	5.467%
53	17.369	2421	2428	2442	rVB	3095995	4420137	86.65%	10.258%
54	17.563	2458	2461	2463	rBV4	4143	5717	0.11%	0.013%
55	17.680	2477	2481	2485	rVB	13131	20926	0.41%	0.049%
56	17.775	2493	2497	2499	rBV5	4446	5604	0.11%	0.013%
57	17.845	2504	2509	2514	rBV4	9679	19137	0.38%	0.044%
58	17.886	2514	2516	2520	rVB4	5118	5144	0.10%	0.012%
59	17.939	2520	2525	2528	rBV7	6873	9804	0.19%	0.023%
60	18.104	2550	2553	2556	rBV5	3640	5189	0.10%	0.012%
61	18.157	2557	2562	2566	rBV4	29243	45365	0.89%	0.105%
62	19.180	2730	2736	2740	rBV3	41622	63986	1.25%	0.149%
63	19.245	2744	2747	2752	rBV	34752	49357	0.97%	0.115%
64	19.380	2768	2770	2773	rBV3	12404	15745	0.31%	0.037%
65	19.533	2792	2796	2800	rBV3	18788	24750	0.49%	0.057%
66	19.604	2801	2808	2822	rBV	3694645	5101395	100.00%	11.840%
67	21.057	3052	3055	3062	rBV3	82632	132964	2.61%	0.309%
68	21.351	3100	3105	3112	rBV	1535602	2067461	40.53%	4.798%
69	23.027	3387	3390	3395	rVB2	104945	149121	2.92%	0.346%
70	23.615	3483	3490	3507	rVB2	1599589	3551994	69.63%	8.244%
71	23.774	3510	3517	3531	rVB	765117	1672379	32.78%	3.881%
72	24.392	3620	3622	3632	rVB2	126131	214344	4.20%	0.497%


Sum of corrected areas: 43087874

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010524.D
Acq On : 24 May 2022 19:41
Operator : CG/JU
Sample : N2950-06
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

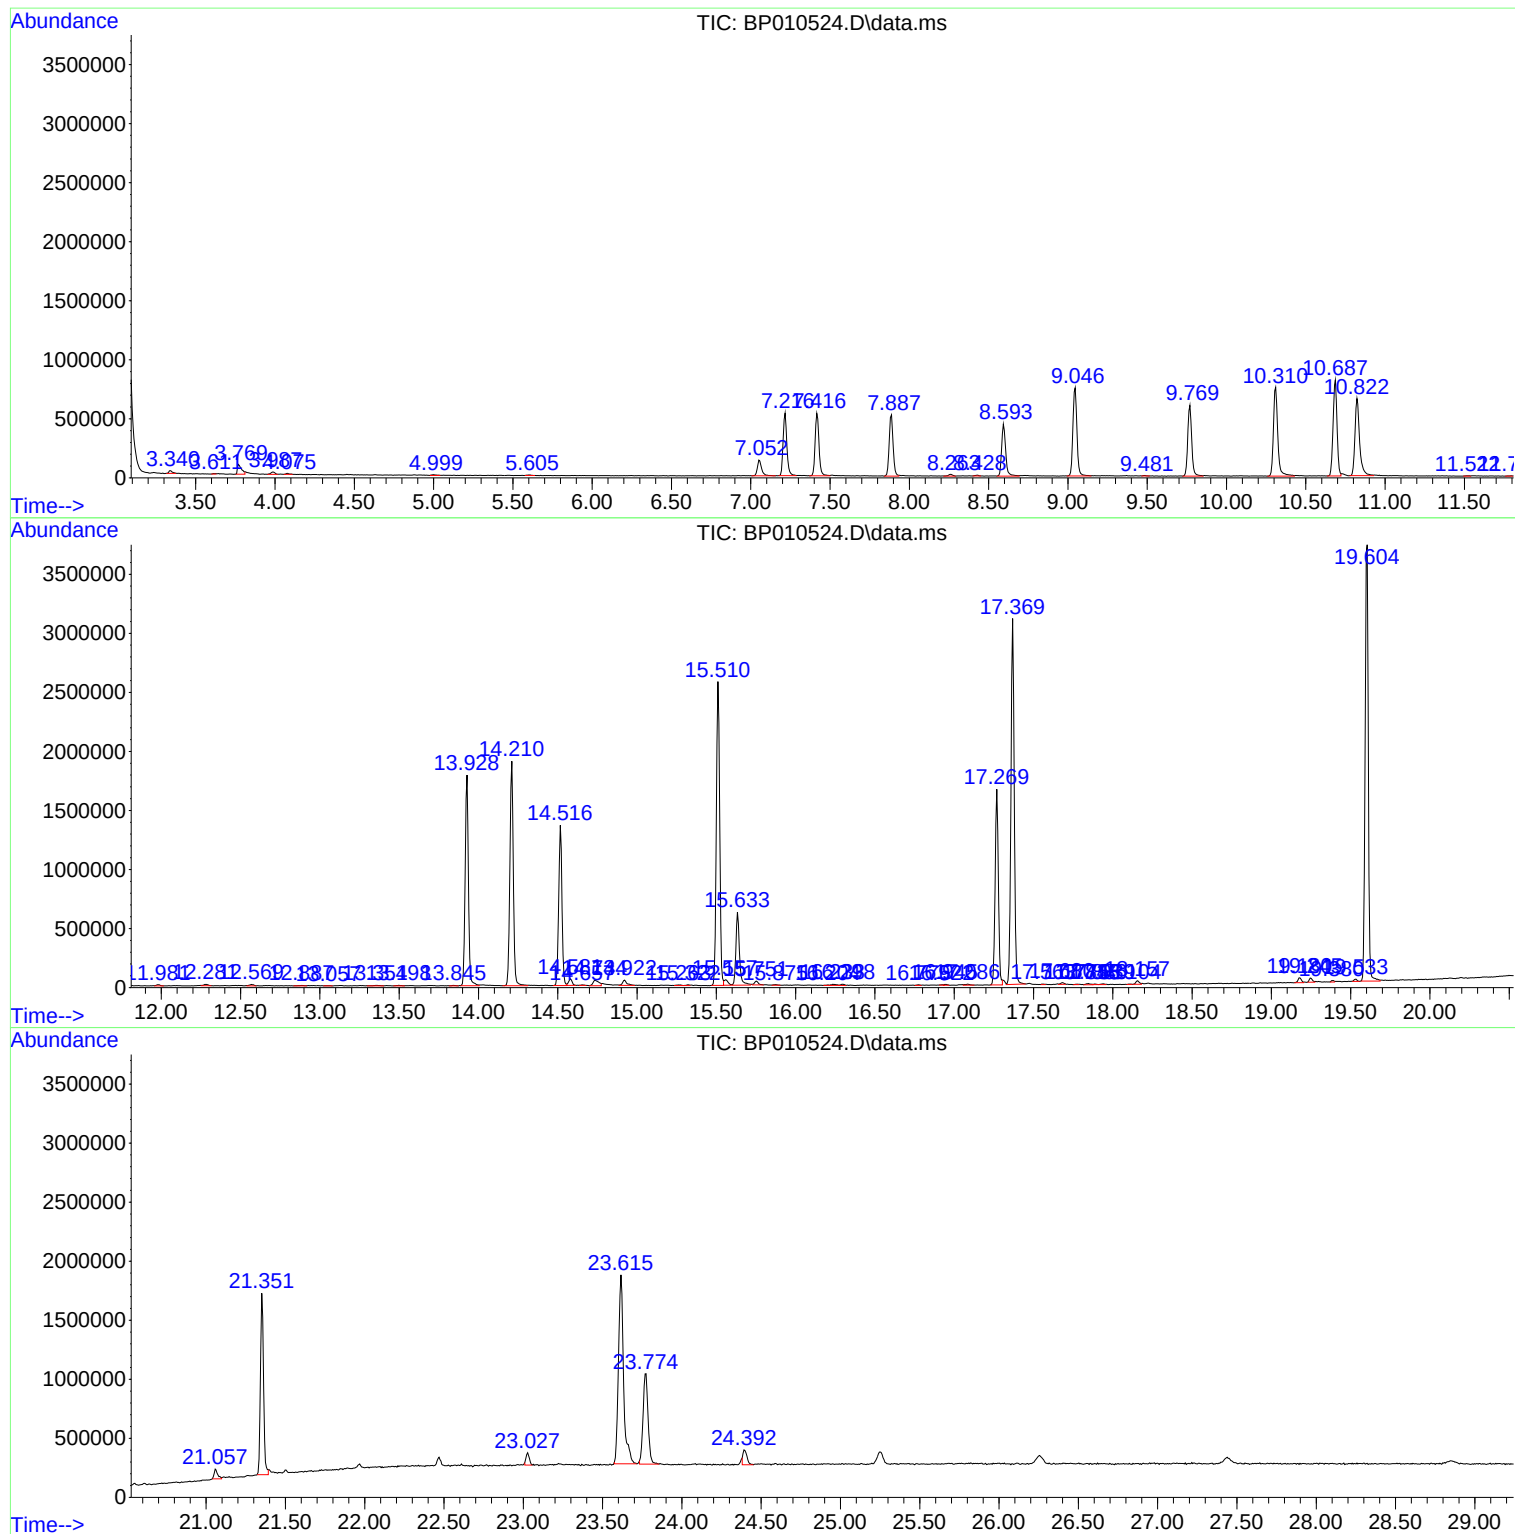

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010524.D
Acq On : 24 May 2022 19:41
Operator : CG/JU
Sample : N2950-06
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTG4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.392	2.56 ng/ul	214344	Perylene-d12	23.774

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Octadecane	254	C18H38	000593-45-3	96
2			Tridecane, 1-iodo-	310	C13H27I	035599-77-0	86
3			Heptadecane, 9-octyl-	352	C25H52	007225-64-1	86
4			Octadecane, 5,14-dibutyl-	366	C26H54	055282-13-8	86
5			Docosane, 5-butyl-	366	C26H54	055282-16-1	86

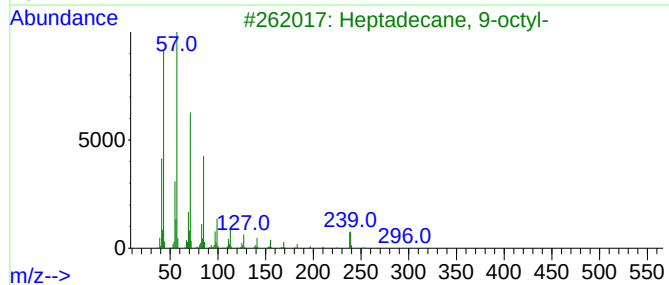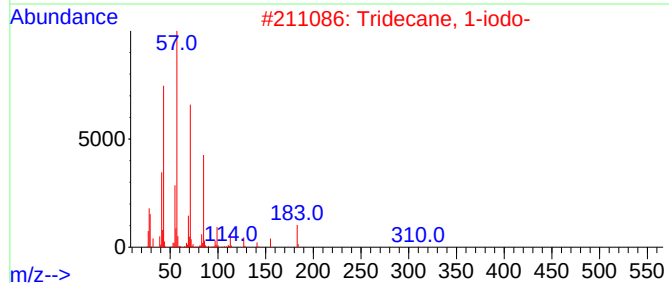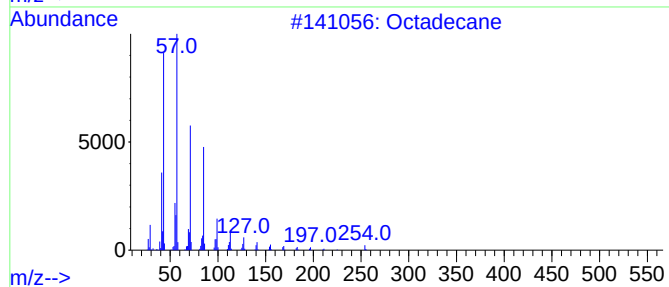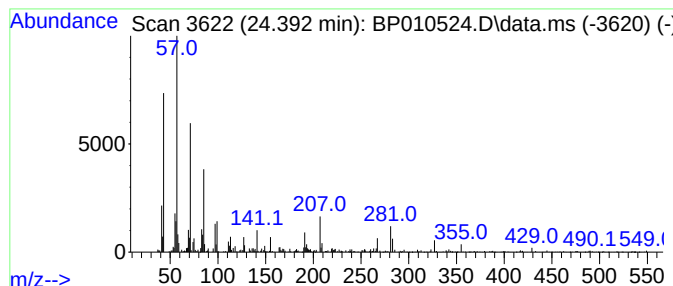

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010524.D
Acq On : 24 May 2022 19:41
Operator : CG/JU
Sample : N2950-06
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.392	2.6	ng/u1	214344	6	23.774	1672380	20.0