

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010525.D
 Acq On : 24 May 2022 20:14
 Operator : CG/JU
 Sample : N2950-11
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	51	rVB	22561	35734	0.76%	0.092%
2	3.769	113	116	131	rBV	87905	198002	4.23%	0.510%
3	3.987	149	153	159	rVB	16133	25532	0.55%	0.066%
4	4.081	166	169	175	rVB3	9782	14741	0.31%	0.038%
5	4.998	319	325	328	rBV6	5901	9659	0.21%	0.025%
6	5.475	401	406	409	rBV7	3470	5115	0.11%	0.013%
7	5.604	424	428	434	rVB4	6598	9874	0.21%	0.025%
8	7.051	668	674	684	rBV	110265	198471	4.24%	0.511%
9	7.216	695	702	714	rBV	453761	762177	16.28%	1.963%
10	7.416	729	736	749	rBV	450181	763129	16.30%	1.965%
11	7.887	808	816	825	rBV	458483	761445	16.26%	1.961%
12	7.957	825	828	833	rVB4	6140	10261	0.22%	0.026%
13	8.592	929	936	953	rBV	371007	653585	13.96%	1.683%
14	8.734	955	960	964	rVB8	4510	8700	0.19%	0.022%
15	9.045	1005	1013	1025	rBV	656527	1158638	24.74%	2.984%
16	9.481	1084	1087	1091	rVB6	4358	6663	0.14%	0.017%
17	9.769	1128	1136	1151	rBV	524828	917255	19.59%	2.362%
18	10.310	1219	1228	1245	rBV	668977	1260126	26.91%	3.246%
19	10.686	1283	1292	1308	rBV	696912	1240105	26.48%	3.194%
20	10.822	1308	1315	1335	rBV	598099	1200084	25.63%	3.091%
21	11.057	1347	1355	1356	rBV7	7217	11126	0.24%	0.029%
22	11.275	1387	1392	1397	rBV7	4632	7843	0.17%	0.020%
23	11.516	1428	1433	1435	rBV6	2903	5362	0.11%	0.014%
24	11.980	1507	1512	1516	rBV6	4552	7347	0.16%	0.019%
25	12.092	1524	1531	1535	rBV8	7342	14120	0.30%	0.036%
26	12.245	1553	1557	1559	rBV4	3909	5483	0.12%	0.014%
27	12.286	1559	1564	1569	rVB2	11983	22572	0.48%	0.058%
28	12.880	1662	1665	1670	rBV7	2712	5029	0.11%	0.013%
29	13.369	1742	1748	1750	rBV6	3996	6799	0.15%	0.018%
30	13.927	1832	1843	1855	rBV	1569023	2250159	48.05%	5.795%
31	14.210	1880	1891	1906	rBV	1716971	2535607	54.15%	6.531%
32	14.516	1936	1943	1958	rBV	1164961	1736926	37.09%	4.474%
33	14.657	1961	1967	1972	rVB2	9443	18210	0.39%	0.047%
34	14.733	1972	1980	1995	rBV2	48345	154749	3.30%	0.399%
35	14.951	2015	2017	2023	rVB6	5317	7291	0.16%	0.019%
36	15.180	2054	2056	2062	rVB6	3494	5385	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
 Data File : BP010525.D
 Acq On : 24 May 2022 20:14
 Operator : CG/JU
 Sample : N2950-11
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBTD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
 Title : SVOA CALIBRATION

37	15.263	2065	2070	2076	rVV	17463	28359	0.61%	0.073%
38	15.333	2077	2082	2086	rVB6	4840	8944	0.19%	0.023%
39	15.510	2104	2112	2127	rBV	2385157	3330555	71.13%	8.578%
40	15.633	2127	2133	2147	rVV	638761	993295	21.21%	2.558%
41	15.751	2149	2153	2162	rVB	28147	49444	1.06%	0.127%
42	15.868	2169	2173	2177	rVB5	4522	8182	0.17%	0.021%
43	16.010	2191	2197	2200	rBV5	5549	10135	0.22%	0.026%
44	16.233	2232	2235	2242	rVV9	4349	9568	0.20%	0.025%
45	16.298	2242	2246	2252	rVB4	10271	14833	0.32%	0.038%
46	16.545	2284	2288	2294	rBV8	7135	13185	0.28%	0.034%
47	16.774	2322	2327	2332	rBV9	4120	7352	0.16%	0.019%
48	16.933	2349	2354	2355	rBV5	5897	8464	0.18%	0.022%
49	17.063	2367	2376	2387	rBV5	21988	77872	1.66%	0.201%
50	17.268	2404	2411	2421	rVV	1474191	2138076	45.66%	5.507%
51	17.368	2421	2428	2445	rVB	2812094	3980032	85.00%	10.251%
52	17.651	2472	2476	2477	rBV3	4464	5146	0.11%	0.013%
53	17.780	2493	2498	2502	rBV7	7572	13941	0.30%	0.036%
54	17.839	2505	2508	2512	rVV5	7718	10191	0.22%	0.026%
55	17.939	2521	2525	2529	rVB6	8983	12243	0.26%	0.032%
56	18.104	2550	2553	2556	rBV5	5268	7772	0.17%	0.020%
57	18.157	2558	2562	2566	rVV6	18300	27094	0.58%	0.070%
58	18.221	2570	2573	2578	rVB2	9959	14768	0.32%	0.038%
59	18.633	2639	2643	2645	rBV5	4169	6255	0.13%	0.016%
60	19.180	2731	2736	2742	rVB4	36258	53397	1.14%	0.138%
61	19.262	2743	2750	2760	rBV2	91921	192121	4.10%	0.495%
62	19.598	2801	2807	2819	rBV	3349664	4682573	100.00%	12.060%
63	21.233	3083	3085	3093	rBV7	32358	47139	1.01%	0.121%
64	21.351	3100	3105	3120	rBV	1569529	2132089	45.53%	5.491%
65	23.615	3483	3490	3497	rBV2	1574136	3271993	69.88%	8.427%
66	23.774	3510	3517	3528	rVB2	738915	1638345	34.99%	4.220%




Sum of corrected areas: 38826667

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010525.D
Acq On : 24 May 2022 20:14
Operator : CG/JU
Sample : N2950-11
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

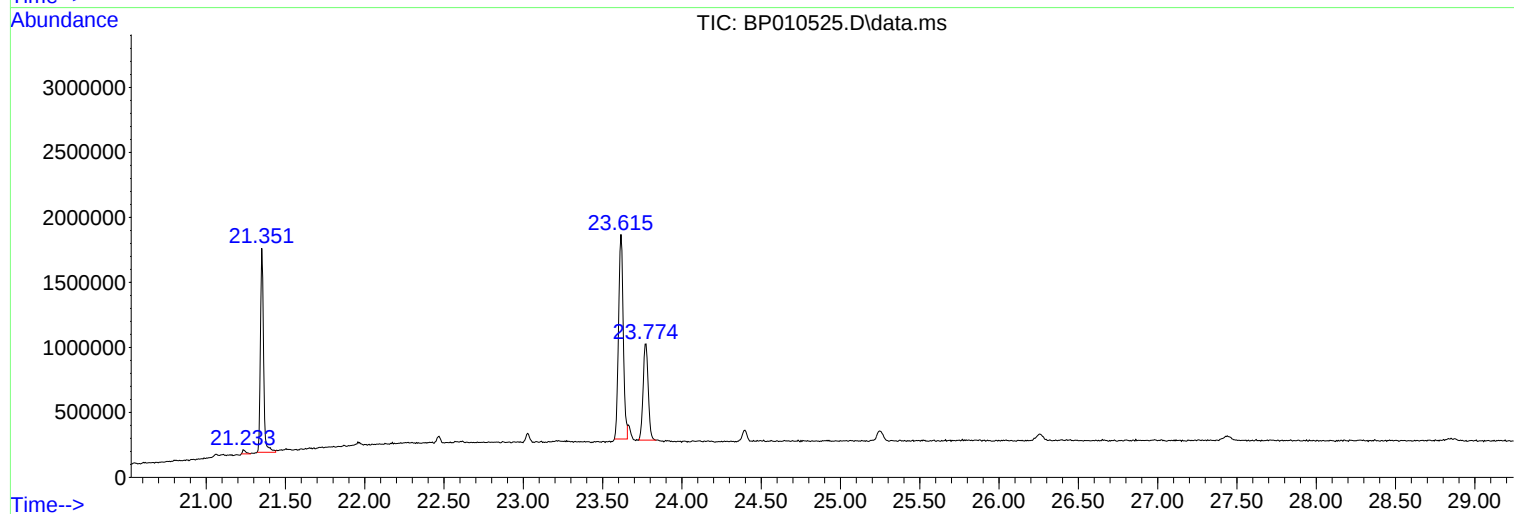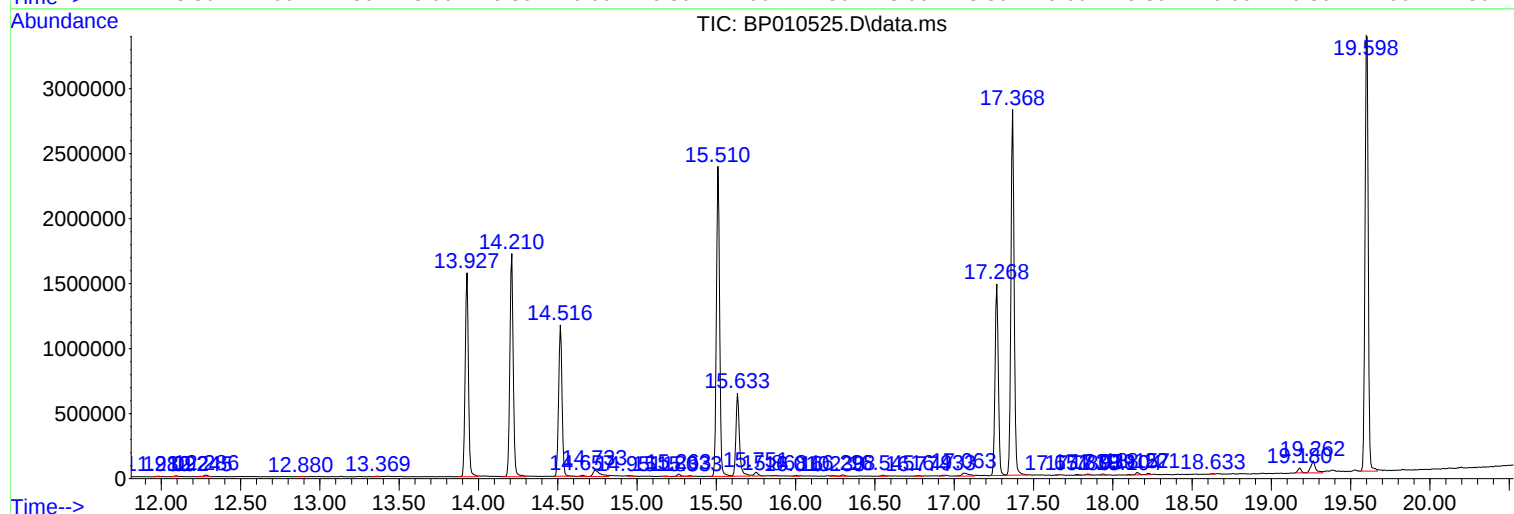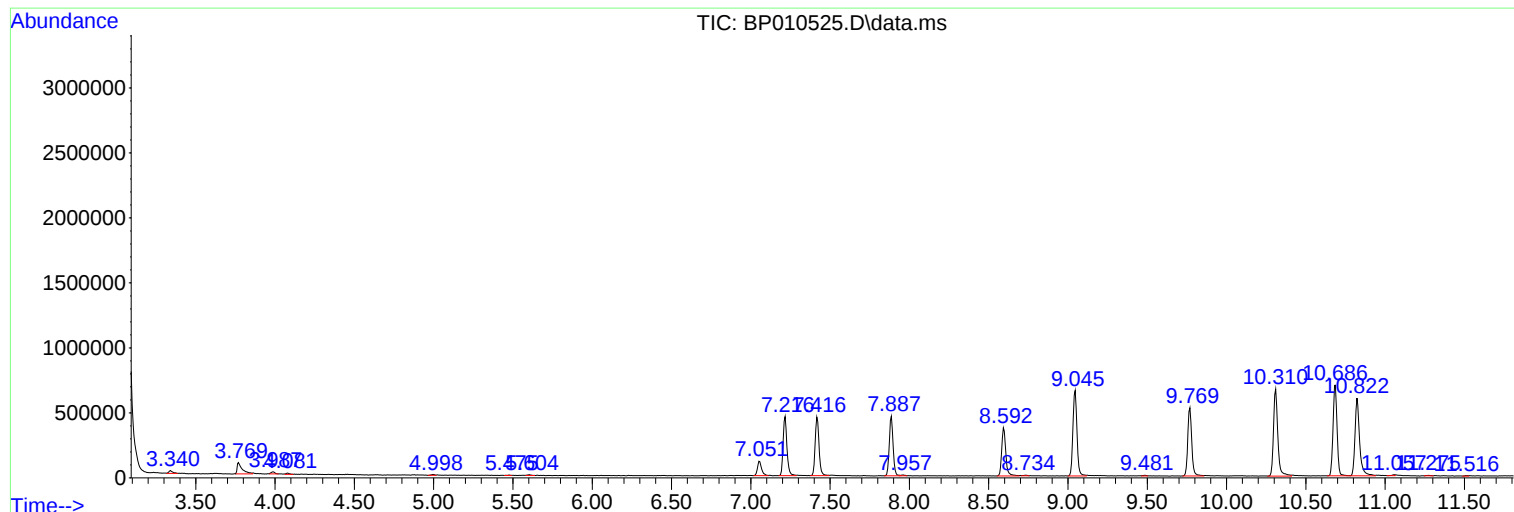

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010525.D
Acq On : 24 May 2022 20:14
Operator : CG/JU
Sample : N2950-11
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052322\
Data File : BP010525.D
Acq On : 24 May 2022 20:14
Operator : CG/JU
Sample : N2950-11
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBTD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051322.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------